

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090519\
 Data File : VU034260.D
 Acq On : 04 Sep 2019 16:07
 Operator : JC/SP
 Sample : K4547-31
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T7-S-G1-(0)

Quant Time: Sep 05 04:58:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 29 04:11:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	430654	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	694253	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	695780	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.46	152	339307	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	265249	48.07	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.14%	
35) Dibromofluoromethane	4.86	113	227052	47.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.30%	
50) Toluene-d8	7.55	98	903283	50.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.20%	
62) 4-Bromofluorobenzene	10.29	95	311104	44.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.72%	
Target Compounds						
43) Isopropyl Acetate	5.53	43	58008	5.185	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090519\
Data File : VU034260.D
Acq On : 04 Sep 2019 16:07
Operator : JC/SP
Sample : K4547-31
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T7-S-G1-(0)

Quant Time: Sep 05 04:58:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U082919W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 29 04:11:12 2019
Response via : Initial Calibration

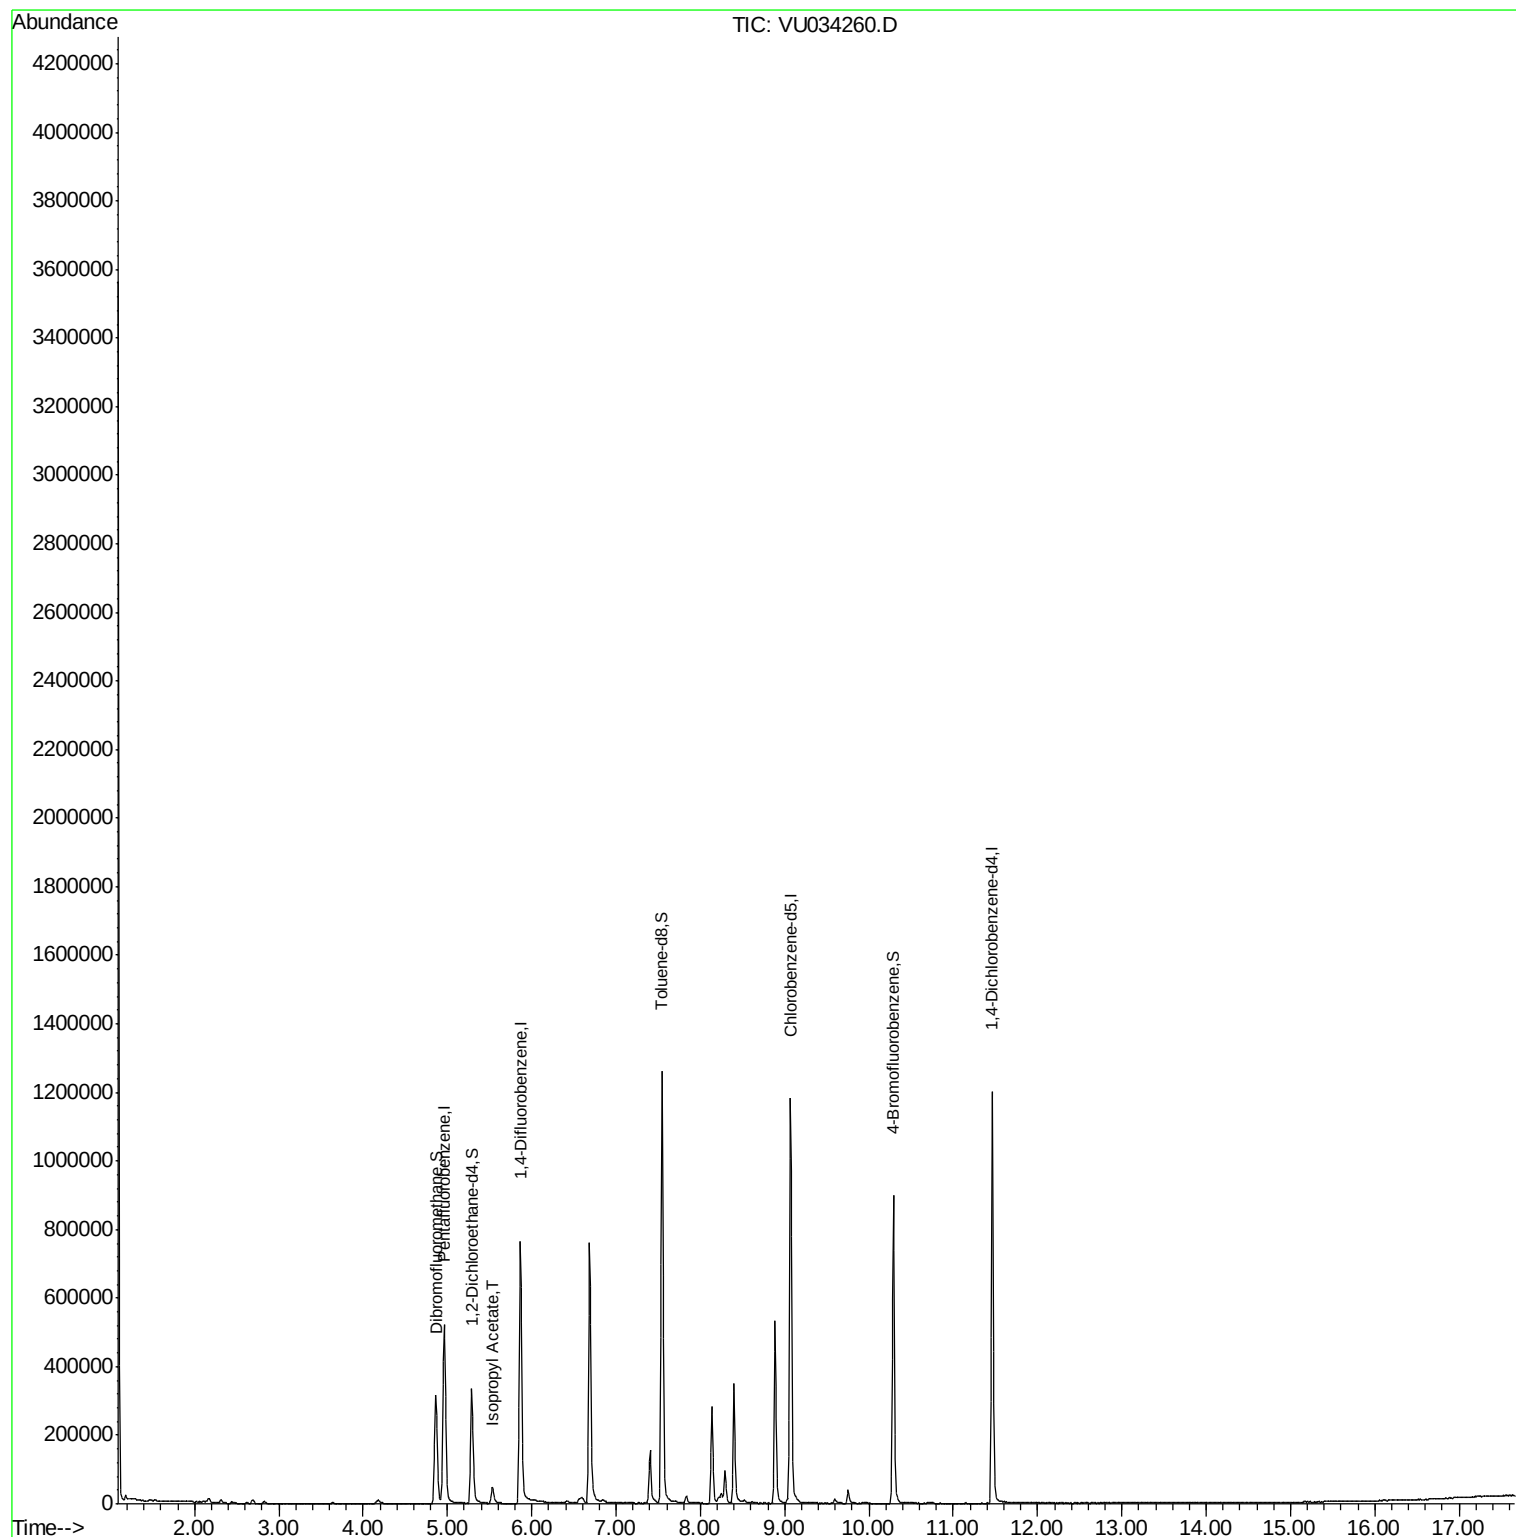

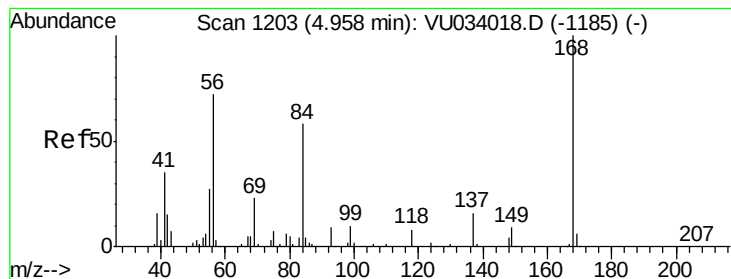

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. 0.00 min

Lab File: VU034260.D

Acq: 04 Sep 2019 16:07

Instrument :

MSVOA_U

ClientSampleId :


T7-S-G1-(0)

Tot Ion:168 Resp: 430654

Ion Ratio Lower Upper

168 100

99 52.2 42.3 63.5

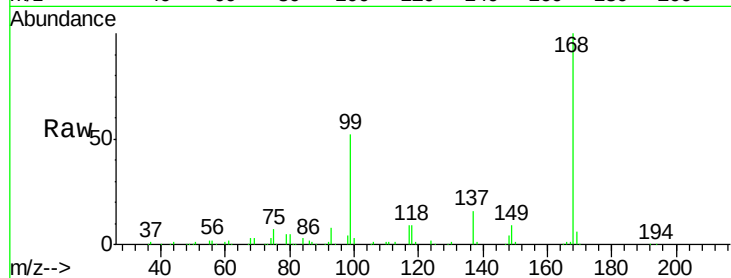

Abundance Ion 167.90 (167.60 to 168.60): VU034260.D (-1185) (-)

Ion 98.90 (98.60 to 99.60): VU034260.D (-1185) (-)

4.96

200000

150000



100000

50000

0

4.90 5.00 5.10

Time-->

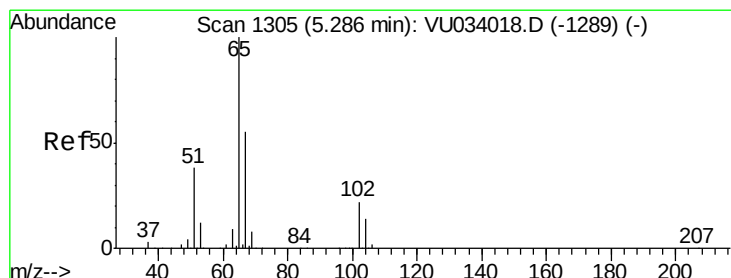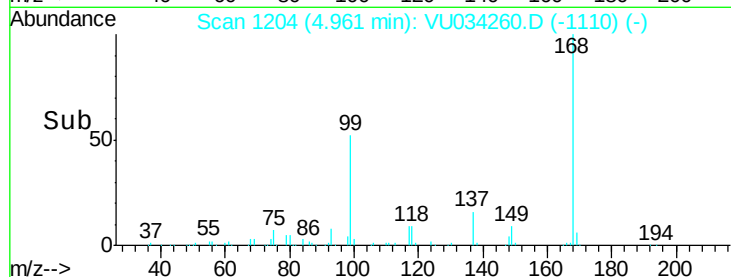

#33

1,2-Dichloroethane-d4

Concen: 48.069 ug/l

RT: 5.29 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU034260.D


Acq: 04 Sep 2019 16:07

Tgt Ion: 65 Resp: 265249

Ion Ratio Lower Upper

65 100

67 55.5 0.0 110.6

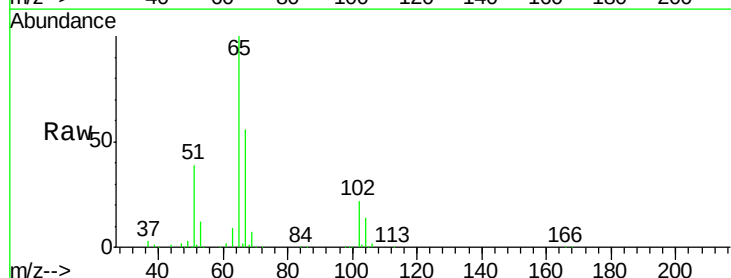

Abundance Ion 64.90 (64.60 to 65.60): VU034260.D (-1289) (-)

Ion 66.90 (66.60 to 67.60): VU034260.D (-1289) (-)

5.29


100000


50000

0

5.20 5.30 5.40

Time-->

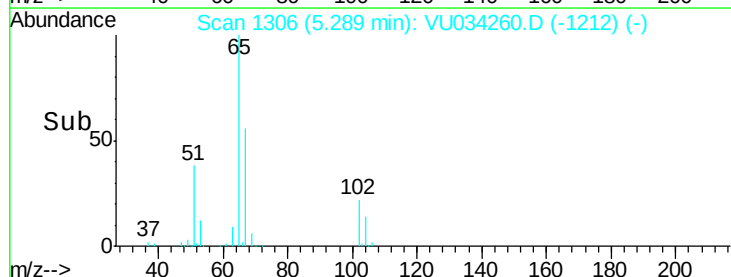

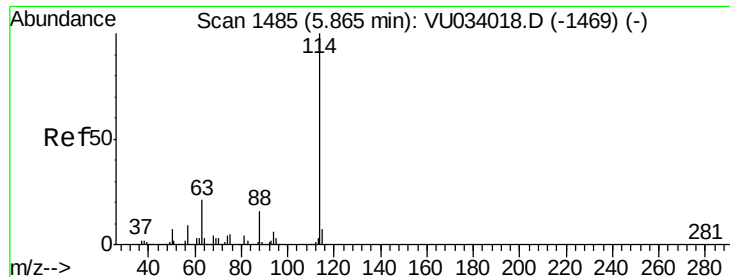

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.87 min Scan# 1486

Delta R.T. 0.00 min

Lab File: VU034260.D

Acq: 04 Sep 2019 16:07

Instrument :

MSVOA_U

ClientSampleId :

T7-S-G1-(0)


Tot Ion:114 Resp: 694253

Ion Ratio Lower Upper

114 100

63 20.2 0.0 42.0




88 16.0 0.0 32.0

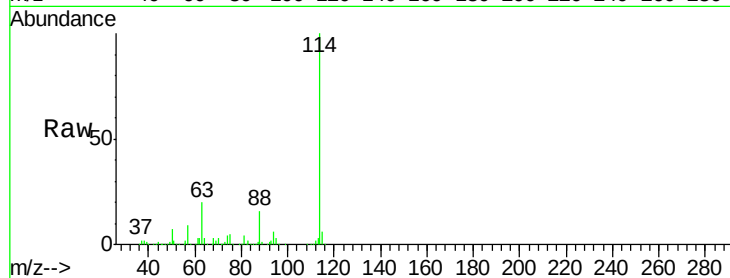

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VU0

Ion 87.90 (87.60 to 88.60): VU0

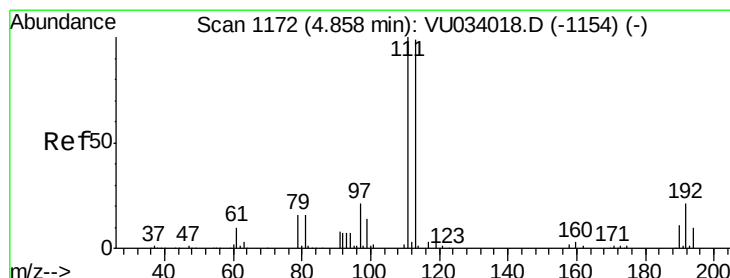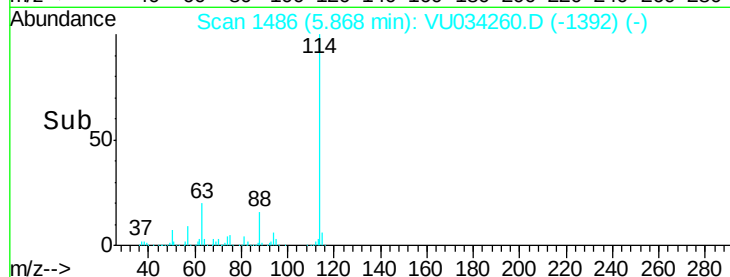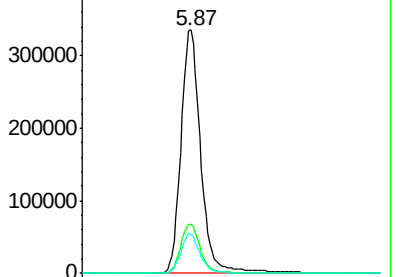

#35

Dibromofluoromethane

Concen: 47.152 ug/l

RT: 4.86 min Scan# 1173

Delta R.T. 0.00 min

Lab File: VU034260.D

Acq: 04 Sep 2019 16:07


Tgt Ion:113 Resp: 227052

Ion Ratio Lower Upper

113 100

111 102.5 81.7 122.5



192 21.7 17.1 25.7

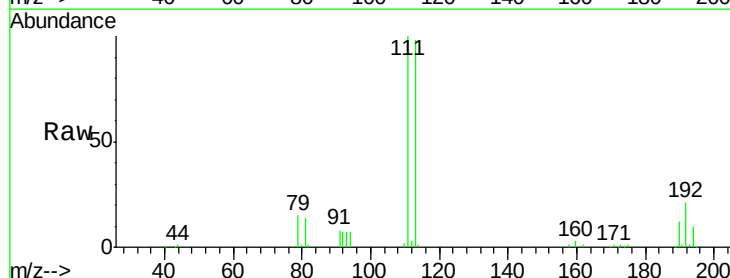


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



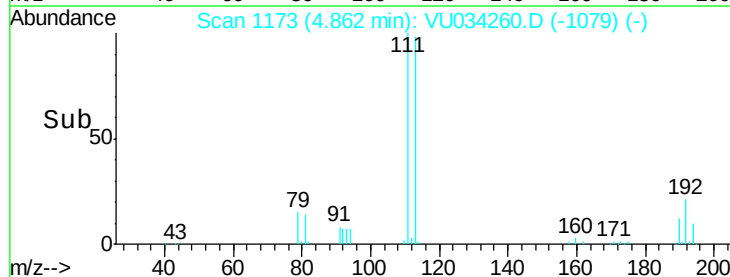
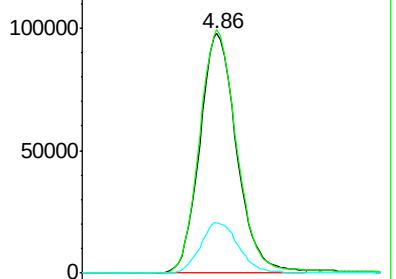


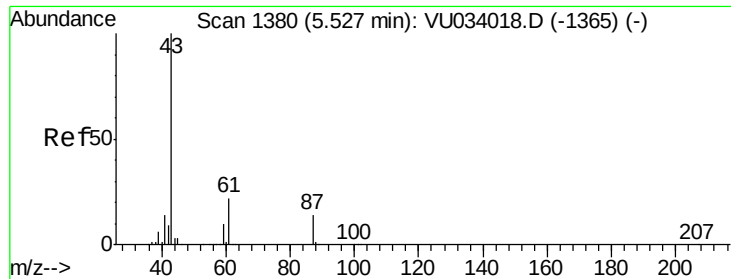

#43
Isopropyl Acetate
Concen: 5.185 ug/l
RT: 5.53 min Scan# 1382
Delta R.T. 0.01 min
Lab File: VU034260.D
Acq: 04 Sep 2019 16:07




Instrument :
MSVOA_U
ClientSampleId :
T7-S-G1-(0)


Tot Ion	43	Resp	58008
Ion Ratio	Lower	Upper	
43	100		
61	21.1	17.2	25.8
87	13.2	10.8	16.2

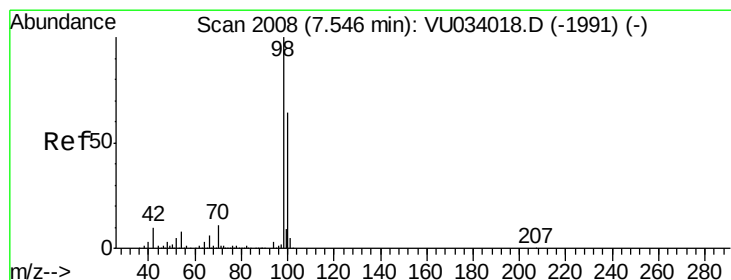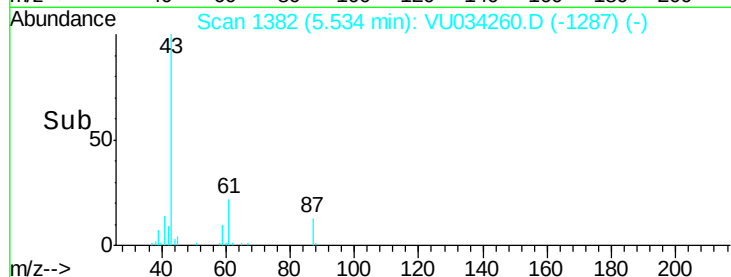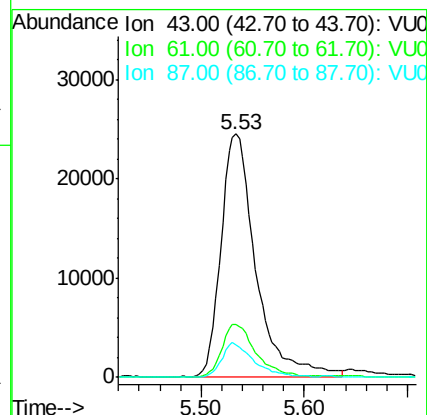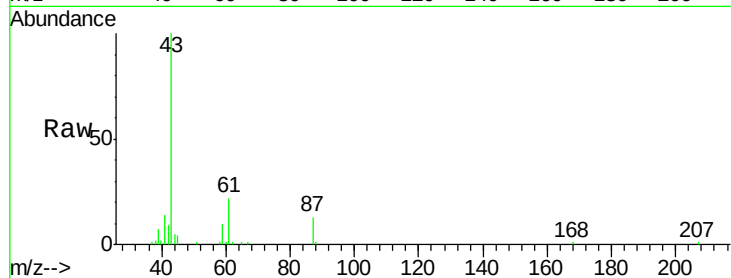

#50
Toluene-d8
Concen: 50.098 ug/l
RT: 7.55 min Scan# 2008
Delta R.T. 0.00 min
Lab File: VU034260.D
Acq: 04 Sep 2019 16:07

Tgt Ion	98	Resp	903283
Ion Ratio	Lower	Upper	
98	100		
100	63.9	50.3	75.5

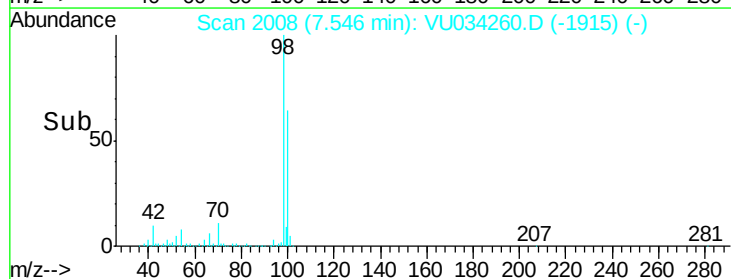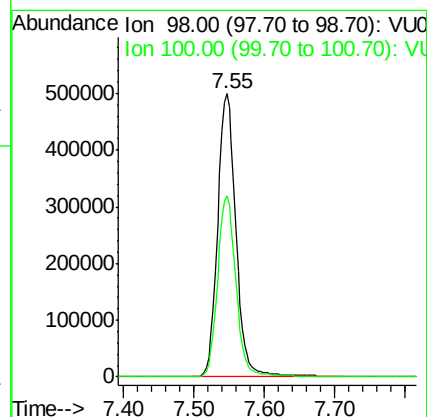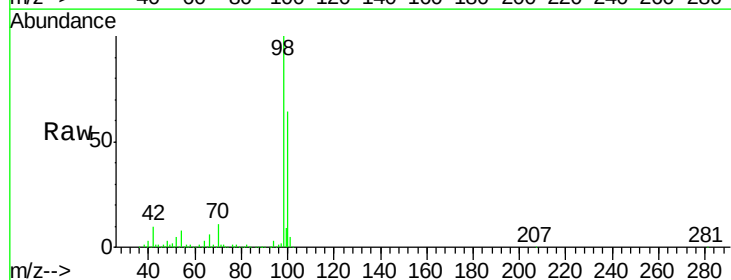

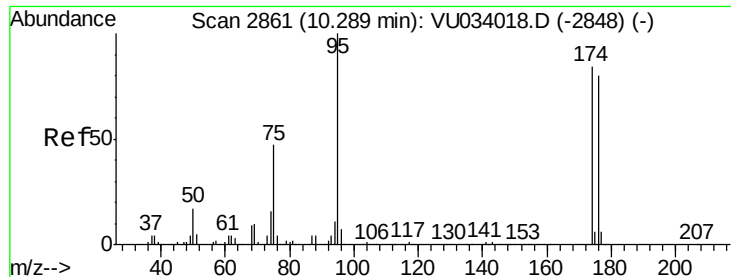

#62

4-Bromofluorobenzene

Concen: 44.358 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. 0.00 min

Lab File: VU034260.D

Acq: 04 Sep 2019 16:07

Instrument :

MSVOA_U

ClientSampleId :

T7-S-G1-(0)


Tot Ion: 95 Resp: 311104

Ion Ratio Lower Upper

95 100

174 86.7 0.0 168.8

176 83.6 0.0 161.8

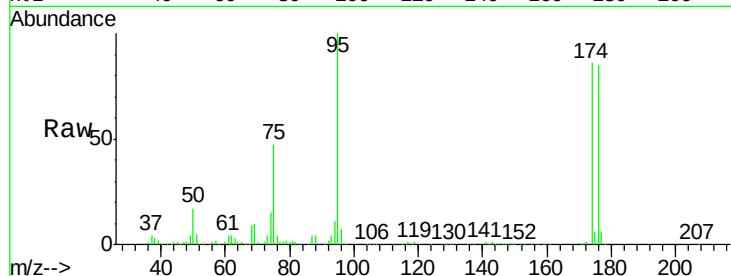


Abundance Ion 94.90 (94.60 to 95.60): VU034018.D (-2848) (-)

Ion 173.80 (173.50 to 174.50): VU034018.D (-2848) (-)

Ion 175.80 (175.50 to 176.50): VU034018.D (-2848) (-)

Time-->

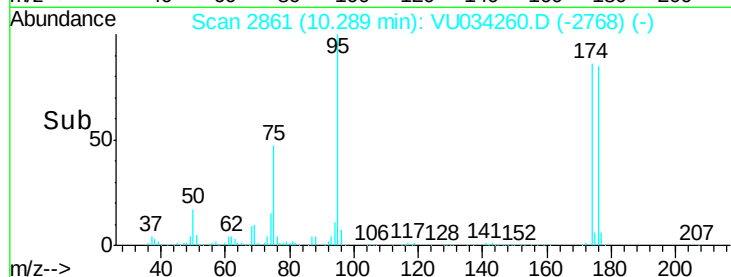


Abundance Ion 94.90 (94.60 to 95.60): VU034260.D (-2768) (-)

Ion 173.80 (173.50 to 174.50): VU034260.D (-2768) (-)

Ion 175.80 (175.50 to 176.50): VU034260.D (-2768) (-)

Time-->

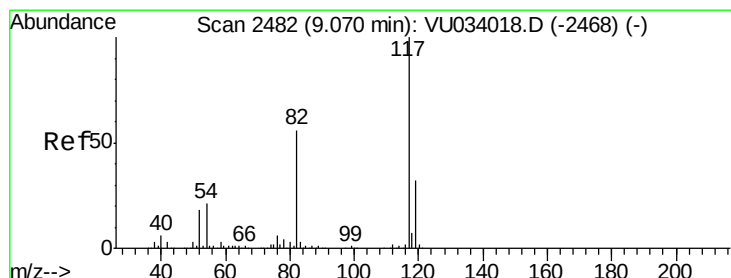

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.07 min Scan# 2482

Delta R.T. 0.00 min

Lab File: VU034260.D

Acq: 04 Sep 2019 16:07


Tgt Ion: 117 Resp: 695780

Ion Ratio Lower Upper

117 100

82 56.1 45.1 67.7

119 31.8 25.4 38.0

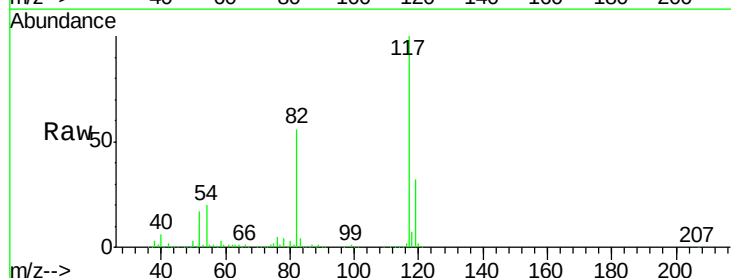


Abundance Ion 116.90 (116.60 to 117.60): VU034018.D (-2468) (-)

Ion 82.00 (81.70 to 82.70): VU034018.D (-2468) (-)

Ion 118.90 (118.60 to 119.60): VU034018.D (-2468) (-)

Time-->

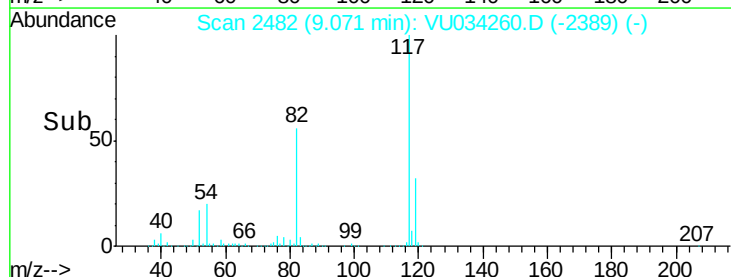


Abundance Ion 116.90 (116.60 to 117.60): VU034260.D (-2389) (-)

Ion 82.00 (81.70 to 82.70): VU034260.D (-2389) (-)

Ion 118.90 (118.60 to 119.60): VU034260.D (-2389) (-)

Time-->

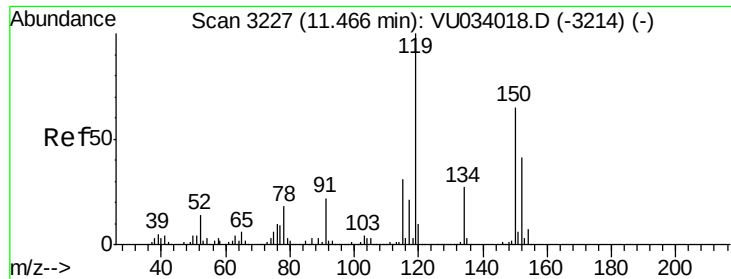

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.46 min Scan# 3226

Delta R.T. -0.00 min

Lab File: VU034260.D

Acq: 04 Sep 2019 16:07

Instrument :

MSVOA_U

ClientSampleId :

T7-S-G1-(0)


Tot Ion:152 Resp: 339307

Ion Ratio Lower Upper

152 100

115 56.7 41.1 123.3

150 155.2 0.0 348.8

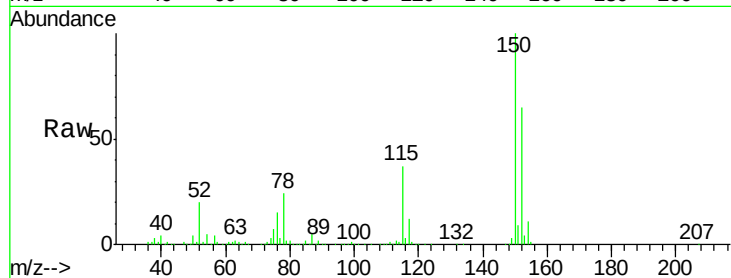

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

