

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
 Data File : VU055084.D
 Acq On : 05 Sep 2023 11:11
 Operator : MD/SY
 Sample : VU0905WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK025

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU055084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	108	rVB	59391	69312	10.42%	1.204%
2	1.907	184	192	207	rVB	70446	92490	13.91%	1.607%
3	2.560	384	395	412	rBV	130773	216493	32.55%	3.762%
4	3.042	534	545	557	rBV4	7916	15094	2.27%	0.262%
5	4.624	1027	1037	1071	rBV	96882	266606	40.09%	4.632%
6	5.062	1157	1173	1193	rBV	128739	291266	43.79%	5.061%
7	5.724	1359	1379	1400	rBV2	258729	665100	100.00%	11.556%
8	6.245	1527	1541	1563	rBV	243264	468269	70.41%	8.136%
9	6.537	1621	1632	1647	rVB10	8442	17334	2.61%	0.301%
10	6.689	1664	1679	1698	rBV	164367	330438	49.68%	5.741%
11	7.566	1940	1952	1970	rBV	62000	117151	17.61%	2.036%
12	7.897	2042	2055	2073	rBV	307337	542724	81.60%	9.430%
13	8.180	2132	2143	2162	rBV	37216	65344	9.82%	1.135%
14	8.634	2272	2284	2323	rBV2	282319	639284	96.12%	11.108%
15	9.415	2514	2527	2550	rBV	361774	622340	93.57%	10.813%
16	10.753	2930	2943	2958	rBV	118035	196167	29.49%	3.408%
17	11.810	3260	3272	3291	rBV	375638	614638	92.41%	10.679%
18	12.193	3379	3391	3411	rBV	282002	479357	72.07%	8.329%
19	13.846	3897	3905	3915	rBV6	8673	13310	2.00%	0.231%
20	14.093	3974	3982	3995	rBV2	11204	18661	2.81%	0.324%
21	14.335	4048	4057	4068	rVB6	8107	13947	2.10%	0.242%




Sum of corrected areas: 5755325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055084.D
Acq On : 05 Sep 2023 11:11
Operator : MD/SY
Sample : VU0905WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

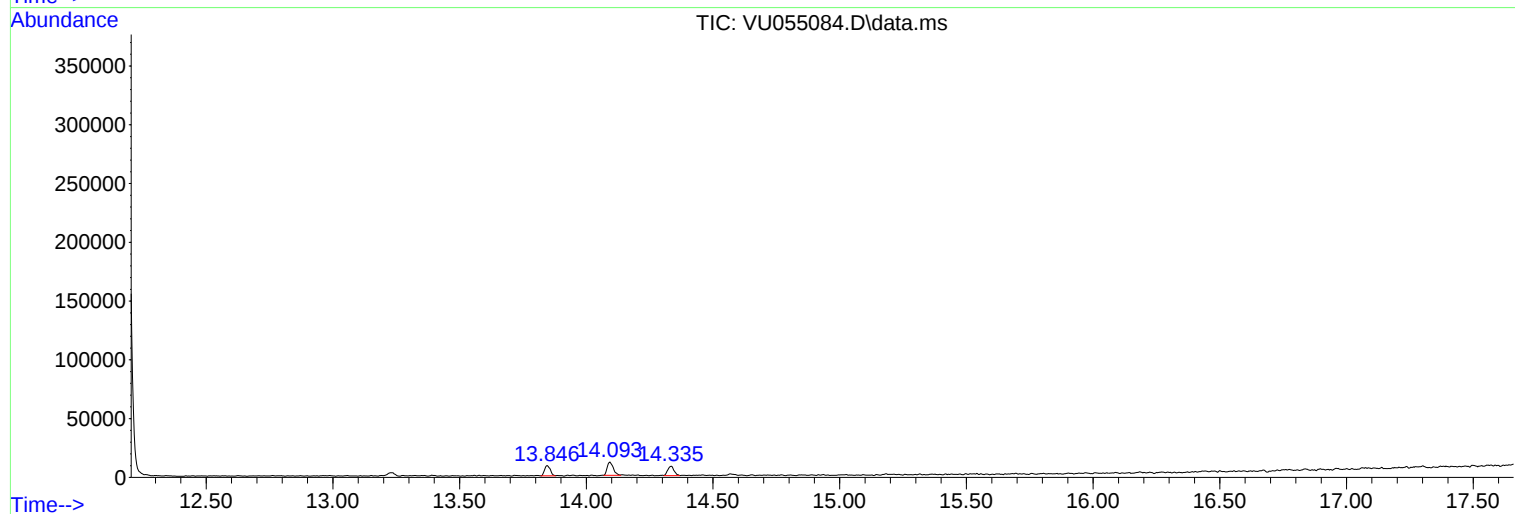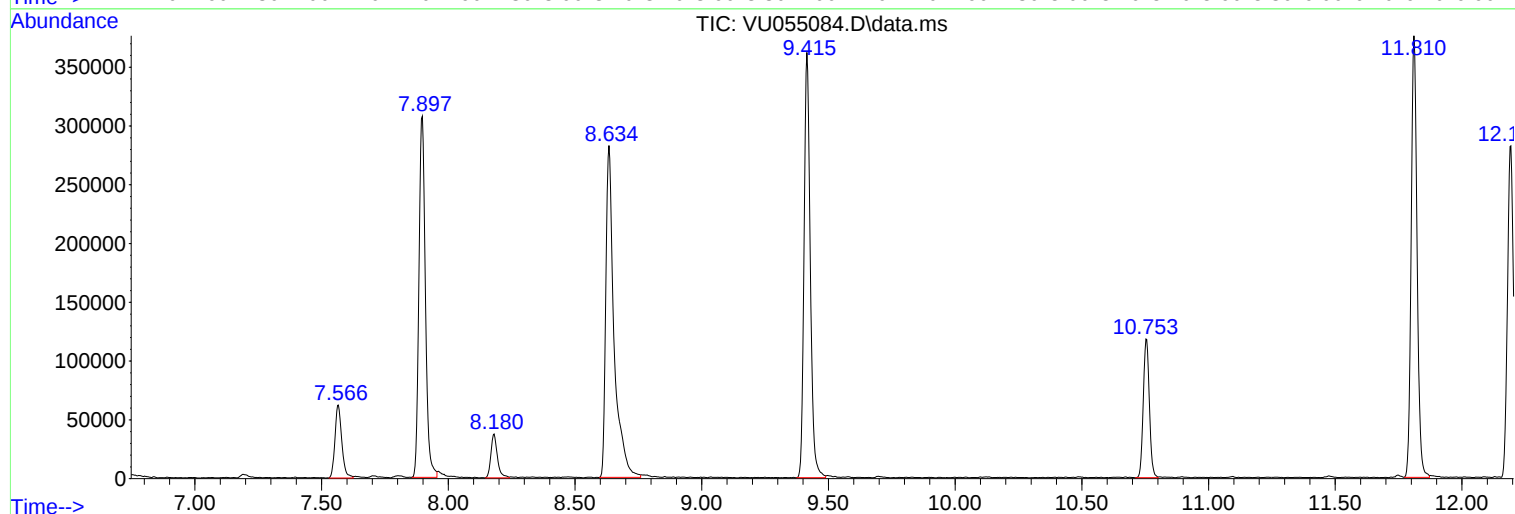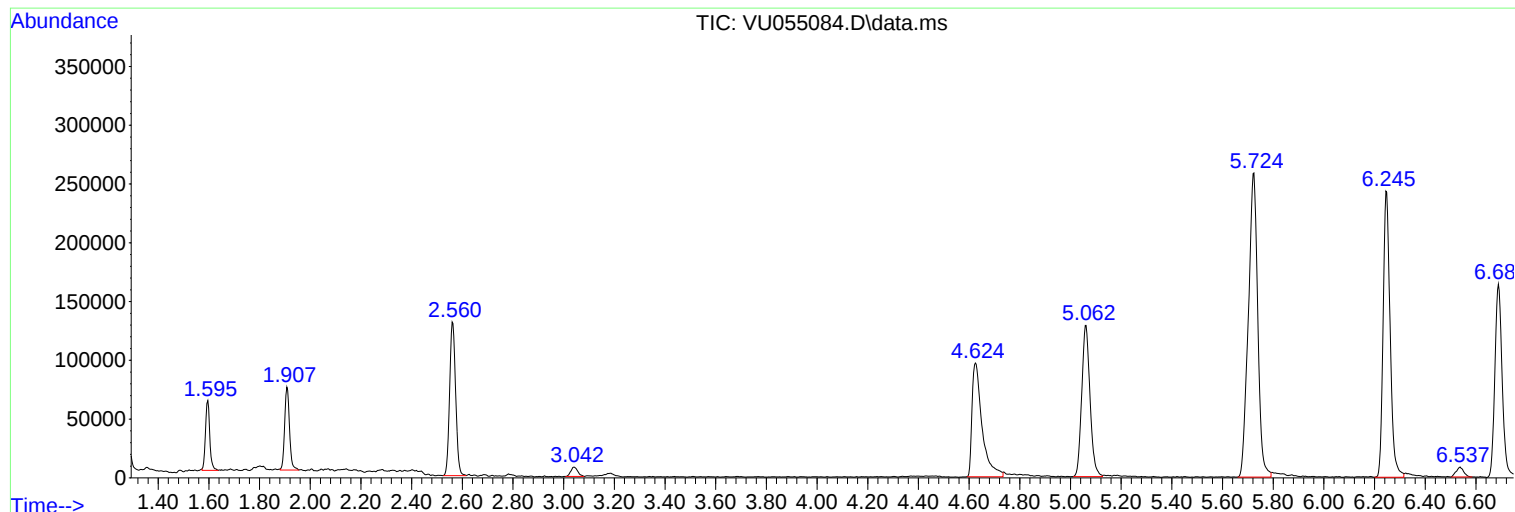

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055084.D
Acq On : 05 Sep 2023 11:11
Operator : MD/SY
Sample : VU0905WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055084.D
Acq On : 05 Sep 2023 11:11
Operator : MD/SY
Sample : VU0905WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc