

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
 Data File : VU055085.D
 Acq On : 05 Sep 2023 11:35
 Operator : MD/SY
 Sample : 04153-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	109	rBV	59852	68973	10.36%	1.205%
2	1.907	184	192	208	rVB	71918	94638	14.22%	1.653%
3	2.563	383	396	412	rBV	132526	217998	32.75%	3.808%
4	3.039	531	544	554	rBV4	7790	13974	2.10%	0.244%
5	4.624	1027	1037	1072	rBV	95682	258185	38.78%	4.510%
6	5.058	1156	1172	1192	rBV	130409	292179	43.89%	5.103%
7	5.724	1355	1379	1401	rBV2	254127	665687	100.00%	11.627%
8	6.248	1529	1542	1561	rBV	237625	463213	69.58%	8.091%
9	6.534	1620	1631	1646	rVB7	8799	17665	2.65%	0.309%
10	6.689	1665	1679	1699	rBV	162755	327621	49.22%	5.723%
11	7.566	1937	1952	1972	rBV2	62021	115845	17.40%	2.023%
12	7.897	2035	2055	2076	rBV	306904	555836	83.50%	9.709%
13	8.180	2131	2143	2157	rBV2	35351	64080	9.63%	1.119%
14	8.634	2271	2284	2326	rBV2	279649	645738	97.00%	11.279%
15	9.415	2514	2527	2557	rBV	354869	610418	91.70%	10.662%
16	10.753	2931	2943	2962	rBV	116781	195288	29.34%	3.411%
17	11.810	3260	3272	3289	rBV2	378524	623266	93.63%	10.887%
18	12.193	3379	3391	3410	rBV	291137	487606	73.25%	8.517%
19	14.100	3976	3984	3996	rVB3	4342	6901	1.04%	0.121%




Sum of corrected areas: 5725111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055085.D
Acq On : 05 Sep 2023 11:35
Operator : MD/SY
Sample : 04153-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

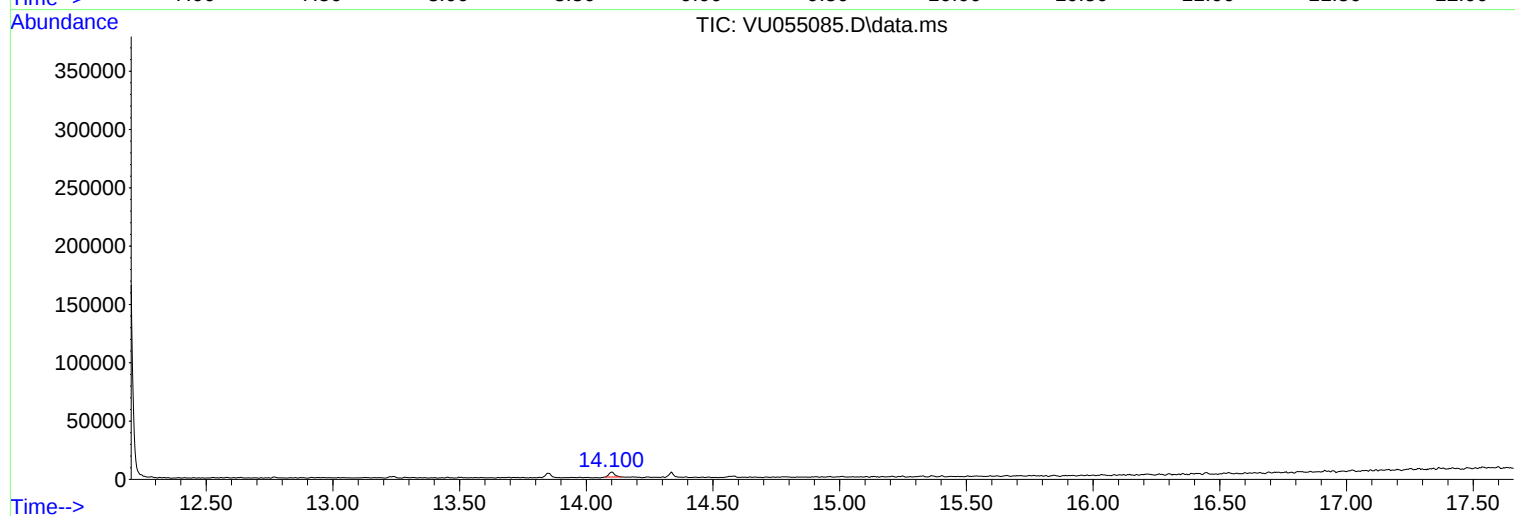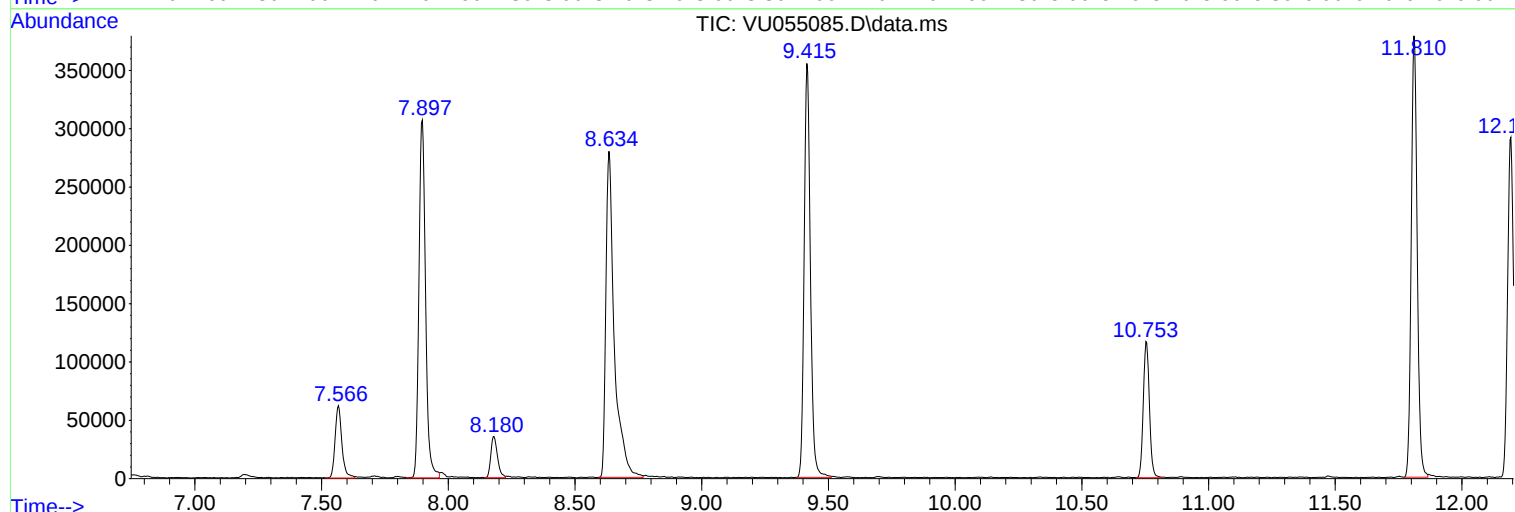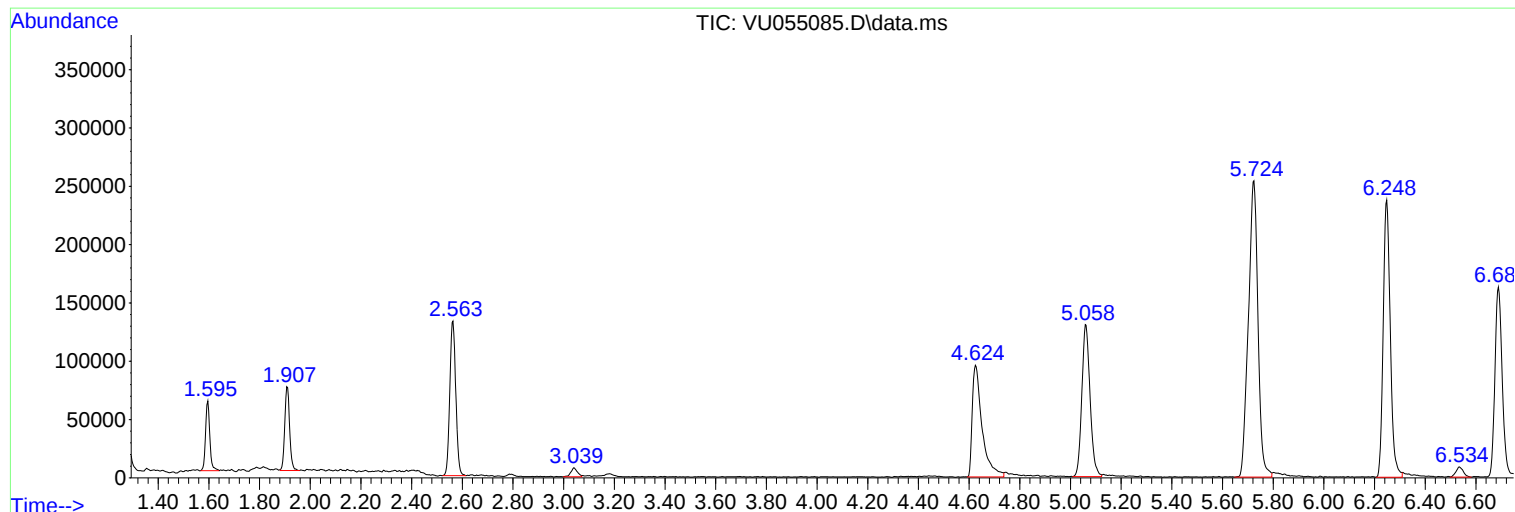

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055085.D
Acq On : 05 Sep 2023 11:35
Operator : MD/SY
Sample : 04153-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055085.D
Acq On : 05 Sep 2023 11:35
Operator : MD/SY
Sample : 04153-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc