

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
 Data File : VU055086.D
 Acq On : 05 Sep 2023 11:59
 Operator : MD/SY
 Sample : 04250-01DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4A0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	54355	62718	8.46%	1.034%
2	1.908	184	192	207	rVB	62292	79300	10.70%	1.307%
3	2.560	384	395	412	rVB	117452	192611	25.99%	3.174%
4	3.043	531	545	559	rBV3	13951	28185	3.80%	0.464%
5	3.184	573	589	616	rVB2	18766	47398	6.40%	0.781%
6	4.628	1021	1038	1043	rBV2	120476	250307	33.78%	4.125%
7	5.059	1156	1172	1194	rBV	116034	261571	35.30%	4.310%
8	5.721	1357	1378	1400	rBV3	230553	605325	81.68%	9.975%
9	6.245	1524	1541	1560	rBV	279457	540946	73.00%	8.914%
10	6.541	1620	1633	1652	rBV	191470	373585	50.41%	6.156%
11	6.689	1665	1679	1700	rBV2	145378	292115	39.42%	4.814%
12	7.566	1940	1952	1970	rBV2	56595	106656	14.39%	1.758%
13	7.898	2041	2055	2073	rBV	273256	490909	66.24%	8.090%
14	8.181	2133	2143	2159	rBV2	33990	58527	7.90%	0.964%
15	8.634	2272	2284	2320	rBV3	256811	588727	79.44%	9.702%
16	9.415	2513	2527	2564	rBV	412711	718182	96.91%	11.835%
17	10.753	2928	2943	2959	rBV	108062	178186	24.04%	2.936%
18	11.811	3259	3272	3290	rBV	451542	741071	100.00%	12.212%
19	12.190	3379	3390	3408	rBV	268336	451920	60.98%	7.447%




Sum of corrected areas: 6068239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055086.D
Acq On : 05 Sep 2023 11:59
Operator : MD/SY
Sample : 04250-01DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

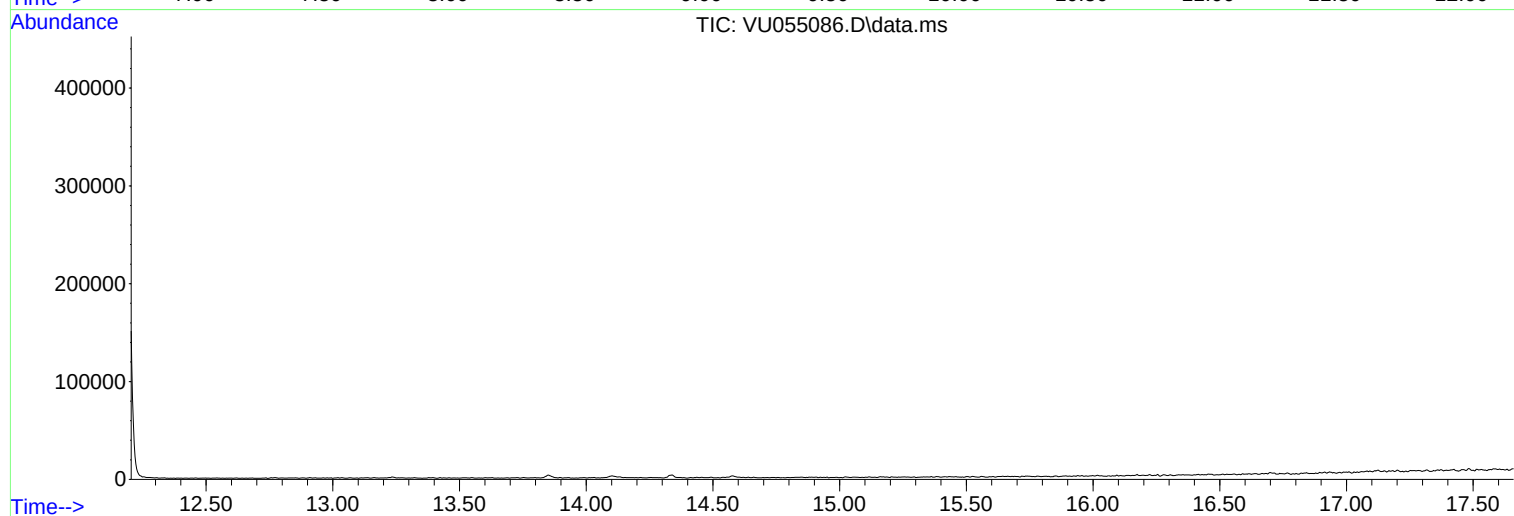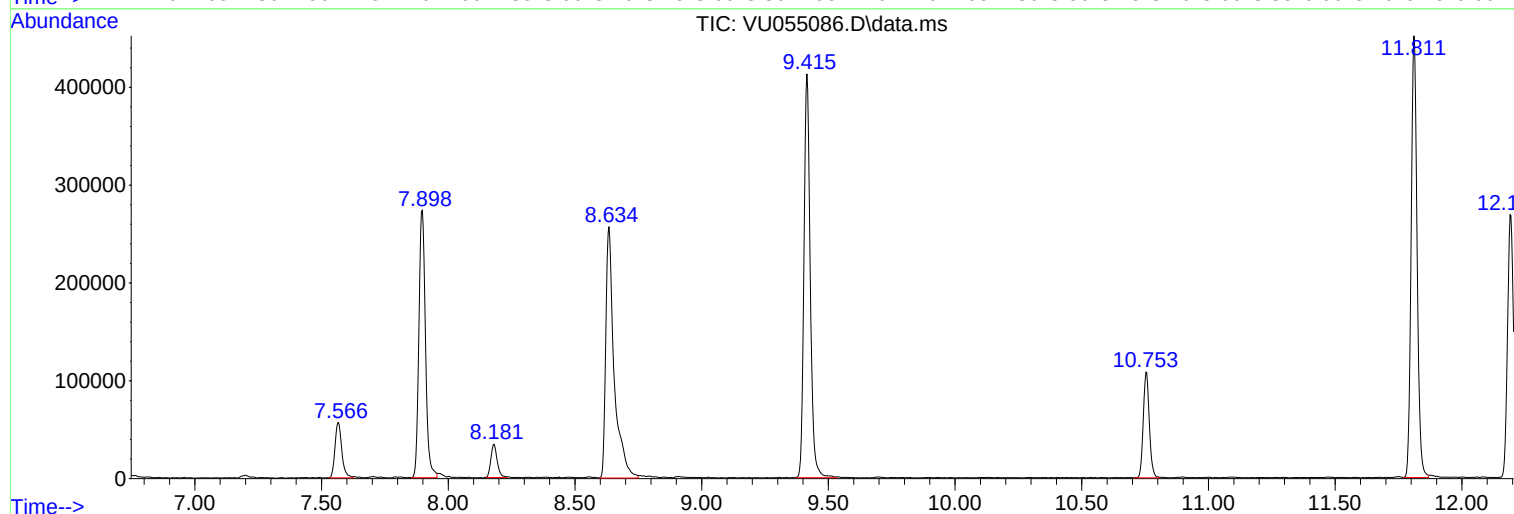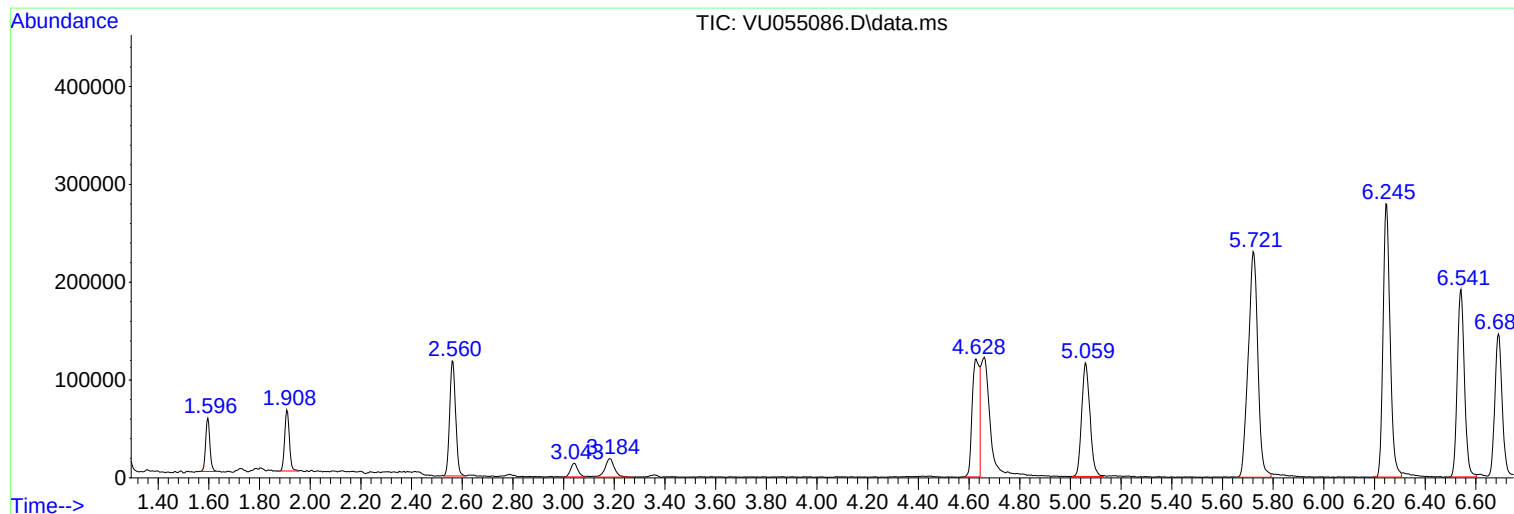

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055086.D
Acq On : 05 Sep 2023 11:59
Operator : MD/SY
Sample : 04250-01DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055086.D
Acq On : 05 Sep 2023 11:59
Operator : MD/SY
Sample : 04250-01DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4A0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc