


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090523\
Data File : VU055082.D
Acq On : 05 Sep 2023 09:07
Operator : MD/SY
Sample : BFB039
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB039

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 06 05:03:37 2023

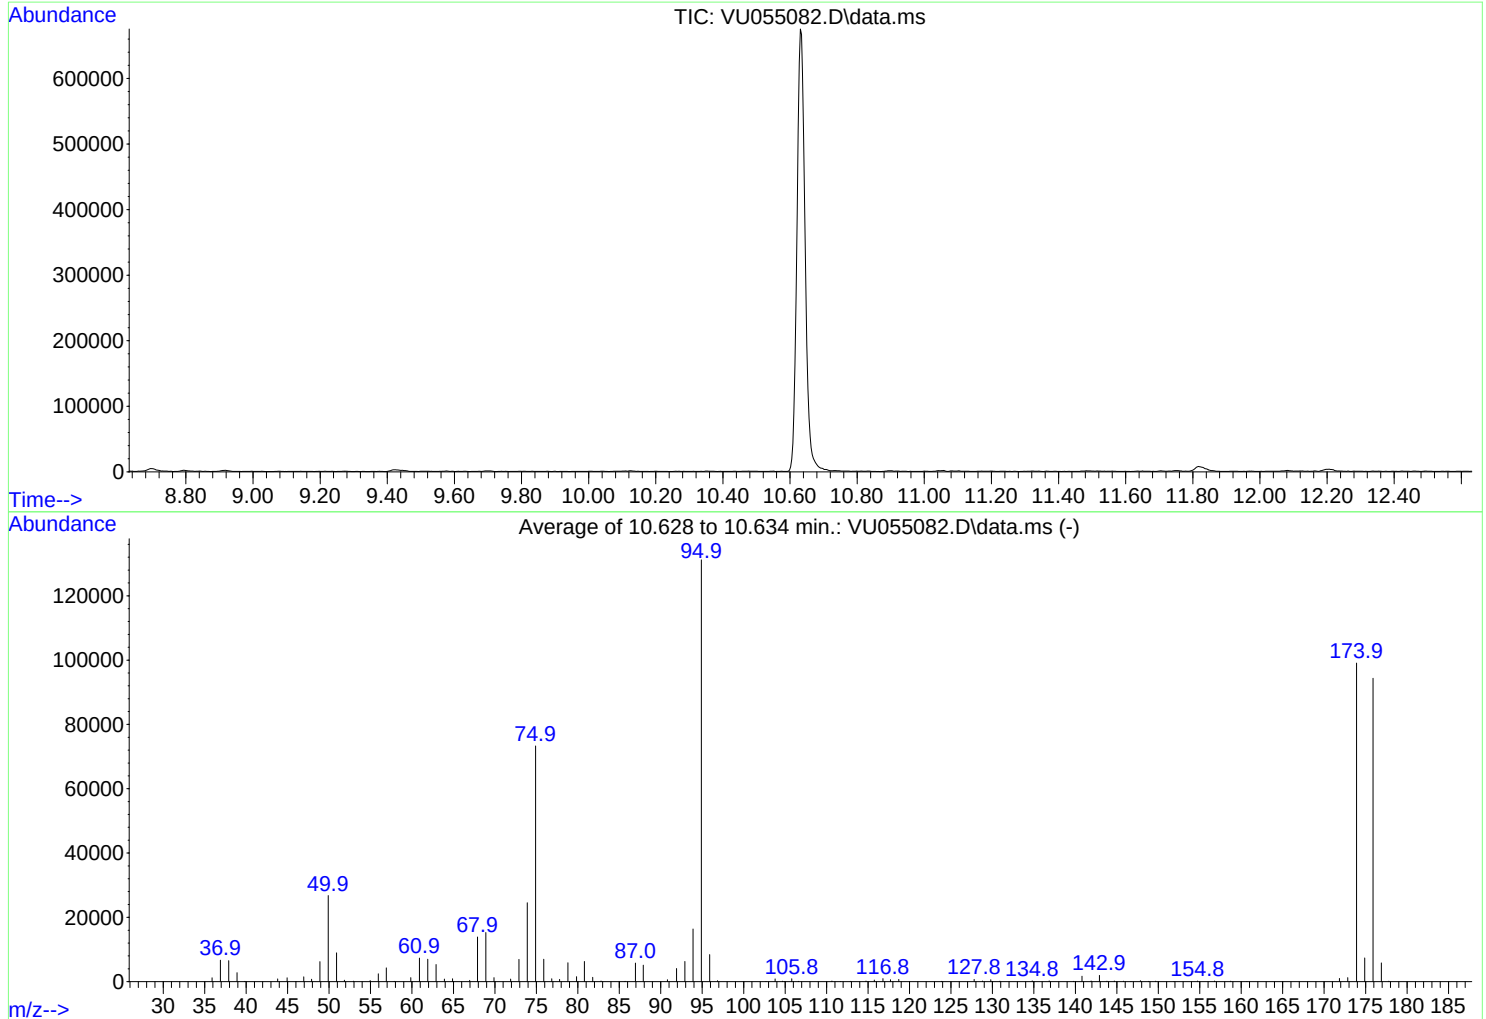

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	26784	PASS
75	95	30	80	55.9	73293	PASS
95	95	100	100	100.0	131187	PASS
96	95	5	9	6.4	8396	PASS
173	174	0.00	2	1.3	1258	PASS
174	95	50	120	75.5	99093	PASS
175	174	5	9	7.4	7372	PASS
176	174	95	101	95.2	94333	PASS
177	176	5	9	6.2	5813	PASS

Scan 2891 (10.586 min): VU055082.D\data.ms
BFB039

m/z	Abundance
39.80	156.0
43.80	603.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	1204.0
36.90	6810.0
37.90	6666.0
38.90	2836.0
40.00	223.0
43.90	1516.0
44.90	1205.0
47.00	1478.0
47.90	768.0
48.90	6410.0
49.90	27408.0
50.90	9286.0
51.80	474.0
52.90	191.0
54.90	348.0
55.90	2533.0
56.90	4394.0
57.80	142.0
59.90	1284.0
60.90	7531.0
61.90	7083.0
62.90	5404.0
63.90	830.0
64.90	923.0
66.90	382.0
67.90	14052.0
68.90	15821.0
69.90	1283.0
71.90	832.0
72.90	7205.0
73.90	25320.0
74.90	75552.0
75.90	7261.0
76.80	980.0
77.80	744.0
78.80	6026.0
79.90	1597.0
80.80	6492.0
81.80	1378.0
82.80	177.0
85.70	123.0
86.90	5961.0
87.90	5317.0
90.80	604.0
91.90	4168.0
92.90	6462.0
93.90	16840.0
94.90	135488.0
95.90	8657.0
96.90	356.0
102.70	118.0
103.80	872.0
104.70	236.0
105.80	894.0
106.60	137.0
110.60	262.0
112.90	129.0
114.70	200.0
115.70	499.0
116.80	947.0
117.70	591.0
118.70	684.0
123.90	134.0
127.80	761.0
128.80	205.0
129.80	590.0
130.90	152.0
134.80	285.0
136.80	234.0
139.80	131.0
140.80	1746.0
141.90	179.0
142.90	2053.0
143.80	142.0
144.70	208.0
145.80	165.0
147.90	328.0
148.90	123.0
149.70	163.0
154.70	204.0
156.80	222.0
158.80	181.0
171.90	988.0
172.90	1314.0
173.90	102328.0
174.90	7619.0
175.90	97208.0
176.90	5990.0
177.80	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	1285.0
36.90	6592.0
37.90	6664.0
38.90	2656.0
40.00	265.0
43.80	1567.0
45.00	1177.0
46.00	218.0
46.90	1546.0
47.90	809.0
48.90	6255.0
49.90	27048.0
50.90	9046.0
51.90	426.0
52.90	178.0
55.00	366.0
56.00	2378.0
56.90	4453.0
57.80	108.0
59.90	1376.0
60.90	7147.0
61.90	6808.0
62.90	5546.0
63.90	831.0
64.90	1035.0
67.00	315.0
67.90	14093.0
68.90	15381.0
69.90	1299.0
71.90	715.0
72.90	6712.0
73.90	24952.0
74.90	73848.0
75.90	6936.0
76.90	800.0
77.80	675.0
78.80	5856.0
79.80	1650.0
80.80	6245.0
81.80	1359.0
82.90	192.0
87.00	5802.0
87.90	5208.0
90.70	663.0
91.90	4190.0
92.90	6467.0
93.90	16616.0
94.90	134272.0
95.90	7858.0
96.90	295.0
103.80	807.0
104.90	225.0
105.80	940.0
106.60	132.0
110.60	224.0
112.80	147.0
114.70	197.0
115.70	487.0
116.80	1016.0
117.70	535.0
118.70	702.0
127.80	670.0
128.80	214.0
129.80	699.0
130.80	143.0
134.80	215.0
136.90	261.0
139.80	118.0
140.80	1747.0
141.80	184.0
142.90	2001.0
143.80	122.0
144.70	184.0
145.80	182.0
147.80	386.0
148.80	177.0
149.70	162.0
151.90	127.0
154.80	323.0
156.80	201.0
158.80	163.0
160.70	106.0
171.90	1037.0
172.90	1273.0
173.90	102296.0
174.90	7352.0
175.90	97304.0
176.90	5790.0
177.80	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	1158.0
36.90	6602.0
37.90	6165.0
38.90	2885.0
39.90	249.0
43.90	1318.0
44.90	1154.0
47.00	1464.0
47.90	686.0
48.90	5968.0
49.90	25896.0
50.90	8579.0
51.80	478.0
53.00	157.0
54.90	348.0
55.90	2419.0
56.90	4036.0
57.90	123.0
59.80	1129.0
60.90	7225.0
61.90	6990.0
62.90	5030.0
63.90	725.0
64.90	684.0
66.90	456.0
67.90	13542.0
68.90	14579.0
69.90	1172.0
71.90	833.0
72.90	6795.0
73.90	23368.0
74.90	70480.0
75.90	6724.0
76.80	998.0
77.80	699.0
78.80	5692.0
79.80	1463.0
80.80	6032.0
81.80	1253.0
82.70	177.0
85.70	133.0
86.90	5569.0
87.90	4903.0
90.90	583.0
91.90	3849.0
92.90	5886.0
93.90	15620.0
94.90	123800.0
95.90	8672.0
96.80	322.0
102.70	115.0
103.80	877.0
104.70	232.0
105.80	818.0
106.60	111.0
110.70	199.0
111.70	103.0
114.80	181.0
115.80	533.0
116.80	891.0
117.70	660.0
118.70	694.0
123.80	140.0
127.80	710.0
128.80	199.0
129.80	463.0
131.00	194.0
134.80	302.0
136.80	234.0
139.80	119.0
140.80	1619.0
142.00	165.0
142.90	1783.0
143.80	129.0
144.70	223.0
145.80	153.0
146.70	126.0
147.80	250.0
149.70	122.0
154.70	131.0
156.80	216.0
158.70	164.0
171.80	943.0
172.80	1187.0
173.90	92656.0
174.90	7144.0
175.90	88488.0
176.90	5660.0
177.80	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039