

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090524\
 Data File : VU060619.D
 Acq On : 05 Sep 2024 12:46
 Operator : MD/SY
 Sample : P3842-03 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0UE7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU060619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rVB	43201	49607	13.02%	1.639%
2	1.911	184	193	206	rBV	40648	53600	14.07%	1.771%
3	2.563	383	396	413	rBV	69514	113904	29.90%	3.764%
4	3.043	536	545	555	rBV3	3231	5726	1.50%	0.189%
5	4.634	1030	1040	1078	rBV	39941	129664	34.04%	4.285%
6	5.055	1156	1171	1198	rBV	69458	156626	41.12%	5.176%
7	5.718	1358	1377	1411	rBV2	132258	349658	91.80%	11.556%
8	6.242	1528	1540	1563	rBV	146102	290589	76.29%	9.604%
9	6.682	1664	1677	1705	rBV3	85427	170858	44.86%	5.647%
10	7.563	1940	1951	1971	rBV2	31952	60447	15.87%	1.998%
11	7.891	2042	2053	2076	rBV	138529	258156	67.78%	8.532%
12	8.177	2132	2142	2166	rVB3	18248	35064	9.21%	1.159%
13	8.463	2220	2231	2240	rBV4	3385	5829	1.53%	0.193%
14	8.631	2272	2283	2316	rBV	144833	308490	80.99%	10.195%
15	9.412	2514	2526	2549	rBV	212453	380893	100.00%	12.588%
16	10.750	2930	2942	2959	rVB	60958	102826	27.00%	3.398%
17	10.888	2971	2985	2999	rBV3	10390	16490	4.33%	0.545%
18	11.807	3259	3271	3293	rBV	182255	310972	81.64%	10.277%
19	12.187	3377	3389	3409	rBV	123450	216431	56.82%	7.153%
20	12.766	3559	3569	3578	rVB3	6218	9976	2.62%	0.330%




Sum of corrected areas: 3025806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090524\
Data File : VU060619.D
Acq On : 05 Sep 2024 12:46
Operator : MD/SY
Sample : P3842-03 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0UE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

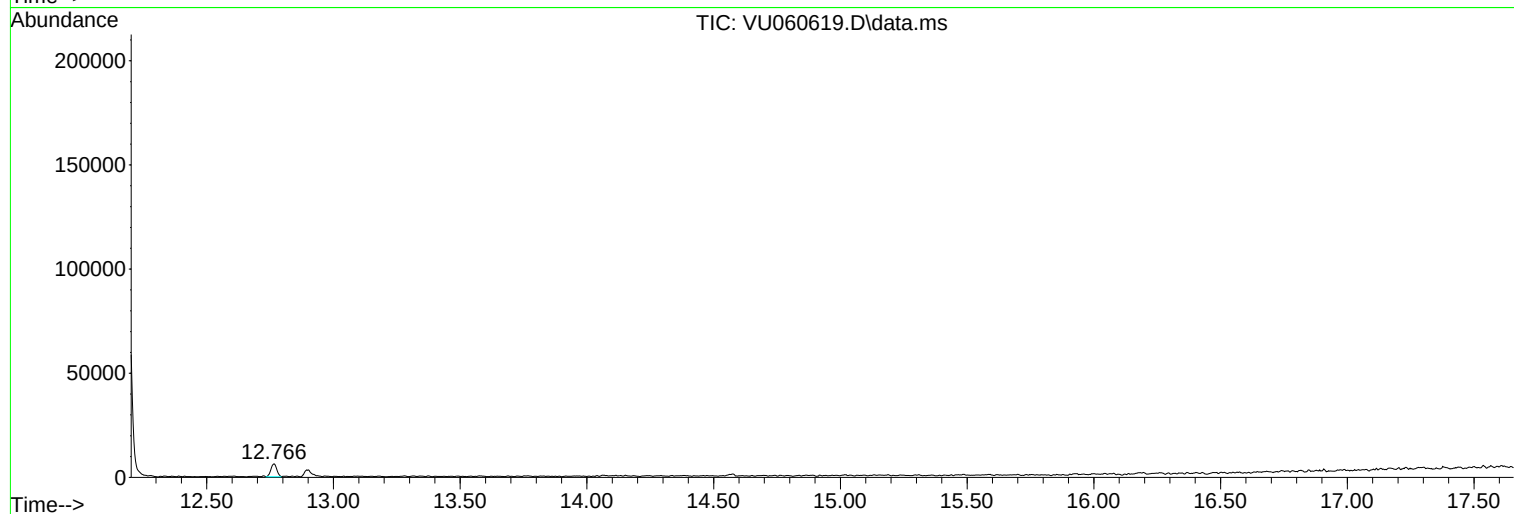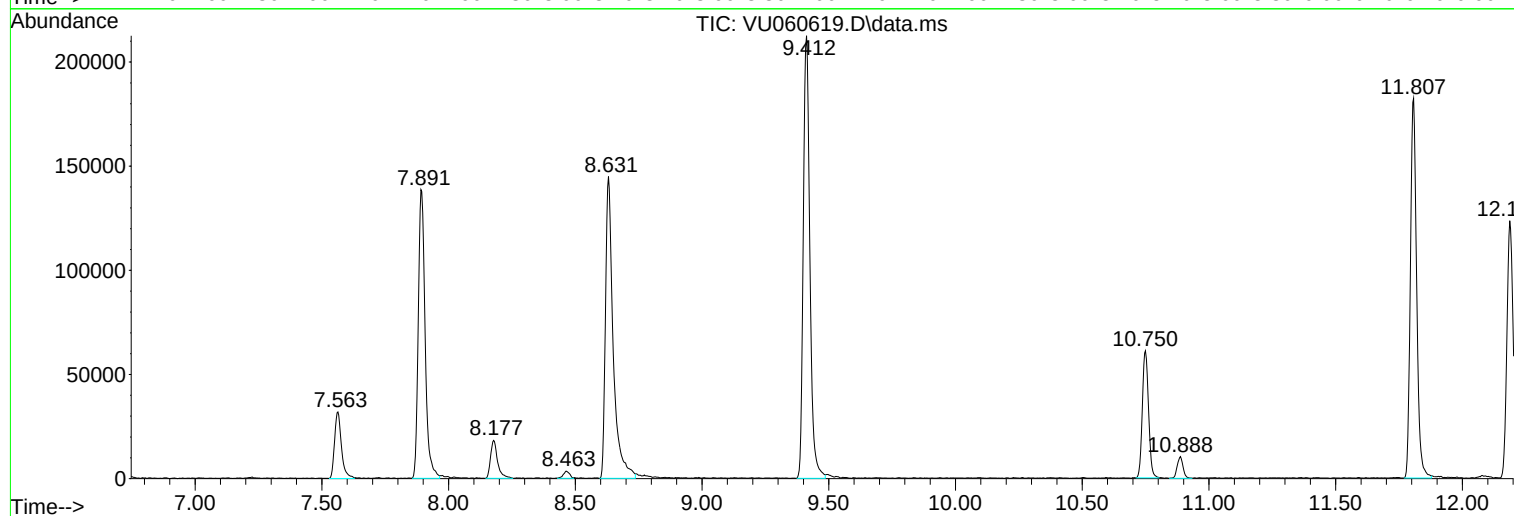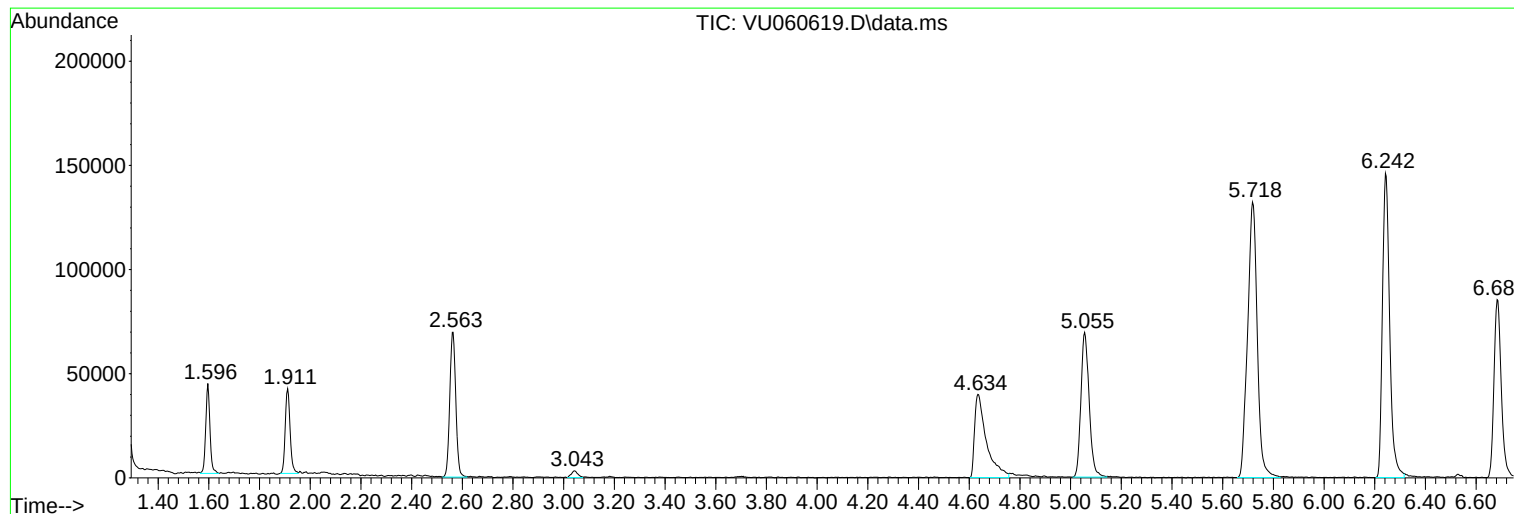

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090524\
Data File : VU060619.D
Acq On : 05 Sep 2024 12:46
Operator : MD/SY
Sample : P3842-03 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0UE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090524\
Data File : VU060619.D
Acq On : 05 Sep 2024 12:46
Operator : MD/SY
Sample : P3842-03 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0UE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR082324WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc