

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090618\
 Data File : VU026574.D
 Acq On : 06 Sep 2018 12:35
 Operator : MD/SY
 Sample : VU0906WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	85	rVB	81563	85199	15.85%	1.990%
2	1.678	150	157	175	rVB	64278	83503	15.53%	1.951%
3	2.270	331	341	355	rVB	136021	201508	37.49%	4.708%
4	2.579	432	437	443	rBV2	243	376	0.07%	0.009%
5	2.701	469	475	482	rVB4	1108	1403	0.26%	0.033%
6	2.742	486	488	491	rVB2	161	97	0.02%	0.002%
7	2.836	509	517	528	rBV3	1328	2631	0.49%	0.061%
8	2.906	537	539	543	rVB	204	116	0.02%	0.003%
9	2.926	543	545	547	rBV	155	92	0.02%	0.002%
10	2.945	547	551	552	rBV	168	122	0.02%	0.003%
11	2.987	560	564	565	rBV	239	139	0.03%	0.003%
12	3.019	572	574	580	rVB	217	157	0.03%	0.004%
13	3.048	580	583	585	rBV	181	131	0.02%	0.003%
14	3.106	598	601	606	rVV	158	91	0.02%	0.002%
15	3.270	648	652	657	rVB	69	65	0.01%	0.002%
16	3.315	664	666	668	rVV	128	54	0.01%	0.001%
17	3.344	672	675	680	rBV	114	110	0.02%	0.003%
18	3.463	709	712	713	rBV	134	56	0.01%	0.001%
19	3.569	741	745	751	rBV	115	120	0.02%	0.003%
20	3.598	751	754	755	rBV	144	64	0.01%	0.001%
21	3.884	840	843	847	rBV	163	87	0.02%	0.002%
22	3.942	859	861	862	rBV	111	52	0.01%	0.001%
23	4.019	882	885	886	rVV	137	58	0.01%	0.001%
24	4.180	921	935	965	rBV	48950	130610	24.30%	3.051%
25	4.398	1000	1003	1011	rVB4	404	394	0.07%	0.009%
26	4.456	1019	1021	1023	rVB	148	59	0.01%	0.001%
27	4.482	1023	1029	1032	rBV	68	61	0.01%	0.001%
28	4.508	1032	1037	1038	rBV	57	54	0.01%	0.001%
29	4.543	1046	1048	1051	rVB	141	59	0.01%	0.001%
30	4.578	1056	1059	1065	rBV	56	63	0.01%	0.001%
31	4.652	1065	1082	1104	rBV	89406	211479	39.34%	4.941%
32	4.948	1171	1174	1177	rBV	152	135	0.03%	0.003%
33	4.974	1180	1182	1184	rBV2	206	68	0.01%	0.002%
34	5.051	1203	1206	1209	rBV	119	86	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090618\
 Data File : VU026574.D
 Acq On : 06 Sep 2018 12:35
 Operator : MD/SY
 Sample : VU0906WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.115	1224	1226	1230	rVB	138	66	0.01%	0.002%
36	5.160	1236	1240	1243	rBV	75	62	0.01%	0.001%
37	5.344	1273	1297	1322	rBV2	183375	537536	100.00%	12.558%
38	5.498	1343	1345	1348	rVB	184	76	0.01%	0.002%
39	5.540	1356	1358	1361	rBV	189	71	0.01%	0.002%
40	5.585	1369	1372	1376	rBV	97	62	0.01%	0.001%
41	5.710	1406	1411	1412	rBV	135	69	0.01%	0.002%
42	5.768	1428	1429	1432	rVB	167	60	0.01%	0.001%
43	5.890	1453	1467	1482	rBV	197818	381459	70.96%	8.912%
44	6.096	1528	1531	1537	rBV	67	66	0.01%	0.002%
45	6.141	1542	1545	1548	rVB	96	57	0.01%	0.001%
46	6.167	1548	1553	1554	rBV	296	185	0.03%	0.004%
47	6.183	1554	1558	1562	rVB3	373	342	0.06%	0.008%
48	6.241	1572	1576	1578	rBV	72	49	0.01%	0.001%
49	6.334	1589	1605	1624	rBV	124925	247130	45.97%	5.774%
50	6.450	1636	1641	1643	rBV	86	64	0.01%	0.001%
51	6.508	1655	1659	1664	rVB	110	101	0.02%	0.002%
52	6.778	1740	1743	1747	rBV	114	88	0.02%	0.002%
53	6.803	1747	1751	1754	rBV	99	77	0.01%	0.002%
54	6.890	1774	1778	1780	rBV	174	110	0.02%	0.003%
55	6.967	1800	1802	1804	rVB	113	62	0.01%	0.001%
56	6.983	1804	1807	1813	rVB	67	52	0.01%	0.001%
57	7.016	1813	1817	1820	rBV	69	54	0.01%	0.001%
58	7.045	1823	1826	1829	rBV	92	60	0.01%	0.001%
59	7.083	1834	1838	1847	rVB	109	126	0.02%	0.003%
60	7.125	1847	1851	1853	rBV	76	63	0.01%	0.001%
61	7.164	1859	1863	1866	rBV	110	80	0.01%	0.002%
62	7.231	1871	1884	1905	rBV	65958	117353	21.83%	2.742%
63	7.373	1921	1928	1929	rBV	69	71	0.01%	0.002%
64	7.385	1929	1932	1934	rVB	119	82	0.02%	0.002%
65	7.466	1954	1957	1961	rBV	125	111	0.02%	0.003%
66	7.488	1961	1964	1967	rVB	89	62	0.01%	0.001%
67	7.524	1971	1975	1976	rBV	77	51	0.01%	0.001%
68	7.569	1976	1989	2007	rBV	241546	415035	77.21%	9.696%
69	7.736	2037	2041	2043	rBV	232	133	0.02%	0.003%
70	7.852	2066	2077	2098	rBV	48910	80215	14.92%	1.874%
71	7.945	2103	2106	2109	rBV2	265	192	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090618\
 Data File : VU026574.D
 Acq On : 06 Sep 2018 12:35
 Operator : MD/SY
 Sample : VU0906WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	7.971	2112	2114	2117	rBV2	99	63	0.01%	0.001%
73	8.183	2166	2180	2190	rBV3	11150	23385	4.35%	0.546%
74	8.315	2211	2221	2246	rVB	159943	273704	50.92%	6.394%
75	8.469	2267	2269	2273	rVB	179	105	0.02%	0.002%
76	8.623	2309	2317	2327	rBV4	1528	2498	0.46%	0.058%
77	8.707	2340	2343	2344	rBV	285	126	0.02%	0.003%
78	8.742	2351	2354	2358	rBV	189	106	0.02%	0.002%
79	8.848	2384	2387	2390	rVB	100	66	0.01%	0.002%
80	8.974	2420	2426	2430	rBV	194	247	0.05%	0.006%
81	9.093	2450	2463	2491	rBV	278214	453472	84.36%	10.594%
82	9.228	2503	2505	2508	rBV	210	106	0.02%	0.002%
83	9.247	2508	2511	2516	rBV2	257	290	0.05%	0.007%
84	9.289	2522	2524	2527	rBV	170	57	0.01%	0.001%
85	9.363	2544	2547	2549	rBV	118	73	0.01%	0.002%
86	9.491	2583	2587	2590	rVB2	176	113	0.02%	0.003%
87	9.765	2669	2672	2673	rBV2	179	83	0.02%	0.002%
88	9.852	2697	2699	2705	rVB	157	92	0.02%	0.002%
89	10.048	2758	2760	2763	rBV	168	51	0.01%	0.001%
90	10.434	2869	2880	2897	rVB	169582	266602	49.60%	6.228%
91	10.614	2929	2936	2949	rVB2	3783	6600	1.23%	0.154%
92	10.739	2971	2975	2980	rBV	171	188	0.03%	0.004%
93	10.771	2980	2985	2987	rBV	489	406	0.08%	0.009%
94	11.237	3128	3130	3133	rBV	162	88	0.02%	0.002%
95	11.417	3184	3186	3187	rBB	104	75	0.01%	0.002%
96	11.485	3195	3207	3226	rBV	253473	387265	72.04%	9.047%
97	11.861	3312	3324	3343	rBV	227932	360759	67.11%	8.428%
98	11.974	3356	3359	3362	rBV	260	207	0.04%	0.005%
99	12.189	3424	3426	3427	rBV	195	93	0.02%	0.002%
100	12.482	3507	3517	3528	rBV2	1502	2664	0.50%	0.062%


Sum of corrected areas: 4280415

Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090618\
Data File : VU026574.D
Acq On : 06 Sep 2018 12:35
Operator : MD/SY
Sample : VU0906WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

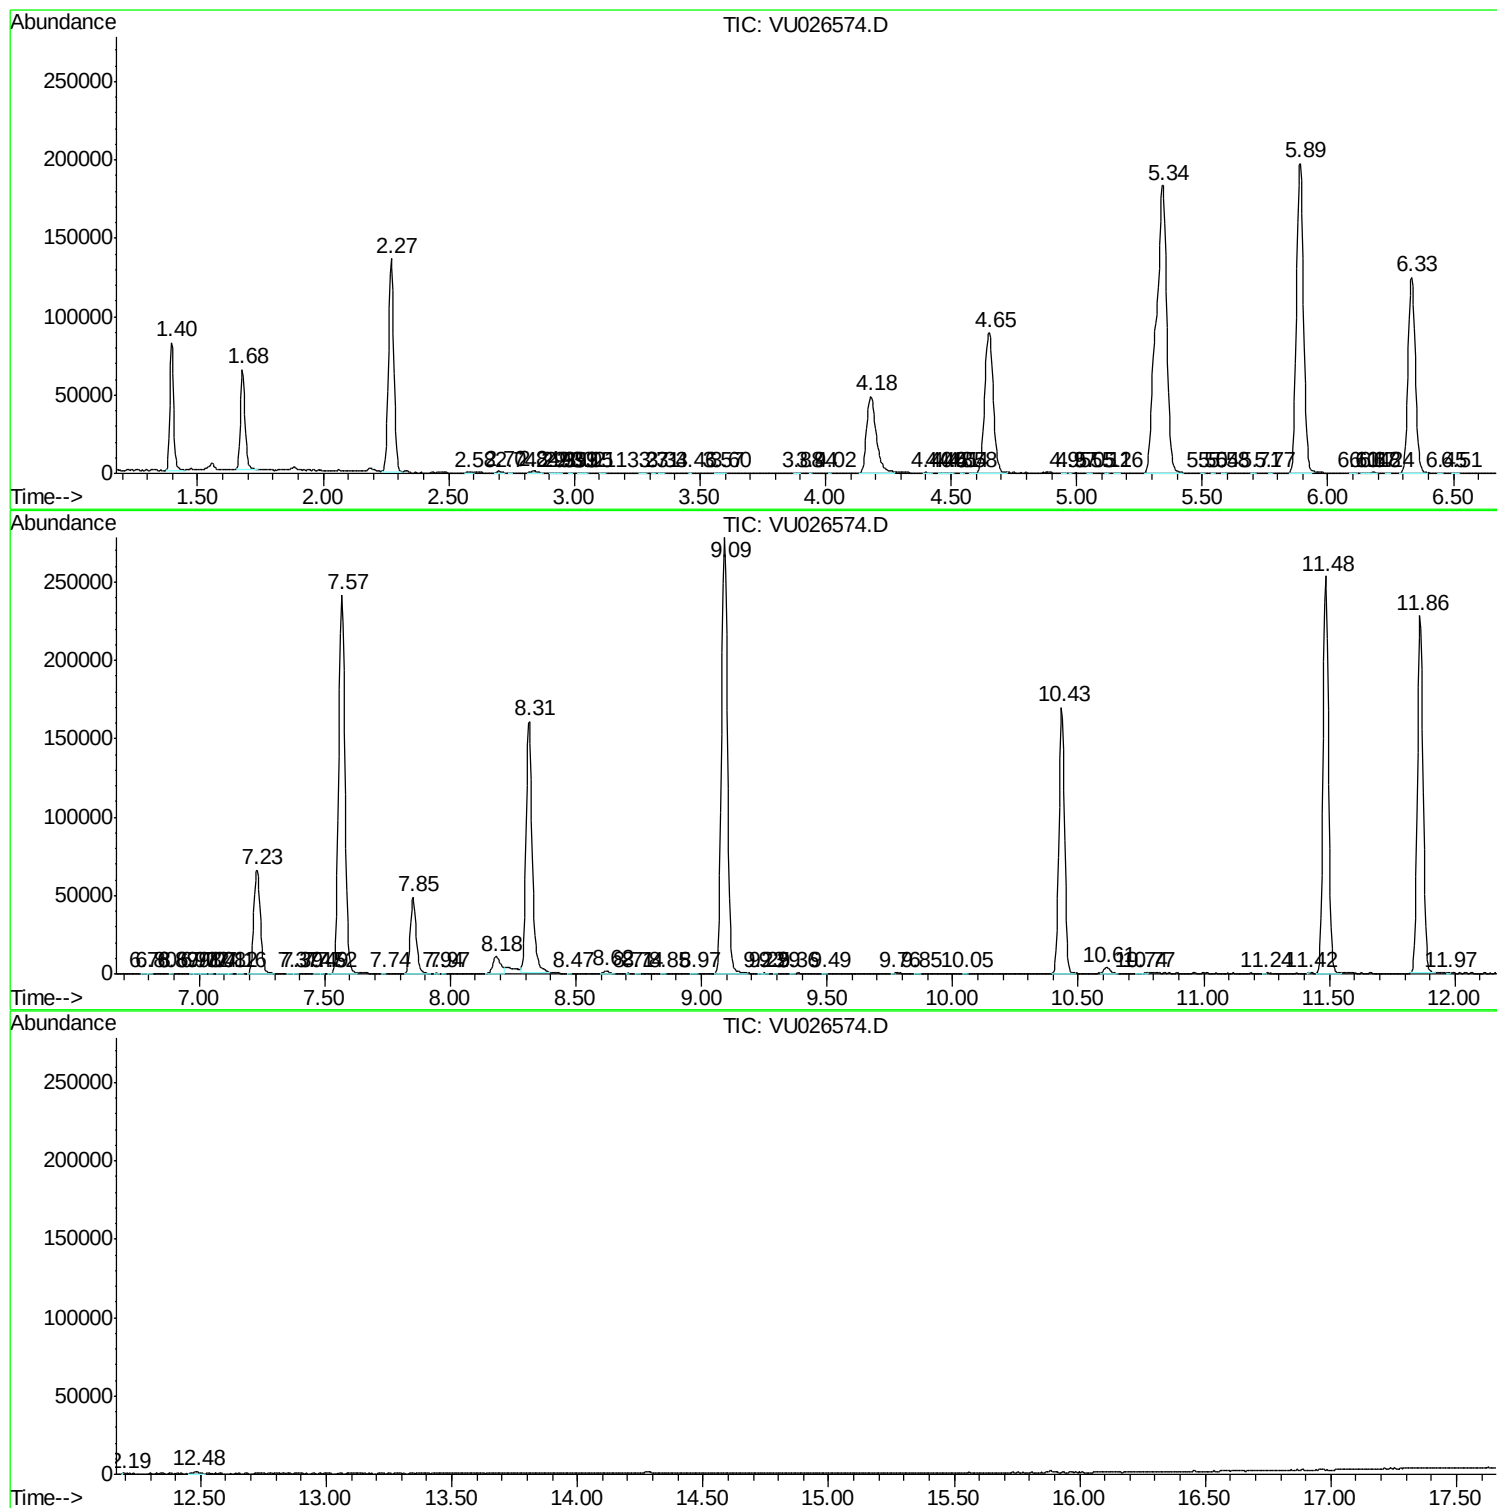

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090618\
Data File : VU026574.D
Acq On : 06 Sep 2018 12:35
Operator : MD/SY
Sample : VU0906WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090618\
Data File : VU026574.D
Acq On : 06 Sep 2018 12:35
Operator : MD/SY
Sample : VU0906WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK46

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc