

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
 Data File : VU026583.D
 Acq On : 06 Sep 2018 16:21
 Operator : MD/SY
 Sample : J4718-16DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEGD2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	63	70	82	rVB2	106891	115318	18.20%	2.399%
2	1.678	150	157	174	rVB	72816	96742	15.27%	2.012%
3	2.270	331	341	357	rBV	150473	224568	35.45%	4.671%
4	2.450	393	397	400	rBV2	237	197	0.03%	0.004%
5	2.475	400	405	412	rVV2	411	510	0.08%	0.011%
6	2.537	422	424	429	rVB	196	92	0.01%	0.002%
7	2.617	445	449	459	rVB2	378	553	0.09%	0.012%
8	2.678	466	468	469	rVV	228	84	0.01%	0.002%
9	2.697	471	474	484	rVB3	896	1168	0.18%	0.024%
10	2.839	508	518	529	rVB2	1925	4186	0.66%	0.087%
11	2.942	545	550	556	rBV2	425	612	0.10%	0.013%
12	3.025	574	576	578	rBV	101	72	0.01%	0.001%
13	3.109	599	602	604	rBV2	157	96	0.02%	0.002%
14	3.147	611	614	618	rVB2	191	138	0.02%	0.003%
15	3.180	622	624	626	rVB	133	56	0.01%	0.001%
16	3.221	635	637	643	rVB2	158	153	0.02%	0.003%
17	3.286	654	657	661	rBV	171	123	0.02%	0.003%
18	3.324	664	669	672	rBV	231	211	0.03%	0.004%
19	3.401	690	693	698	rBV	208	147	0.02%	0.003%
20	3.443	703	706	709	rVV	143	67	0.01%	0.001%
21	3.601	753	755	761	rVB2	248	173	0.03%	0.004%
22	3.649	768	770	773	rVB2	167	91	0.01%	0.002%
23	3.672	773	777	779	rBV	80	67	0.01%	0.001%
24	3.700	783	786	789	rVB	161	82	0.01%	0.002%
25	3.736	795	797	798	rBV	163	74	0.01%	0.002%
26	3.864	833	837	838	rBV	137	56	0.01%	0.001%
27	3.887	841	844	846	rVV	145	93	0.01%	0.002%
28	3.977	868	872	876	rBV	153	98	0.02%	0.002%
29	4.022	881	886	890	rBV2	234	214	0.03%	0.004%
30	4.099	904	910	911	rBV2	283	290	0.05%	0.006%
31	4.180	920	935	940	rBV	61714	127801	20.18%	2.658%
32	4.414	1006	1008	1014	rVB3	358	244	0.04%	0.005%
33	4.453	1016	1020	1022	rBV	171	116	0.02%	0.002%
34	4.501	1033	1035	1043	rVB2	166	152	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
 Data File : VU026583.D
 Acq On : 06 Sep 2018 16:21
 Operator : MD/SY
 Sample : J4718-16DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEGD2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	4.540	1044	1047	1050	rBV	188	107	0.02%	0.002%
36	4.575	1055	1058	1065	rVB	88	73	0.01%	0.002%
37	4.649	1065	1081	1105	rBV	107488	248308	39.20%	5.165%
38	4.980	1182	1184	1187	rVB3	348	158	0.02%	0.003%
39	5.048	1202	1205	1207	rBV	172	112	0.02%	0.002%
40	5.083	1214	1216	1219	rVB	286	126	0.02%	0.003%
41	5.176	1242	1245	1247	rVB	127	72	0.01%	0.001%
42	5.244	1263	1266	1272	rBV	81	86	0.01%	0.002%
43	5.343	1272	1297	1326	rVV2	214078	633450	100.00%	13.176%
44	5.459	1330	1333	1336	rBV2	160	112	0.02%	0.002%
45	5.536	1354	1357	1363	rBV	62	59	0.01%	0.001%
46	5.733	1412	1418	1421	rBV	64	68	0.01%	0.001%
47	5.890	1452	1467	1495	rBV	199794	388223	61.29%	8.075%
48	6.192	1551	1561	1571	rVB2	6560	12515	1.98%	0.260%
49	6.253	1576	1580	1583	rBV	101	86	0.01%	0.002%
50	6.334	1590	1605	1627	rBV	148750	292245	46.14%	6.079%
51	6.440	1632	1638	1642	rBV	107	115	0.02%	0.002%
52	6.462	1642	1645	1648	rVB	210	121	0.02%	0.003%
53	6.511	1654	1660	1663	rBV	63	72	0.01%	0.001%
54	6.536	1664	1668	1673	rBV	115	90	0.01%	0.002%
55	6.617	1687	1693	1699	rBV	112	173	0.03%	0.004%
56	6.858	1760	1768	1777	rVV2	417	696	0.11%	0.014%
57	6.919	1783	1787	1791	rBV	111	95	0.01%	0.002%
58	7.051	1826	1828	1831	rVB2	149	83	0.01%	0.002%
59	7.089	1837	1840	1844	rBV	121	84	0.01%	0.002%
60	7.167	1859	1864	1870	rVV	110	131	0.02%	0.003%
61	7.231	1871	1884	1904	rBV	78063	137487	21.70%	2.860%
62	7.318	1909	1911	1914	rVB	218	121	0.02%	0.003%
63	7.372	1920	1928	1930	rBV2	432	400	0.06%	0.008%
64	7.395	1934	1935	1938	rVB	131	70	0.01%	0.001%
65	7.443	1948	1950	1954	rVB	157	88	0.01%	0.002%
66	7.466	1954	1957	1959	rBV2	172	123	0.02%	0.003%
67	7.568	1976	1989	2007	rBV	285980	489599	77.29%	10.184%
68	7.739	2039	2042	2046	rBV	89	65	0.01%	0.001%
69	7.765	2046	2050	2052	rBV	88	65	0.01%	0.001%
70	7.851	2066	2077	2095	rBV	56323	93537	14.77%	1.946%
71	8.009	2123	2126	2130	rBV	76	57	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
 Data File : VU026583.D
 Acq On : 06 Sep 2018 16:21
 Operator : MD/SY
 Sample : J4718-16DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEGD2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	8.183	2167	2180	2188	rBV2	3944	8093	1.28%	0.168%
73	8.314	2210	2221	2250	rVB	197545	329286	51.98%	6.849%
74	8.604	2306	2311	2314	rBV2	406	421	0.07%	0.009%
75	8.742	2351	2354	2355	rBV2	190	87	0.01%	0.002%
76	8.819	2373	2378	2381	rBV	110	109	0.02%	0.002%
77	8.855	2385	2389	2393	rVV2	206	211	0.03%	0.004%
78	8.880	2394	2397	2400	rVB	147	78	0.01%	0.002%
79	8.935	2411	2414	2417	rVB	250	140	0.02%	0.003%
80	9.093	2448	2463	2482	rBV	282000	459238	72.50%	9.552%
81	9.237	2504	2508	2510	rBV	114	90	0.01%	0.002%
82	9.340	2536	2540	2546	rBV2	269	296	0.05%	0.006%
83	9.382	2548	2553	2561	rVV2	489	574	0.09%	0.012%
84	9.417	2561	2564	2567	rVV2	186	139	0.02%	0.003%
85	9.446	2571	2573	2576	rVB	121	74	0.01%	0.002%
86	9.498	2586	2589	2594	rBV	181	99	0.02%	0.002%
87	9.777	2674	2676	2679	rBV	246	197	0.03%	0.004%
88	9.941	2724	2727	2730	rVV	131	102	0.02%	0.002%
89	10.009	2745	2748	2751	rBV	199	128	0.02%	0.003%
90	10.025	2751	2753	2755	rBV	161	98	0.02%	0.002%
91	10.260	2822	2826	2829	rBV	162	147	0.02%	0.003%
92	10.298	2834	2838	2840	rBV2	220	175	0.03%	0.004%
93	10.366	2856	2859	2863	rVB	194	133	0.02%	0.003%
94	10.433	2868	2880	2897	rVV	202333	317506	50.12%	6.604%
95	10.613	2927	2936	2948	rVB	1876	2786	0.44%	0.058%
96	10.668	2950	2953	2956	rVV	219	194	0.03%	0.004%
97	10.694	2959	2961	2964	rVB	176	65	0.01%	0.001%
98	11.182	3111	3113	3120	rVB	148	82	0.01%	0.002%
99	11.485	3195	3207	3225	rBV	253144	389329	61.46%	8.098%
100	11.861	3312	3324	3344	rBV	269256	423973	66.93%	8.819%


Sum of corrected areas: 4807566

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090618\
Data File : VU026583.D
Acq On : 06 Sep 2018 16:21
Operator : MD/SY
Sample : J4718-16DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEGD2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

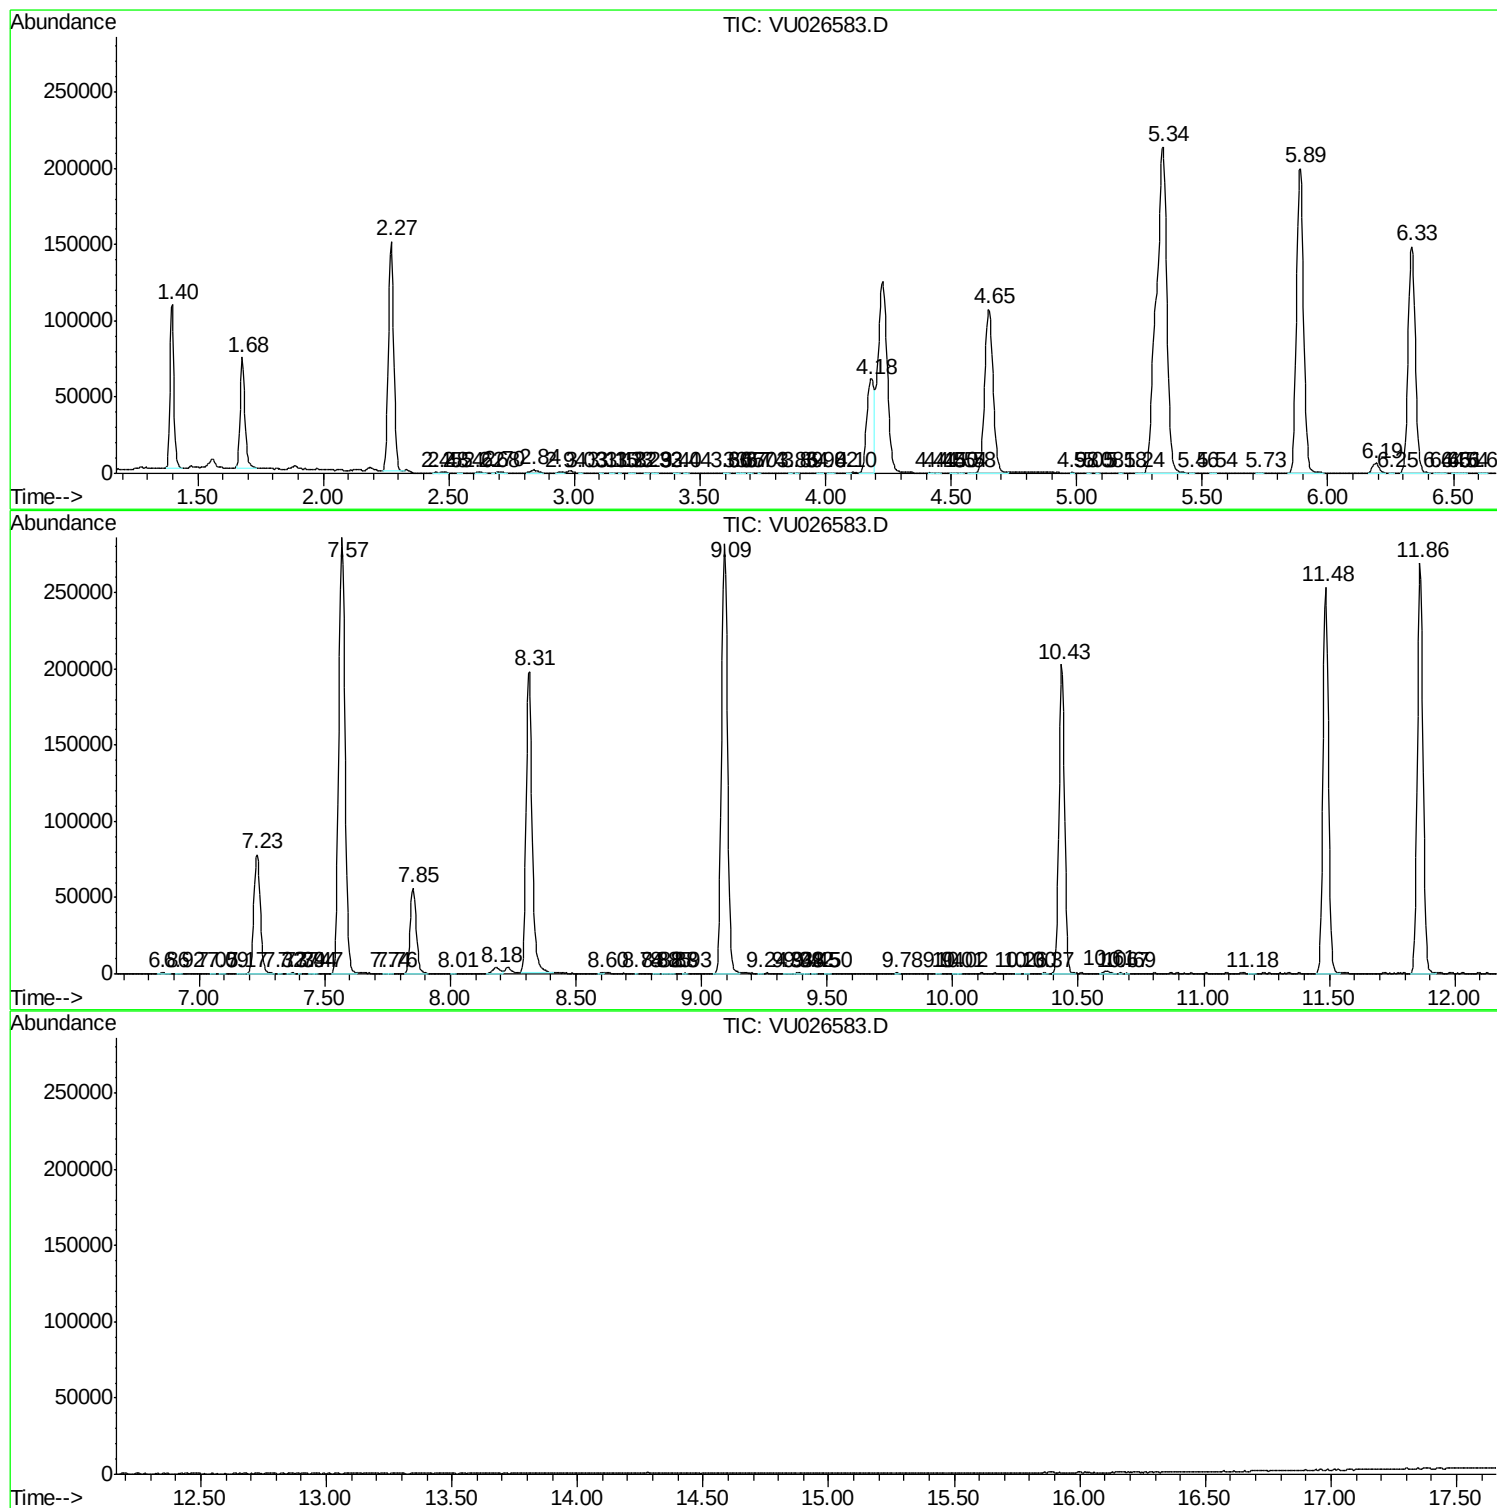

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090618\
Data File : VU026583.D
Acq On : 06 Sep 2018 16:21
Operator : MD/SY
Sample : J4718-16DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEGD2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090618\
Data File : VU026583.D
Acq On : 06 Sep 2018 16:21
Operator : MD/SY
Sample : J4718-16DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEGD2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc