

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
 Data File : VU026587.D
 Acq On : 06 Sep 2018 19:15
 Operator : MD/SY
 Sample : J4618-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	63	69	83	rBV	79954	82398	13.95%	1.771%
2	1.678	150	157	170	rVB	65800	83394	14.12%	1.792%
3	2.270	331	341	354	rVB	127000	192174	32.54%	4.130%
4	2.569	432	434	435	rBV	133	54	0.01%	0.001%
5	2.623	443	451	455	rBV2	444	604	0.10%	0.013%
6	2.701	468	475	484	rVV3	887	1151	0.19%	0.025%
7	2.746	487	489	491	rVB	158	63	0.01%	0.001%
8	2.800	503	506	508	rBV	134	63	0.01%	0.001%
9	2.839	508	518	532	rVB2	1973	4235	0.72%	0.091%
10	2.916	539	542	545	rVB	184	102	0.02%	0.002%
11	2.971	556	559	560	rBV	120	55	0.01%	0.001%
12	3.006	569	570	576	rVB	266	151	0.03%	0.003%
13	3.074	589	591	594	rVB2	208	109	0.02%	0.002%
14	3.193	624	628	630	rBV	183	96	0.02%	0.002%
15	3.209	631	633	635	rVV	163	52	0.01%	0.001%
16	3.231	637	640	643	rVV	108	65	0.01%	0.001%
17	3.279	651	655	657	rBV	113	79	0.01%	0.002%
18	3.389	687	689	691	rVB	122	47	0.01%	0.001%
19	3.643	764	768	773	rVB	63	71	0.01%	0.002%
20	3.672	773	777	779	rBV	78	57	0.01%	0.001%
21	3.852	830	833	837	rVB	70	50	0.01%	0.001%
22	3.929	855	857	860	rVB	164	97	0.02%	0.002%
23	3.983	868	874	877	rBV	96	113	0.02%	0.002%
24	4.003	877	880	884	rVB	100	62	0.01%	0.001%
25	4.048	892	894	897	rVB	102	52	0.01%	0.001%
26	4.070	898	901	908	rVB	118	120	0.02%	0.003%
27	4.102	908	911	913	rBV	200	169	0.03%	0.004%
28	4.180	919	935	962	rBV	59502	154510	26.16%	3.320%
29	4.405	1003	1005	1008	rVB	224	130	0.02%	0.003%
30	4.427	1008	1012	1014	rBV	122	105	0.02%	0.002%
31	4.543	1045	1048	1053	rBV	100	85	0.01%	0.002%
32	4.588	1058	1062	1065	rBV	114	89	0.02%	0.002%
33	4.649	1065	1081	1110	rBV	102770	238572	40.39%	5.127%
34	4.983	1182	1185	1186	rBV	158	92	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
 Data File : VU026587.D
 Acq On : 06 Sep 2018 19:15
 Operator : MD/SY
 Sample : J4618-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

35	5.205	1251	1254	1257	rBV	72	57	0.01%	0.001%
36	5.263	1269	1272	1273	rBV	158	97	0.02%	0.002%
37	5.344	1273	1297	1315	rBV2	200233	590629	100.00%	12.693%
38	5.475	1337	1338	1341	rVB	124	67	0.01%	0.001%
39	5.511	1347	1349	1352	rBV	162	63	0.01%	0.001%
40	5.646	1388	1391	1398	rVV	53	68	0.01%	0.001%
41	5.890	1451	1467	1489	rBV	217179	416297	70.48%	8.946%
42	6.016	1503	1506	1508	rBV	168	135	0.02%	0.003%
43	6.038	1511	1513	1516	rVB	123	52	0.01%	0.001%
44	6.061	1516	1520	1524	rBV2	136	104	0.02%	0.002%
45	6.250	1576	1579	1587	rVB	61	71	0.01%	0.002%
46	6.334	1591	1605	1625	rBV	142156	278807	47.21%	5.992%
47	6.440	1631	1638	1639	rBV	51	46	0.01%	0.001%
48	6.463	1639	1645	1652	rVV3	285	383	0.06%	0.008%
49	6.530	1663	1666	1671	rVB	62	50	0.01%	0.001%
50	6.684	1708	1714	1719	rBV	67	90	0.02%	0.002%
51	6.726	1725	1727	1732	rVB	186	89	0.02%	0.002%
52	6.839	1758	1762	1765	rVV	111	74	0.01%	0.002%
53	6.868	1765	1771	1776	rVV2	302	444	0.08%	0.010%
54	6.926	1785	1789	1792	rBV	103	83	0.01%	0.002%
55	6.954	1796	1798	1803	rVB2	130	89	0.02%	0.002%
56	6.980	1803	1806	1809	rBV	89	54	0.01%	0.001%
57	7.012	1812	1816	1820	rBV	63	52	0.01%	0.001%
58	7.144	1855	1857	1862	rVB	80	50	0.01%	0.001%
59	7.231	1872	1884	1903	rBV	65896	114726	19.42%	2.465%
60	7.376	1926	1929	1936	rVB	246	333	0.06%	0.007%
61	7.469	1954	1958	1964	rVB2	247	247	0.04%	0.005%
62	7.501	1964	1968	1971	rBV	71	64	0.01%	0.001%
63	7.517	1971	1973	1975	rBV	133	70	0.01%	0.002%
64	7.569	1975	1989	2006	rBV	266387	450619	76.29%	9.684%
65	7.723	2034	2037	2043	rBV2	248	163	0.03%	0.004%
66	7.852	2066	2077	2091	rBV	47373	78855	13.35%	1.695%
67	7.958	2108	2110	2114	rVB	162	77	0.01%	0.002%
68	8.186	2166	2181	2190	rBV3	5047	11295	1.91%	0.243%
69	8.311	2210	2220	2251	rVB	195605	330490	55.96%	7.102%
70	8.527	2285	2287	2288	rBV	130	53	0.01%	0.001%
71	8.668	2329	2331	2334	rVB	175	58	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
 Data File : VU026587.D
 Acq On : 06 Sep 2018 19:15
 Operator : MD/SY
 Sample : J4618-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
 Title : VOC Analysis

72	8.691	2337	2338	2340	rBV	226	95	0.02%	0.002%
73	8.726	2347	2349	2351	rVB	150	63	0.01%	0.001%
74	8.742	2351	2354	2359	rBV	247	282	0.05%	0.006%
75	8.816	2373	2377	2380	rBV	241	188	0.03%	0.004%
76	8.884	2395	2398	2403	rBV	167	99	0.02%	0.002%
77	8.932	2411	2413	2415	rVB	132	55	0.01%	0.001%
78	8.951	2415	2419	2422	rVB	59	47	0.01%	0.001%
79	9.032	2442	2444	2450	rVB2	193	128	0.02%	0.003%
80	9.093	2450	2463	2482	rBV	302688	491343	83.19%	10.559%
81	9.302	2523	2528	2534	rBV2	186	234	0.04%	0.005%
82	9.427	2564	2567	2571	rBV2	186	148	0.03%	0.003%
83	9.446	2571	2573	2575	rBV2	116	62	0.01%	0.001%
84	9.591	2616	2618	2622	rVB	131	79	0.01%	0.002%
85	9.639	2630	2633	2636	rBV2	169	103	0.02%	0.002%
86	9.781	2674	2677	2680	rBV2	197	174	0.03%	0.004%
87	10.093	2772	2774	2778	rVB	129	82	0.01%	0.002%
88	10.112	2778	2780	2781	rBV	129	53	0.01%	0.001%
89	10.212	2808	2811	2814	rBV	127	78	0.01%	0.002%
90	10.228	2814	2816	2818	rBV2	178	102	0.02%	0.002%
91	10.269	2826	2829	2832	rBV	182	113	0.02%	0.002%
92	10.433	2868	2880	2897	rBV	201510	312567	52.92%	6.717%
93	10.552	2915	2917	2920	rBV	183	69	0.01%	0.001%
94	10.610	2926	2935	2945	rVB3	2076	3120	0.53%	0.067%
95	10.874	3014	3017	3019	rBV	181	138	0.02%	0.003%
96	11.060	3073	3075	3077	rBV	149	46	0.01%	0.001%
97	11.417	3184	3186	3190	rVB	285	173	0.03%	0.004%
98	11.485	3195	3207	3222	rBV	263297	405321	68.63%	8.710%
99	11.861	3312	3324	3342	rBV	254685	403693	68.35%	8.675%
100	12.472	3510	3514	3515	rBV	576	403	0.07%	0.009%


Sum of corrected areas: 4653325

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090618\
Data File : VU026587.D
Acq On : 06 Sep 2018 19:15
Operator : MD/SY
Sample : J4618-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

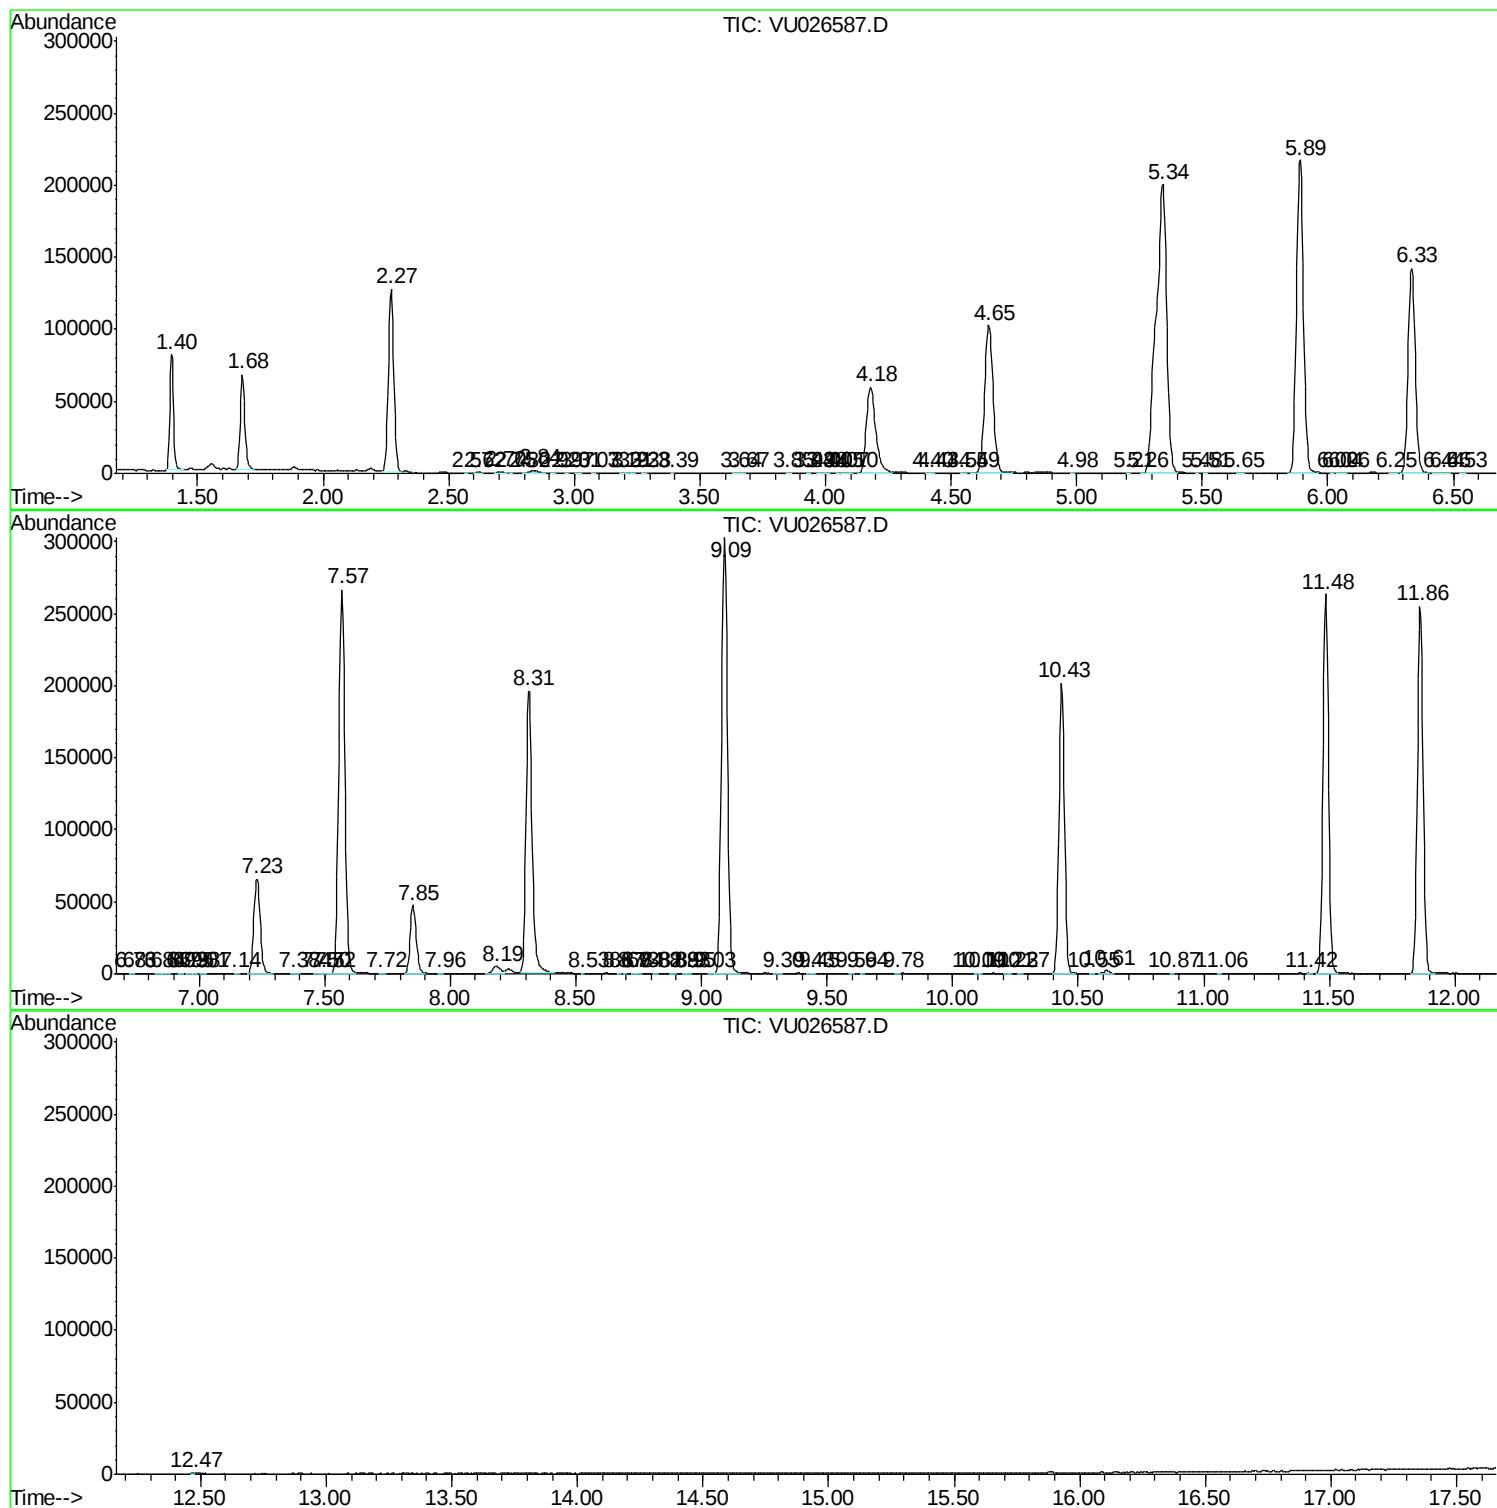

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090618\
Data File : VU026587.D
Acq On : 06 Sep 2018 19:15
Operator : MD/SY
Sample : J4618-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU090618\
Data File : VU026587.D
Acq On : 06 Sep 2018 19:15
Operator : MD/SY
Sample : J4618-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc