


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090618\
Data File : VU026572.D
Acq On : 06 Sep 2018 09:49
Operator : MD/SY
Sample : BFB50
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM082918WMA.M
Title : VOC Analysis
Last Update : Fri Sep 07 05:26:58 2018

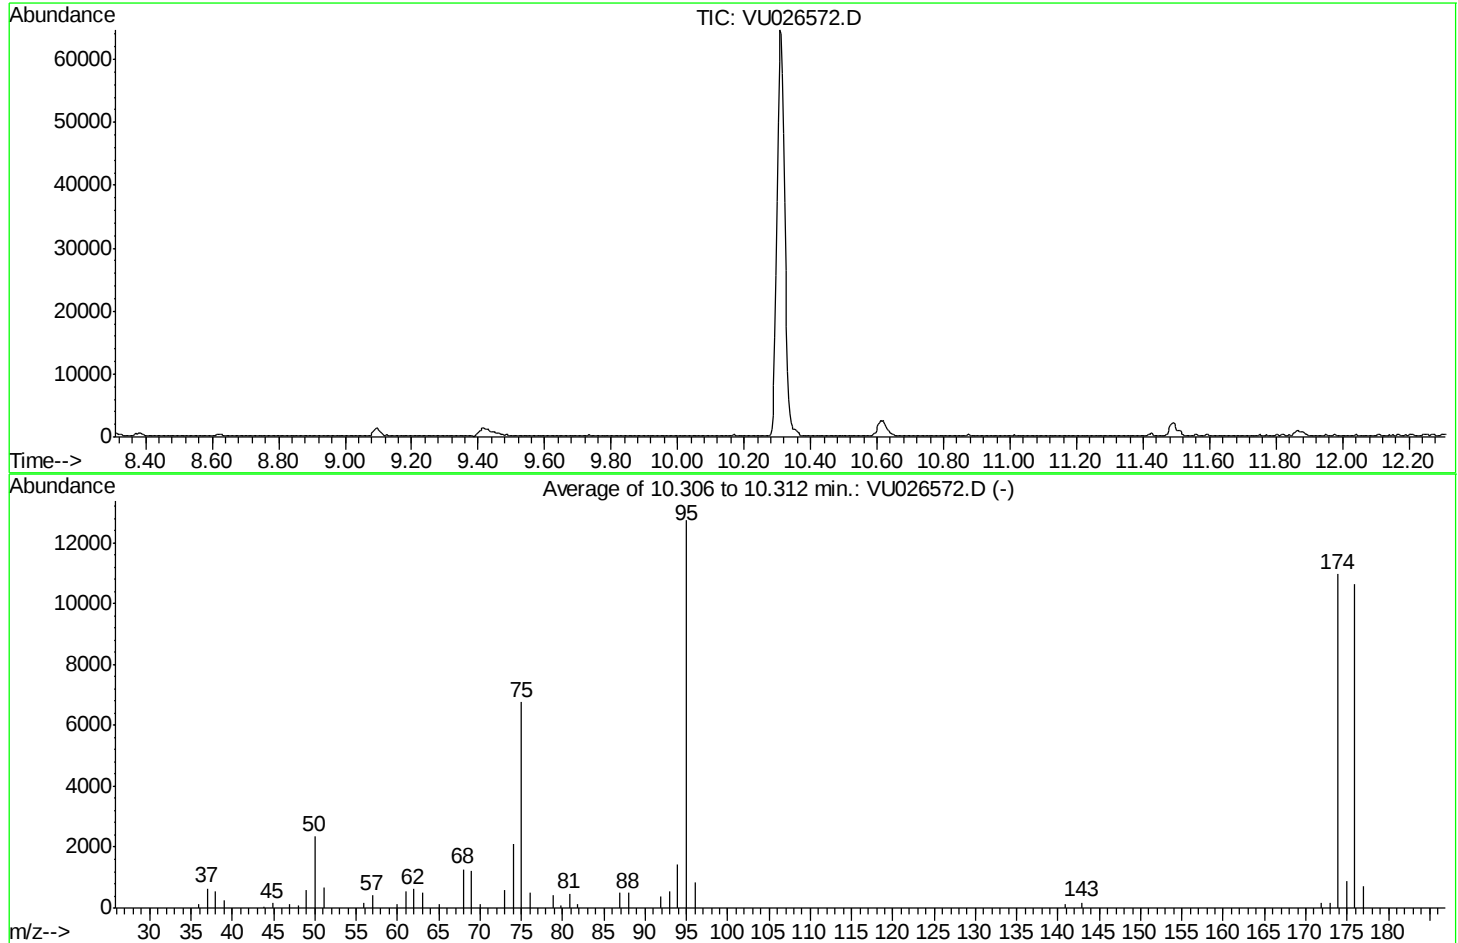

AutoFind: Scans 2835, 2836, 2837; Background Corrected with Scan 2825

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	2345	PASS
75	95	30	80	53.0	6754	PASS
95	95	100	100	100.0	12738	PASS
96	95	5	9	6.7	854	PASS
173	174	0.00	2	1.7	182	PASS
174	95	50	120	86.0	10960	PASS
175	174	5	9	8.1	883	PASS
176	174	95	101	97.1	10643	PASS
177	176	5	9	6.6	707	PASS

m/z	Abundance
43.90	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	123.0
37.00	624.0
38.00	477.0
39.00	194.0
43.90	266.0
44.90	153.0
46.90	133.0
48.00	102.0
49.00	574.0
50.00	2357.0
51.00	733.0
55.90	175.0
57.00	422.0
59.90	112.0
61.00	562.0
61.90	593.0
63.00	462.0
65.10	143.0
68.00	1186.0
69.00	1157.0
70.00	113.0
73.00	521.0
74.00	2086.0
75.00	6440.0
76.00	498.0
78.90	384.0
80.80	444.0
81.80	117.0
86.90	480.0
87.90	498.0
91.90	371.0
93.00	494.0
93.90	1315.0
95.00	12108.0
96.00	859.0
140.90	179.0
142.90	156.0
171.90	170.0
173.00	155.0
173.90	10328.0
174.90	856.0
175.90	9828.0
176.90	649.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	137.0
37.00	655.0
38.00	548.0
38.90	238.0
43.90	256.0
44.90	151.0
46.90	147.0
48.00	106.0
48.90	621.0
50.00	2392.0
51.00	682.0
55.90	178.0
56.90	432.0
60.00	114.0
61.00	565.0
61.90	644.0
63.00	491.0
65.00	143.0
68.00	1319.0
69.00	1237.0
69.90	120.0
73.00	592.0
74.00	2161.0
75.00	6984.0
76.00	527.0
78.90	438.0
79.80	128.0
80.90	491.0
81.90	118.0
86.90	521.0
88.00	530.0
91.90	401.0
93.00	537.0
94.00	1447.0
95.00	13130.0
96.00	857.0
140.90	155.0
142.90	182.0
171.90	180.0
173.00	175.0
173.90	11259.0
175.00	930.0
175.90	11014.0
176.90	727.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	135.0
37.00	654.0
38.00	619.0
38.90	274.0
43.90	270.0
44.90	144.0
46.90	134.0
47.90	102.0
48.90	562.0
50.00	2286.0
51.10	605.0
55.90	163.0
56.90	392.0
60.00	111.0
61.00	534.0
62.00	612.0
63.00	510.0
64.90	126.0
68.00	1294.0
69.00	1249.0
69.90	123.0
72.90	598.0
74.00	2061.0
75.00	6840.0
76.00	515.0
78.90	423.0
79.90	150.0
80.90	517.0
81.90	114.0
86.80	495.0
88.00	484.0
91.90	408.0
92.90	557.0
94.00	1487.0
95.00	12977.0
96.00	847.0
140.90	100.0
142.90	178.0
171.80	171.0
173.00	218.0
173.90	11293.0
175.00	864.0
175.90	11089.0
176.90	746.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50