

Data File : VU034294.D
Acq On : 05 Sep 2019 19:24
Operator : JC/SP
Sample : K4548-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T11-2-(0)

Quant Time: Sep 06 07:40:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 06 05:10:13 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.96	168	437254	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.87	114	694710	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.07	117	683495	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.46	152	340126	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.29	65	276523	41.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	83.60%	
35) Dibromofluoromethane	4.86	113	240956	37.27	ug/l	0.00
Spiked Amount	50.000		Recovery	=	74.54%	
50) Toluene-d8	7.55	98	971637	40.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	80.02%	
62) 4-Bromofluorobenzene	10.29	95	344367	36.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	73.46%	


Target Compounds			Qvalue			
5) Bromomethane	1.63	94	493	Below Cal	#	68
6) Chloroethane	1.68	64	338	Below Cal	#	43
8) Diethyl Ether	2.10	74	818	0.243	ug/l	72
10) Methyl Iodide	2.41	142	356	3.917	ug/l #	90
11) Tert butyl alcohol	2.82	59	4050	2.898	ug/l #	76
16) Acetone	2.31	43	11592	3.386	ug/l	99
18) Methyl Acetate	2.61	43	3016	0.362	ug/l #	87
20) Methylene Chloride	2.69	84	6170	0.706	ug/l	91
31) Cyclohexane	4.96	56	7724	0.997	ug/l #	1
36) 1,1-Dichloropropene	4.96	75	30073	3.992	ug/l #	48
38) Carbon Tetrachloride	4.96	117	38332	4.765	ug/l #	15
43) Isopropyl Acetate	5.53	43	84652	6.092	ug/l	99
48) Methyl methacrylate	6.68	41	124482	18.861	ug/l #	37
49) 1,4-Dioxane	6.69	88	40	0.278	ug/l #	1
51) 4-Methyl-2-Pentanone	7.40	43	81925	8.517	ug/l #	45
54) cis-1,3-Dichloropropene	7.40	75	40709	3.896	ug/l #	62
56) Ethyl methacrylate	8.01	69	142	3.089	ug/l #	28
57) 1,3-Dichloropropane	8.40	76	5988	0.531	ug/l #	43
59) 2-Hexanone	8.40	43	82299	11.453	ug/l #	54
74) N-amyl acetate	9.92	43	2266	0.254	ug/l #	45
76) 1,2,3-Trichloropropane	10.29	75	162151	21.840	ug/l #	36
81) trans-1,4-Dichloro-2-buten	10.29	75	162151	73.448	ug/l #	100
93) 1,2,4-Trichlorobenzene	13.52	180	571	3.518	ug/l #	92
95) Naphthalene	13.77	128	2271	4.058	ug/l #	76
96) 1,2,3-Trichlorobenzene	13.98	180	594	2.711	ug/l	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU034294.D
Acq On : 05 Sep 2019 19:24
Operator : JC/SP
Sample : K4548-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
T11-2-(0)

Quant Time: Sep 06 07:40:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Quant Title : SW846 8260
QLast Update : Fri Sep 06 05:10:13 2019
Response via : Initial Calibration

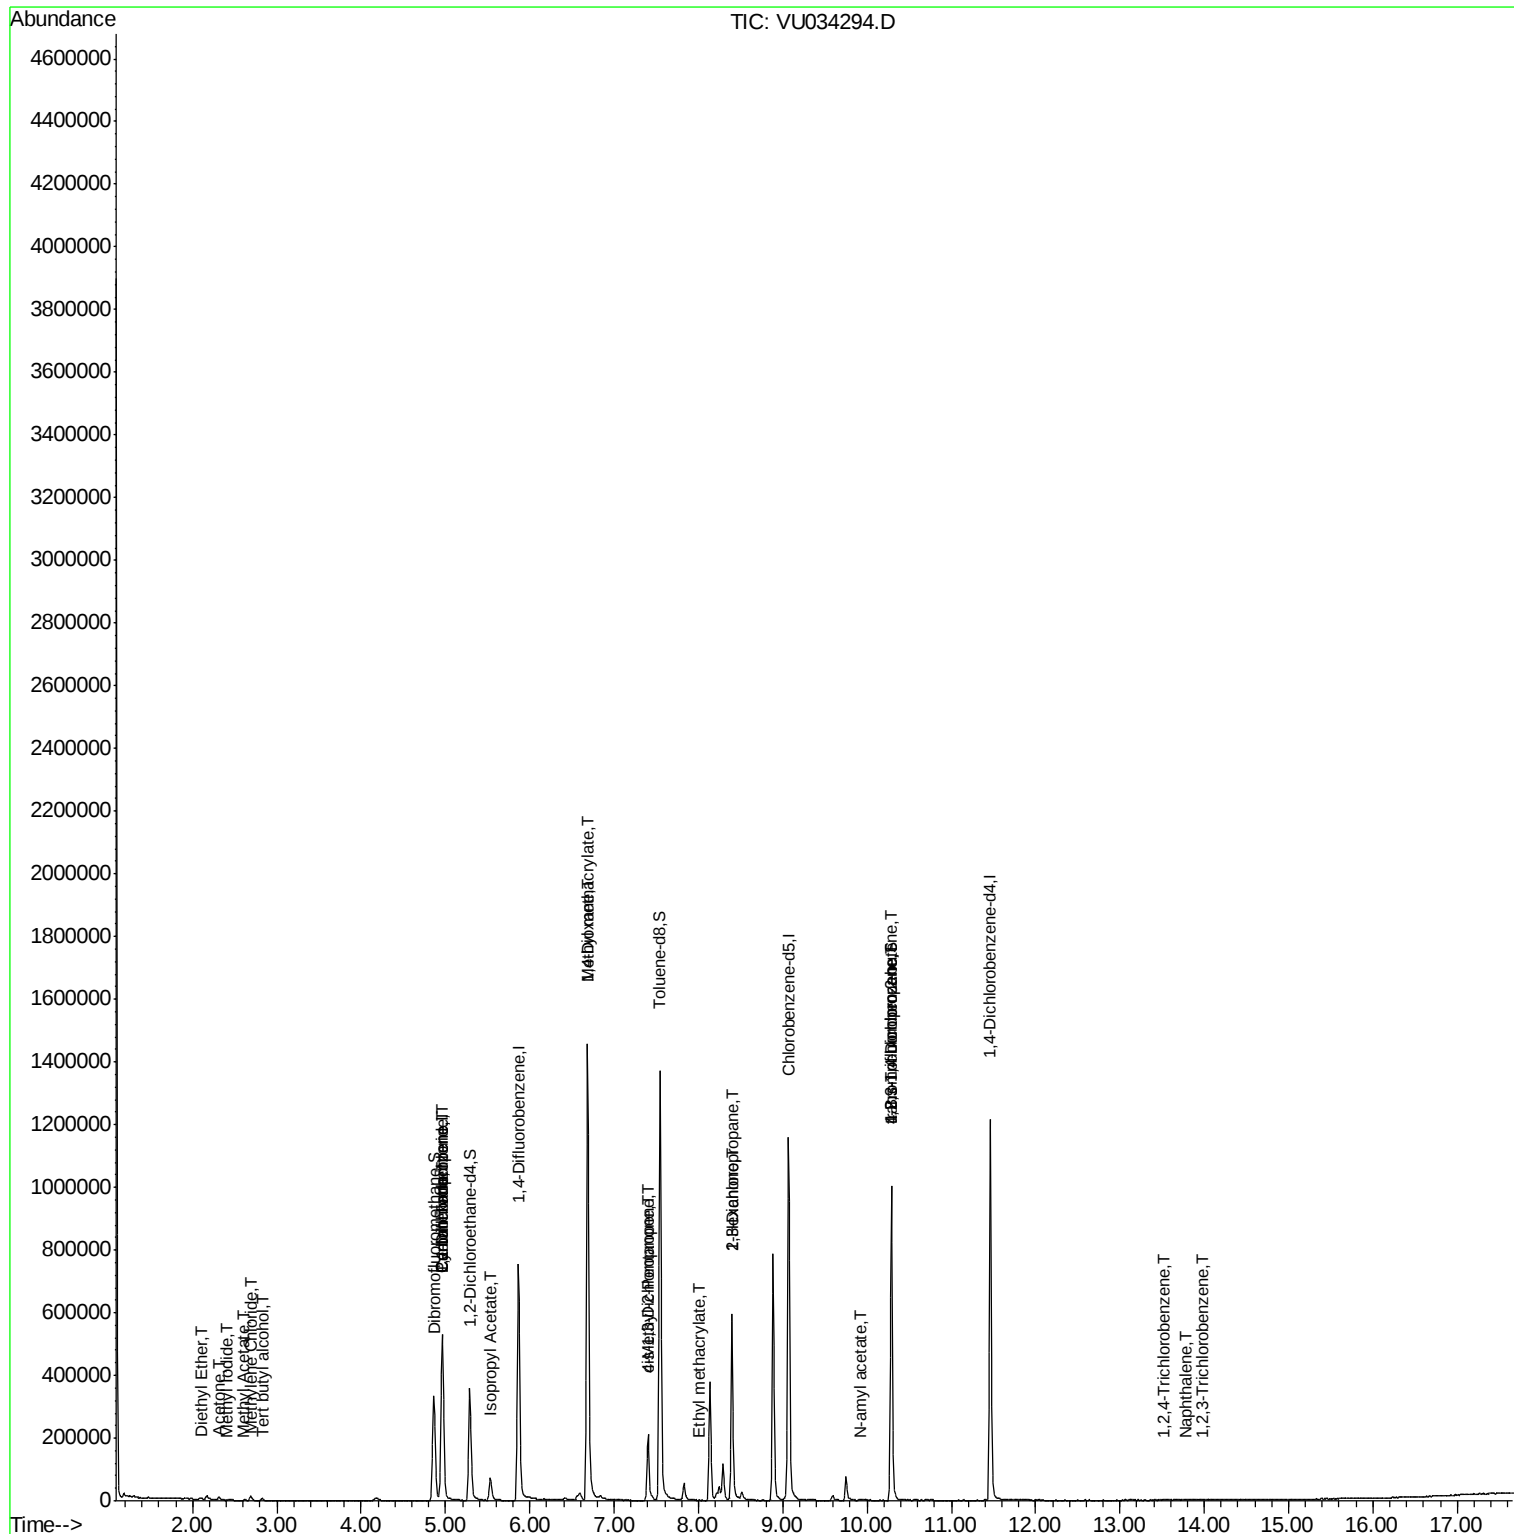

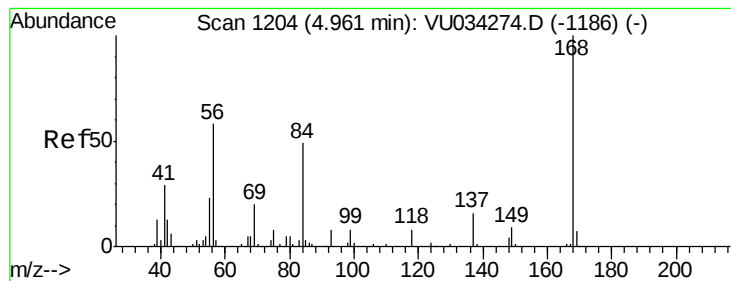

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.96 min Scan# 1205

Delta R.T. 0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :


T11-2-(0)

Tgt Ion:168 Resp: 437254

Ion Ratio Lower Upper

168 100

99 51.8 41.6 62.4



Abundance Ion 167.90 (167.60 to 168.60): VU034274.D (-1186) (-)

Ion 98.90 (98.60 to 99.60): VU034274.D (-1186) (-)

4.96

200000

150000

100000



50000

0

4.90

5.00

Time-->

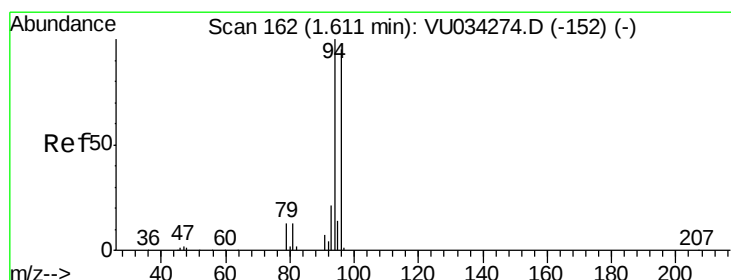

#5

Bromomethane

Concen: Below Cal

RT: 1.63 min Scan# 169

Delta R.T. 0.02 min

Lab File: VU034294.D


Acq: 05 Sep 2019 19:24

Tgt Ion: 94 Resp: 493

Ion Ratio Lower Upper

94 100

96 64.0 75.7 113.5#

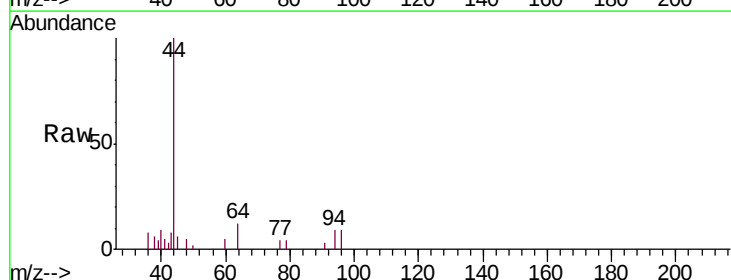

Abundance Ion 93.90 (93.60 to 94.60): VU034274.D (-152) (-)

Ion 95.90 (95.60 to 96.60): VU034274.D (-152) (-)

1.63

400

300

200

100


0


1.60

1.62

1.64

Time-->

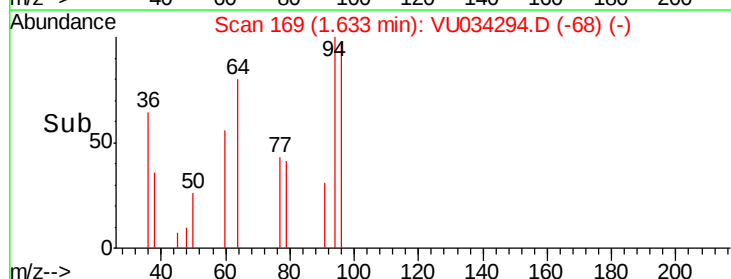

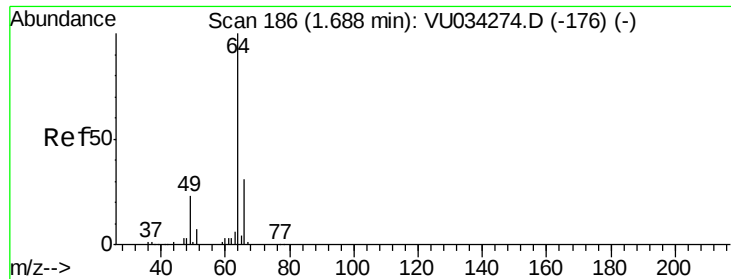

#6

Chloroethane

Concen: Below Cal

RT: 1.68 min Scan# 182

Delta R.T. -0.01 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :





T11-2-(0)

Tgt Ion: 64 Resp: 338

Ion Ratio Lower Upper

64 100

66 0.0 25.0 37.6#

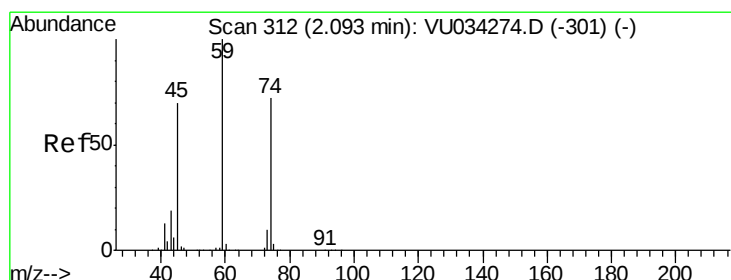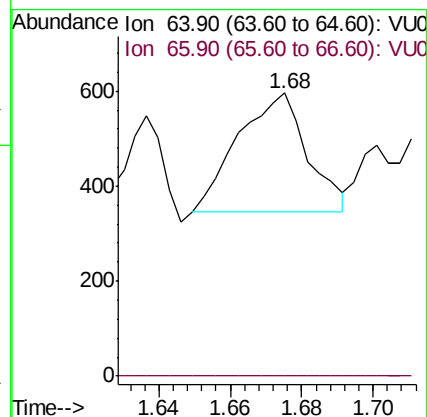

#8

Diethyl Ether

Concen: 0.243 ug/l

RT: 2.10 min Scan# 313

Delta R.T. 0.00 min

Lab File: VU034294.D




Acq: 05 Sep 2019 19:24


Tgt Ion: 74 Resp: 818

Ion Ratio Lower Upper

74 100

45 124.0 48.2 144.6



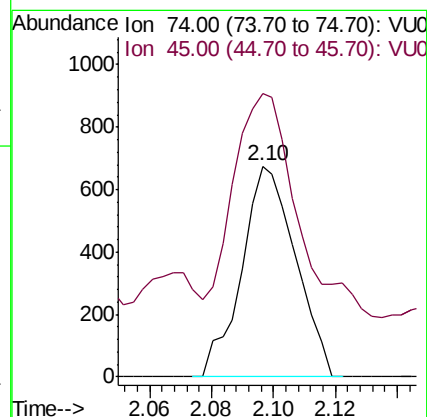



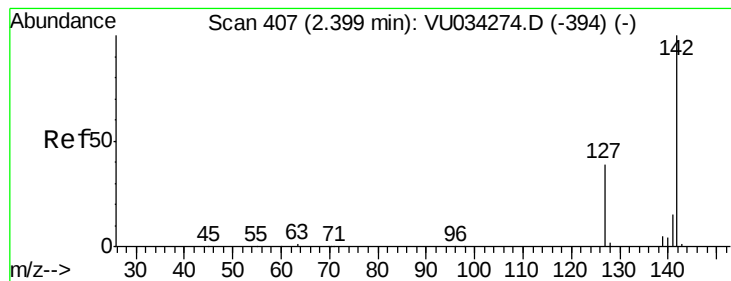

#10
Methyl Iodide
Concen: 3.917 ug/l
RT: 2.41 min Scan# 409
Delta R.T. 0.01 min
Lab File: VU034294.D
Acq: 05 Sep 2019 19:24




Instrument :
MSVOA_U
ClientSampleId :
T11-2-(0)


Tgt Ion: 142 Resp: 356
Ion Ratio Lower Upper
142 100
127 40.4 32.1 48.1
141 0.0 11.5 17.3#

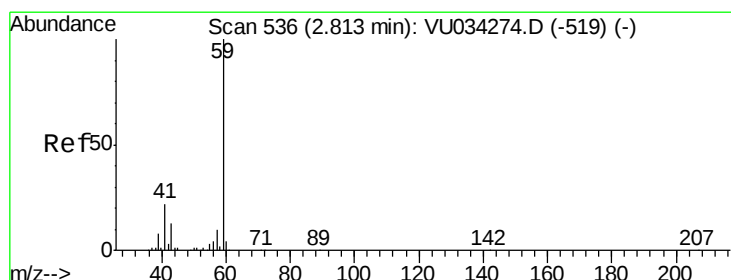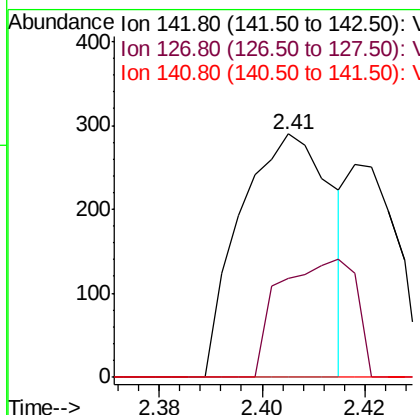

#11
Tert butyl alcohol
Concen: 2.898 ug/l
RT: 2.82 min Scan# 539
Delta R.T. 0.01 min
Lab File: VU034294.D
Acq: 05 Sep 2019 19:24

Tgt Ion: 59 Resp: 4050
Ion Ratio Lower Upper
59 100
57 1.0 7.9 11.9#

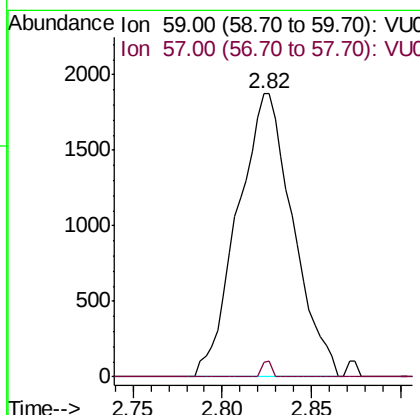

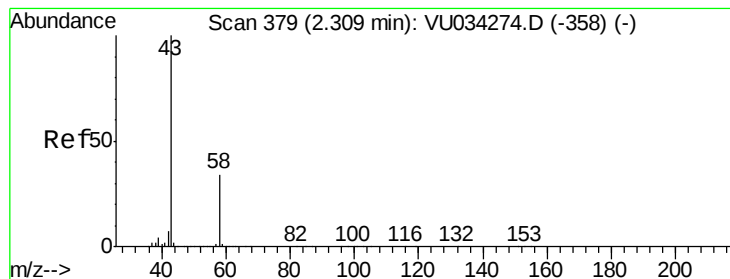

#16

Acetone

Concen: 3.386 ug/l

RT: 2.31 min Scan# 380

Delta R.T. 0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :


T11-2-(0)

Tgt Ion: 43 Resp: 11592

Ion Ratio Lower Upper

43 100

58 34.0 27.6 41.4



Abundance Ion 43.00 (42.70 to 43.70): VU034294.D (-380) (-)

Ion 58.00 (57.70 to 58.70): VU034294.D (-380) (-)

2.31

6000



4000

2000

0

2.25 2.30 2.35 2.40

Time-->



#18

Methyl Acetate

Concen: 0.362 ug/l

RT: 2.61 min Scan# 474

Delta R.T. 0.01 min

Lab File: VU034294.D


Acq: 05 Sep 2019 19:24

Tgt Ion: 43 Resp: 3016

Ion Ratio Lower Upper

43 100

74 17.0 18.9 28.3#



Abundance Ion 43.00 (42.70 to 43.70): VU034294.D (-474) (-)

Ion 74.00 (73.70 to 74.70): VU034294.D (-474) (-)

2.61

1500


1000


500

0

2.60 2.65

Time-->



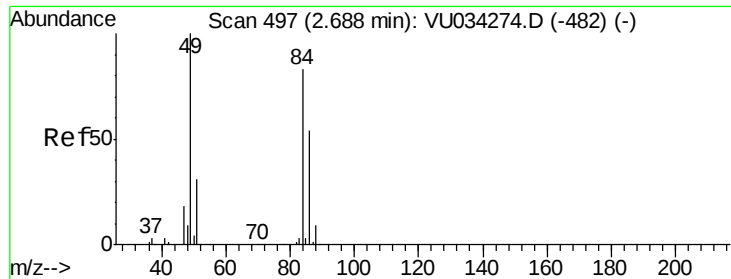

#20

Methylene Chloride

Concen: 0.706 ug/l

RT: 2.69 min Scan# 497

Delta R.T. 0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :
MSVOA_U
ClientSampleId :
T11-2-(0)

Tgt Ion: 84 Resp: 6170


Ion Ratio Lower Upper

84 100

49 106.0 96.0 144.0

51 32.1 30.0 45.0

86 62.1 51.4 77.0






Abundance Ion 83.90 (83.60 to 84.60): VU0

Ion 48.90 (48.60 to 49.60): VU0

Ion 50.90 (50.60 to 51.60): VU0

Ion 85.90 (85.60 to 86.60): VU0

Time-->

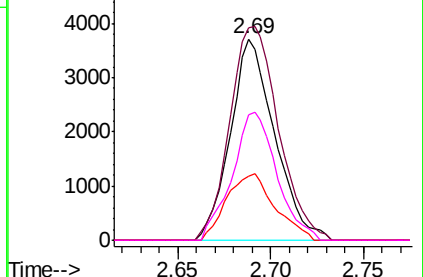

#31

Cyclohexane

Concen: 0.997 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. -0.01 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24


Tgt Ion: 56 Resp: 7724

Ion Ratio Lower Upper

56 100

69 174.0 26.7 40.1#

84 160.0 68.2 102.4#






Abundance Ion 56.00 (55.70 to 56.70): VU0

Ion 69.00 (68.70 to 69.70): VU0

Ion 84.00 (83.70 to 84.70): VU0

Time-->

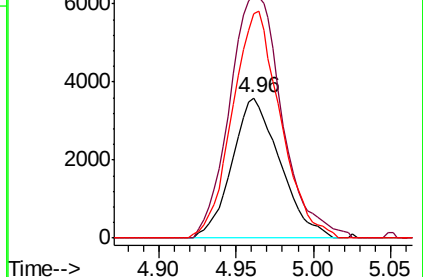

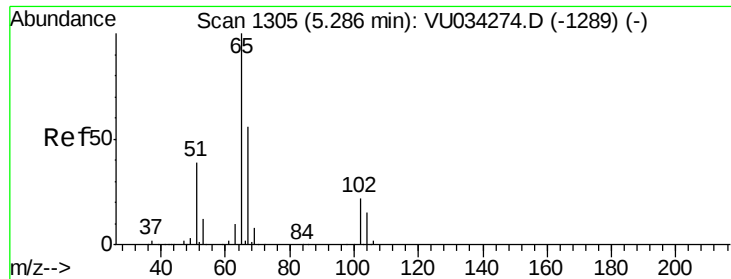

#33

1,2-Dichloroethane-d4

Concen: 41.797 ug/l

RT: 5.29 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :





T11-2-(0)

Tgt Ion: 65 Resp: 276523

Ion Ratio Lower Upper

65 100

67 55.8 0.0 112.4

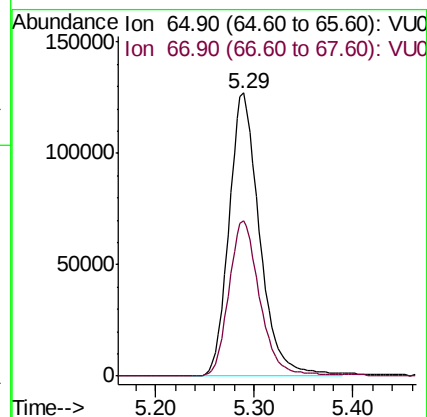

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 5.87 min Scan# 1486

Delta R.T. 0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24




Tgt Ion: 114 Resp: 694710


Ion Ratio Lower Upper

114 100

63 20.6 0.0 42.4

88 16.1 0.0 32.4



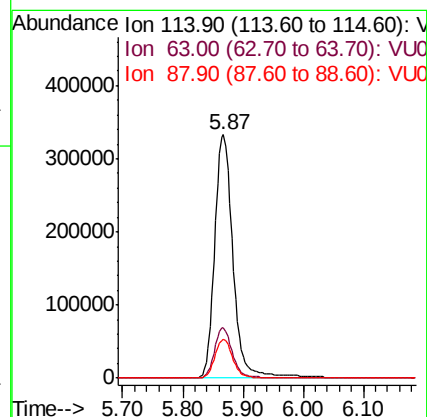





#35
 Dibromofluoromethane
 Concen: 37.275 ug/l
 RT: 4.86 min Scan# 1173
 Delta R.T. 0.00 min
 Lab File: VU034294.D
 Acq: 05 Sep 2019 19:24




Instrument :
 MSVOA_U
 ClientSampleId :
 T11-2-(0)


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.5	81.5	122.3
192	21.9	17.8	26.8

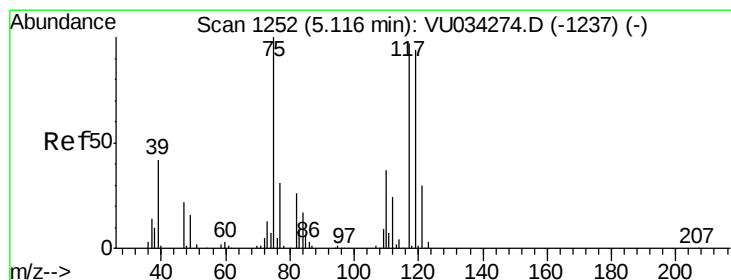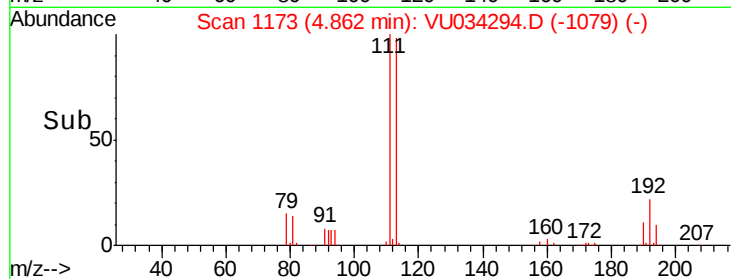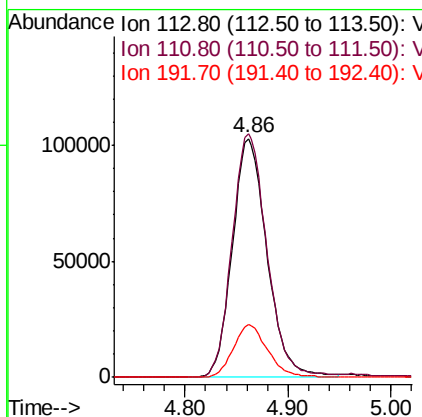

#36
 1,1-Dichloropropene
 Concen: 3.992 ug/l
 RT: 4.96 min Scan# 1204
 Delta R.T. -0.15 min
 Lab File: VU034294.D
 Acq: 05 Sep 2019 19:24

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.0	18.3	54.9#
77	0.0	24.9	37.3#

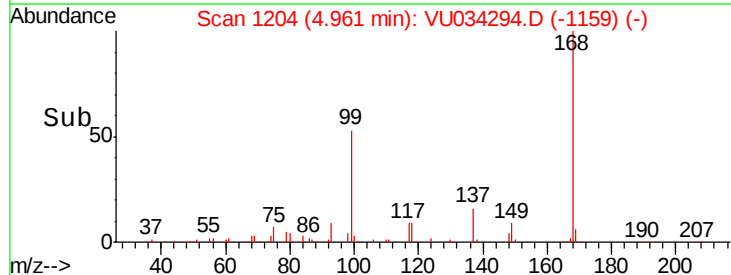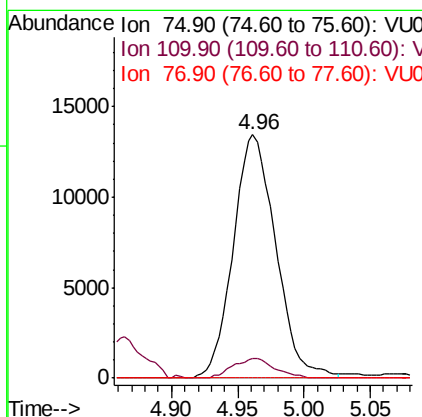

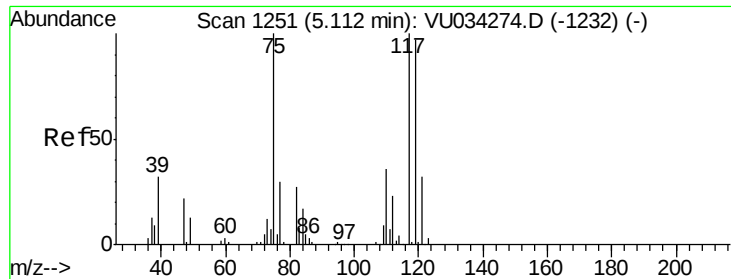

#38

Carbon Tetrachloride

Concen: 4.765 ug/l

RT: 4.96 min Scan# 1204

Delta R.T. -0.15 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :

T11-2-(0)


Tgt Ion:117 Resp: 38332

Ion Ratio Lower Upper

117 100

119 4.8 77.8 116.6#




121 0.0 25.2 37.8#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

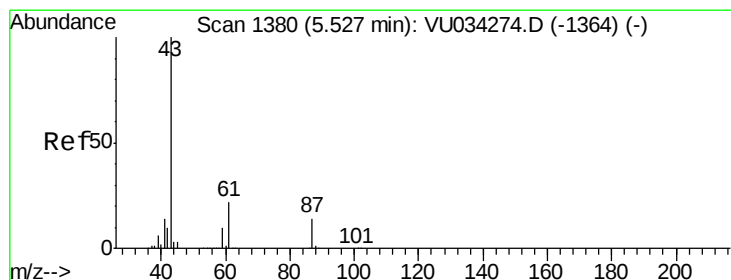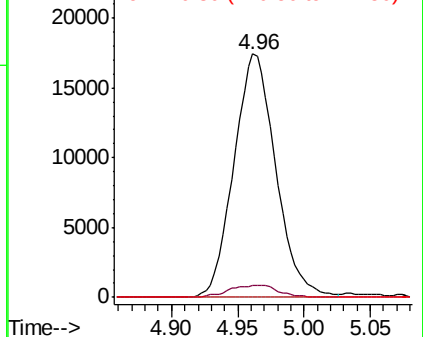

#43

Isopropyl Acetate

Concen: 6.092 ug/l

RT: 5.53 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24


Tgt Ion: 43 Resp: 84652

Ion Ratio Lower Upper

43 100

61 22.1 17.1 25.7



87 13.8 11.1 16.7




Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 87.00 (86.70 to 87.70): VU0




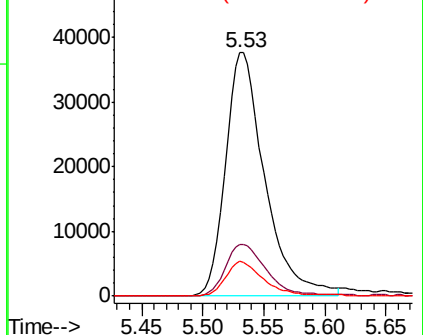




#48
Methyl methacrylate
Concen: 18.861 ug/l
RT: 6.68 min Scan# 1740
Delta R.T. 0.08 min
Lab File: VU034294.D
Acq: 05 Sep 2019 19:24




Instrument :
MSVOA_U
ClientSampleId :
T11-2-(0)


Tgt Ion: 41 Resp: 124482
Ion Ratio Lower Upper
41 100
69 0.1 72.8 109.2#
39 47.3 38.6 58.0

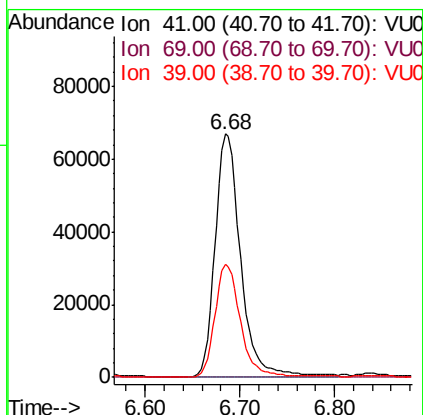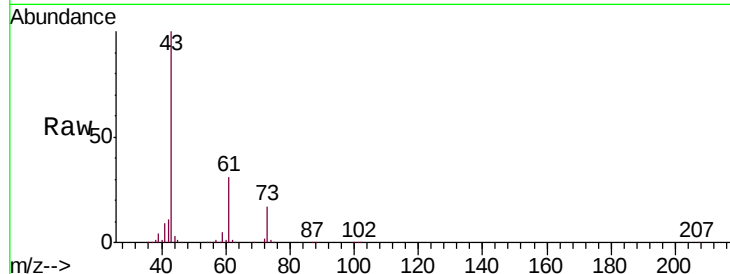

#49
1,4-Dioxane
Concen: 0.278 ug/l
RT: 6.69 min Scan# 1741
Delta R.T. 0.10 min
Lab File: VU034294.D
Acq: 05 Sep 2019 19:24

Tgt Ion: 88 Resp: 40
Ion Ratio Lower Upper
88 100
43 3600895.0 23.8 35.6#
58 18957.5 58.4 87.6#



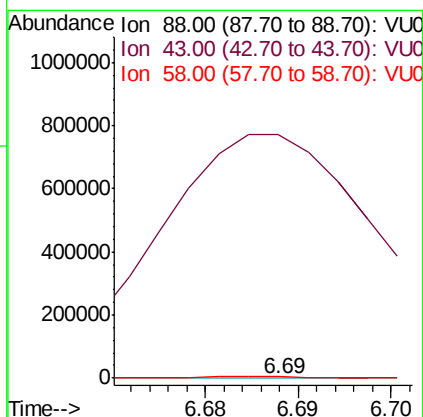
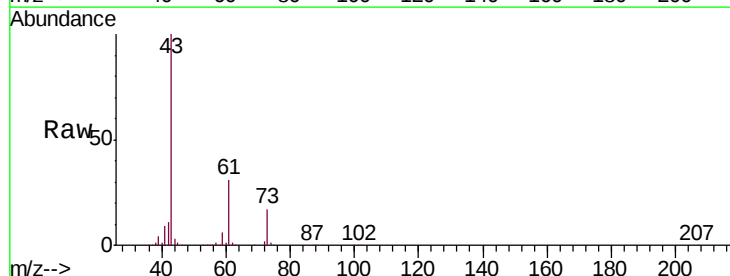




#50
Toluene-d8
Concen: 40.007 ug/l
RT: 7.55 min Scan# 2008
Delta R.T. -0.00 min
Lab File: VU034294.D
Acq: 05 Sep 2019 19:24




Instrument :
MSVOA_U
ClientSampleId :
T11-2-(0)


Tgt Ion: 98 Resp: 971637
Ion Ratio Lower Upper
98 100
100 65.0 51.7 77.5

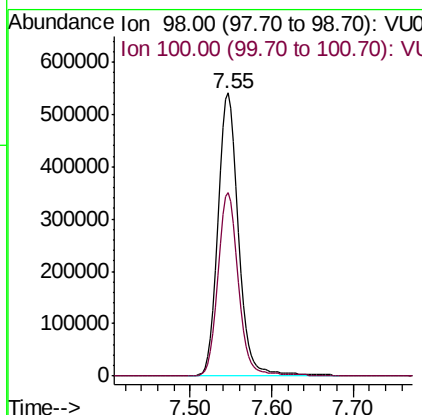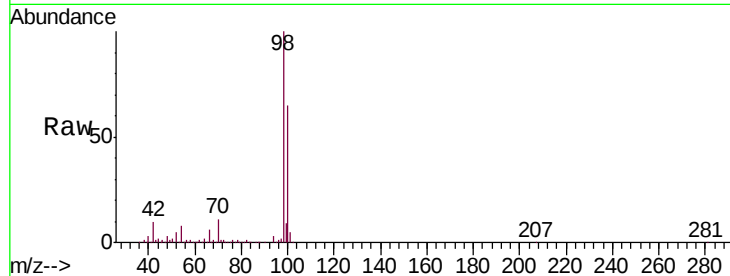

#51
4-Methyl-2-Pentanone
Concen: 8.517 ug/l
RT: 7.40 min Scan# 1963
Delta R.T. -0.04 min
Lab File: VU034294.D
Acq: 05 Sep 2019 19:24

Tgt Ion: 43 Resp: 81925
Ion Ratio Lower Upper
43 100
58 6.9 33.0 49.4#

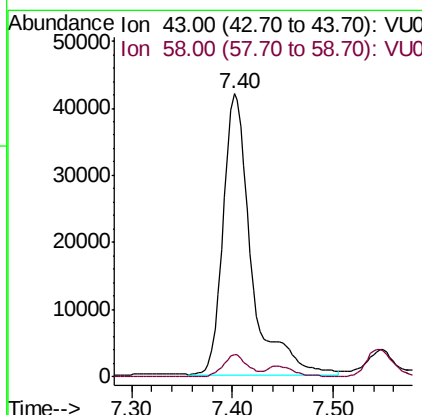



#54

cis-1,3-Dichloropropene

Concen: 3.896 ug/l

RT: 7.40 min Scan# 1963

Delta R.T. 0.15 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :

T11-2-(0)


Tgt Ion: 75 Resp: 40709

Ion Ratio Lower Upper

75 100

77 0.5 25.1 37.7#




39 24.4 31.2 46.8#

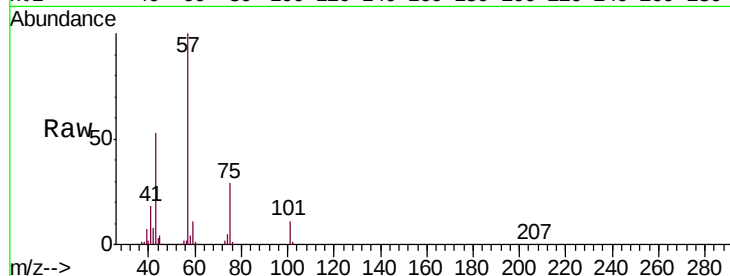

Abundance Ion 74.90 (74.60 to 75.60): VU034294.D (-1963) (-)

Ion 76.90 (76.60 to 77.60): VU034294.D (-1963) (-)

Ion 39.00 (38.70 to 39.70): VU034294.D (-1963) (-)

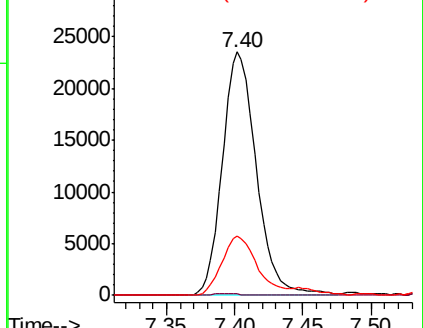

#56

Ethyl methacrylate

Concen: 3.089 ug/l

RT: 8.01 min Scan# 2151

Delta R.T. 0.01 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24


Tgt Ion: 69 Resp: 142

Ion Ratio Lower Upper

69 100

41 0.0 49.5 74.3#



39 0.0 22.5 33.7#




Abundance Ion 69.00 (68.70 to 69.70): VU034294.D (-2151) (-)

Ion 41.00 (40.70 to 41.70): VU034294.D (-2151) (-)

Ion 39.00 (38.70 to 39.70): VU034294.D (-2151) (-)

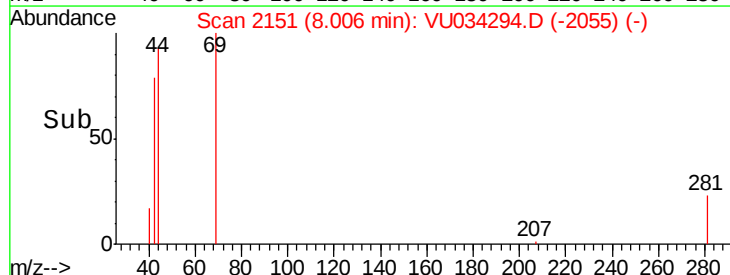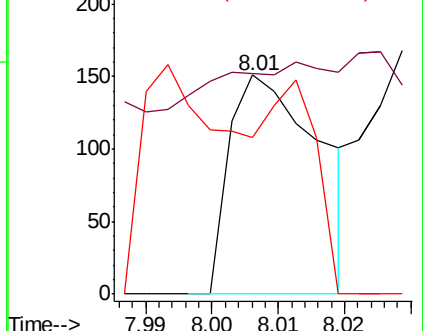



#57

1,3-Dichloropropane

Concen: 0.531 ug/l

RT: 8.40 min Scan# 2272

Delta R.T. 0.17 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :


T11-2-(0)

Tgt Ion: 76 Resp: 5988

Ion Ratio Lower Upper




76 100

78 0.0 25.4 38.2#



Abundance Ion 75.90 (75.60 to 76.60): VU034294.D (-2125) (-)

Ion 77.90 (77.60 to 78.60): VU034294.D (-2125) (-)

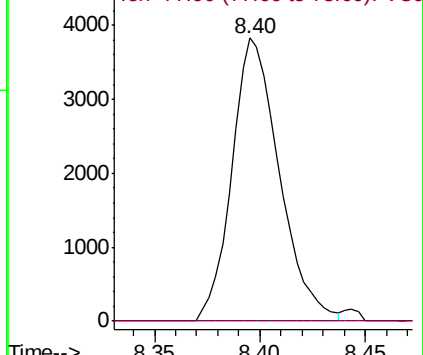

#59

2-Hexanone

Concen: 11.453 ug/l

RT: 8.40 min Scan# 2273

Delta R.T. 0.05 min

Lab File: VU034294.D


Acq: 05 Sep 2019 19:24

Tgt Ion: 43 Resp: 82299

Ion Ratio Lower Upper



43 100


58 23.8 28.8 86.5#



Abundance Ion 43.00 (42.70 to 43.70): VU034294.D (-2163) (-)

Ion 58.00 (57.70 to 58.70): VU034294.D (-2163) (-)

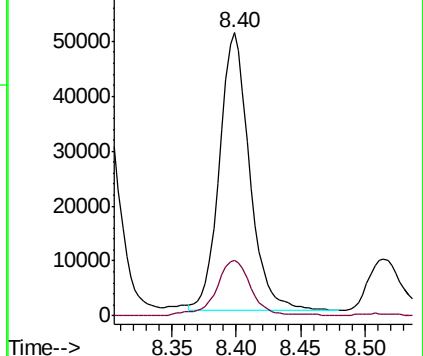



#62

4-Bromofluorobenzene

Concen: 36.725 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :

T11-2-(0)


Tgt Ion: 95 Resp: 344367

Ion Ratio Lower Upper

95 100

174 87.2 0.0 175.2

176 83.8 0.0 168.0






Abundance Ion 94.90 (94.60 to 95.60): VU034274.D (-2846) (-)

Ion 173.80 (173.50 to 174.50): VU034274.D (-2846) (-)

Ion 175.80 (175.50 to 176.50): VU034274.D (-2846) (-)

Time-->

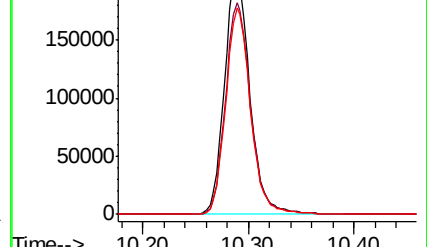

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 9.07 min Scan# 2482

Delta R.T. -0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24


Tgt Ion: 117 Resp: 683495

Ion Ratio Lower Upper

117 100

82 55.0 44.6 67.0

119 32.7 25.9 38.9






Abundance Ion 116.90 (116.60 to 117.60): VU034274.D (-2468) (-)

Ion 82.00 (81.70 to 82.70): VU034274.D (-2468) (-)

Ion 118.90 (118.60 to 119.60): VU034274.D (-2468) (-)

Time-->

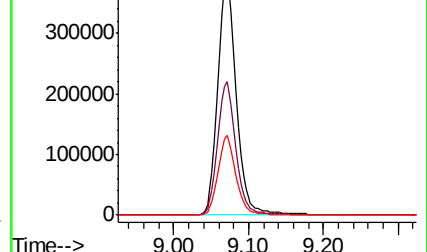



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.46 min Scan# 3226

Delta R.T. -0.00 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :

T11-2-(0)


Tgt Ion:152 Resp: 340126

Ion Ratio Lower Upper

152 100

115 55.6 39.1 117.3




150 157.0 0.0 345.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

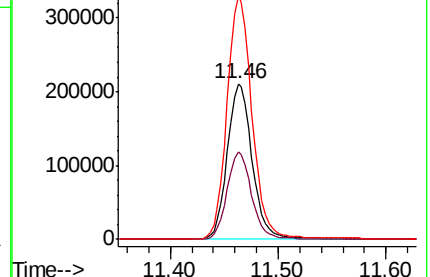

#74

N-ethyl acetate

Concen: 0.254 ug/l

RT: 9.92 min Scan# 2747

Delta R.T. -0.07 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Tgt Ion: 43 Resp: 2266


Ion Ratio Lower Upper

43 100

70 0.0 36.4 54.6#

55 8.3 21.2 31.8#

61 0.0 20.4 30.6#






Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 55.00 (54.70 to 55.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

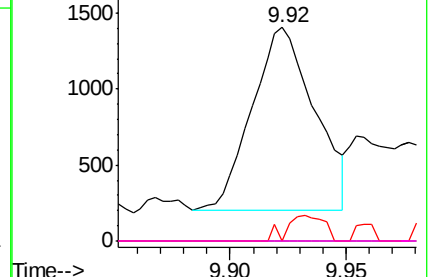

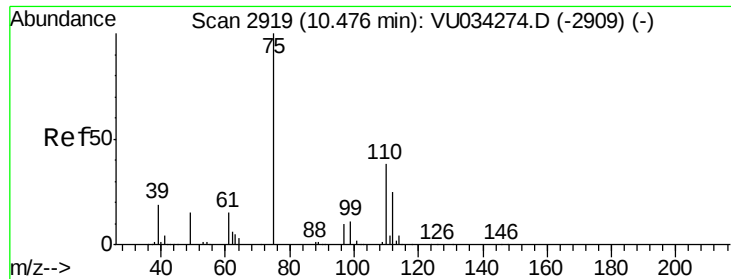

#76

1,2,3-Trichloropropane

Concen: 21.840 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.19 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24

Instrument :

MSVOA_U

ClientSampled :


T11-2-(0)

Tgt Ion: 75 Resp: 162151

Ion Ratio Lower Upper

75 100

77 1.3 20.8 62.2#



Abundance Ion 74.90 (74.60 to 75.60): VU034274.D (-2909) (-)

Ion 77.00 (76.70 to 77.70): VU034274.D (-2909) (-)

10.29

100000

80000



60000

40000

20000

0

Time-->



#81

trans-1,4-Dichloro-2-butene

Concen: 73.448 ug/l

RT: 10.29 min Scan# 2861

Delta R.T. -0.20 min

Lab File: VU034294.D

Acq: 05 Sep 2019 19:24


Tgt Ion: 75 Resp: 162151

Ion Ratio Lower Upper

75 100

53 0.1 0.0 0.0#

89 0.0 0.0 0.0



Abundance Ion 74.90 (74.60 to 75.60): VU034274.D (-2924) (-)

Ion 53.00 (52.70 to 53.70): VU034274.D (-2924) (-)

Ion 88.90 (88.60 to 89.60): VU034274.D (-2924) (-)


10.29


100000

50000

0

Time-->




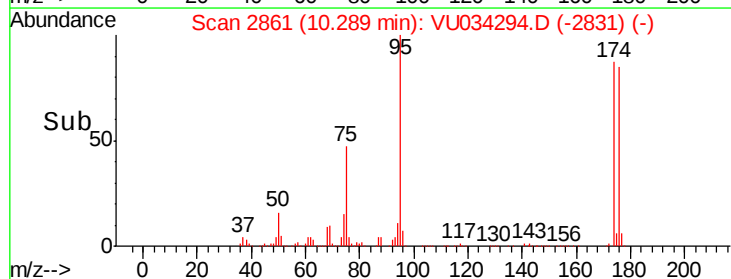




#93
 1,2,4-Trichlorobenzene
 Concen: 3.518 ug/l
 RT: 13.52 min Scan# 3866
 Delta R.T. 0.04 min
 Lab File: VU034294.D
 Acq: 05 Sep 2019 19:24




Instrument :
 MSVOA_U
 ClientSampleId :
 T11-2-(0)


Tgt Ion:180 Resp: 571
 Ion Ratio Lower Upper
 180 100
 182 96.3 47.9 143.8
 145 12.1 14.4 43.0#

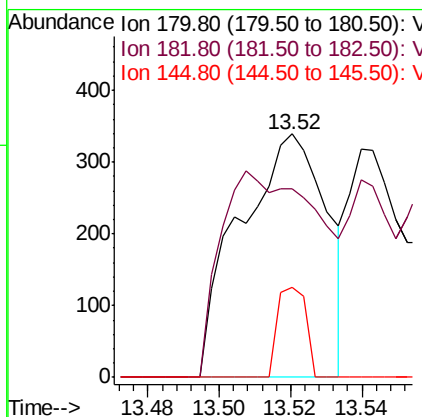

#95
 Naphthalene
 Concen: 4.058 ug/l
 RT: 13.77 min Scan# 3945
 Delta R.T. 0.05 min
 Lab File: VU034294.D
 Acq: 05 Sep 2019 19:24

Tgt Ion:128 Resp: 2271
 Ion Ratio Lower Upper
 128 100
 127 5.2 10.6 15.8#
 129 0.0 8.4 12.6#

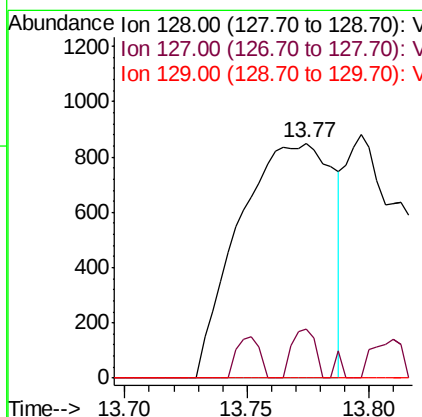

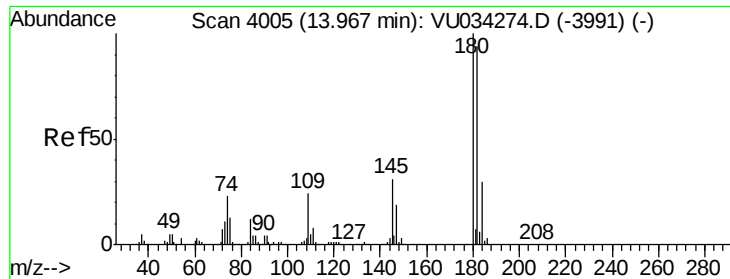

#96
 1,2,3-Trichlorobenzene
 Concen: 2.711 ug/l
 RT: 13.98 min Scan# 4010
 Delta R.T. 0.02 min
 Lab File: VU034294.D
 Acq: 05 Sep 2019 19:24

Instrument :
 MSVOA_U
 ClientSampleId :
 T11-2-(0)

Tgt Ion	Ratio	Lower	Upper
180	100		
182	100.2	48.4	145.0
145	16.8	15.4	46.4

