


Ethyl methacrylate

Response Ratio

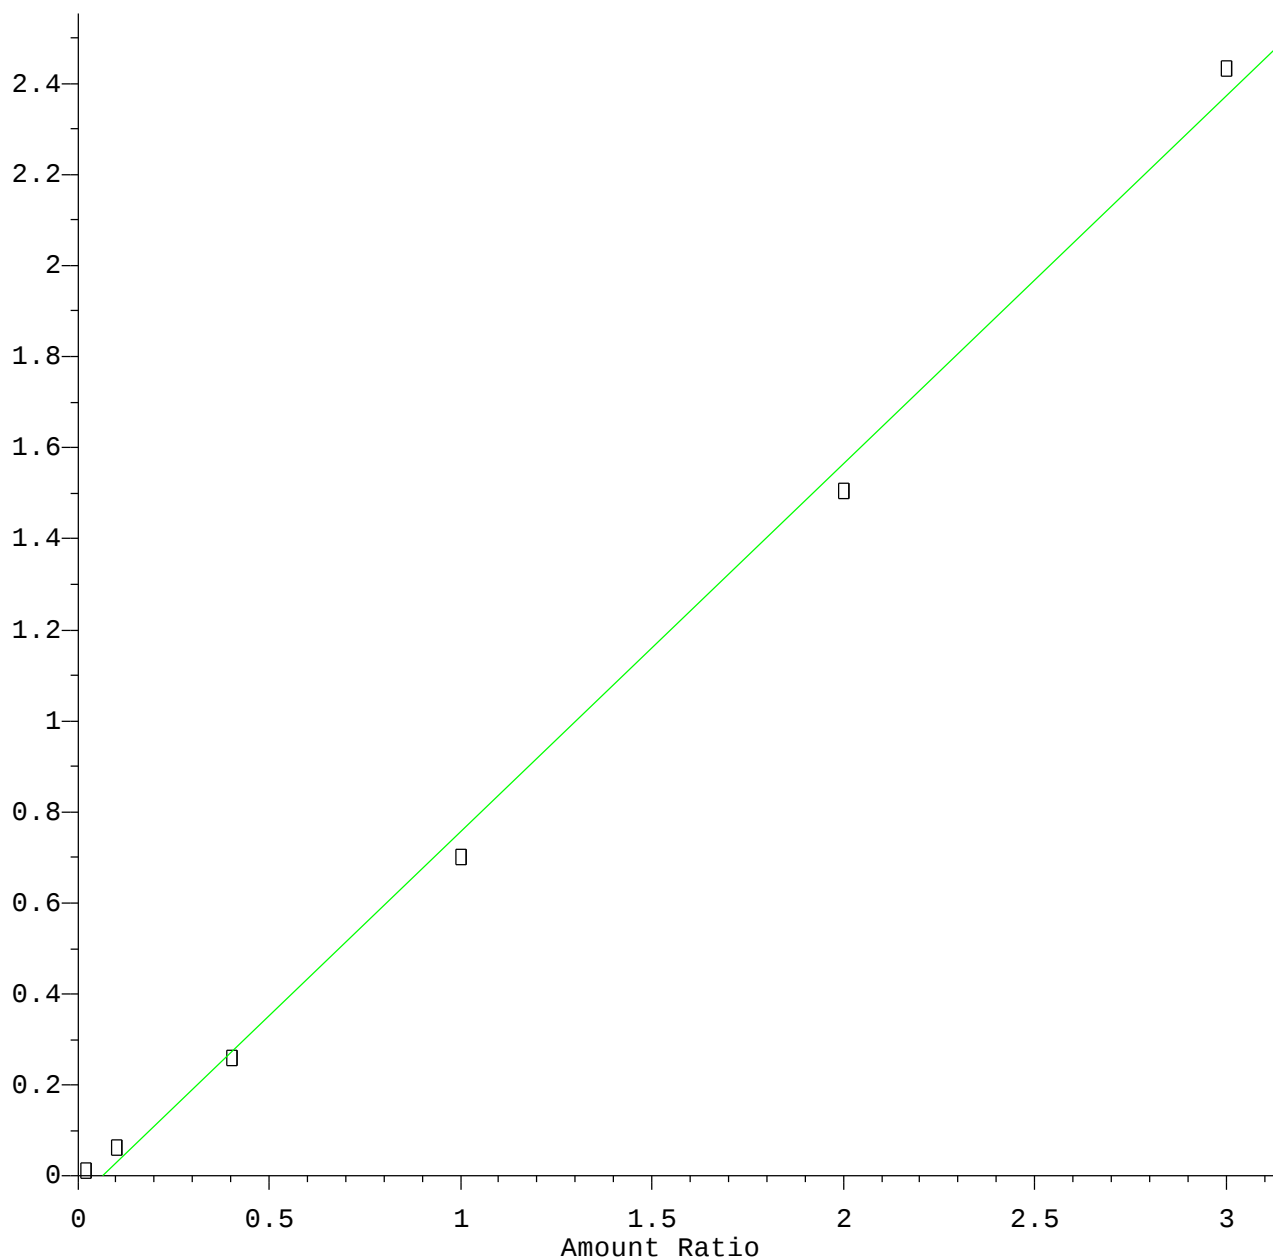


Resp Ratio = $8.07 \times 10^{-1} \times \text{Amt} - 4.96 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

2-Chloroethyl Vinyl ether

Response Ratio

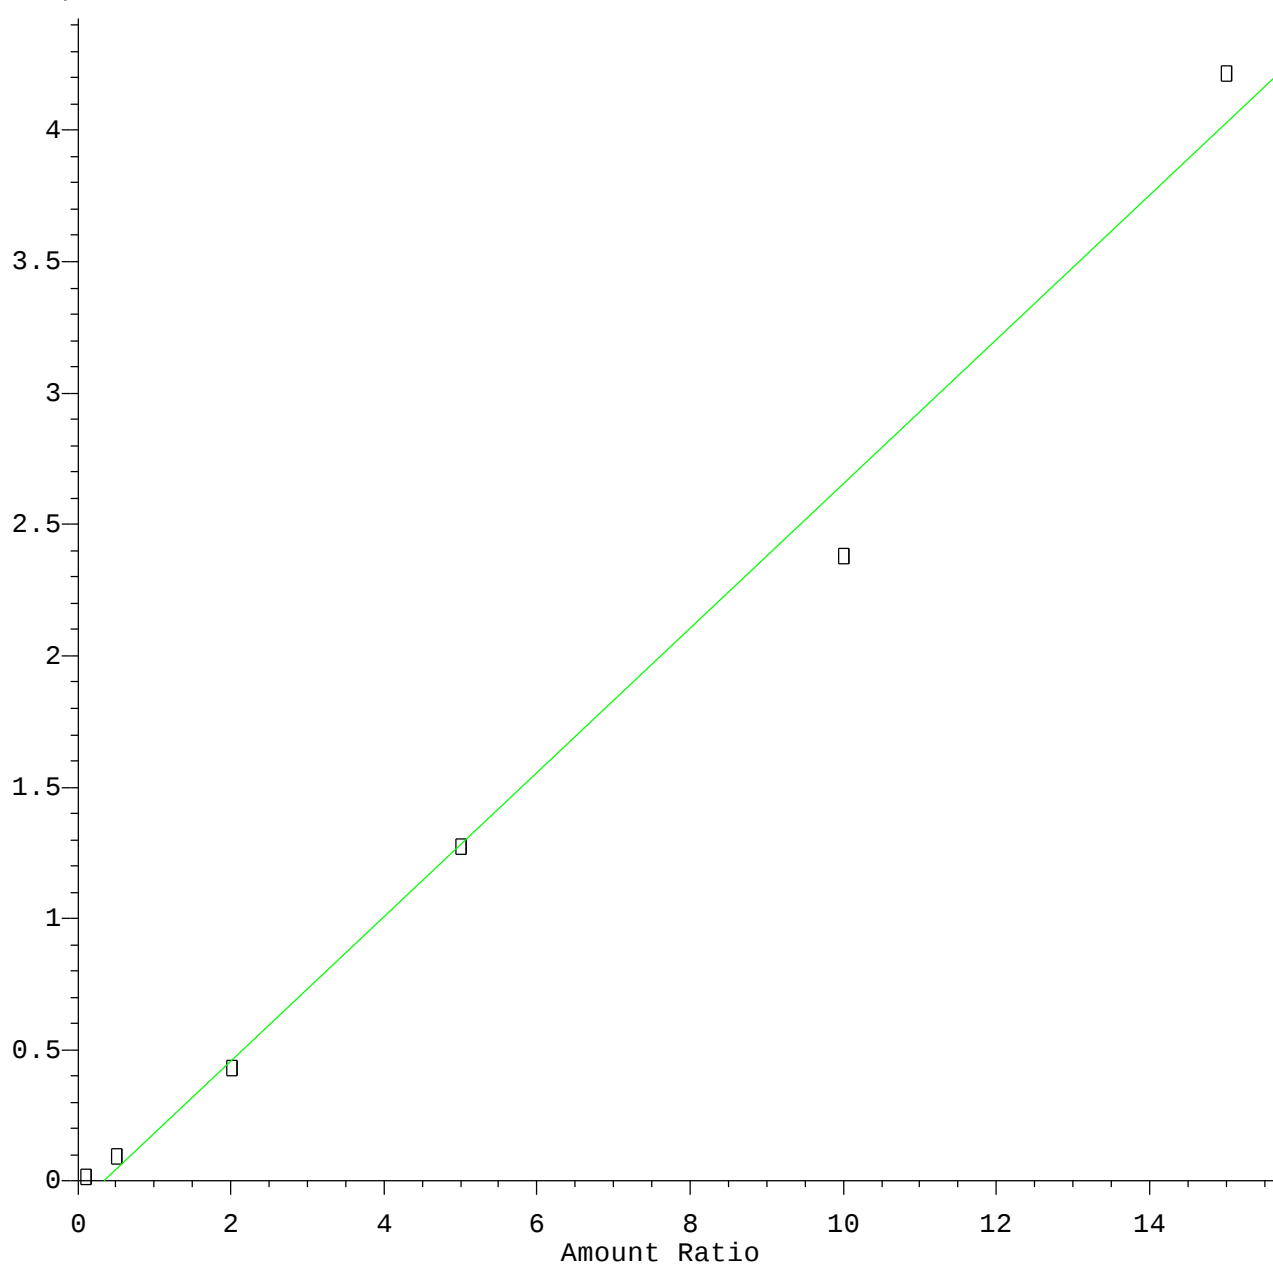


Resp Ratio = $2.74 \times 10^{-1} \times \text{Amt} - 9.12 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

1,2,4-Trichlorobenzene

Response Ratio

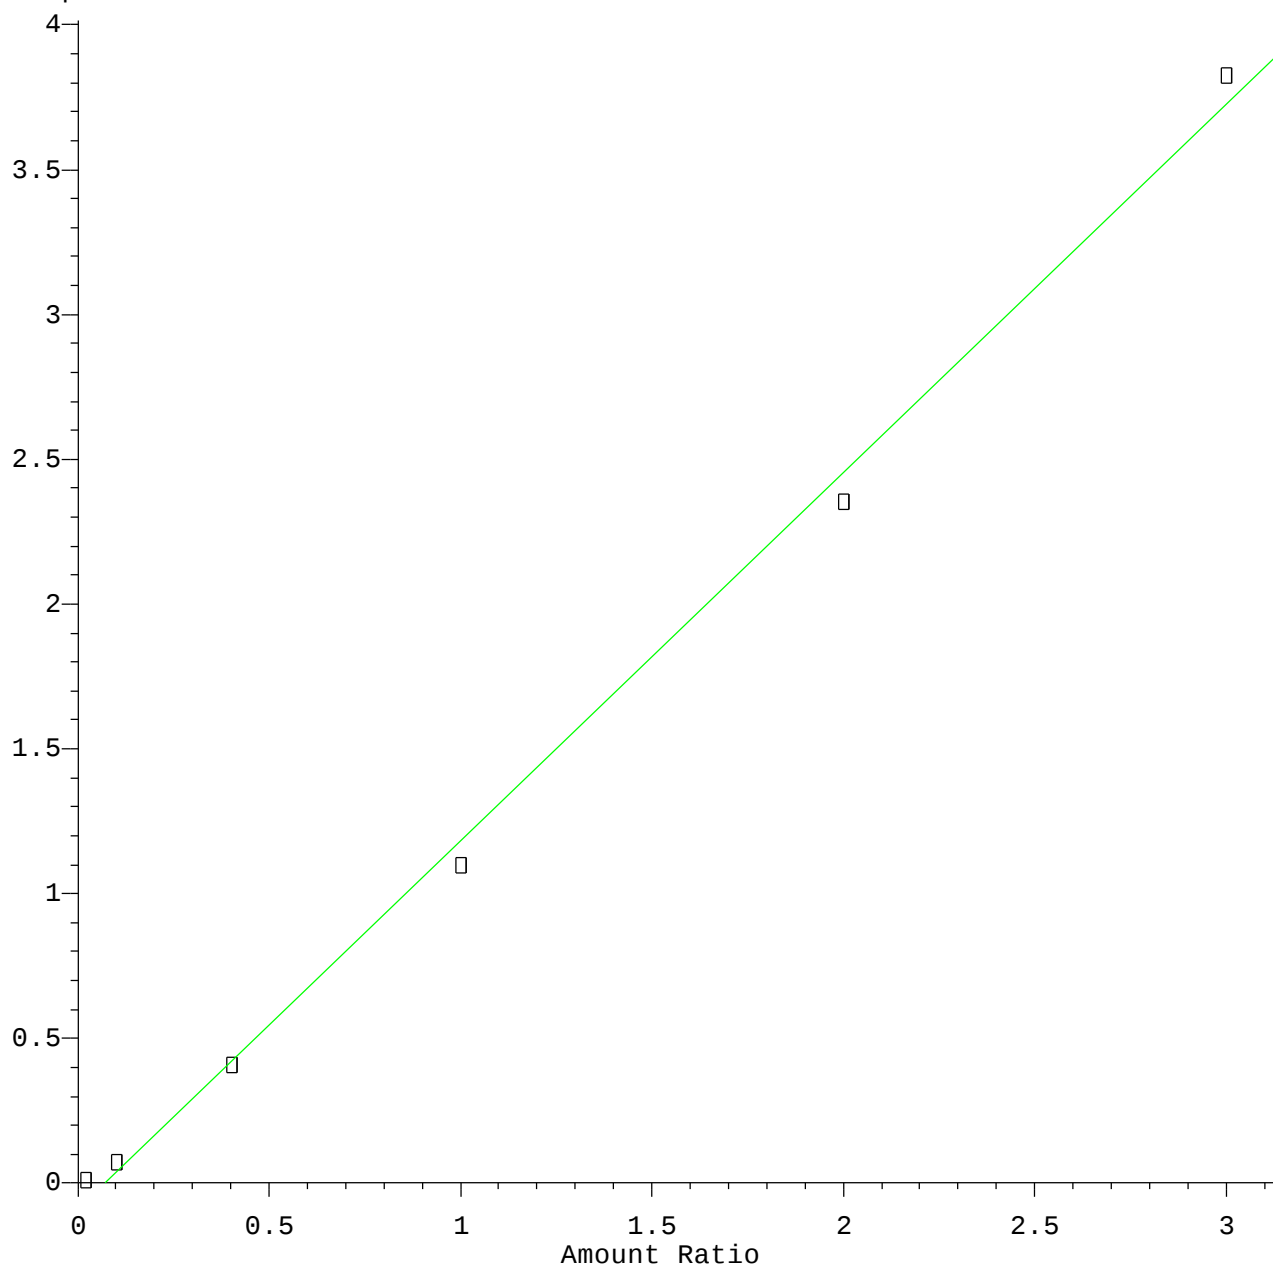


Resp Ratio = 1.27e+000 * Amt - 8.77e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

Naphthalene

Response Ratio

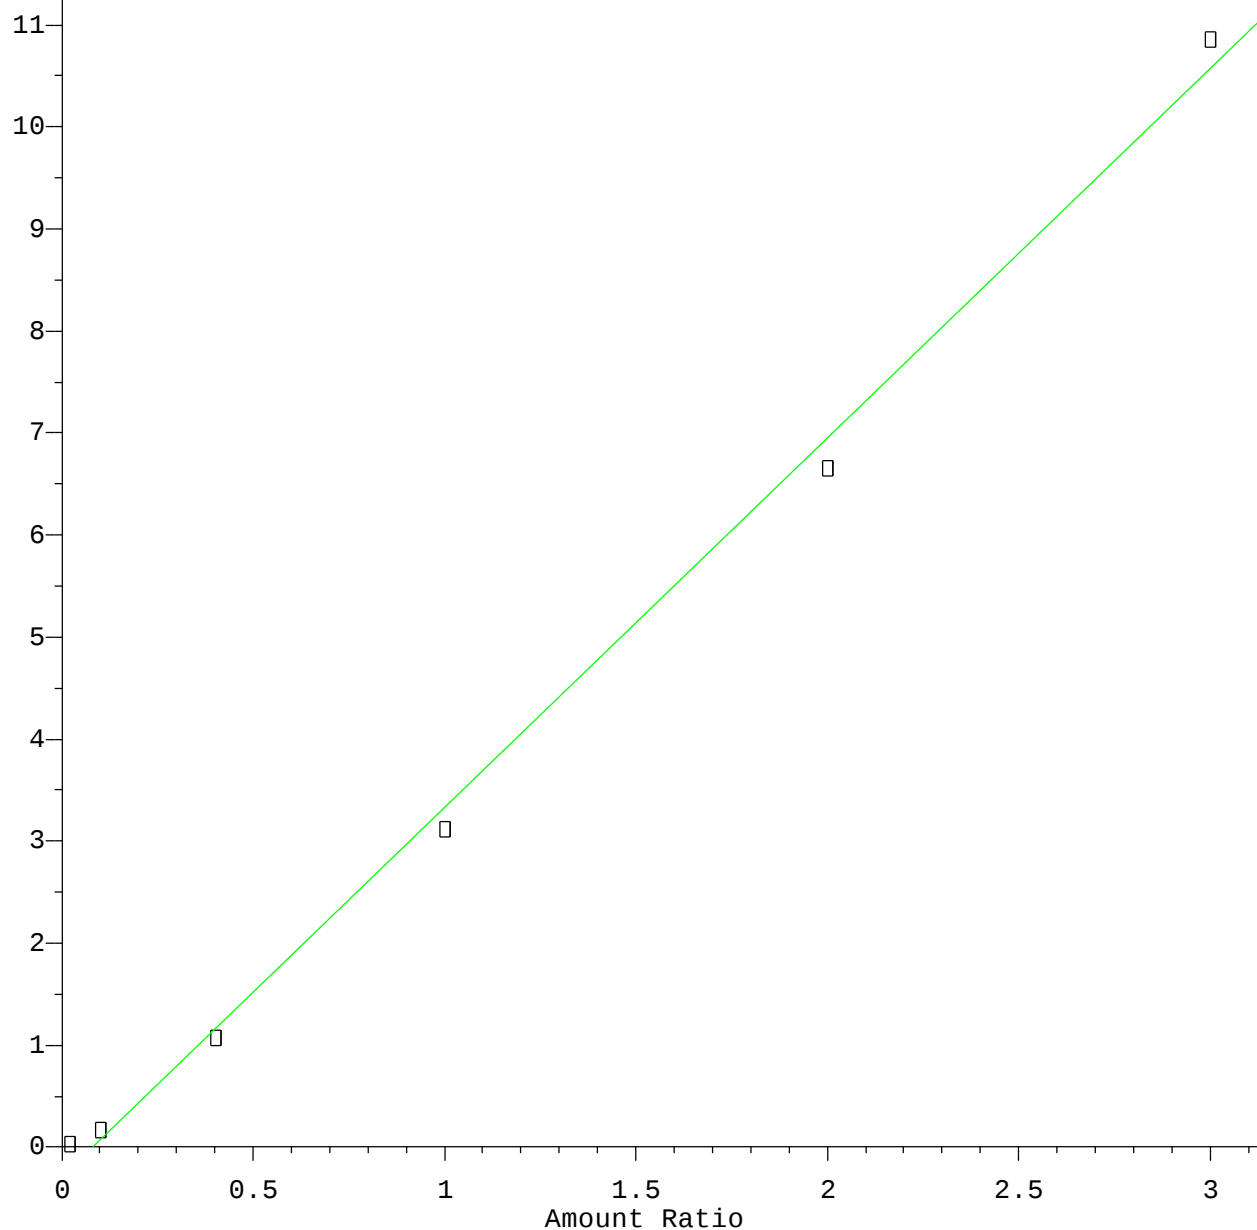


Resp Ratio = 3.62×10^0 * Amt - 2.87×10^{-1}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019


1,2,3-Trichlorobenzene

Response Ratio

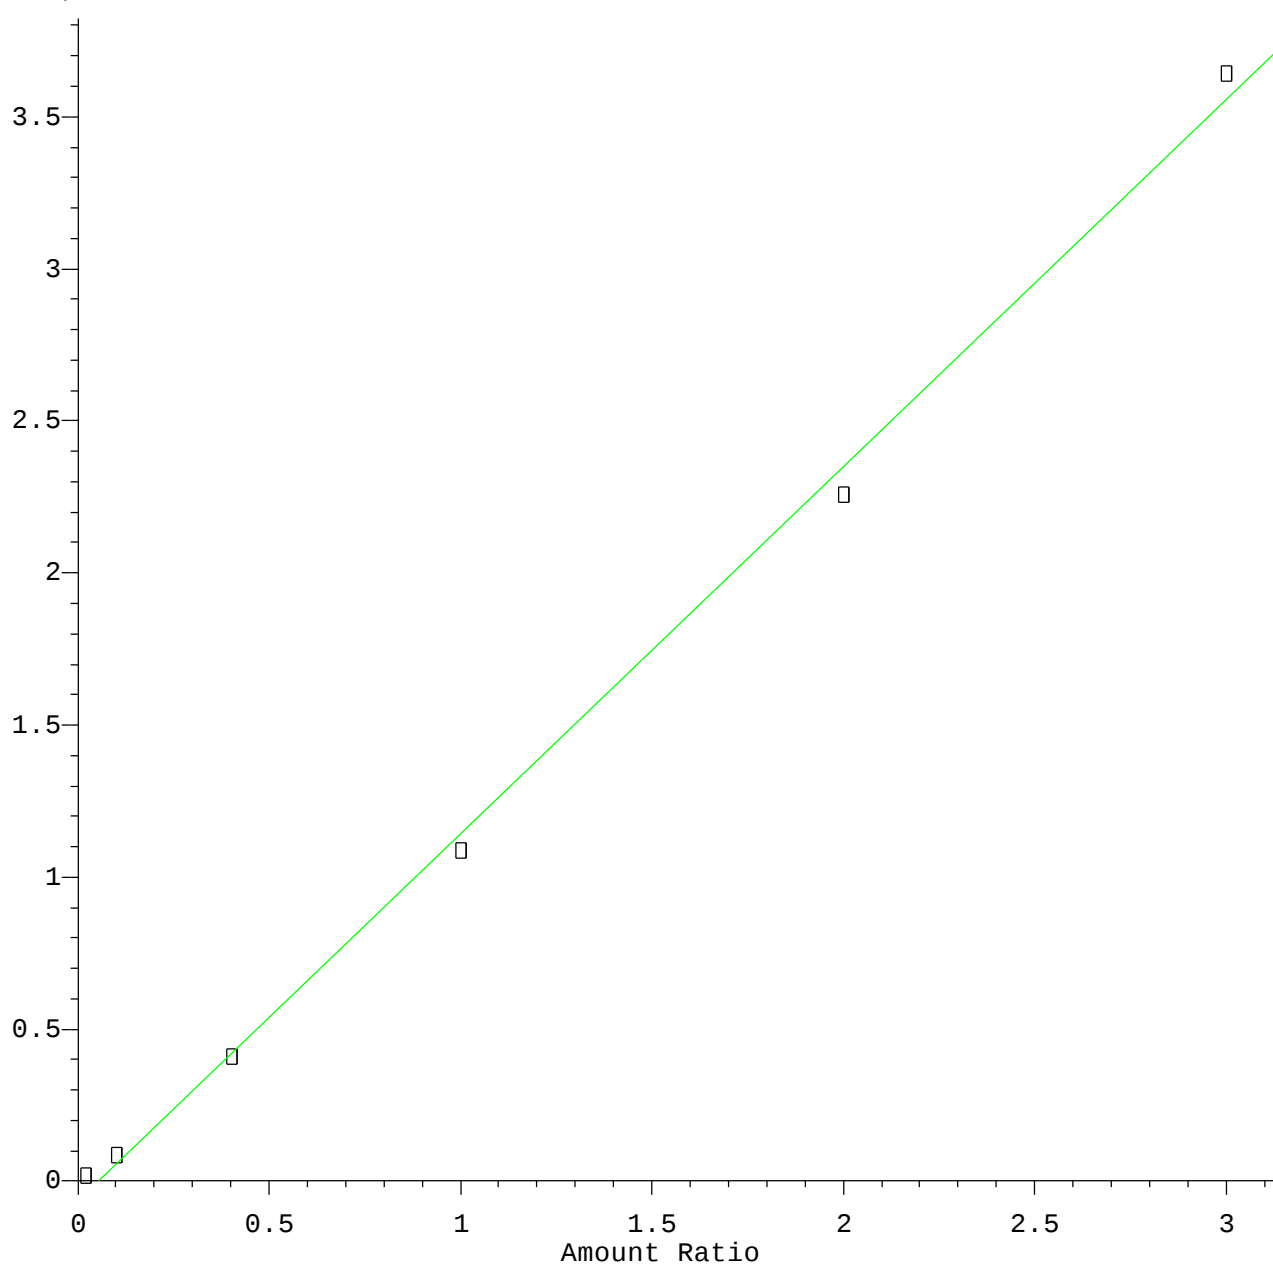


Resp Ratio = 1.21×10^0 * Amt - 6.37×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

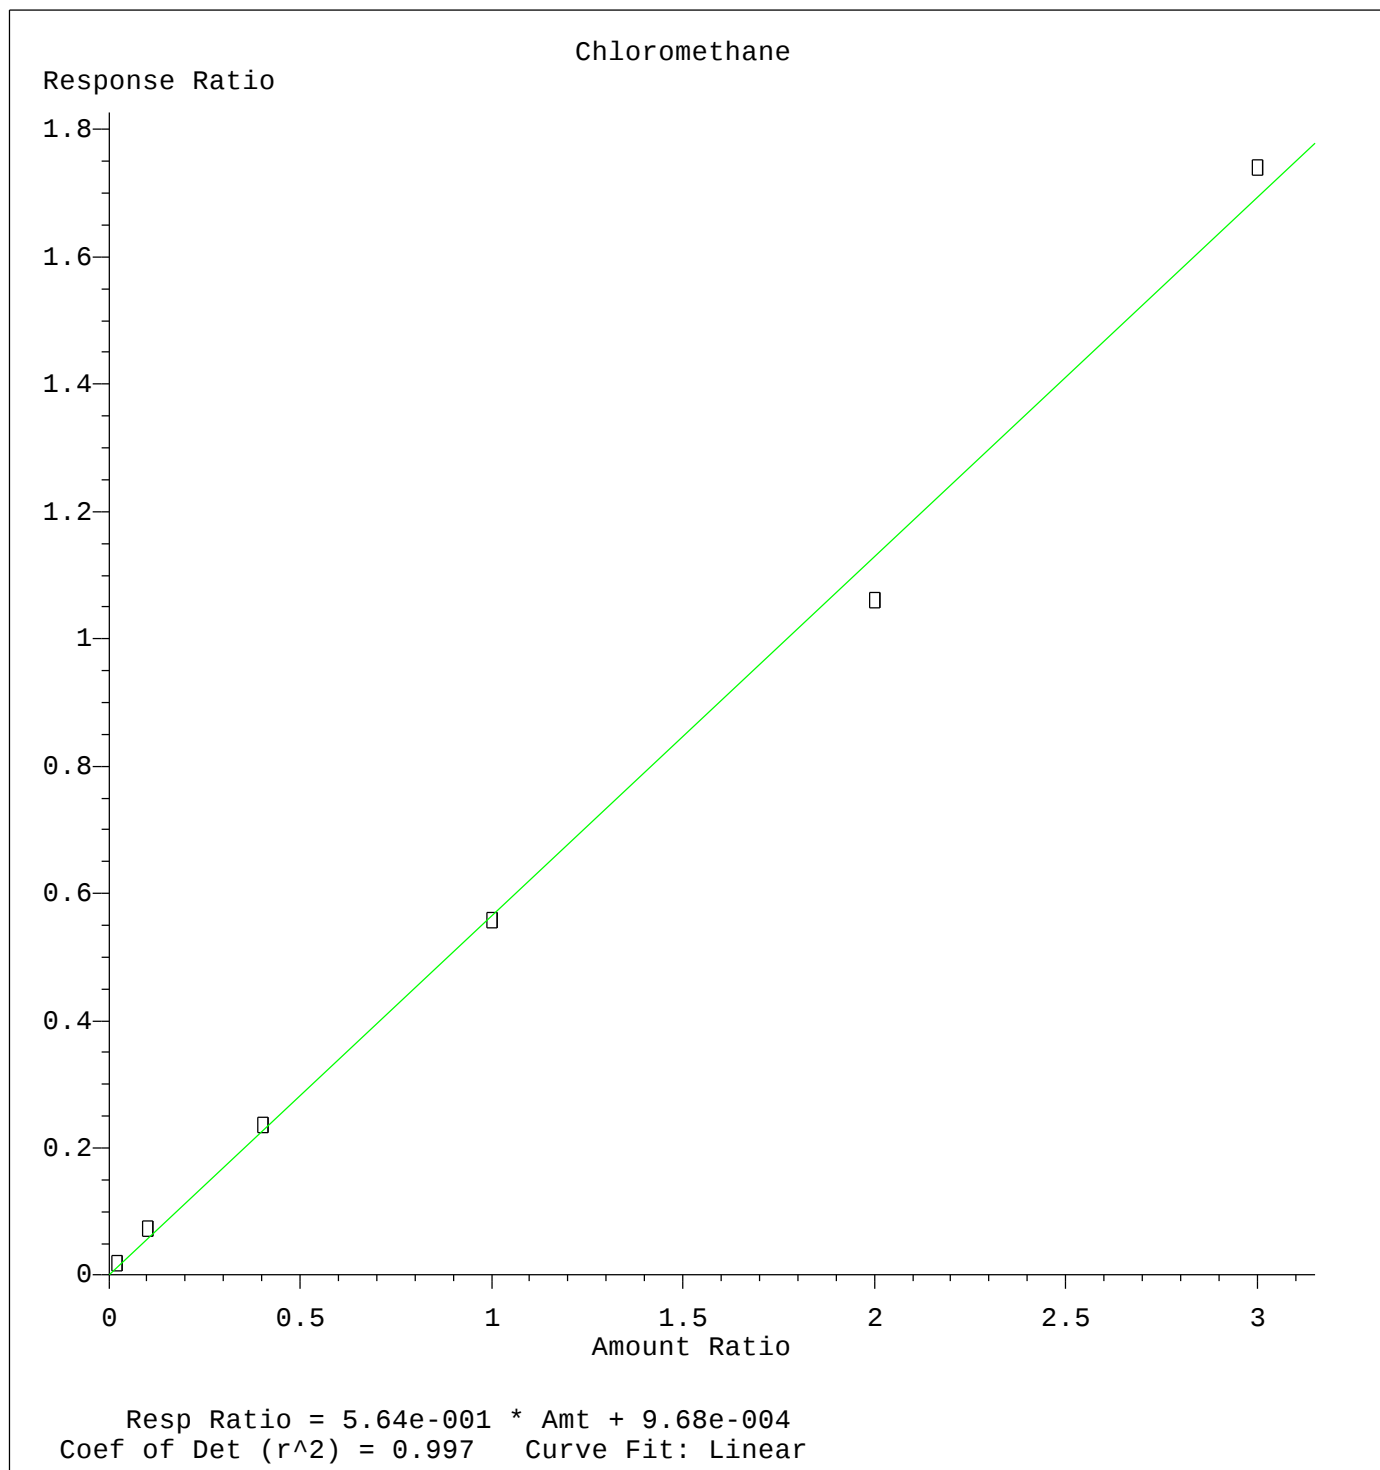


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

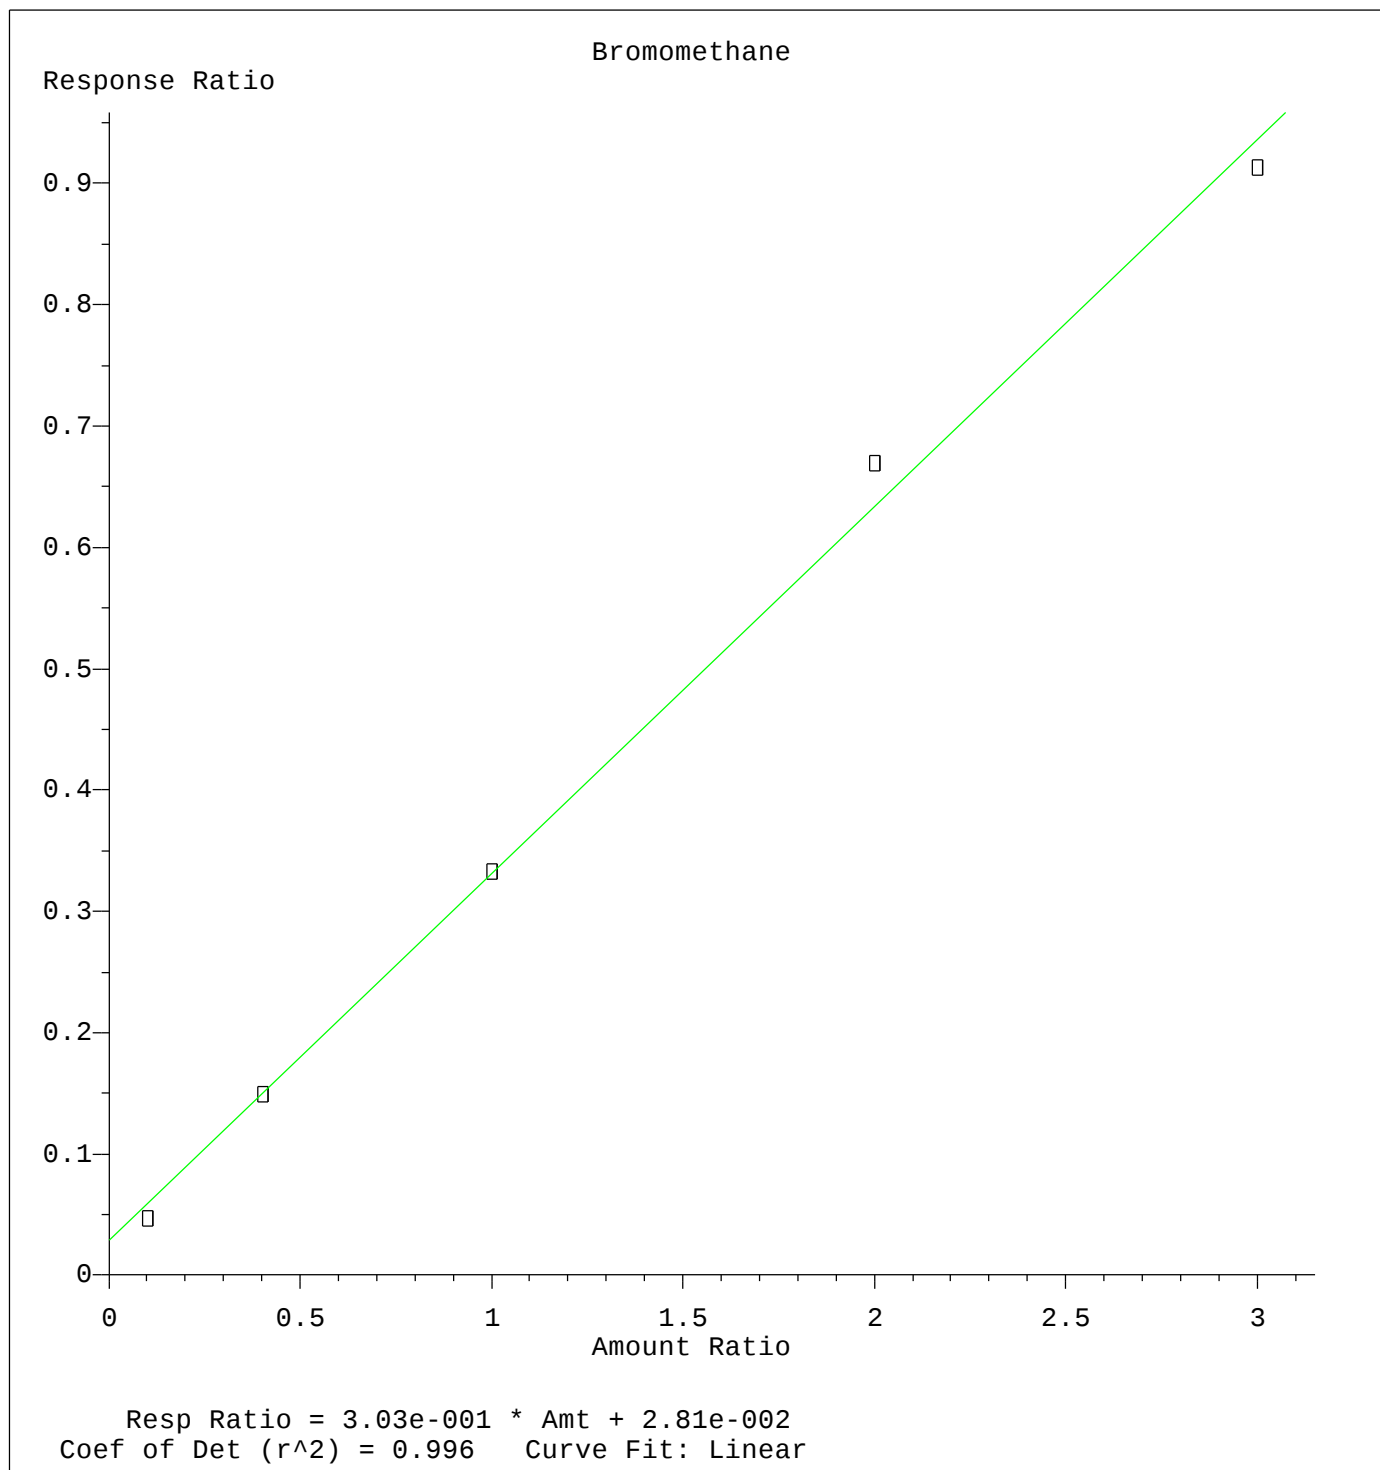

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

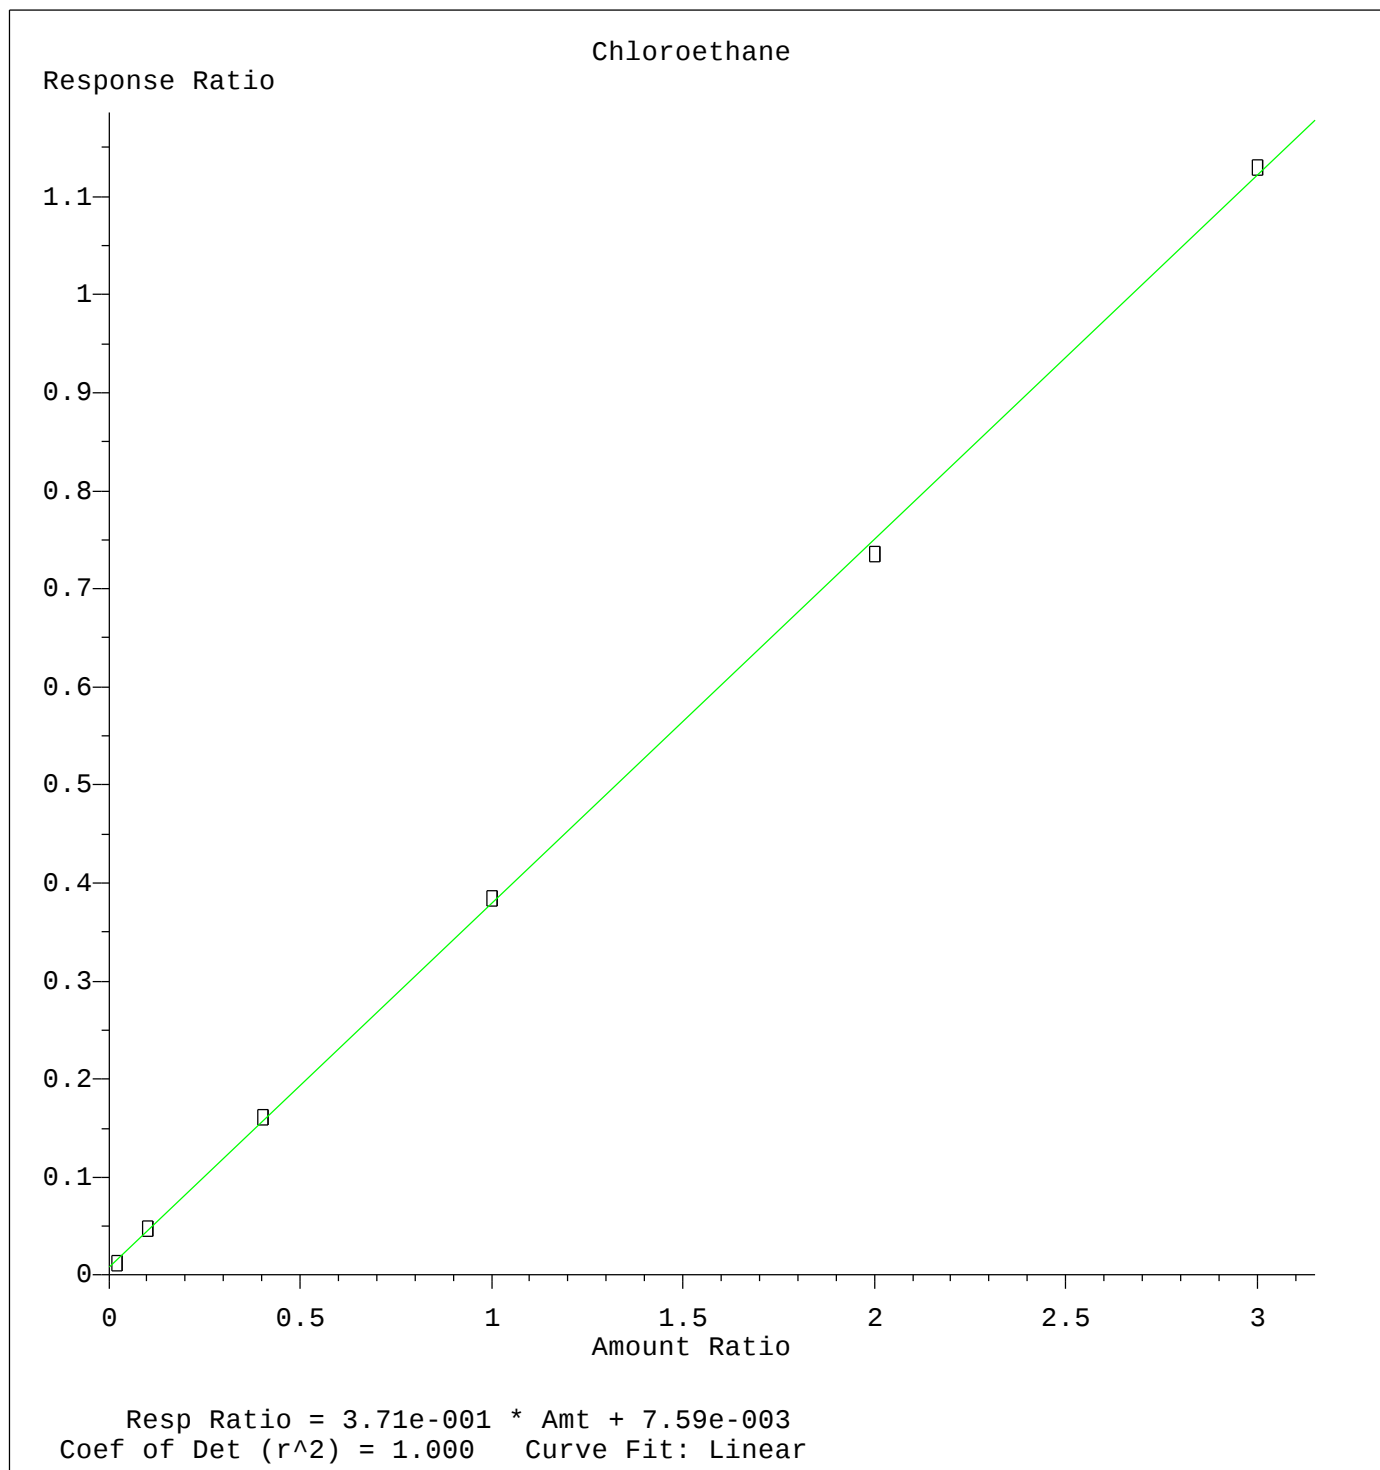


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

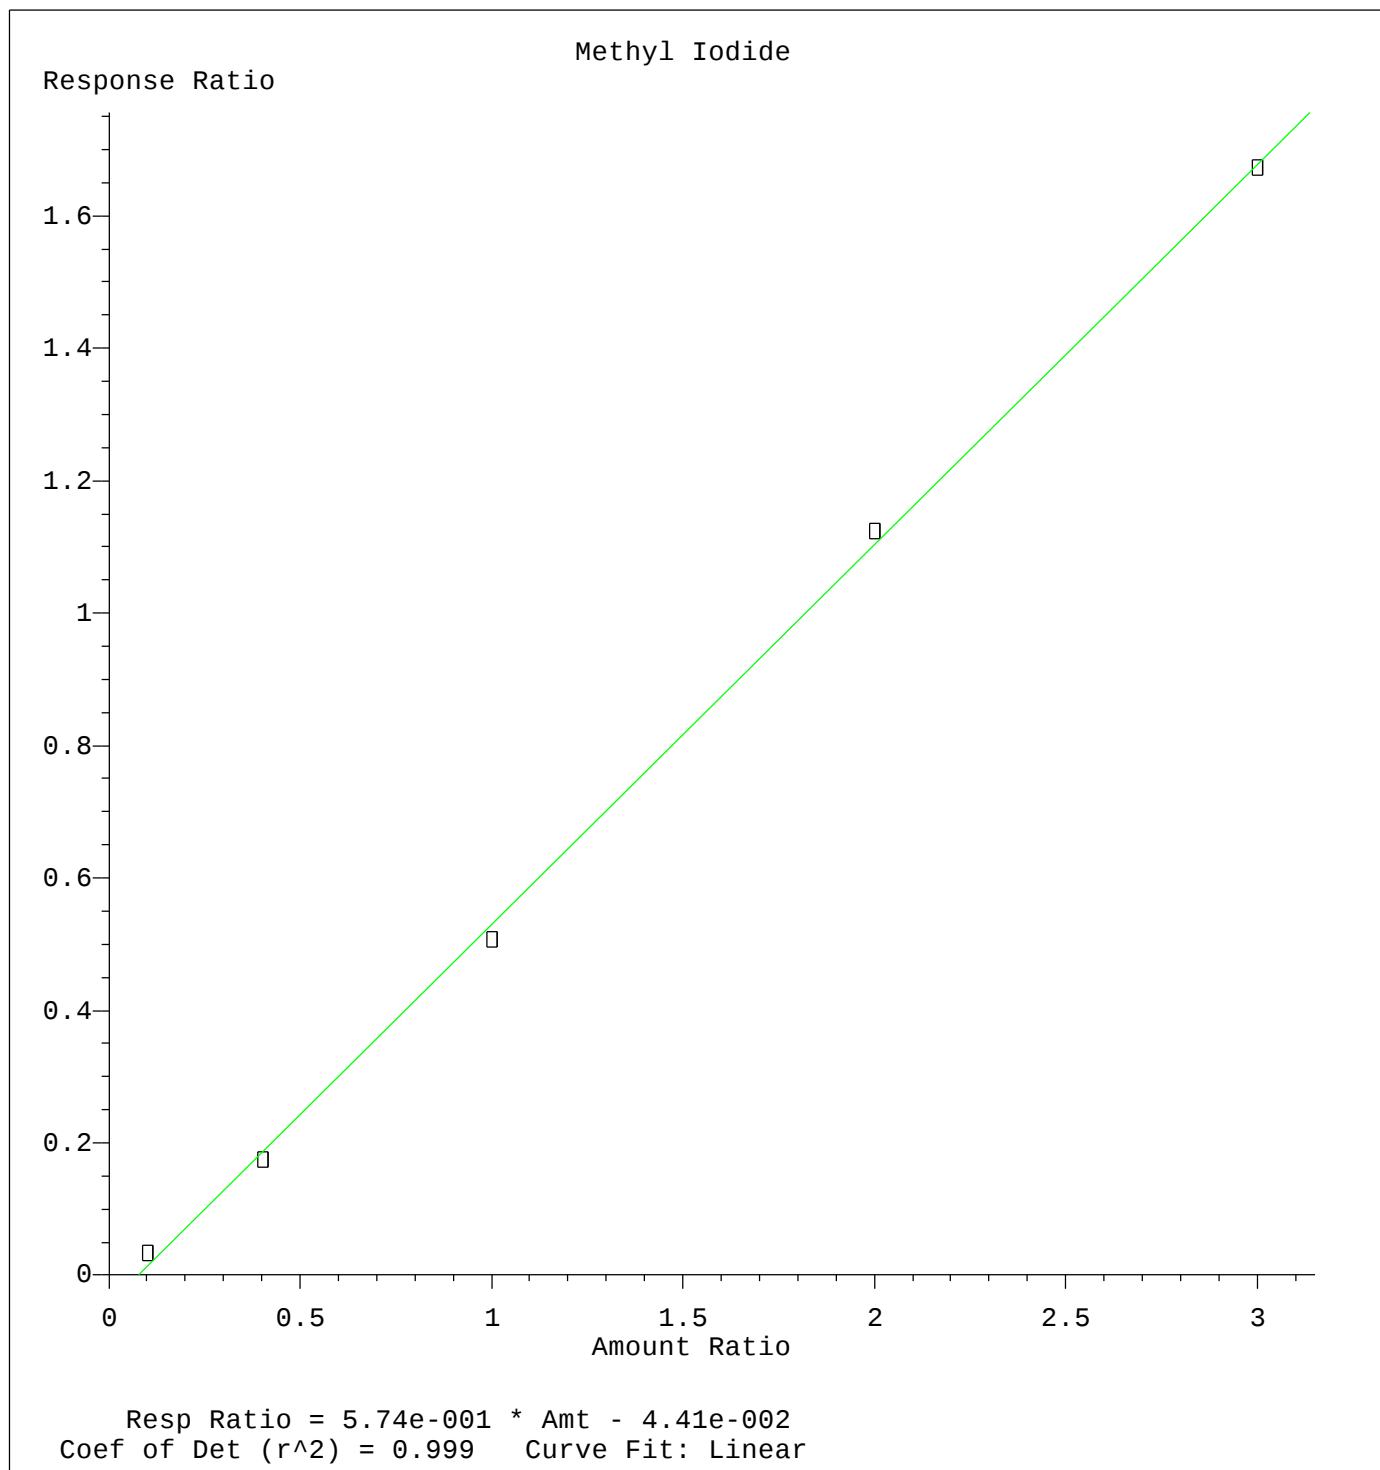

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019

Methylene Chloride

Response Ratio

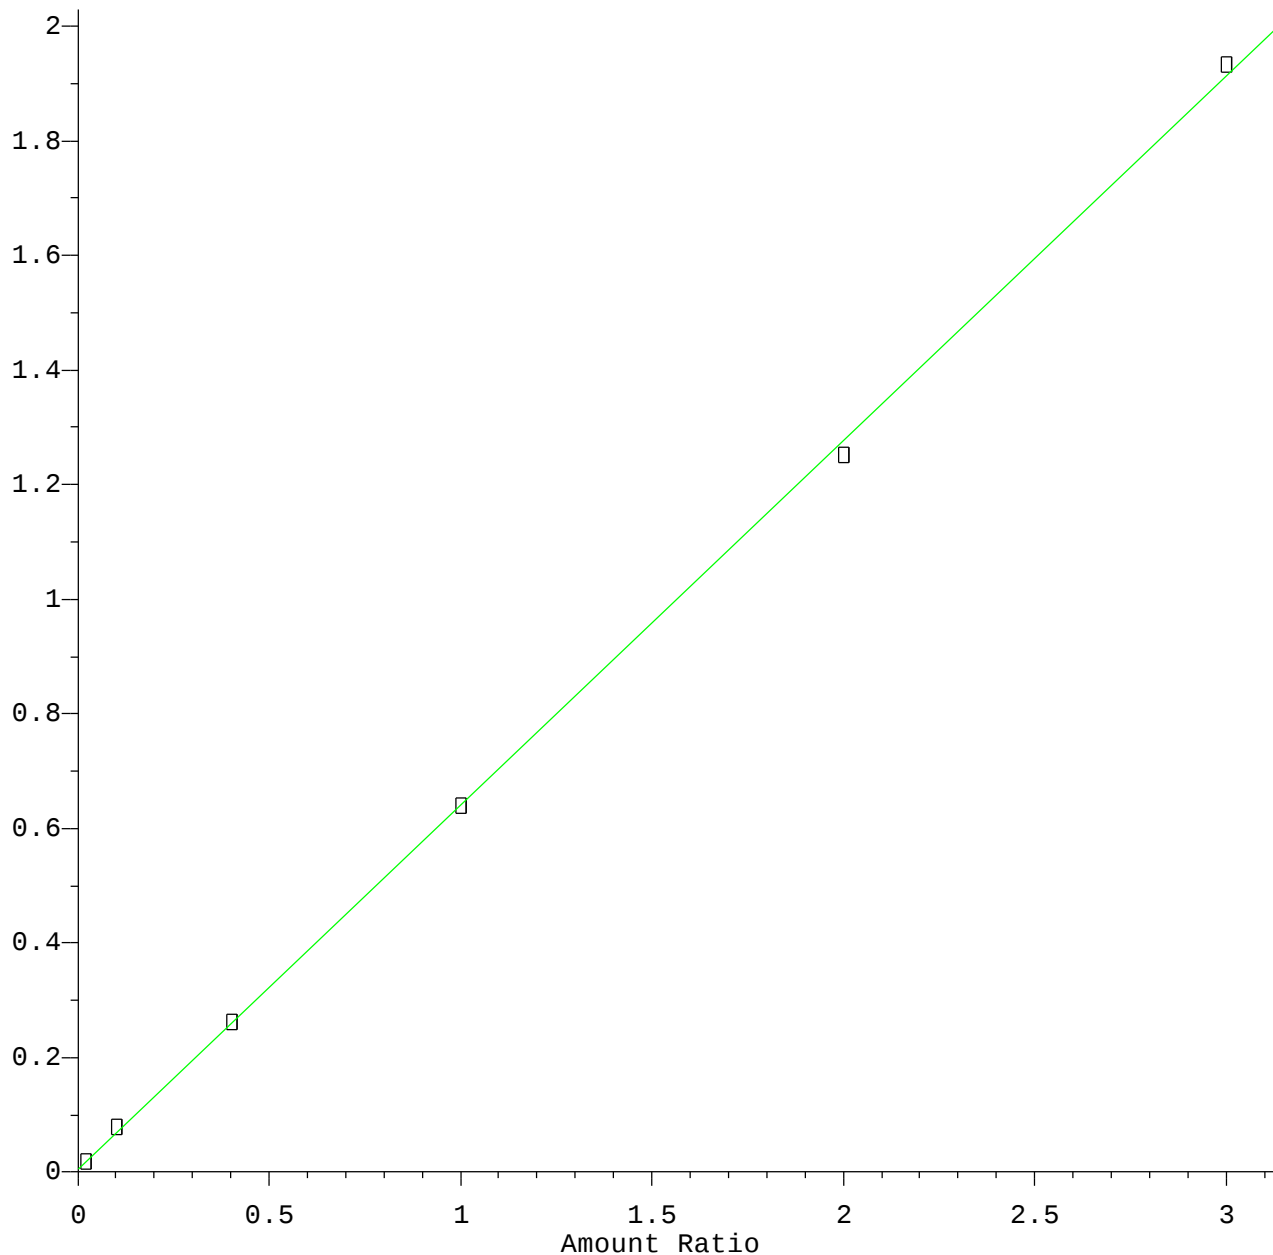

Resp Ratio = 6.36e-001 * Amt + 5.13e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Calibration Table Last Updated: Fri Sep 06 05:10:13 2019