


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090619\
 Data File : VU034270.D
 Acq On : 05 Sep 2019 08:23
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
 Title : SW846 8260
 Last Update : Fri Sep 06 05:10:13 2019

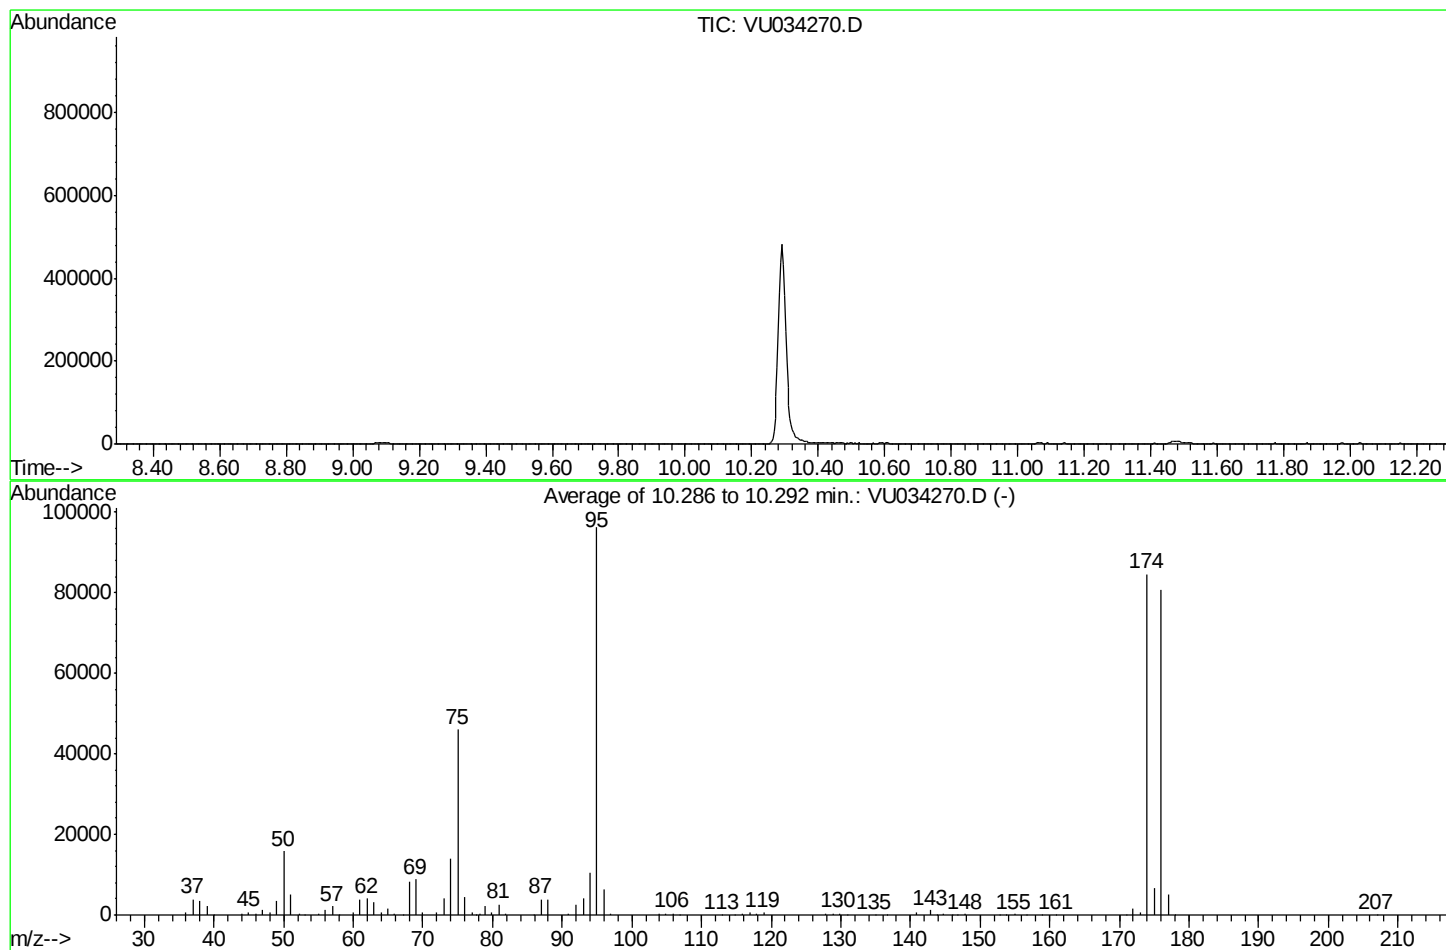

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	15778	PASS
75	95	30	60	47.7	45920	PASS
95	95	100	100	100.0	96221	PASS
96	95	5	9	6.6	6331	PASS
173	174	0.00	2	0.8	642	PASS
174	95	50	100	87.9	84602	PASS
175	174	5	9	7.8	6558	PASS
176	174	95	101	95.3	80592	PASS
177	176	5	9	6.3	5044	PASS