


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090619\
Data File : VU034284.D
Acq On : 05 Sep 2019 15:22
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U090619W.M
Title : SW846 8260
Last Update : Fri Sep 06 05:10:13 2019

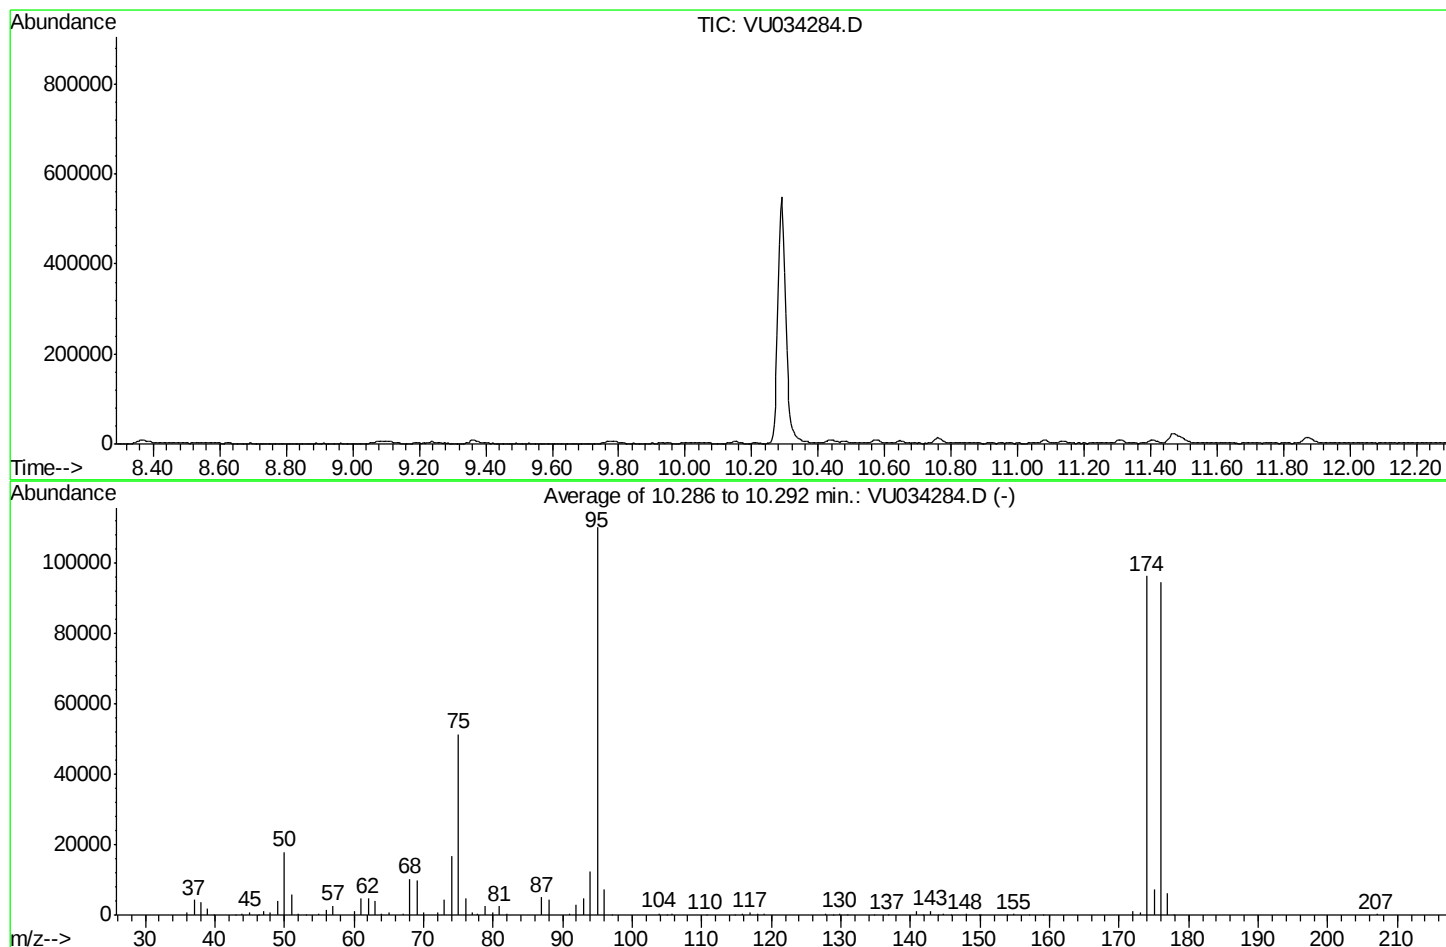

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	18010	PASS
75	95	30	60	46.6	51341	PASS
95	95	100	100	100.0	110154	PASS
96	95	5	9	6.5	7185	PASS
173	174	0.00	2	0.7	721	PASS
174	95	50	100	87.4	96224	PASS
175	174	5	9	7.6	7317	PASS
176	174	95	101	98.2	94509	PASS
177	176	5	9	6.6	6260	PASS