

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050636.D
 Acq On : 06 Sep 2022 16:09
 Operator : SY/MD
 Sample : N4482-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW347

Quant Time: Sep 07 01:39:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 07 01:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	194184	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	195228	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	75290	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	50182	30.214	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	60.420%
7) Chloroethane-d5	1.903	69	46130	41.072	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.140%
11) 1,1-Dichloroethene-d2	2.562	63	82413	28.079	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.160%#
21) 2-Butanone-d5	4.623	46	124257	102.257	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.260%
24) Chloroform-d	5.063	84	161431	51.283	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.560%
26) 1,2-Dichloroethane-d4	5.700	65	108149	56.223	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	112.440%
32) Benzene-d6	5.726	84	300210	46.532	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.060%
36) 1,2-Dichloropropane-d6	6.690	67	103947	49.073	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.140%
41) Toluene-d8	7.896	98	244175	44.257	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.520%
43) trans-1,3-Dichloroprop...	8.179	79	44388	50.647	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.300%
47) 2-Hexanone-d5	8.632	63	51934	97.472	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.470%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	163373	50.967	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.940%
66) 1,2-Dichlorobenzene-d4	12.192	152	95126	53.973	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.940%
Target Compounds						Qvalue
13) Acetone	2.629	43	8385	9.148	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050636.D
Acq On : 06 Sep 2022 16:09
Operator : SY/MD
Sample : N4482-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW347

Quant Time: Sep 07 01:39:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 07 01:37:50 2022
Response via : Initial Calibration

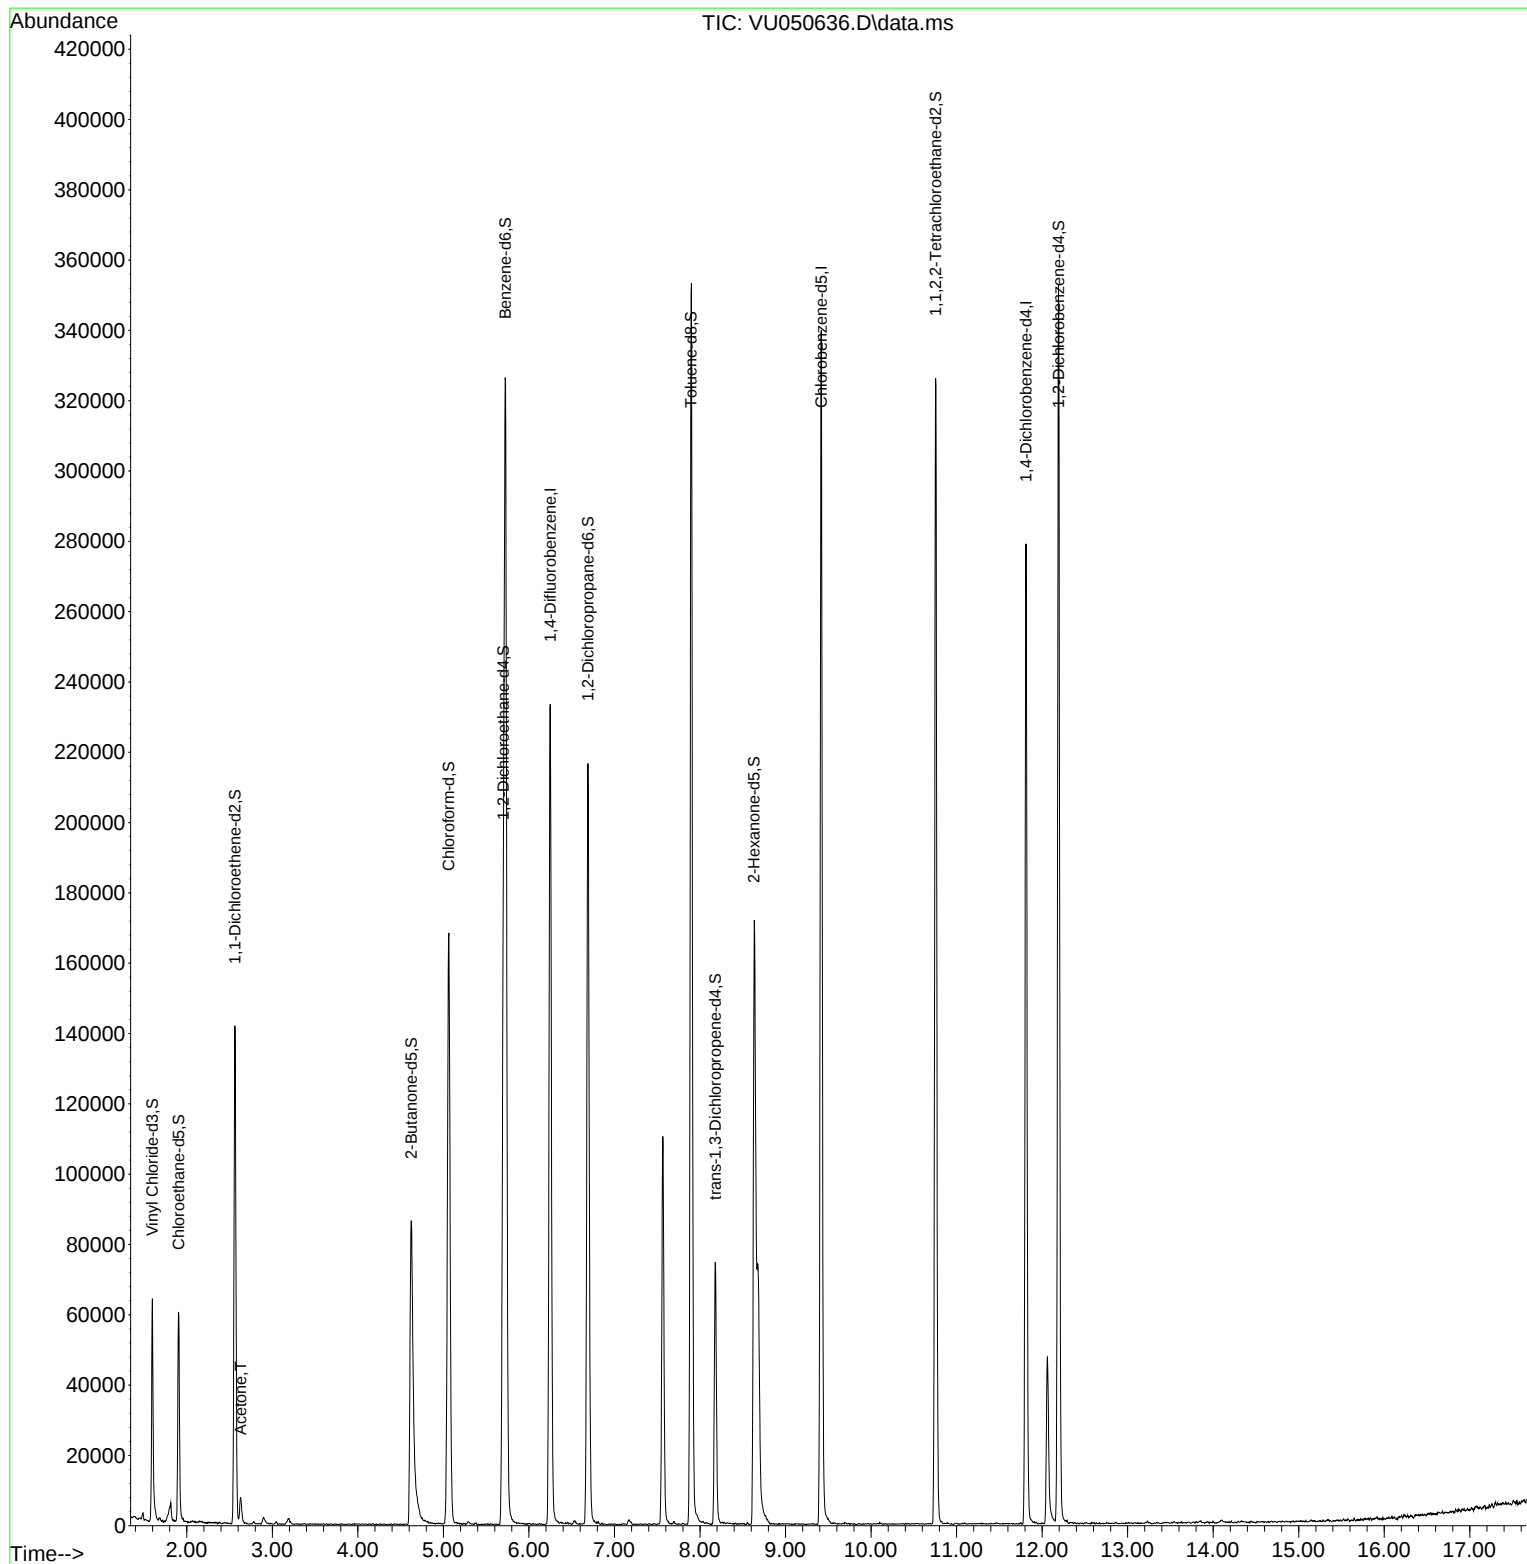

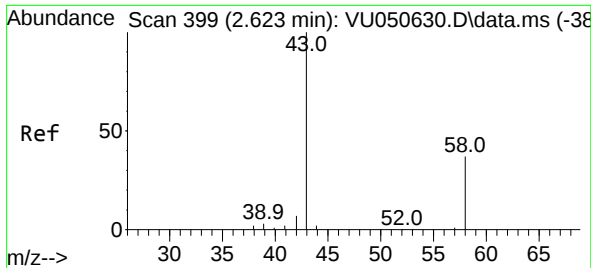

#13
 Acetone
 Concen: 9.148 ug/L
 RT: 2.629 min Scan# 401
 Delta R.T. 0.006 min
 Lab File: VU050636.D
 Acq: 06 Sep 2022 16:09

Instrument :
 MSVOA_U
 ClientSampleId :
 EW347

Tgt Ion: 43 Resp: 8385
 Ion Ratio Lower Upper
 43 100
 58 35.9 0.0 76.2

