

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050639.D
 Acq On : 06 Sep 2022 17:20
 Operator : SY/MD
 Sample : N4482-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW350

Quant Time: Sep 07 01:40:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 07 01:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	202643	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	202644	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	75779	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	49292	28.439	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	56.880%#	
7) Chloroethane-d5	1.900	69	44169	37.684	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	75.360%	
11) 1,1-Dichloroethene-d2	2.562	63	81375	26.568	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	53.140%#	
21) 2-Butanone-d5	4.620	46	123450	97.352	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	97.350%	
24) Chloroform-d	5.060	84	163249	49.696	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.400%	
26) 1,2-Dichloroethane-d4	5.700	65	109942	54.769	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	109.540%	
32) Benzene-d6	5.726	84	303482	45.318	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.640%	
36) 1,2-Dichloropropane-d6	6.690	67	107218	48.765	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	97.520%	
41) Toluene-d8	7.899	98	247707	43.254	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.500%	
43) trans-1,3-Dichloroprop...	8.179	79	45512	50.029	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	100.060%	
47) 2-Hexanone-d5	8.632	63	49439	89.394	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	89.390%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	171391	51.512	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	103.020%	
66) 1,2-Dichlorobenzene-d4	12.192	152	91260	51.445	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	102.880%	
Target Compounds						
13) Acetone	2.626	43	9670	10.109	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050639.D
Acq On : 06 Sep 2022 17:20
Operator : SY/MD
Sample : N4482-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW350

Quant Time: Sep 07 01:40:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 07 01:37:50 2022
Response via : Initial Calibration

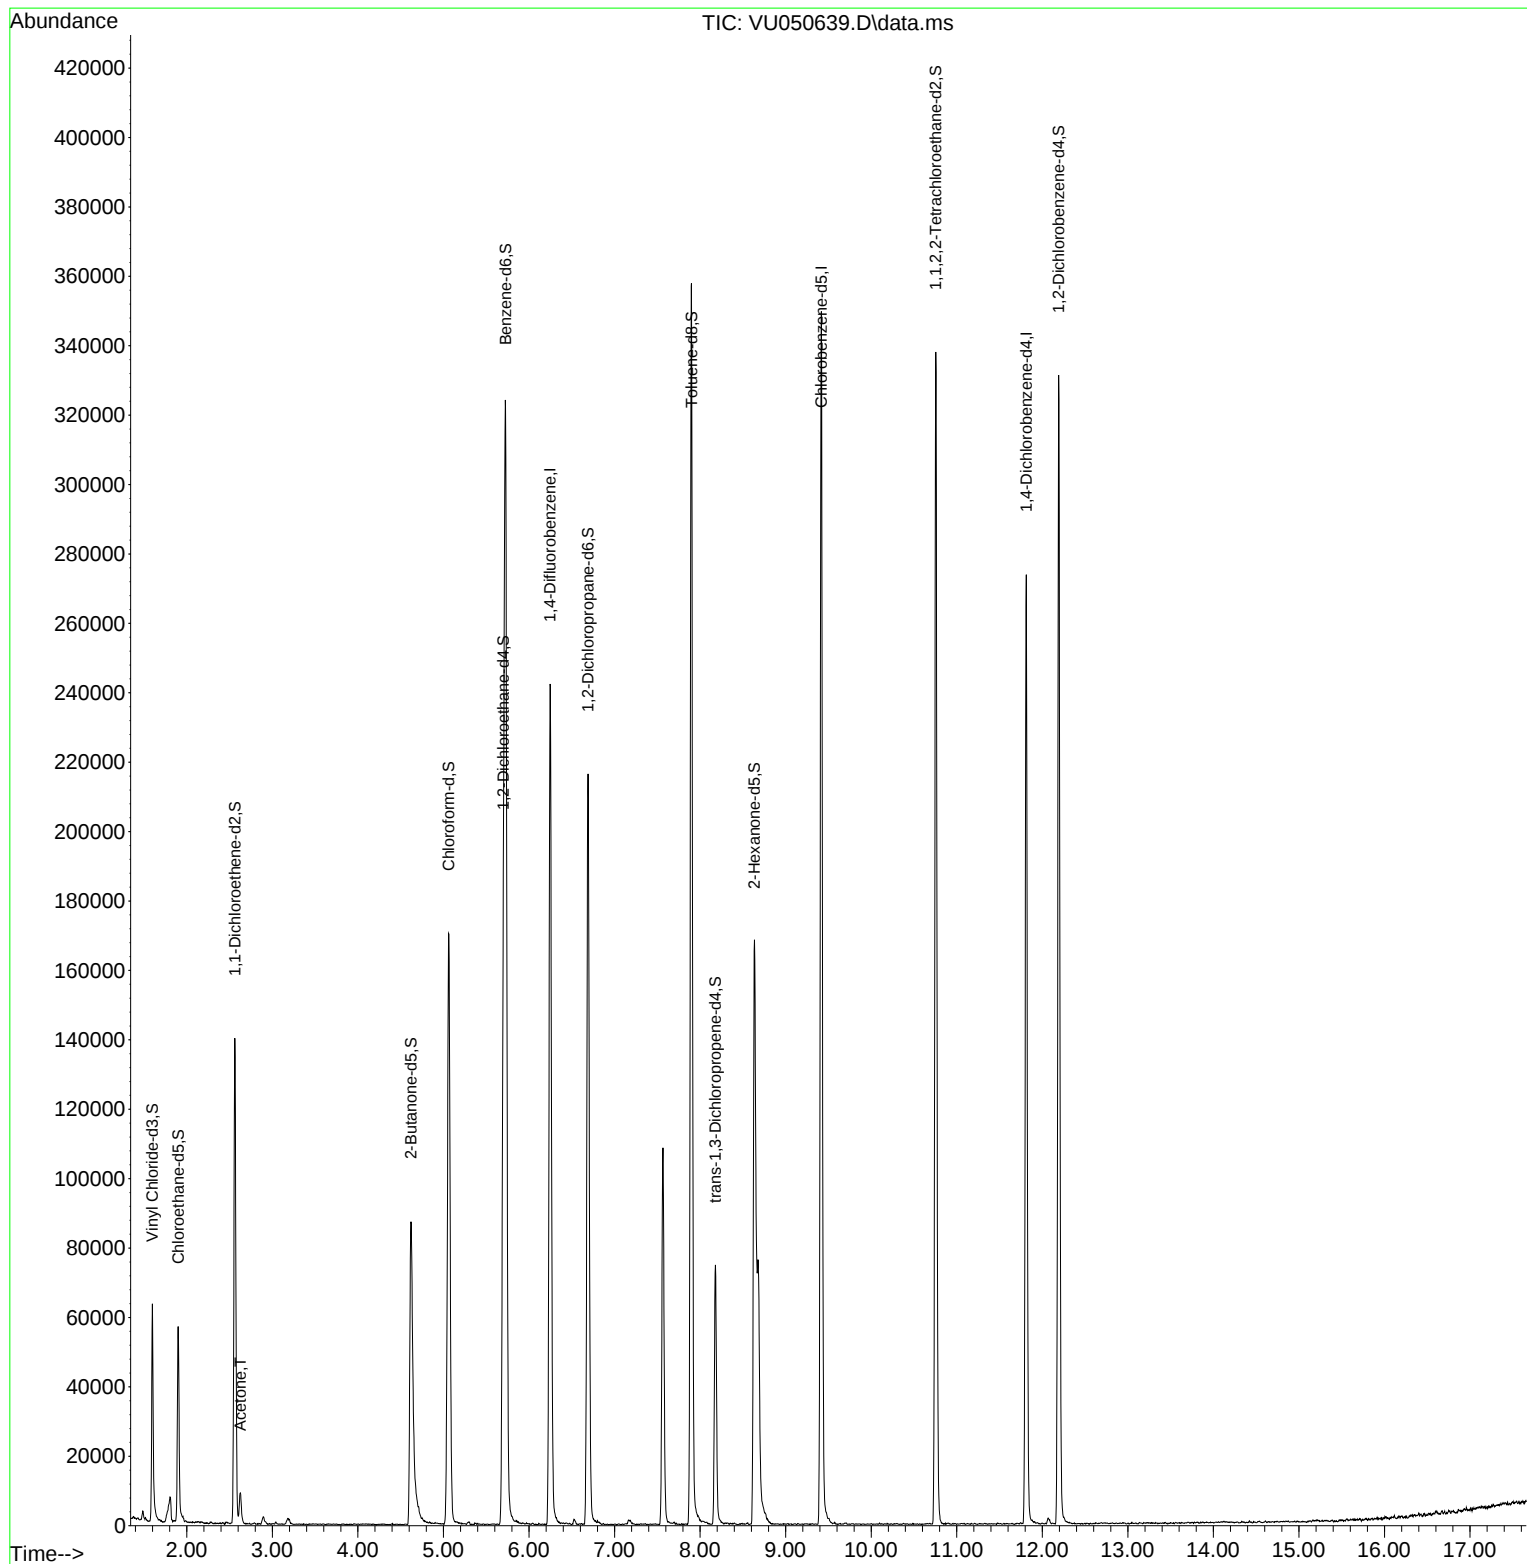

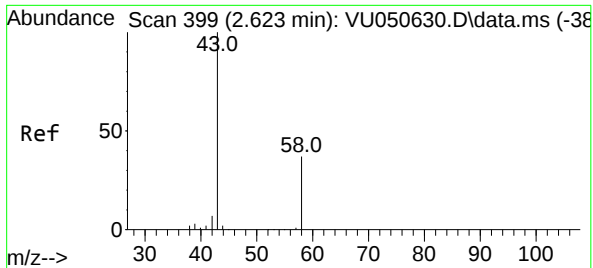

#13
 Acetone
 Concen: 10.109 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU050639.D
 Acq: 06 Sep 2022 17:20

Instrument :
 MSVOA_U
 ClientSampleId :
 EW350

Tgt Ion: 43 Resp: 9670
 Ion Ratio Lower Upper
 43 100
 58 35.2 0.0 76.2

