

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050646.D
 Acq On : 06 Sep 2022 20:06
 Operator : SY/MD
 Sample : N4483-10ME
 Misc : 2.57g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW358ME

Quant Time: Sep 07 01:42:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 07 01:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	213223	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	210586	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	82887	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43565	23.888	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	47.780%#
7) Chloroethane-d5	1.903	69	40880	33.148	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	66.300%#
11) 1,1-Dichloroethene-d2	2.565	63	74998	23.271	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	46.540%#
21) 2-Butanone-d5	4.623	46	116868	87.588	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.590%
24) Chloroform-d	5.063	84	150834	43.638	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.280%
26) 1,2-Dichloroethane-d4	5.700	65	103972	49.225	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.460%
32) Benzene-d6	5.726	84	281711	40.480	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.960%
36) 1,2-Dichloropropane-d6	6.690	67	98220	42.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.980%
41) Toluene-d8	7.899	98	227686	38.259	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.520%#
43) trans-1,3-Dichloroprop...	8.179	79	41358	43.748	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.500%
47) 2-Hexanone-d5	8.632	63	45195	78.638	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.640%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	159960	46.263	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.520%
66) 1,2-Dichlorobenzene-d4	12.192	152	88652	45.689	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.380%
Target Compounds						
13) Acetone	2.629	43	7807	7.756	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050646.D
Acq On : 06 Sep 2022 20:06
Operator : SY/MD
Sample : N4483-10ME
Misc : 2.57g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW358ME

Quant Time: Sep 07 01:42:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 07 01:37:50 2022
Response via : Initial Calibration

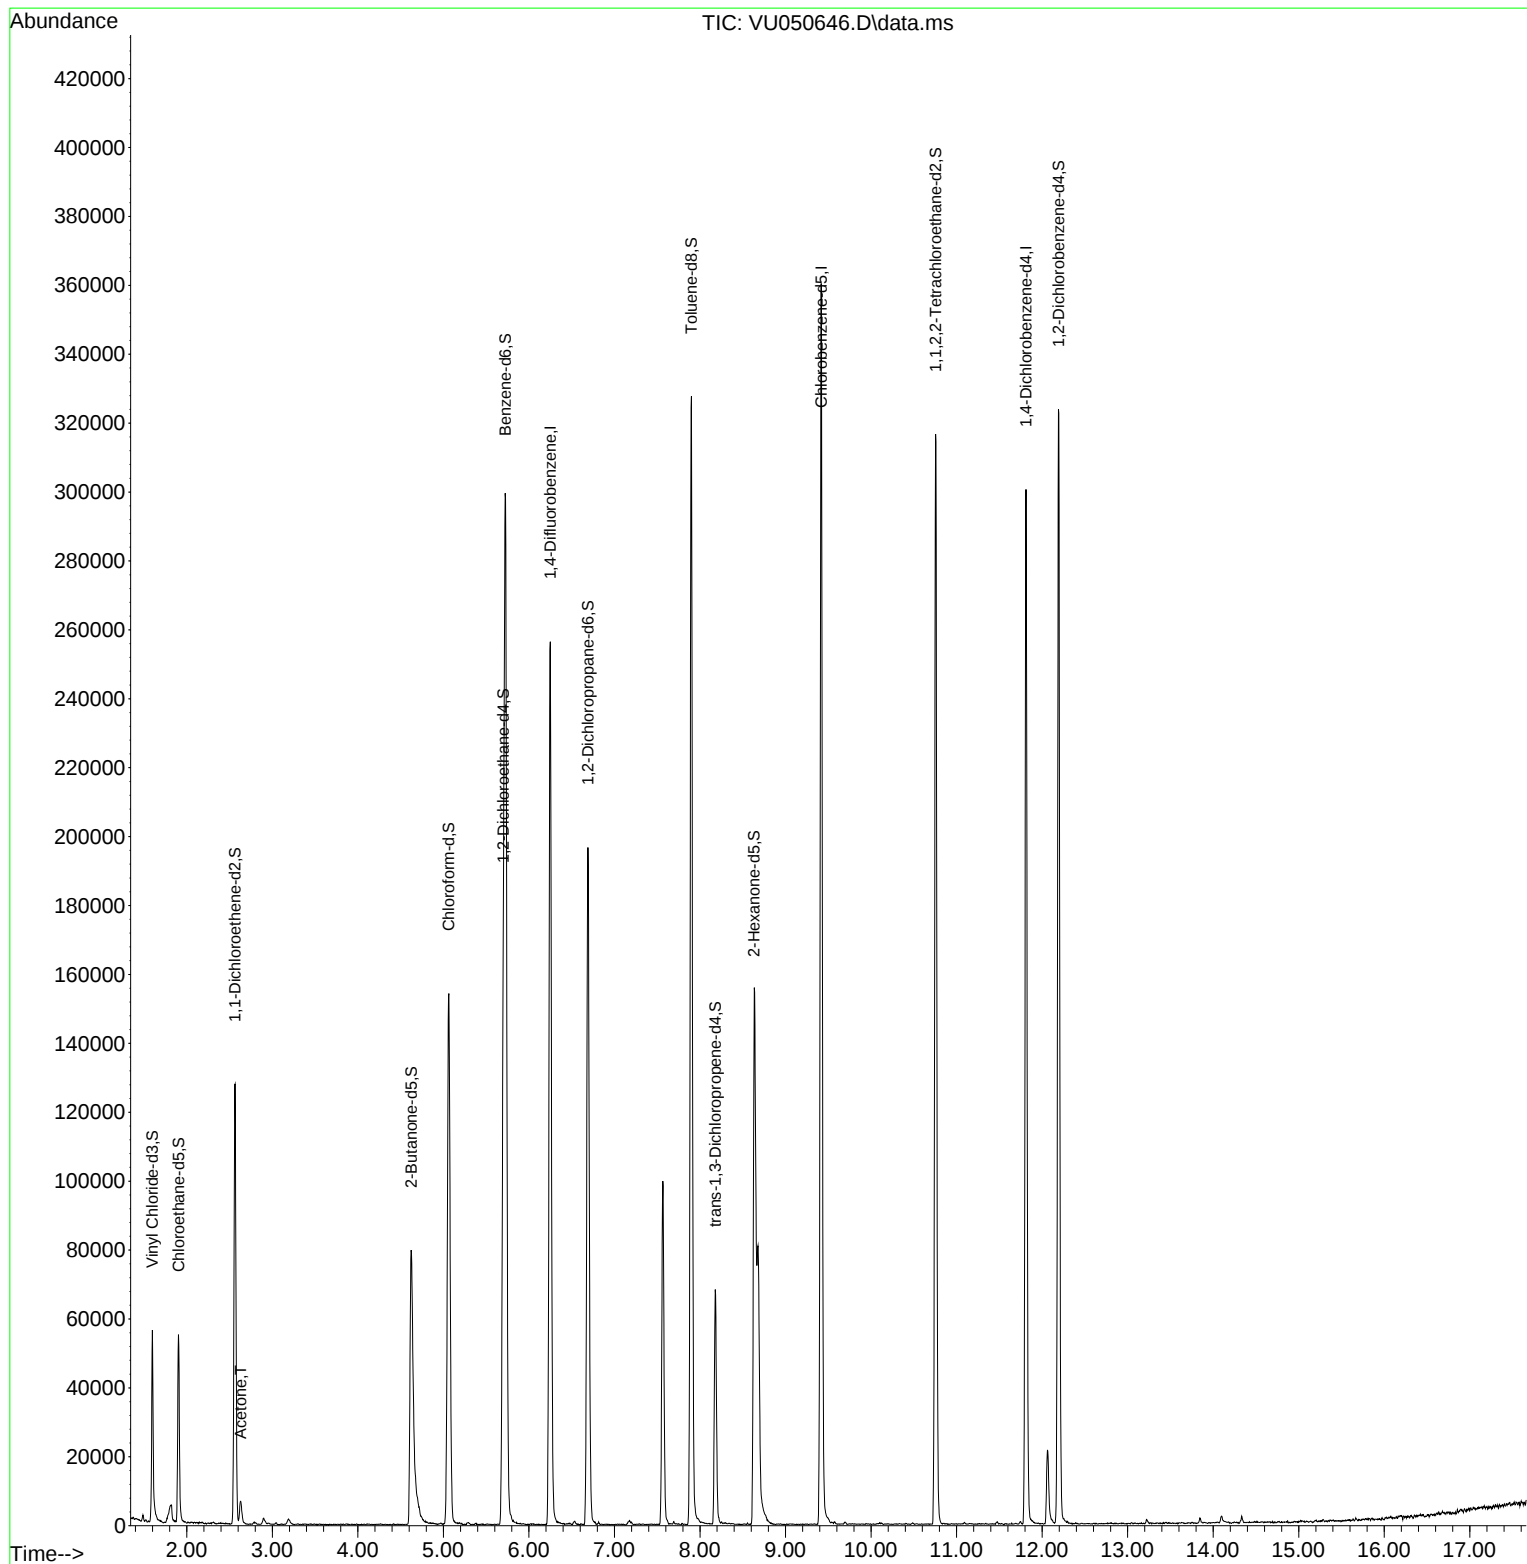

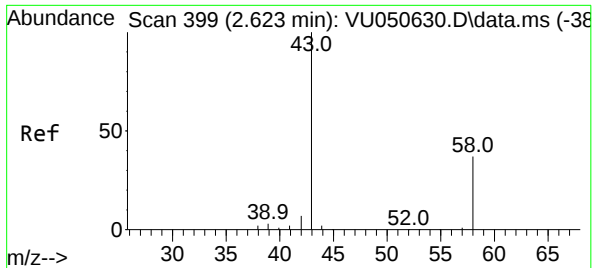

#13
 Acetone
 Concen: 7.756 ug/L
 RT: 2.629 min Scan# 401
 Delta R.T. 0.006 min
 Lab File: VU050646.D
 Acq: 06 Sep 2022 20:06

Instrument :
 MSVOA_U
 ClientSampleId :
 EW358ME

Tgt Ion: 43 Resp: 7807
 Ion Ratio Lower Upper
 43 100
 58 39.7 0.0 76.2

