

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050647.D
 Acq On : 06 Sep 2022 20:29
 Operator : SY/MD
 Sample : N4482-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW366

Quant Time: Sep 07 01:42:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 07 01:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	166785	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	168568	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	63278	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	32899	23.062	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	46.120%#	
7) Chloroethane-d5	1.900	69	31724	32.886	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	65.780%#	
11) 1,1-Dichloroethene-d2	2.562	63	55819	22.143	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	44.280%#	
21) 2-Butanone-d5	4.623	46	110677	106.044	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	106.040%	
24) Chloroform-d	5.063	84	124024	45.872	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.740%	
26) 1,2-Dichloroethane-d4	5.700	65	87482	52.950	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.900%	
32) Benzene-d6	5.726	84	223768	40.169	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	80.340%	
36) 1,2-Dichloropropane-d6	6.690	67	80763	44.158	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	88.320%	
41) Toluene-d8	7.899	98	176147	36.976	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	73.960%#	
43) trans-1,3-Dichloroprop...	8.179	79	33820	44.691	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.380%	
47) 2-Hexanone-d5	8.636	63	39982	86.908	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	86.910%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	137992	49.858	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	99.720%	
66) 1,2-Dichlorobenzene-d4	12.192	152	69486	46.909	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.820%	
Target Compounds						
13) Acetone	2.630	43	2119	2.691	ug/L	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050647.D
Acq On : 06 Sep 2022 20:29
Operator : SY/MD
Sample : N4482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW366

Quant Time: Sep 07 01:42:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 07 01:37:50 2022
Response via : Initial Calibration

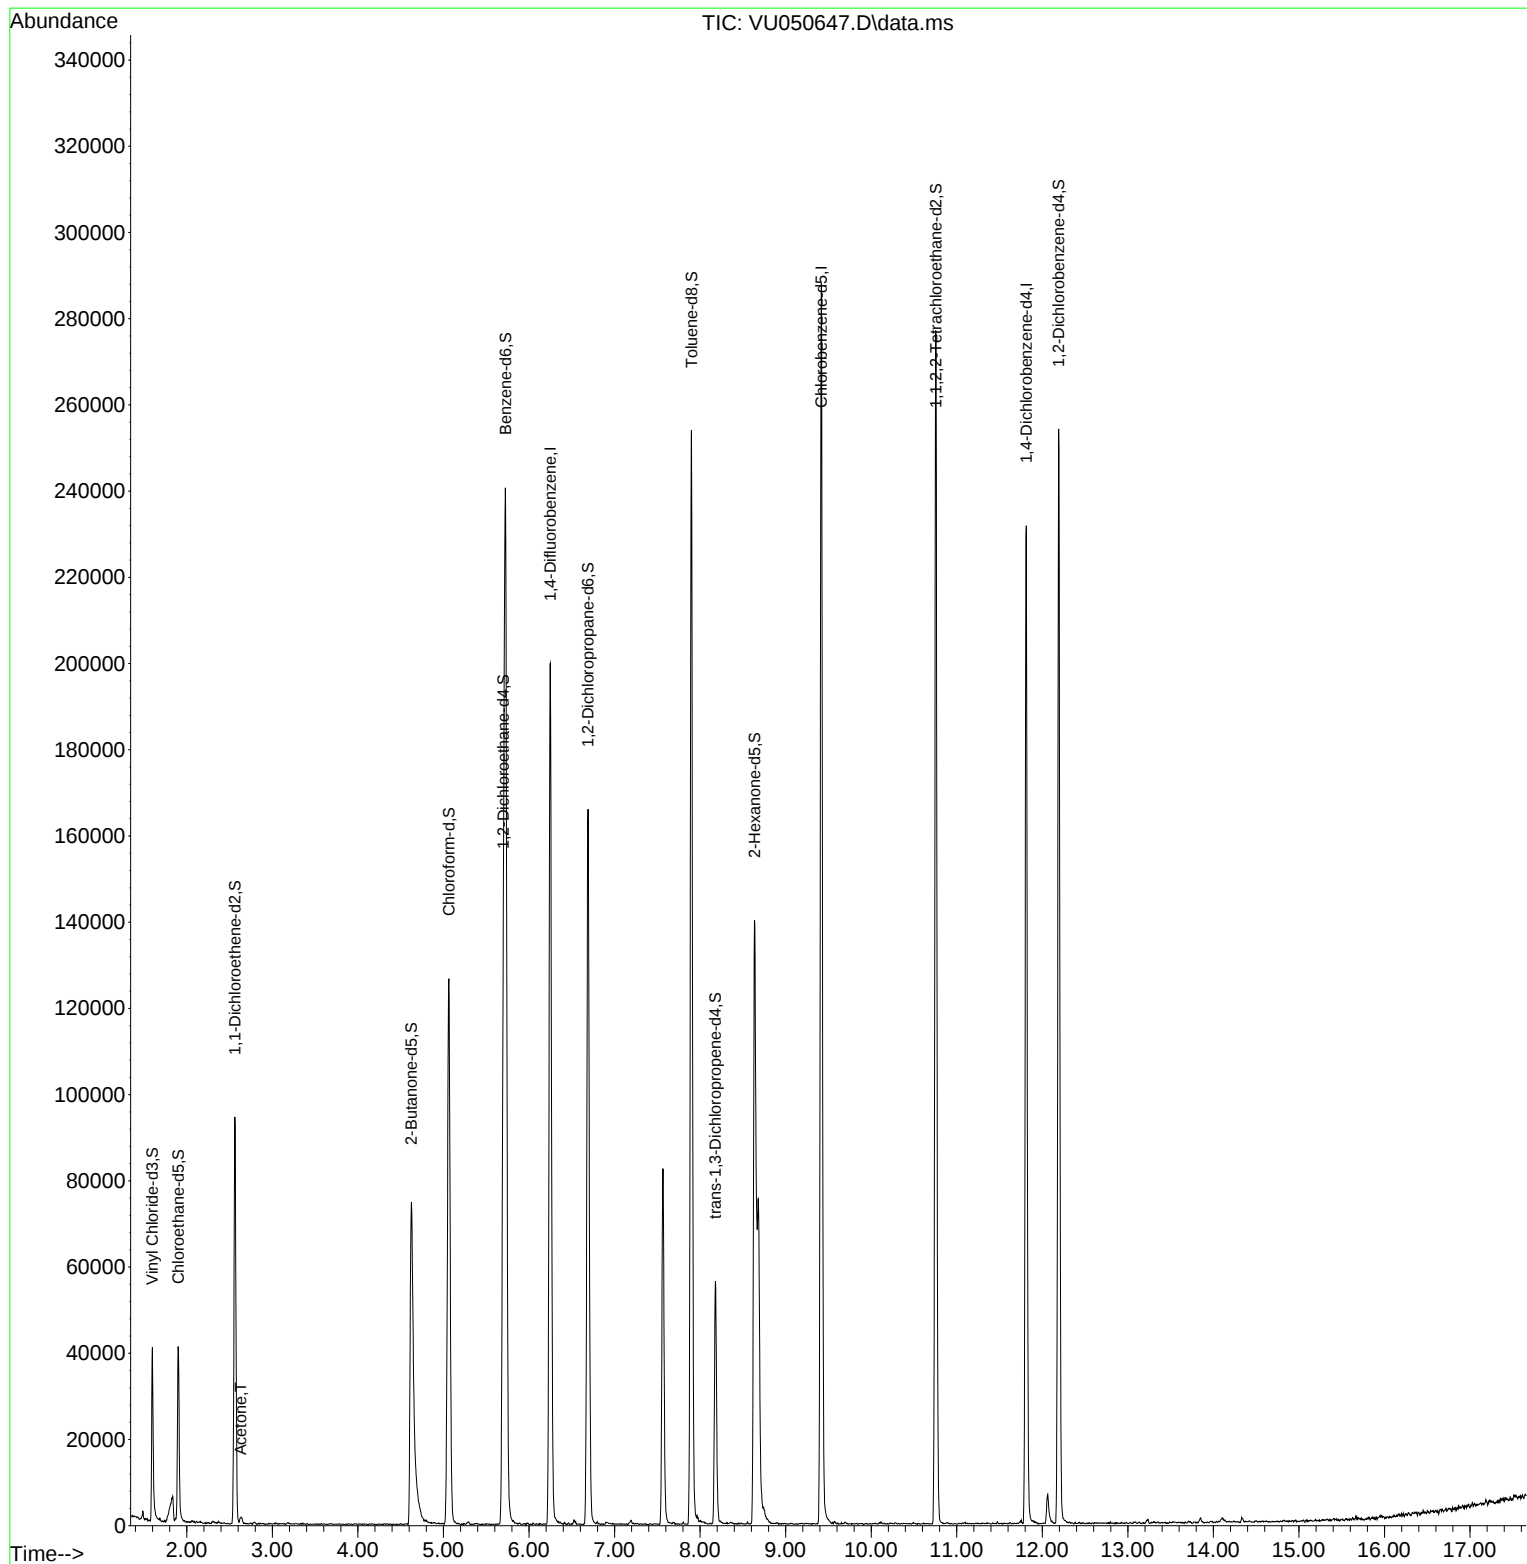

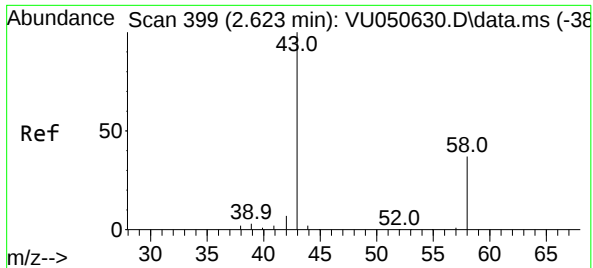

#13
 Acetone
 Concen: 2.691 ug/L
 RT: 2.630 min Scan# 401
 Delta R.T. 0.007 min
 Lab File: VU050647.D
 Acq: 06 Sep 2022 20:29

Instrument :
 MSVOA_U
 ClientSampleId :
 EW366

Tgt Ion: 43 Resp: 2119
 Ion Ratio Lower Upper
 43 100
 58 19.6 0.0 76.2

