

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050632.D
 Acq On : 06 Sep 2022 14:27
 Operator : SY/MD
 Sample : VU0906WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK183

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050632.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rBV	214855	265843	13.66%	1.945%
2	1.906	168	176	200	rVB	193431	263134	13.52%	1.925%
3	2.565	368	381	398	rBV	376298	607460	31.22%	4.444%
4	2.697	420	422	426	rVB2	525	220	0.01%	0.002%
5	2.903	483	486	489	rVV2	389	260	0.01%	0.002%
6	2.954	498	502	507	rVB3	347	406	0.02%	0.003%
7	3.047	519	531	540	rVV6	2963	5594	0.29%	0.041%
8	3.186	562	574	583	rBV5	1157	2366	0.12%	0.017%
9	3.263	594	598	604	rBV2	222	225	0.01%	0.002%
10	3.308	609	612	616	rBV2	338	283	0.01%	0.002%
11	3.398	636	640	644	rVV	699	638	0.03%	0.005%
12	3.957	809	814	817	rBV2	415	353	0.02%	0.003%
13	4.022	832	834	840	rVB2	232	219	0.01%	0.002%
14	4.050	840	843	847	rBV	273	256	0.01%	0.002%
15	4.095	854	857	864	rVB2	293	329	0.02%	0.002%
16	4.189	882	886	888	rBV	308	240	0.01%	0.002%
17	4.478	973	976	984	rVB2	256	254	0.01%	0.002%
18	4.520	984	989	990	rBV	298	266	0.01%	0.002%
19	4.623	1008	1021	1074	rBV	187359	521201	26.78%	3.813%
20	4.822	1080	1083	1086	rBV2	710	485	0.02%	0.004%
21	4.964	1125	1127	1131	rBV3	353	242	0.01%	0.002%
22	5.063	1141	1158	1183	rBV	357974	786834	40.43%	5.757%
23	5.295	1221	1230	1235	rBV5	1377	2087	0.11%	0.015%
24	5.378	1248	1256	1261	rVV3	1107	1489	0.08%	0.011%
25	5.475	1282	1286	1288	rVB2	378	271	0.01%	0.002%
26	5.517	1295	1299	1302	rVB2	302	241	0.01%	0.002%
27	5.568	1313	1315	1325	rVB	258	262	0.01%	0.002%
28	5.726	1338	1364	1387	rBV2	717894	1945947	100.00%	14.237%
29	5.976	1438	1442	1445	rBV3	731	634	0.03%	0.005%
30	6.156	1494	1498	1500	rBV2	339	278	0.01%	0.002%
31	6.192	1506	1509	1512	rBV3	331	250	0.01%	0.002%
32	6.250	1512	1527	1548	rBV	511013	974472	50.08%	7.130%
33	6.497	1601	1604	1606	rBV2	324	256	0.01%	0.002%
34	6.533	1606	1615	1626	rVB8	3183	6235	0.32%	0.046%
35	6.607	1637	1638	1644	rBV3	309	327	0.02%	0.002%
36	6.690	1649	1664	1690	rBV	470102	909980	46.76%	6.658%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050632.D
 Acq On : 06 Sep 2022 14:27
 Operator : SY/MD
 Sample : VU0906WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK183

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.890	1723	1726	1730	rVB2	367	272	0.01%	0.002%
38	6.992	1754	1758	1764	rVV2	330	264	0.01%	0.002%
39	7.018	1764	1766	1772	rVB	260	237	0.01%	0.002%
40	7.182	1813	1817	1819	rBV4	888	711	0.04%	0.005%
41	7.433	1893	1895	1902	rVB3	330	269	0.01%	0.002%
42	7.481	1902	1910	1913	rBV	276	249	0.01%	0.002%
43	7.568	1924	1937	1959	rBV	225532	405982	20.86%	2.970%
44	7.790	2001	2006	2007	rBV2	837	682	0.04%	0.005%
45	7.899	2025	2040	2079	rBV	811952	1430301	73.50%	10.465%
46	8.179	2115	2127	2142	rBV	151285	261729	13.45%	1.915%
47	8.359	2180	2183	2189	rVB3	502	455	0.02%	0.003%
48	8.391	2189	2193	2195	rBV	481	354	0.02%	0.003%
49	8.635	2256	2269	2304	rBV7	351936	1029340	52.90%	7.531%
50	8.893	2347	2349	2359	rVB3	800	830	0.04%	0.006%
51	8.973	2369	2374	2377	rVB2	499	431	0.02%	0.003%
52	9.086	2404	2409	2413	rVB3	385	338	0.02%	0.002%
53	9.121	2417	2420	2423	rVV2	299	228	0.01%	0.002%
54	9.304	2474	2477	2480	rBV2	296	230	0.01%	0.002%
55	9.417	2498	2512	2545	rBV	707771	1198209	61.57%	8.767%
56	9.626	2575	2577	2580	rBV2	324	254	0.01%	0.002%
57	9.677	2589	2593	2595	rBV2	405	333	0.02%	0.002%
58	9.697	2595	2599	2603	rVV3	636	570	0.03%	0.004%
59	9.745	2611	2614	2619	rVB3	354	270	0.01%	0.002%
60	9.867	2648	2652	2655	rBV2	301	283	0.01%	0.002%
61	9.918	2664	2668	2675	rVB3	471	464	0.02%	0.003%
62	10.066	2708	2714	2717	rBV	368	472	0.02%	0.003%
63	10.487	2842	2845	2851	rVB3	709	797	0.04%	0.006%
64	10.539	2857	2861	2863	rBV	347	235	0.01%	0.002%
65	10.651	2893	2896	2900	rBV2	243	259	0.01%	0.002%
66	10.754	2916	2928	2954	rBV	656240	1071298	55.05%	7.838%
67	11.095	3026	3034	3040	rBV3	1034	1223	0.06%	0.009%
68	11.394	3119	3127	3129	rBV	522	587	0.03%	0.004%
69	11.413	3130	3133	3138	rVV2	622	506	0.03%	0.004%
70	11.475	3148	3152	3155	rBV4	666	547	0.03%	0.004%
71	11.558	3170	3178	3181	rBV	373	459	0.02%	0.003%
72	11.616	3188	3196	3199	rBV3	417	567	0.03%	0.004%
73	11.719	3224	3228	3230	rBV	376	323	0.02%	0.002%
74	11.754	3231	3239	3244	rVB5	1294	1666	0.09%	0.012%
75	11.812	3244	3257	3292	rBV	533540	878512	45.15%	6.428%
76	12.024	3321	3323	3326	rBV	427	268	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050632.D
 Acq On : 06 Sep 2022 14:27
 Operator : SY/MD
 Sample : VU0906WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK183

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	12.053	3330	3332	3335	rVB2	639	326	0.02%	0.002%
78	12.195	3362	3376	3395	rBV	646135	1051843	54.05%	7.696%
79	12.401	3437	3440	3442	rBV2	427	279	0.01%	0.002%
80	12.561	3484	3490	3493	rBV3	405	555	0.03%	0.004%
81	12.719	3535	3539	3546	rVB3	528	651	0.03%	0.005%
82	12.757	3548	3551	3553	rBV2	416	221	0.01%	0.002%
83	12.774	3553	3556	3558	rBV2	402	289	0.01%	0.002%
84	12.819	3566	3570	3577	rVB3	662	591	0.03%	0.004%
85	12.860	3577	3583	3588	rVB3	587	819	0.04%	0.006%
86	12.893	3588	3593	3597	rBV2	231	231	0.01%	0.002%
87	12.918	3597	3601	3603	rBV2	401	386	0.02%	0.003%
88	13.002	3622	3627	3629	rBV	427	391	0.02%	0.003%
89	13.060	3641	3645	3650	rBV3	458	426	0.02%	0.003%
90	13.121	3661	3664	3667	rBV3	517	354	0.02%	0.003%
91	13.227	3694	3697	3704	rVB5	1334	1346	0.07%	0.010%
92	13.417	3752	3756	3760	rBV3	499	506	0.03%	0.004%
93	13.507	3781	3784	3786	rVV2	300	223	0.01%	0.002%
94	13.613	3814	3817	3820	rBV	442	348	0.02%	0.003%
95	13.774	3864	3867	3870	rBV2	459	324	0.02%	0.002%
96	13.851	3885	3891	3897	rVB3	2118	2639	0.14%	0.019%
97	14.095	3958	3967	3975	rBV5	5265	8929	0.46%	0.065%
98	14.333	4034	4041	4049	rBV5	2961	4818	0.25%	0.035%
99	14.828	4193	4195	4197	rBV2	564	296	0.02%	0.002%
100	15.085	4273	4275	4278	rBV2	565	275	0.01%	0.002%




Sum of corrected areas: 13667907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050632.D
Acq On : 06 Sep 2022 14:27
Operator : SY/MD
Sample : VU0906WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

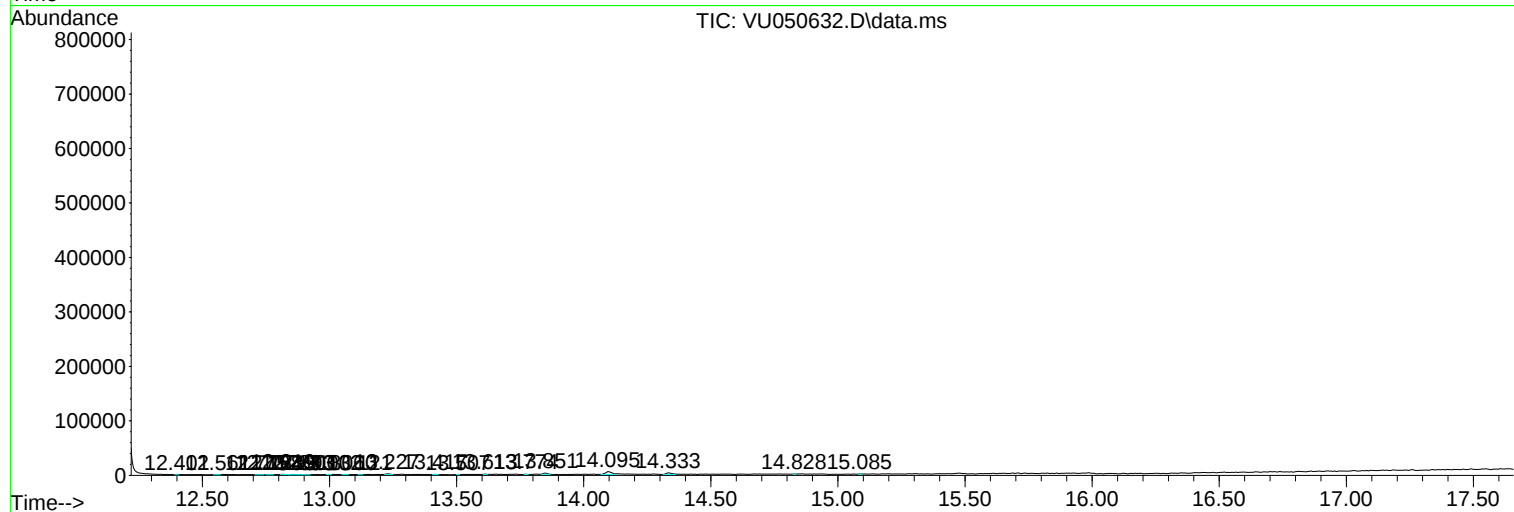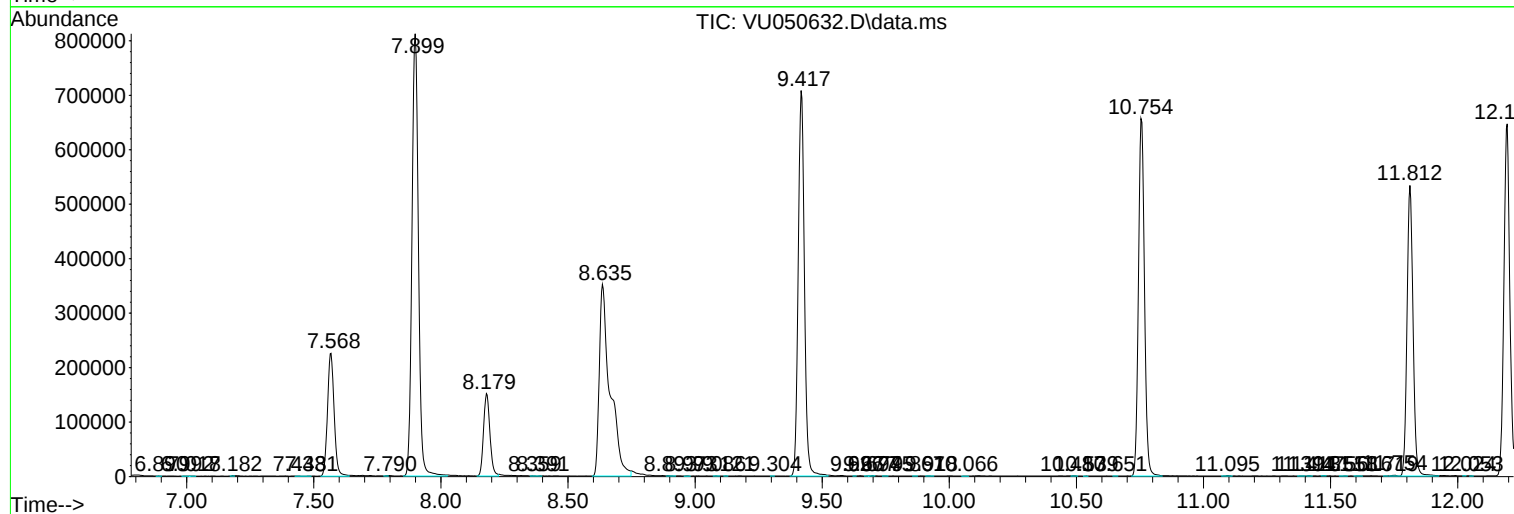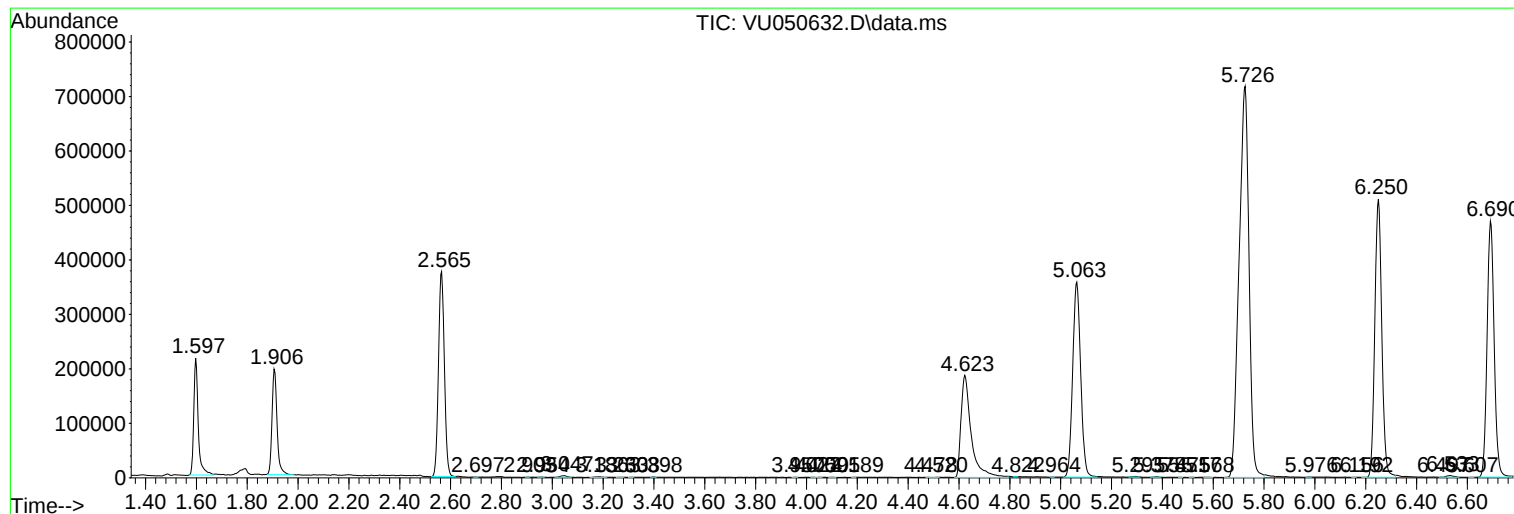

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050632.D
Acq On : 06 Sep 2022 14:27
Operator : SY/MD
Sample : VU0906WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050632.D
Acq On : 06 Sep 2022 14:27
Operator : SY/MD
Sample : VU0906WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------