

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050637.D
 Acq On : 06 Sep 2022 16:33
 Operator : SY/MD
 Sample : N4399-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	51	rBV3	2184	2506	0.26%	0.037%
2	1.517	52	55	63	rVB	1263	1093	0.11%	0.016%
3	1.597	72	80	94	rBV	78016	94702	9.89%	1.395%
4	1.719	116	118	121	rBV2	438	233	0.02%	0.003%
5	1.800	129	143	148	rVB8	6078	10722	1.12%	0.158%
6	1.903	166	175	193	rBV	67469	91368	9.54%	1.346%
7	2.057	219	223	226	rBV4	853	729	0.08%	0.011%
8	2.128	242	245	252	rBV3	477	593	0.06%	0.009%
9	2.186	259	263	266	rBV2	492	372	0.04%	0.005%
10	2.208	266	270	273	rVV	241	237	0.02%	0.003%
11	2.228	273	276	278	rVV2	344	212	0.02%	0.003%
12	2.256	283	285	289	rVV	273	198	0.02%	0.003%
13	2.279	290	292	295	rVB	434	233	0.02%	0.003%
14	2.366	316	319	323	rVV2	353	267	0.03%	0.004%
15	2.424	334	337	340	rVV	231	174	0.02%	0.003%
16	2.562	368	380	398	rBV	173277	283103	29.55%	4.171%
17	2.739	431	435	437	rBV	260	189	0.02%	0.003%
18	2.781	444	448	451	rBV2	449	397	0.04%	0.006%
19	2.797	451	453	457	rVV2	455	284	0.03%	0.004%
20	2.896	479	484	487	rBV2	196	209	0.02%	0.003%
21	2.954	500	502	512	rVB2	417	408	0.04%	0.006%
22	3.006	512	518	521	rBV2	253	285	0.03%	0.004%
23	3.038	521	528	531	rBV3	1093	1379	0.14%	0.020%
24	3.182	562	573	585	rBV2	2086	4471	0.47%	0.066%
25	3.517	674	677	685	rVB2	221	249	0.03%	0.004%
26	3.604	694	704	707	rBV	270	370	0.04%	0.005%
27	4.073	846	850	856	rBV2	207	215	0.02%	0.003%
28	4.128	861	867	871	rBV2	186	224	0.02%	0.003%
29	4.189	880	886	888	rBV2	188	223	0.02%	0.003%
30	4.494	978	981	988	rVB	248	248	0.03%	0.004%
31	4.620	1008	1020	1065	rBV	85667	243713	25.44%	3.591%
32	5.063	1140	1158	1177	rBV	179148	395075	41.24%	5.820%
33	5.256	1215	1218	1222	rBV3	259	196	0.02%	0.003%
34	5.279	1222	1225	1227	rBV2	419	335	0.03%	0.005%
35	5.375	1250	1255	1259	rVV3	456	463	0.05%	0.007%
36	5.533	1300	1304	1310	rVB2	238	234	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050637.D
 Acq On : 06 Sep 2022 16:33
 Operator : SY/MD
 Sample : N4399-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	5.723	1342	1363	1389	rBV2	346735	957951	100.00%	14.113%
38	5.915	1421	1423	1428	rVB	423	246	0.03%	0.004%
39	5.977	1439	1442	1448	rBV3	342	344	0.04%	0.005%
40	6.250	1512	1527	1549	rBV	264888	513640	53.62%	7.567%
41	6.401	1571	1574	1577	rVB2	288	195	0.02%	0.003%
42	6.533	1607	1615	1622	rVB3	1388	2263	0.24%	0.033%
43	6.610	1634	1639	1642	rVB	251	225	0.02%	0.003%
44	6.690	1649	1664	1685	rBV	226247	441825	46.12%	6.509%
45	6.954	1742	1746	1752	rVB2	170	184	0.02%	0.003%
46	7.092	1783	1789	1794	rBV2	248	286	0.03%	0.004%
47	7.176	1812	1815	1817	rBV	405	303	0.03%	0.004%
48	7.218	1824	1828	1830	rBV2	296	232	0.02%	0.003%
49	7.308	1854	1856	1861	rVB	288	245	0.03%	0.004%
50	7.340	1861	1866	1870	rBV	342	364	0.04%	0.005%
51	7.375	1870	1877	1883	rVV2	266	400	0.04%	0.006%
52	7.565	1924	1936	1958	rVV	111415	198187	20.69%	2.920%
53	7.745	1986	1992	1994	rBV2	179	206	0.02%	0.003%
54	7.899	2025	2040	2064	rBV	405315	714416	74.58%	10.525%
55	8.179	2116	2127	2145	rVV	77259	131894	13.77%	1.943%
56	8.369	2181	2186	2190	rVB2	350	325	0.03%	0.005%
57	8.520	2230	2233	2237	rVB2	257	191	0.02%	0.003%
58	8.636	2256	2269	2278	rBV3	166309	350103	36.55%	5.158%
59	8.835	2329	2331	2336	rVB3	438	270	0.03%	0.004%
60	9.041	2391	2395	2398	rBV	282	213	0.02%	0.003%
61	9.089	2407	2410	2415	rVV2	185	218	0.02%	0.003%
62	9.111	2415	2417	2420	rVV2	290	189	0.02%	0.003%
63	9.234	2452	2455	2460	rBV	227	221	0.02%	0.003%
64	9.311	2474	2479	2482	rBV2	238	262	0.03%	0.004%
65	9.417	2499	2512	2530	rBV	374221	635044	66.29%	9.356%
66	9.574	2558	2561	2570	rVB3	531	619	0.06%	0.009%
67	9.616	2570	2574	2577	rBV	220	182	0.02%	0.003%
68	9.825	2633	2639	2646	rBV2	241	285	0.03%	0.004%
69	9.951	2675	2678	2685	rBV2	145	201	0.02%	0.003%
70	10.099	2721	2724	2728	rVB2	323	289	0.03%	0.004%
71	10.317	2789	2792	2796	rVB2	221	192	0.02%	0.003%
72	10.391	2810	2815	2818	rBV2	189	221	0.02%	0.003%
73	10.472	2836	2840	2843	rBV2	234	179	0.02%	0.003%
74	10.755	2915	2928	2950	rBV	342564	558644	58.32%	8.230%
75	11.054	3017	3021	3027	rVB3	403	297	0.03%	0.004%
76	11.086	3027	3031	3034	rBV	427	356	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050637.D
 Acq On : 06 Sep 2022 16:33
 Operator : SY/MD
 Sample : N4399-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.468	3147	3150	3155	rVB	291	240	0.03%	0.004%
78	11.504	3158	3161	3168	rVB2	258	278	0.03%	0.004%
79	11.812	3241	3257	3280	rBV	308740	502867	52.49%	7.409%
80	12.063	3325	3335	3344	rBV5	9620	17636	1.84%	0.260%
81	12.192	3363	3375	3394	rBV	369274	612551	63.94%	9.024%
82	12.626	3504	3510	3514	rVB	204	231	0.02%	0.003%
83	12.652	3515	3518	3525	rBV2	225	279	0.03%	0.004%
84	12.690	3525	3530	3532	rBV3	279	239	0.02%	0.004%
85	12.719	3535	3539	3542	rBV2	200	225	0.02%	0.003%
86	12.816	3566	3569	3573	rBV2	274	215	0.02%	0.003%
87	13.230	3694	3698	3703	rBV3	259	275	0.03%	0.004%
88	13.330	3721	3729	3731	rBV3	493	535	0.06%	0.008%
89	13.343	3731	3733	3737	rVV2	395	350	0.04%	0.005%
90	13.362	3737	3739	3743	rVB3	330	217	0.02%	0.003%
91	13.459	3766	3769	3772	rBV2	356	224	0.02%	0.003%
92	13.610	3810	3816	3819	rBV3	481	543	0.06%	0.008%
93	13.664	3830	3833	3834	rBV	282	174	0.02%	0.003%
94	13.722	3847	3851	3854	rBV2	395	350	0.04%	0.005%
95	13.806	3873	3877	3880	rBV	428	397	0.04%	0.006%
96	13.889	3898	3903	3909	rBV2	363	542	0.06%	0.008%
97	13.951	3920	3922	3925	rBV2	375	271	0.03%	0.004%
98	14.343	4041	4044	4049	rVB2	599	448	0.05%	0.007%
99	15.368	4361	4363	4368	rVB4	642	431	0.04%	0.006%
100	15.603	4434	4436	4440	rBV4	563	343	0.04%	0.005%




Sum of corrected areas: 6787677

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050637.D
Acq On : 06 Sep 2022 16:33
Operator : SY/MD
Sample : N4399-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

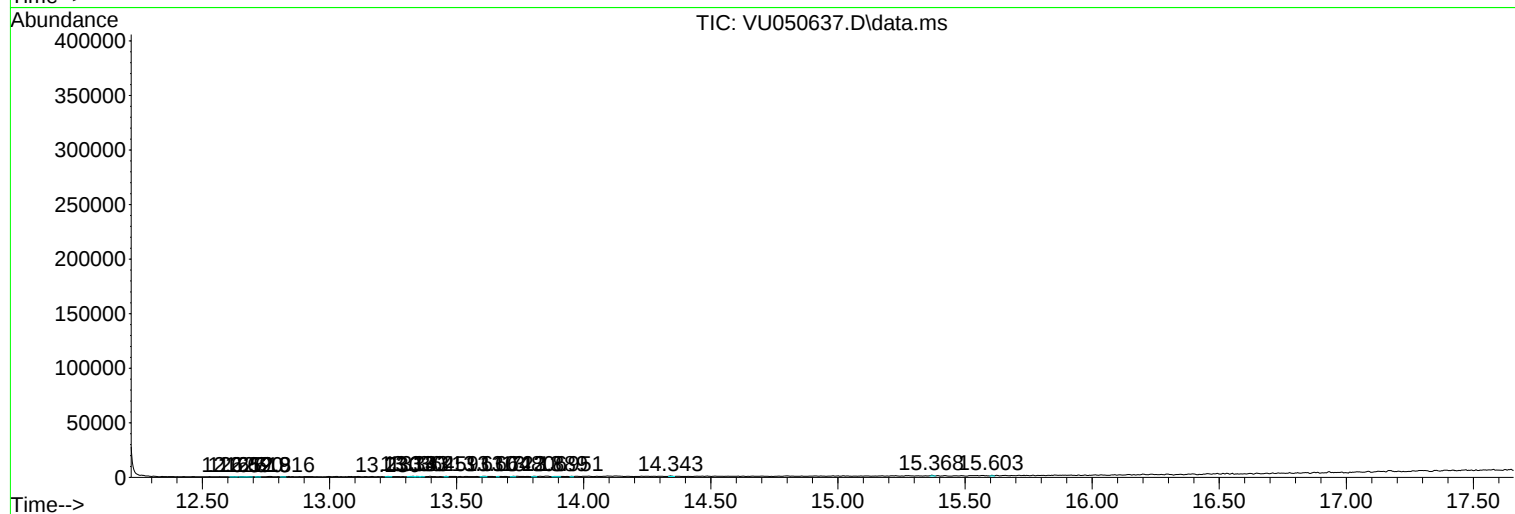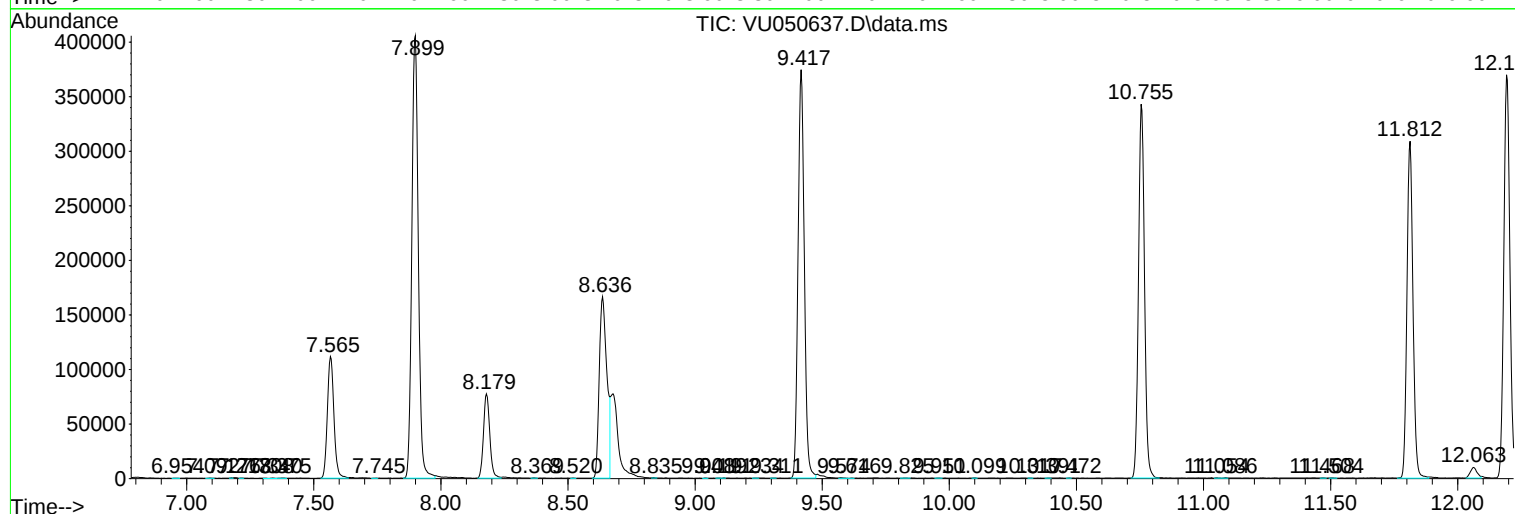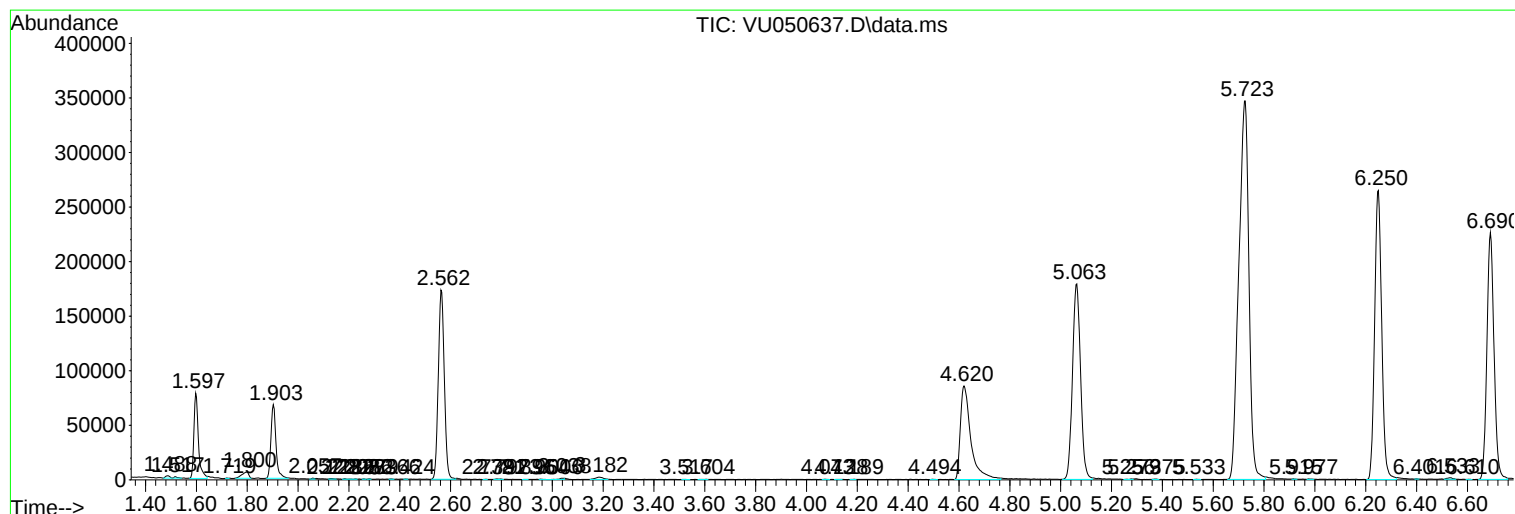

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050637.D
Acq On : 06 Sep 2022 16:33
Operator : SY/MD
Sample : N4399-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050637.D
Acq On : 06 Sep 2022 16:33
Operator : SY/MD
Sample : N4399-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------