

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050642.D
 Acq On : 06 Sep 2022 18:31
 Operator : SY/MD
 Sample : VIBLK131
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK131

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	52	rBV4	2895	3699	0.41%	0.055%
2	1.520	53	56	61	rVB2	1428	1176	0.13%	0.017%
3	1.598	71	80	106	rBV	64335	79838	8.84%	1.185%
4	1.794	126	141	146	rBV7	5247	9296	1.03%	0.138%
5	1.842	153	156	159	rBV3	598	546	0.06%	0.008%
6	1.903	167	175	197	rVB	58454	82178	9.10%	1.220%
7	2.019	209	211	214	rBV2	338	201	0.02%	0.003%
8	2.160	252	255	257	rBV3	345	243	0.03%	0.004%
9	2.231	272	277	281	rBV3	525	627	0.07%	0.009%
10	2.283	286	293	297	rVV4	784	940	0.10%	0.014%
11	2.302	297	299	304	rVV3	338	242	0.03%	0.004%
12	2.363	314	318	320	rBV2	457	360	0.04%	0.005%
13	2.405	328	331	332	rBV	422	213	0.02%	0.003%
14	2.562	368	380	392	rBV	140311	229349	25.40%	3.405%
15	2.627	393	400	411	rVB	9029	15730	1.74%	0.234%
16	2.707	423	425	429	rVB	348	209	0.02%	0.003%
17	2.736	429	434	436	rBV2	174	187	0.02%	0.003%
18	2.791	443	451	460	rBV2	2505	4410	0.49%	0.065%
19	2.893	474	483	497	rVV3	1759	3597	0.40%	0.053%
20	2.996	512	515	519	rVB2	315	208	0.02%	0.003%
21	3.025	519	524	525	rBV	347	267	0.03%	0.004%
22	3.041	525	529	542	rVV3	1266	2026	0.22%	0.030%
23	3.099	545	547	553	rVB2	175	184	0.02%	0.003%
24	3.183	562	573	586	rBV2	2274	5066	0.56%	0.075%
25	3.353	619	626	634	rVV5	1513	2441	0.27%	0.036%
26	3.479	658	665	668	rBV2	179	220	0.02%	0.003%
27	3.575	692	695	698	rBV	241	175	0.02%	0.003%
28	3.819	767	771	775	rBV2	183	203	0.02%	0.003%
29	4.099	852	858	861	rBV2	305	376	0.04%	0.006%
30	4.118	861	864	868	rVV2	241	237	0.03%	0.004%
31	4.257	901	907	910	rBV2	237	227	0.03%	0.003%
32	4.623	1007	1021	1065	rBV	88232	254578	28.19%	3.779%
33	4.868	1095	1097	1101	rVB	346	228	0.03%	0.003%
34	5.064	1141	1158	1183	rBV	167450	371708	41.17%	5.518%
35	5.282	1221	1226	1229	rBV2	566	624	0.07%	0.009%
36	5.343	1239	1245	1248	rBV	350	323	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050642.D
 Acq On : 06 Sep 2022 18:31
 Operator : SY/MD
 Sample : VIBLK131
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK131

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	5.376	1248	1255	1264	rVV4	1028	1771	0.20%	0.026%
38	5.411	1264	1266	1271	rVB3	302	202	0.02%	0.003%
39	5.559	1309	1312	1321	rVB2	252	326	0.04%	0.005%
40	5.723	1342	1363	1396	rBV2	324407	902948	100.00%	13.405%
41	6.041	1455	1462	1464	rBV2	376	411	0.05%	0.006%
42	6.057	1464	1467	1470	rVV	212	182	0.02%	0.003%
43	6.073	1470	1472	1478	rVB2	366	374	0.04%	0.006%
44	6.131	1485	1490	1495	rBV2	286	352	0.04%	0.005%
45	6.250	1512	1527	1548	rBV	248960	476149	52.73%	7.069%
46	6.369	1560	1564	1566	rBV	433	293	0.03%	0.004%
47	6.382	1566	1568	1572	rVV	334	247	0.03%	0.004%
48	6.536	1608	1616	1627	rVB8	2104	4391	0.49%	0.065%
49	6.588	1627	1632	1636	rVB2	392	361	0.04%	0.005%
50	6.691	1647	1664	1683	rBV2	210721	419874	46.50%	6.233%
51	6.842	1709	1711	1714	rBV2	355	190	0.02%	0.003%
52	6.861	1714	1717	1721	rVV	199	184	0.02%	0.003%
53	7.147	1802	1806	1807	rBV2	410	275	0.03%	0.004%
54	7.160	1807	1810	1812	rBV2	562	405	0.04%	0.006%
55	7.565	1923	1936	1955	rBV	110011	198182	21.95%	2.942%
56	7.794	1997	2007	2019	rBV3	5320	9570	1.06%	0.142%
57	7.900	2025	2040	2057	rBV	367868	644672	71.40%	9.571%
58	8.179	2115	2127	2144	rBV	76685	132157	14.64%	1.962%
59	8.398	2192	2195	2205	rBB4	1012	1012	0.11%	0.015%
60	8.472	2215	2218	2219	rBV	254	175	0.02%	0.003%
61	8.556	2236	2244	2252	rVB3	2693	3760	0.42%	0.056%
62	8.636	2256	2269	2278	rBV3	164635	356029	39.43%	5.285%
63	8.919	2353	2357	2364	rVB3	421	649	0.07%	0.010%
64	9.269	2463	2466	2471	rBV2	137	175	0.02%	0.003%
65	9.417	2499	2512	2551	rBV	352411	599290	66.37%	8.897%
66	9.572	2551	2560	2572	rVB2	3674	6226	0.69%	0.092%
67	9.694	2589	2598	2612	rVB3	4013	6690	0.74%	0.099%
68	10.115	2717	2729	2744	rVV4	6146	12282	1.36%	0.182%
69	10.186	2748	2751	2756	rBV2	202	247	0.03%	0.004%
70	10.488	2835	2845	2853	rBV3	5166	7522	0.83%	0.112%
71	10.755	2916	2928	2946	rBV	335241	550398	60.96%	8.171%
72	11.089	3023	3032	3046	rBV2	6285	9472	1.05%	0.141%
73	11.176	3053	3059	3064	rBV2	314	370	0.04%	0.005%
74	11.472	3141	3151	3164	rVB3	8102	11826	1.31%	0.176%
75	11.665	3208	3211	3217	rVB2	229	258	0.03%	0.004%
76	11.745	3228	3236	3244	rBV2	8838	13344	1.48%	0.198%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050642.D
 Acq On : 06 Sep 2022 18:31
 Operator : SY/MD
 Sample : VIBLK131
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK131

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.813	3245	3257	3279	rVB	296117	493009	54.60%	7.319%
78	11.957	3299	3302	3303	rBV2	379	178	0.02%	0.003%
79	12.070	3330	3337	3343	rBV6	1560	2137	0.24%	0.032%
80	12.192	3360	3375	3397	rBV	340572	580717	64.31%	8.621%
81	12.388	3432	3436	3437	rBV	280	183	0.02%	0.003%
82	12.433	3447	3450	3454	rBV2	222	188	0.02%	0.003%
83	12.530	3477	3480	3485	rBV	305	251	0.03%	0.004%
84	12.690	3527	3530	3533	rVB	365	237	0.03%	0.004%
85	12.732	3538	3543	3546	rVB2	269	234	0.03%	0.003%
86	12.761	3546	3552	3556	rBV3	412	635	0.07%	0.009%
87	12.916	3596	3600	3606	rBV2	261	359	0.04%	0.005%
88	13.002	3617	3627	3634	rVB5	1741	2555	0.28%	0.038%
89	13.076	3647	3650	3652	rBV2	282	187	0.02%	0.003%
90	13.112	3658	3661	3666	rBV2	337	268	0.03%	0.004%
91	13.221	3685	3695	3707	rBV3	15771	24441	2.71%	0.363%
92	13.440	3759	3763	3764	rBV	304	199	0.02%	0.003%
93	13.674	3829	3836	3839	rBV3	359	482	0.05%	0.007%
94	13.842	3877	3888	3902	rBV2	25428	41470	4.59%	0.616%
95	14.089	3953	3965	3993	rBV	46237	88039	9.75%	1.307%
96	14.330	4030	4040	4057	rVB2	32529	53385	5.91%	0.793%
97	15.160	4296	4298	4301	rVB	546	287	0.03%	0.004%
98	15.240	4320	4323	4326	rBV3	494	310	0.03%	0.005%
99	15.475	4393	4396	4401	rVB5	709	582	0.06%	0.009%
100	15.501	4401	4404	4405	rBV2	492	282	0.03%	0.004%




Sum of corrected areas: 6735988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050642.D
Acq On : 06 Sep 2022 18:31
Operator : SY/MD
Sample : VIBLK131
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK131

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

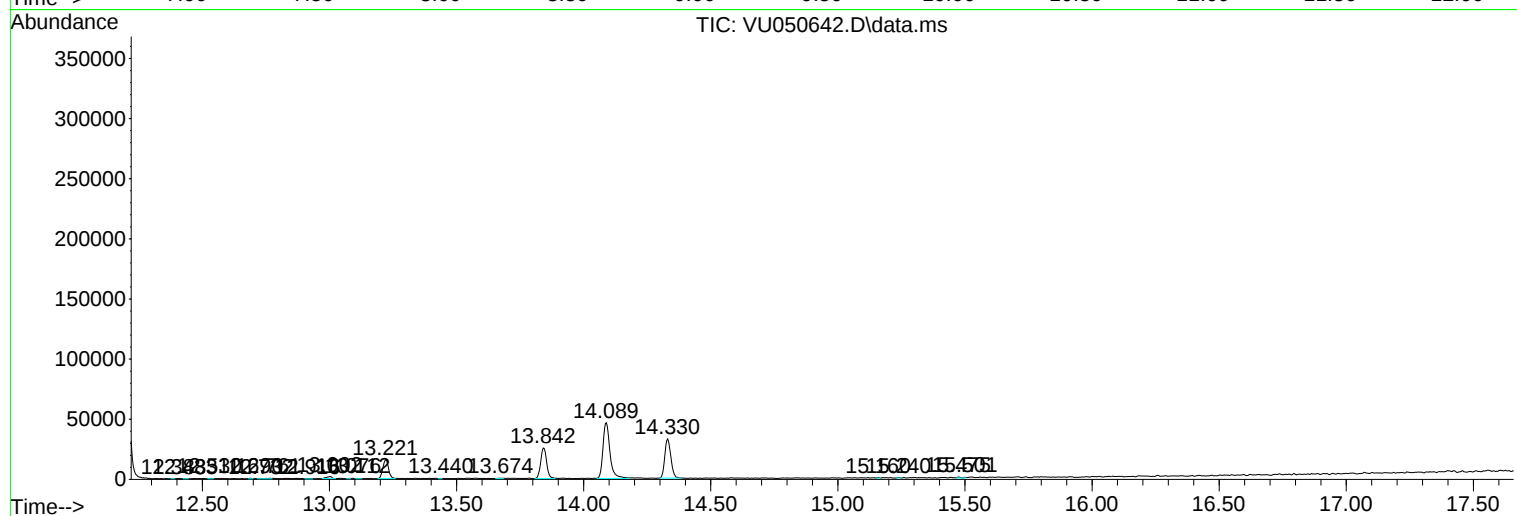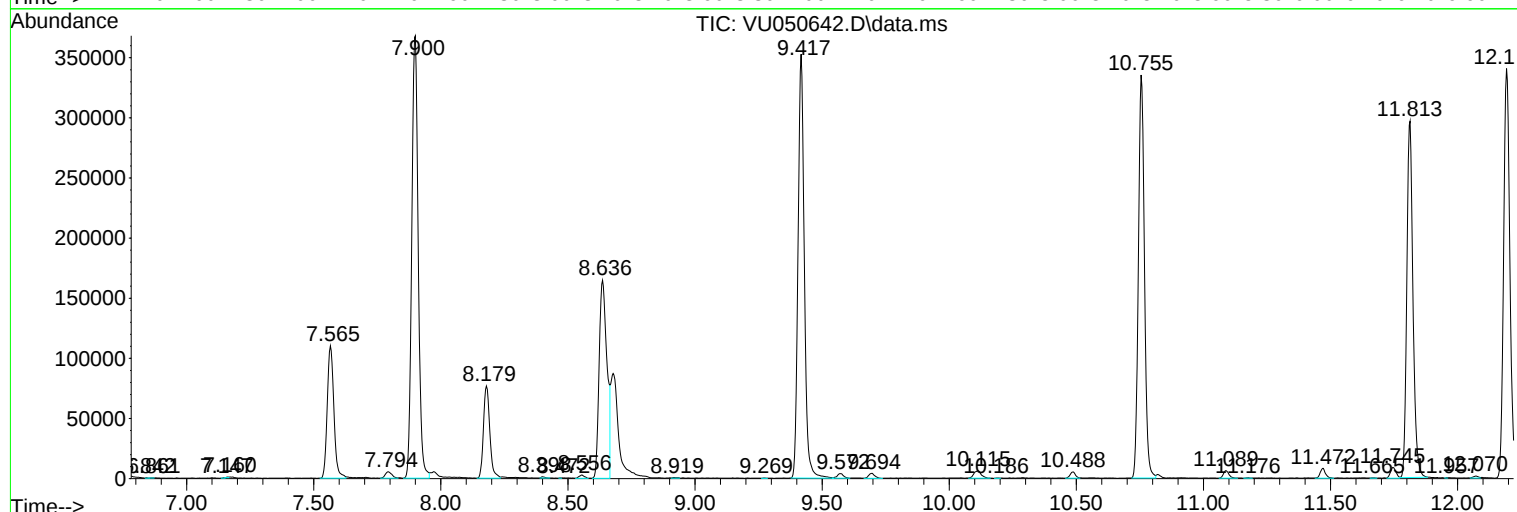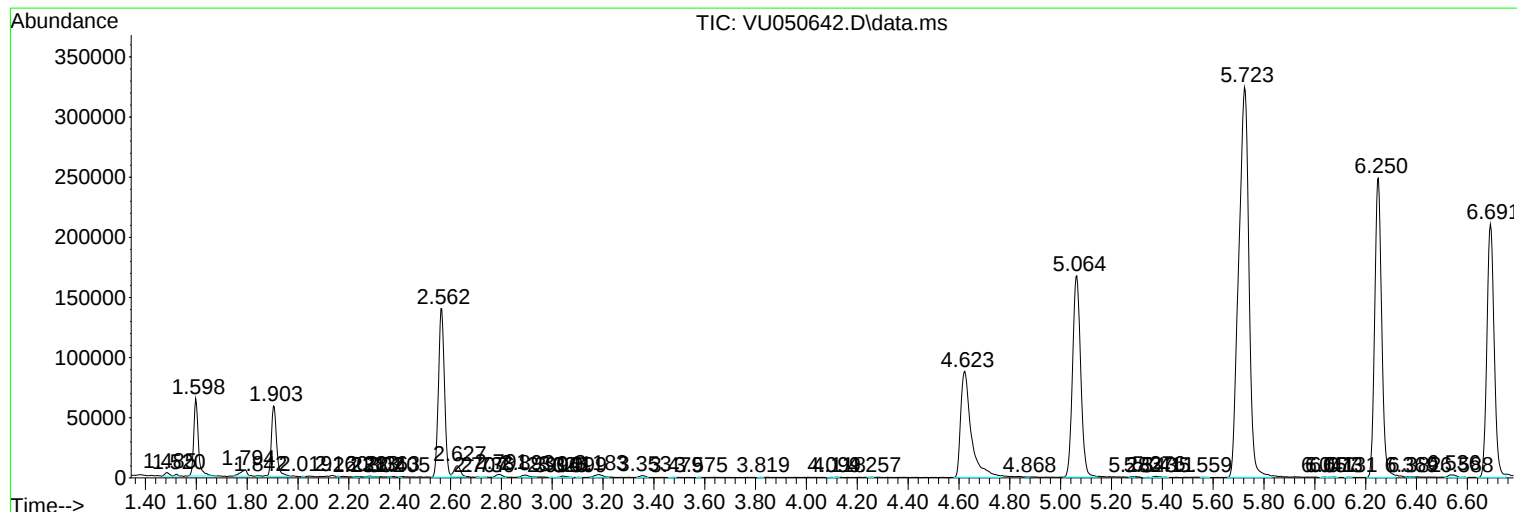

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050642.D
Acq On : 06 Sep 2022 18:31
Operator : SY/MD
Sample : VIBLK131
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK131

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050642.D
Acq On : 06 Sep 2022 18:31
Operator : SY/MD
Sample : VIBLK131
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK131

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------