

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050647.D
 Acq On : 06 Sep 2022 20:29
 Operator : SY/MD
 Sample : N4482-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	43	45	49	rVB2	1606	1001	0.15%	0.020%
2	1.597	73	80	100	rBV	40305	51411	7.66%	1.047%
3	1.742	123	125	128	rVB	423	219	0.03%	0.004%
4	1.826	129	151	152	rBV5	5507	12123	1.81%	0.247%
5	1.900	166	174	194	rVB	40493	56417	8.41%	1.149%
6	2.115	238	241	245	rBV2	353	303	0.05%	0.006%
7	2.240	275	280	282	rBV	237	230	0.03%	0.005%
8	2.289	294	295	297	rBV	292	165	0.02%	0.003%
9	2.562	369	380	395	rVV	94399	151621	22.59%	3.087%
10	2.633	395	402	414	rVB2	1488	3025	0.45%	0.062%
11	2.742	433	436	442	rVB2	255	281	0.04%	0.006%
12	2.790	444	451	460	rVB3	512	907	0.14%	0.018%
13	3.176	567	571	572	rBV2	330	213	0.03%	0.004%
14	3.356	624	627	631	rBV	329	248	0.04%	0.005%
15	3.408	639	643	648	rBV	241	190	0.03%	0.004%
16	3.575	691	695	699	rVB2	196	155	0.02%	0.003%
17	3.893	789	794	800	rVB2	158	184	0.03%	0.004%
18	3.957	808	814	816	rBV2	170	179	0.03%	0.004%
19	4.099	856	858	864	rVB2	235	234	0.03%	0.005%
20	4.134	864	869	874	rBV2	286	380	0.06%	0.008%
21	4.311	921	924	928	rVV2	170	176	0.03%	0.004%
22	4.350	931	936	939	rVB2	190	190	0.03%	0.004%
23	4.379	939	945	948	rBV2	169	161	0.02%	0.003%
24	4.411	952	955	958	rBV2	217	189	0.03%	0.004%
25	4.478	971	976	979	rBV2	158	171	0.03%	0.003%
26	4.626	1010	1022	1067	rBV2	74773	222725	33.18%	4.534%
27	5.063	1140	1158	1177	rBV	126563	278289	41.46%	5.666%
28	5.215	1199	1205	1208	rVB2	233	180	0.03%	0.004%
29	5.234	1208	1211	1213	rBV	307	157	0.02%	0.003%
30	5.247	1213	1215	1220	rVV2	198	165	0.02%	0.003%
31	5.292	1221	1229	1235	rVV4	640	1067	0.16%	0.022%
32	5.562	1310	1313	1315	rBV2	223	176	0.03%	0.004%
33	5.723	1340	1363	1391	rBV2	240417	671229	100.00%	13.666%
34	5.970	1438	1440	1443	rBV2	474	355	0.05%	0.007%
35	6.096	1474	1479	1484	rVB2	190	196	0.03%	0.004%
36	6.250	1512	1527	1554	rBV	199760	383846	57.19%	7.815%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050647.D
 Acq On : 06 Sep 2022 20:29
 Operator : SY/MD
 Sample : N4482-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.417	1575	1579	1583	rBV2	451	362	0.05%	0.007%
38	6.462	1590	1593	1598	rVB2	442	386	0.06%	0.008%
39	6.526	1606	1613	1618	rBV5	1019	1166	0.17%	0.024%
40	6.690	1650	1664	1693	rVV	165886	321377	47.88%	6.543%
41	6.797	1693	1697	1701	rBB3	440	257	0.04%	0.005%
42	6.816	1701	1703	1709	rVB2	331	244	0.04%	0.005%
43	6.899	1725	1729	1733	rBV2	529	553	0.08%	0.011%
44	7.137	1800	1803	1809	rVB2	198	212	0.03%	0.004%
45	7.192	1809	1820	1827	rBV3	1025	1853	0.28%	0.038%
46	7.469	1898	1906	1909	rBV2	201	283	0.04%	0.006%
47	7.565	1925	1936	1955	rBV	82494	145722	21.71%	2.967%
48	7.684	1969	1973	1981	rVB4	454	603	0.09%	0.012%
49	7.803	2005	2010	2013	rBV4	455	364	0.05%	0.007%
50	7.899	2026	2040	2058	rBV	253731	446069	66.46%	9.082%
51	8.124	2105	2110	2114	rVB2	218	235	0.04%	0.005%
52	8.179	2116	2127	2144	rVV	56195	95122	14.17%	1.937%
53	8.552	2240	2243	2247	rBV2	491	331	0.05%	0.007%
54	8.636	2256	2269	2279	rBV3	139925	307675	45.84%	6.264%
55	9.047	2391	2397	2399	rBV2	184	183	0.03%	0.004%
56	9.063	2399	2402	2412	rVB2	242	344	0.05%	0.007%
57	9.227	2449	2453	2455	rBV2	208	169	0.03%	0.003%
58	9.314	2478	2480	2483	rBV2	219	158	0.02%	0.003%
59	9.417	2499	2512	2536	rBV	287749	484765	72.22%	9.869%
60	9.549	2549	2553	2555	rVB2	339	225	0.03%	0.005%
61	9.575	2555	2561	2566	rBB	492	575	0.09%	0.012%
62	9.697	2595	2599	2605	rVB2	367	382	0.06%	0.008%
63	9.938	2666	2674	2678	rBV	272	382	0.06%	0.008%
64	10.092	2719	2722	2724	rBV3	299	196	0.03%	0.004%
65	10.108	2725	2727	2729	rVV2	475	269	0.04%	0.005%
66	10.121	2729	2731	2735	rVV3	394	280	0.04%	0.006%
67	10.282	2776	2781	2789	rVB2	326	436	0.06%	0.009%
68	10.317	2789	2792	2798	rVB2	222	211	0.03%	0.004%
69	10.546	2861	2863	2865	rBV2	239	169	0.03%	0.003%
70	10.658	2895	2898	2903	rVB2	156	160	0.02%	0.003%
71	10.755	2915	2928	2949	rBV	276846	445251	66.33%	9.065%
72	11.066	3021	3025	3029	rBV	208	231	0.03%	0.005%
73	11.221	3069	3073	3075	rBV	204	161	0.02%	0.003%
74	11.301	3095	3098	3102	rBV2	219	227	0.03%	0.005%
75	11.475	3148	3152	3159	rVB2	484	379	0.06%	0.008%
76	11.546	3170	3174	3176	rBV	262	194	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
 Data File : VU050647.D
 Acq On : 06 Sep 2022 20:29
 Operator : SY/MD
 Sample : N4482-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.619	3194	3197	3202	rVB2	327	317	0.05%	0.006%
78	11.745	3233	3236	3238	rBV2	395	232	0.03%	0.005%
79	11.812	3245	3257	3278	rBV	231489	373864	55.70%	7.612%
80	12.063	3326	3335	3349	rBV3	6744	12841	1.91%	0.261%
81	12.192	3363	3375	3392	rBV	253856	417036	62.13%	8.490%
82	12.385	3430	3435	3437	rBV2	396	303	0.05%	0.006%
83	12.584	3494	3497	3502	rBB2	190	175	0.03%	0.004%
84	12.796	3560	3563	3566	rBV	453	248	0.04%	0.005%
85	12.851	3577	3580	3583	rVB2	258	170	0.03%	0.003%
86	12.928	3601	3604	3611	rBV3	298	289	0.04%	0.006%
87	13.063	3644	3646	3649	rBV2	332	229	0.03%	0.005%
88	13.234	3689	3699	3705	rVB4	989	1505	0.22%	0.031%
89	13.443	3762	3764	3767	rVB	334	176	0.03%	0.004%
90	13.642	3824	3826	3831	rVB2	312	239	0.04%	0.005%
91	13.671	3831	3835	3840	rBV2	355	417	0.06%	0.008%
92	13.780	3863	3869	3874	rBV3	289	423	0.06%	0.009%
93	13.851	3882	3891	3896	rBV4	1146	1687	0.25%	0.034%
94	14.008	3937	3940	3945	rBV3	203	201	0.03%	0.004%
95	14.034	3945	3948	3952	rBV2	350	260	0.04%	0.005%
96	14.105	3961	3970	3972	rBV4	964	1356	0.20%	0.028%
97	14.330	4035	4040	4051	rBV6	1195	1906	0.28%	0.039%
98	14.488	4086	4089	4091	rBV2	311	219	0.03%	0.004%
99	14.947	4229	4232	4233	rBV2	342	179	0.03%	0.004%
100	15.086	4270	4275	4278	rBV3	626	610	0.09%	0.012%




Sum of corrected areas: 4911801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050647.D
Acq On : 06 Sep 2022 20:29
Operator : SY/MD
Sample : N4482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

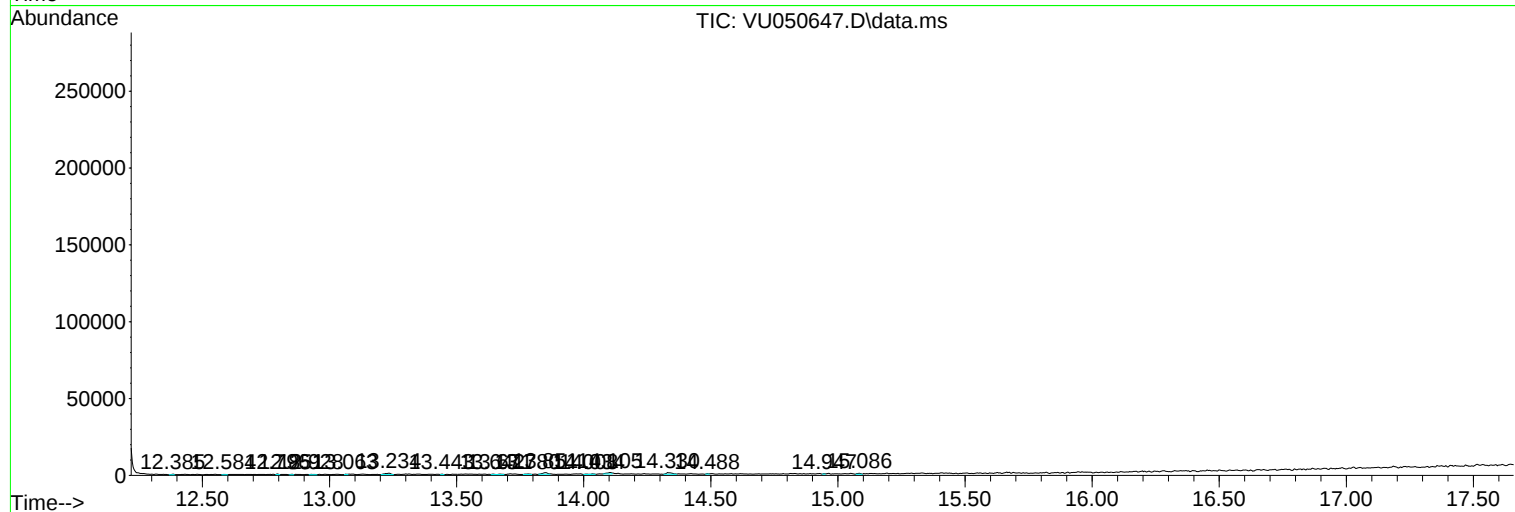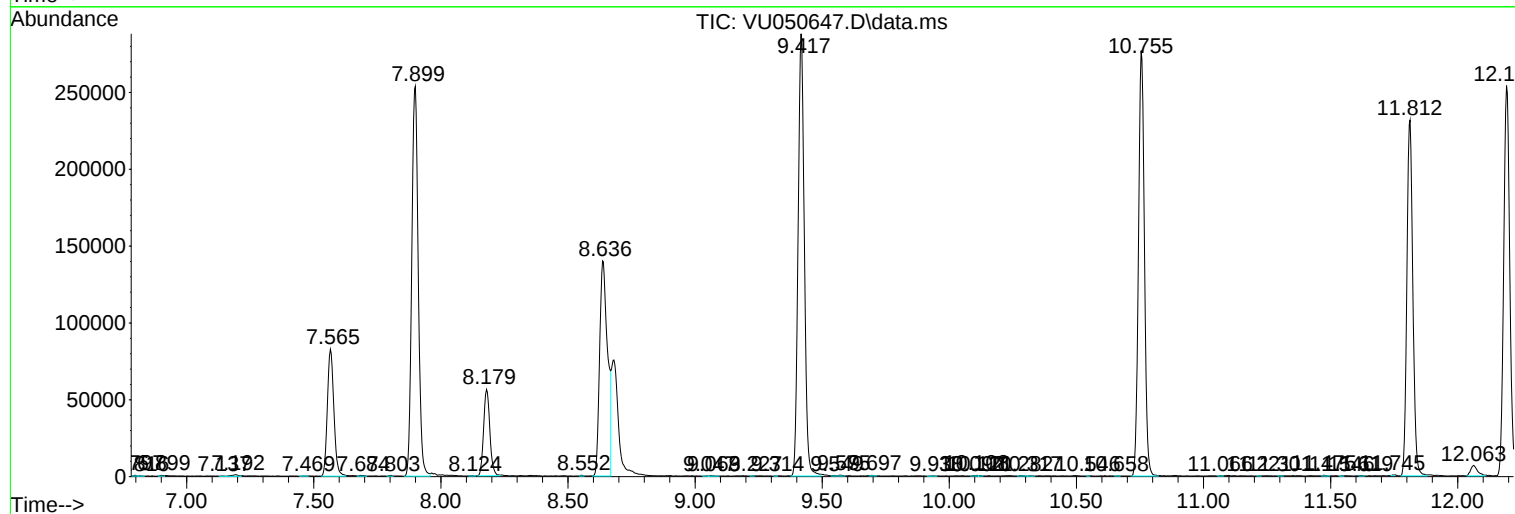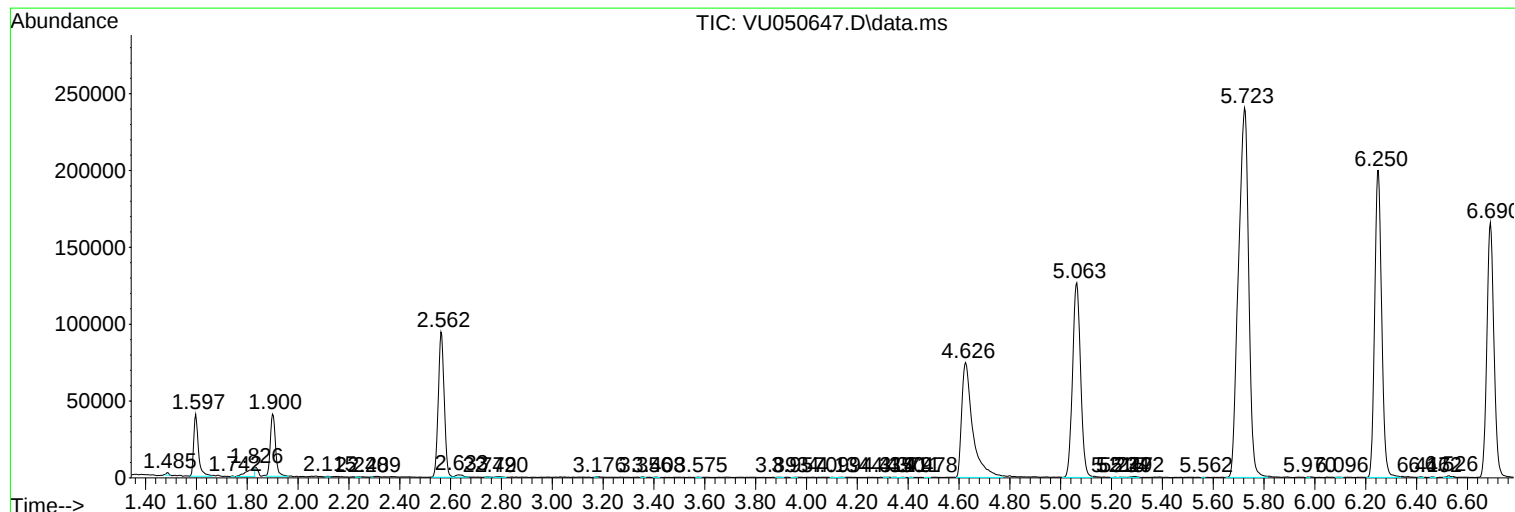

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050647.D
Acq On : 06 Sep 2022 20:29
Operator : SY/MD
Sample : N4482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050647.D
Acq On : 06 Sep 2022 20:29
Operator : SY/MD
Sample : N4482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc