
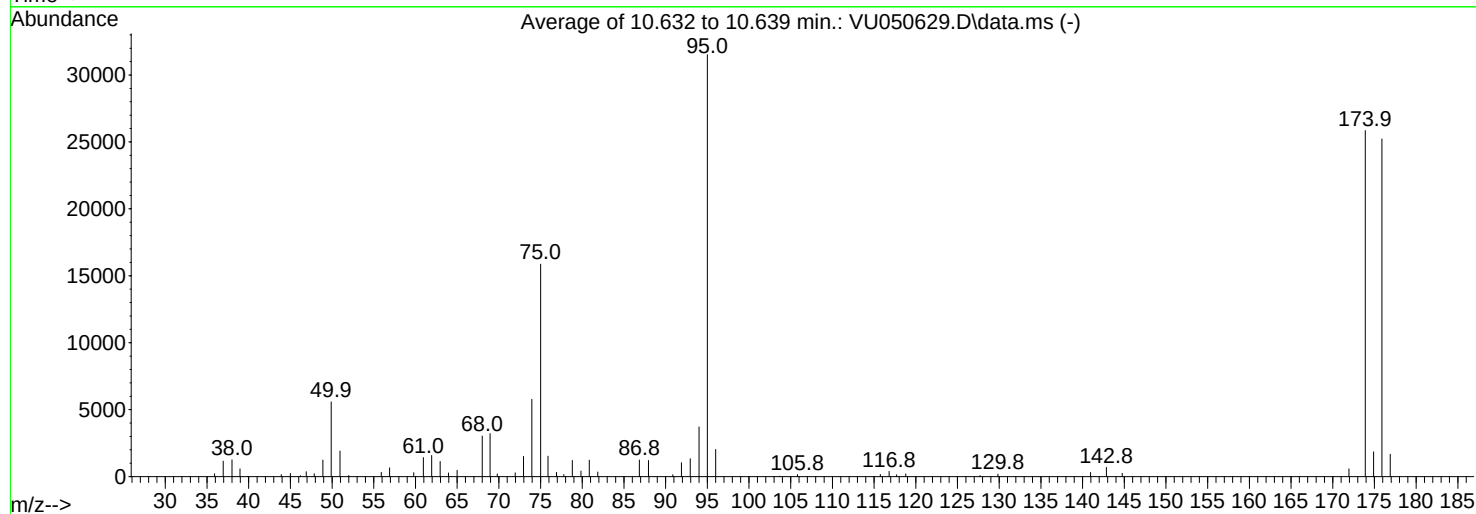


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090622\
Data File : VU050629.D
Acq On : 06 Sep 2022 11:31
Operator : SY/MD
Sample : BFB120
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB120

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Title : VOC Analysis
Last Update : Wed Sep 07 01:37:50 2022

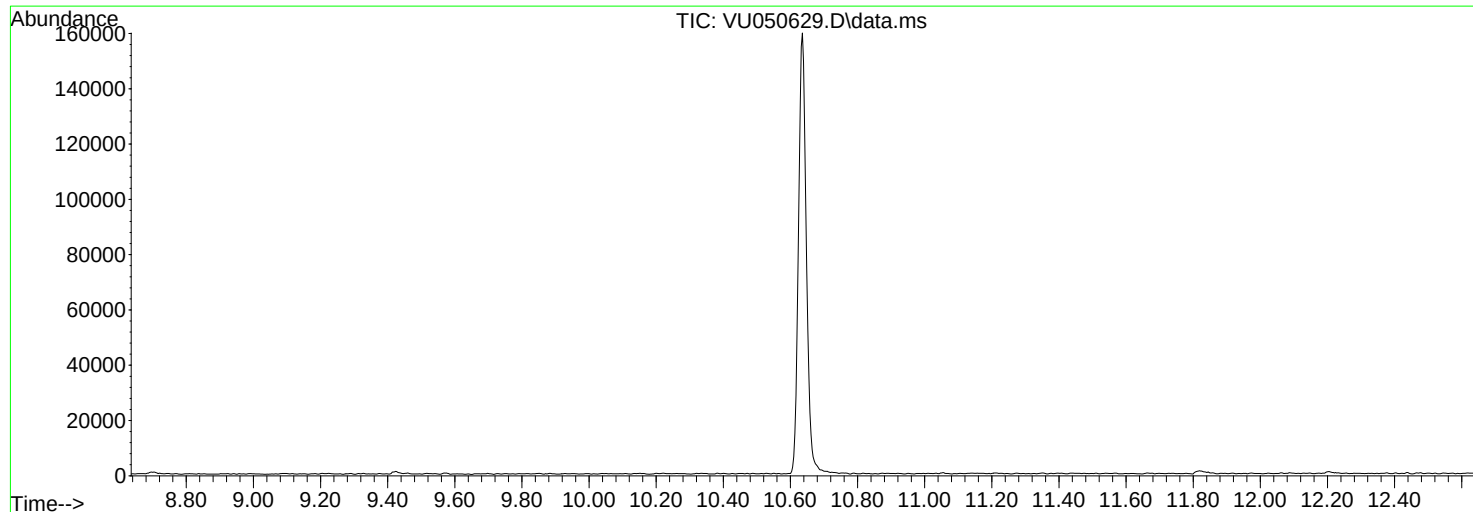

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	5575	PASS
75	95	30	80	50.4	15873	PASS
95	95	100	100	100.0	31512	PASS
96	95	5	9	6.4	2029	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.0	25851	PASS
175	174	5	9	7.1	1848	PASS
176	174	95	101	97.6	25235	PASS
177	176	5	9	6.6	1672	PASS

Scan 2879 (10.597 min): VU050629.D\data.ms
BFB120

m/z	Abundance
39.90	421.0
43.90	435.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120

m/z	Abundance
35.90	203.0
37.00	1249.0
38.00	1295.0
38.90	575.0
39.80	430.0
43.90	543.0
45.00	245.0
46.90	447.0
47.90	246.0
48.90	1281.0
49.90	5684.0
50.90	1934.0
52.00	116.0
55.90	275.0
56.90	639.0
59.80	272.0
61.00	1559.0
61.90	1586.0
63.00	1154.0
63.90	335.0
65.00	460.0
68.00	3125.0
69.00	3164.0
69.80	207.0
71.90	271.0
73.00	1493.0
74.00	5732.0
75.00	16440.0
75.90	1489.0
76.90	281.0
77.80	137.0
78.80	1218.0
79.90	430.0
80.80	1278.0
81.90	325.0
86.80	1276.0
87.90	1221.0
90.80	123.0
91.90	994.0
92.90	1399.0
94.00	3633.0
95.00	31328.0
96.00	2189.0
103.70	112.0
105.80	141.0
115.70	128.0
116.80	381.0
117.70	132.0
118.80	186.0
127.70	124.0
129.90	168.0
140.90	299.0
142.90	644.0
144.80	270.0
172.00	639.0
173.90	25736.0
174.90	1887.0
175.90	24432.0
176.90	1615.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120

m/z	Abundance
35.90	208.0
37.00	1208.0
38.00	1277.0
38.90	597.0
39.90	428.0
43.90	606.0
45.00	238.0
46.20	104.0
46.90	379.0
47.90	215.0
48.90	1278.0
49.90	5814.0
51.00	1992.0
52.00	114.0
55.90	317.0
56.90	674.0
59.80	310.0
60.90	1437.0
61.90	1627.0
62.90	1140.0
63.90	260.0
65.00	486.0
68.00	3148.0
69.00	3319.0
69.80	194.0
71.90	312.0
73.00	1572.0
74.00	6064.0
75.00	16392.0
75.90	1622.0
76.90	357.0
77.80	160.0
78.80	1274.0
79.80	411.0
80.90	1277.0
81.90	361.0
86.90	1242.0
88.00	1217.0
90.80	123.0
91.90	1106.0
92.90	1346.0
94.00	3801.0
95.00	32344.0
96.00	2050.0
105.80	157.0
115.80	172.0
116.80	427.0
117.70	142.0
118.80	206.0
127.70	126.0
129.80	207.0
141.00	310.0
142.80	733.0
144.80	253.0
172.00	597.0
173.90	26688.0
174.90	1876.0
175.90	26136.0
176.90	1741.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120

m/z	Abundance
35.90	225.0
36.90	1019.0
38.00	1190.0
39.00	567.0
39.90	414.0
43.90	603.0
45.00	218.0
46.20	108.0
46.90	276.0
47.80	180.0
48.90	1157.0
49.90	5226.0
51.00	1792.0
55.90	357.0
56.90	651.0
59.80	304.0
60.90	1240.0
62.00	1499.0
62.90	1110.0
64.00	222.0
65.00	459.0
68.00	2805.0
68.90	3144.0
69.80	202.0
72.00	254.0
72.90	1441.0
73.90	5526.0
75.00	14787.0
75.90	1474.0
76.90	322.0
77.80	145.0
78.80	1110.0
79.80	387.0
80.90	1138.0
81.80	343.0
86.90	1199.0
88.00	1178.0
90.90	151.0
91.90	1011.0
93.00	1241.0
94.00	3697.0
95.00	30864.0
96.00	1847.0
105.80	145.0
115.80	197.0
116.80	364.0
117.70	141.0
118.80	206.0
129.80	195.0
141.00	300.0
142.80	673.0
144.70	228.0
171.90	495.0
173.90	25128.0
174.90	1780.0
175.90	25136.0
176.90	1660.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120