

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
 Data File : VU055173.D
 Acq On : 07 Sep 2023 05:00
 Operator : MD/SY
 Sample : 04267-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 07 15:40:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 06 05:03:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	167693	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	171919	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.814	152	87317	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	31897	4.058	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.907	69	38952	4.282	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.560	65	18981	4.239	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.800%
20) 2-Butanone-d5	4.624	46	122723	53.808	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.620%
24) Chloroform-d	5.058	84	100552	4.821	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	5.702	65	51566	4.942	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.800%
32) Benzene-d6	5.724	84	198223	4.671	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	6.685	67	67754	5.020	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.898	98	170973	4.374	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.400%
43) trans-1,3-Dichloroprop...	8.181	79	14112	3.797	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.000%
46) 2-Hexanone-d5	8.634	63	70876	46.968	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.940%
56) 1,1,2,2-Tetrachloroeth...	10.756	84	48889	5.150	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.000%
66) 1,2-Dichlorobenzene-d4	12.193	152	61429	4.820	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds						
					Qvalue	
3) Chloromethane	1.518	50	1795	0.181	ug/L	98
5) Vinyl chloride	1.599	62	1153	0.110	ug/L #	74
12) 1,1-Dichloroethene	2.573	96	6179	0.797	ug/L #	1
17) Methyl tert-butyl Ether	3.361	73	4055	0.199	ug/L #	69
18) trans-1,2-Dichloroethene	3.351	96	2274	0.289	ug/L	92
22) cis-1,2-Dichloroethene	4.663	96	439587	45.655	ug/L	95
34) Trichloroethene	6.537	95	2636563	259.277	ug/L	96
35) Methylcyclohexane	6.689	83	15117	1.060	ug/L #	29
37) 1,2-Dichloropropane	6.689	63	7764	0.779	ug/L #	88
42) Toluene	7.968	91	19299	0.495	ug/L	89
45) 1,1,2-Trichloroethane	8.399	97	764	0.114	ug/L #	80
47) Tetrachloroethene	8.553	164	2994	0.426	ug/L	93
48) 2-Hexanone	8.682	43	18483	4.153	ug/L	89
49) Dibromochloromethane	8.553	129	2767	0.378	ug/L #	9
51) Chlorobenzene	9.451	112	4288	0.166	ug/L	92
61) 1,2,3-Trichloropropane	11.811	75	12318	2.126	ug/L #	70
69) 1,3,5-Trichlorobenzene	13.843	180	11435	0.774	ug/L	97
70) 1,2,4-trichlorobenzene	13.843	180	11435	0.826	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055173.D
Acq On : 07 Sep 2023 05:00
Operator : MD/SY
Sample : 04267-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Sep 07 15:40:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 06 05:03:37 2023
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055173.D
Acq On : 07 Sep 2023 05:00
Operator : MD/SY
Sample : 04267-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Sep 07 15:40:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 06 05:03:37 2023
Response via : Initial Calibration




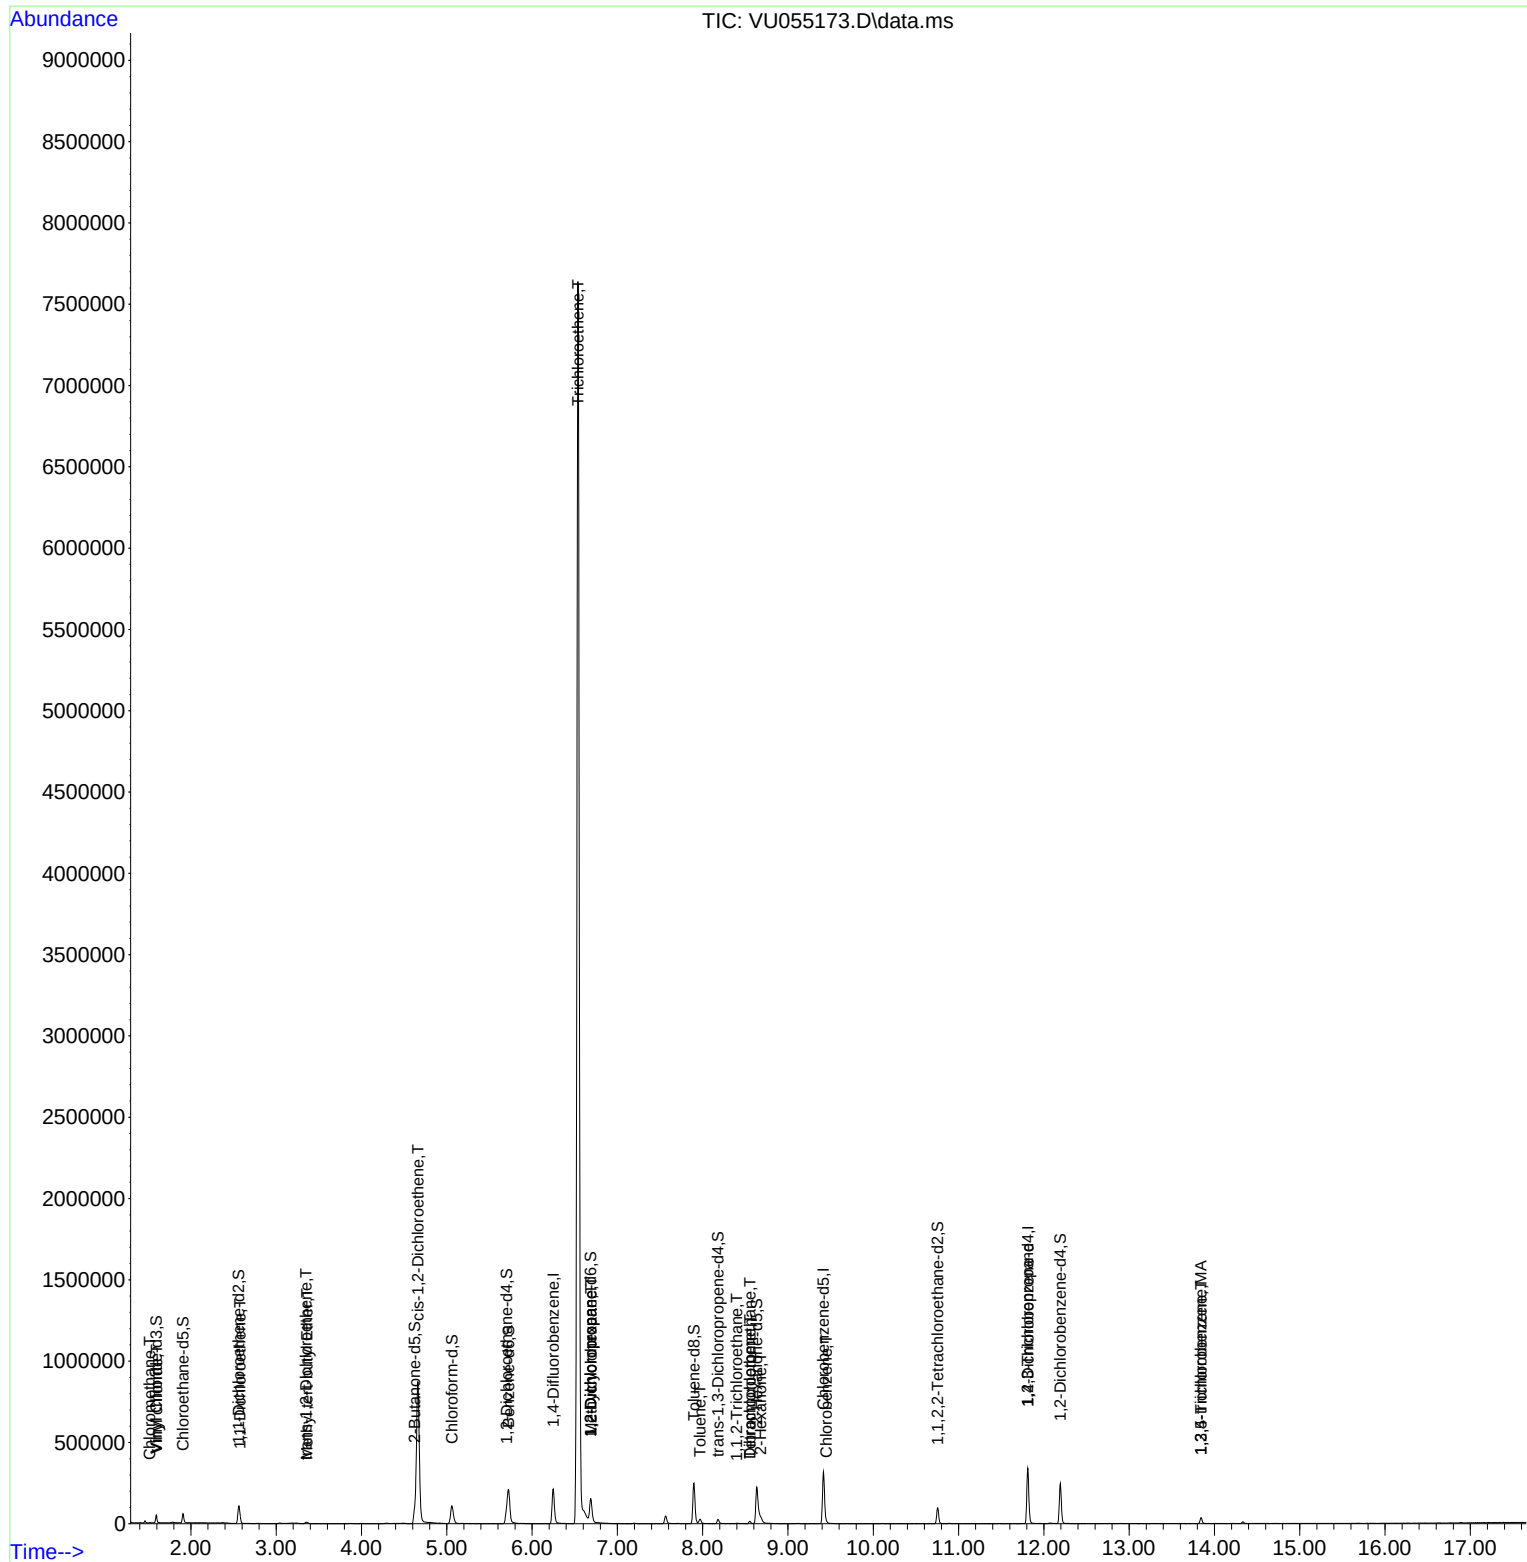


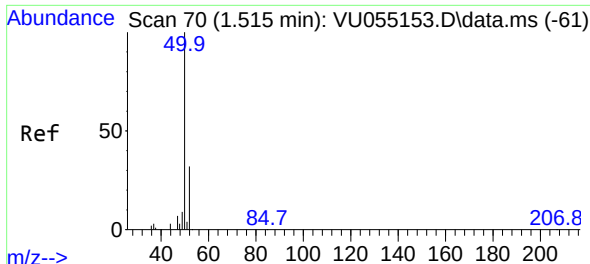

#3
Chloromethane
Concen: 0.181 ug/L
RT: 1.518 min Scan# 70
Delta R.T. 0.003 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 50 Resp: 1795
Ion Ratio Lower Upper
50 100
52 33.3 22.5 41.7

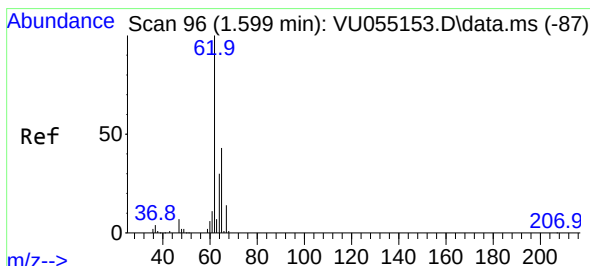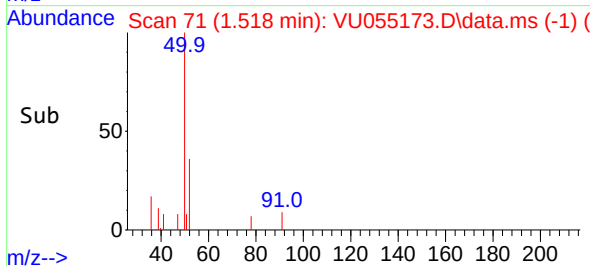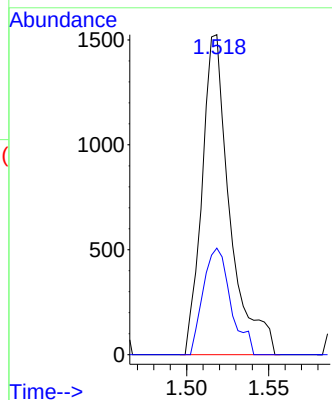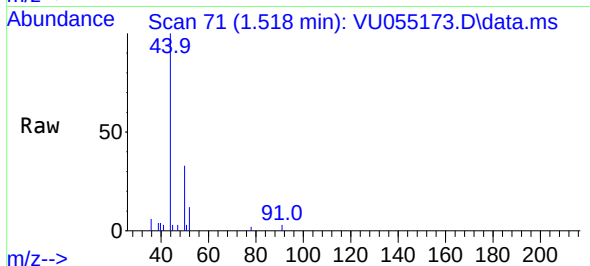

#5
Vinyl chloride
Concen: 0.110 ug/L
RT: 1.599 min Scan# 96
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00


Tgt Ion: 62 Resp: 1153
Ion Ratio Lower Upper
62 100
64 49.7 24.2 45.0#

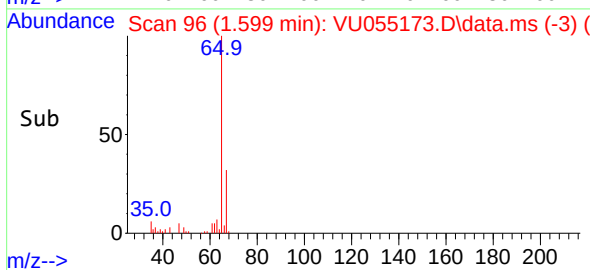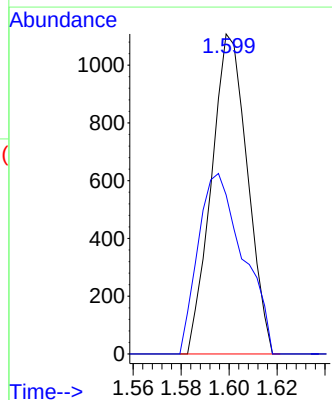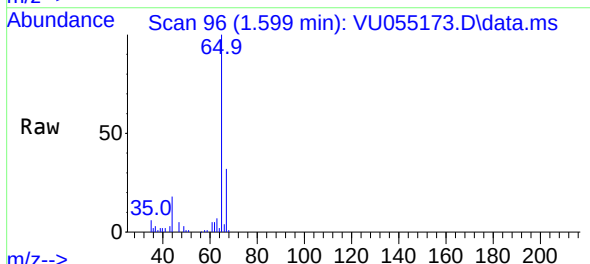



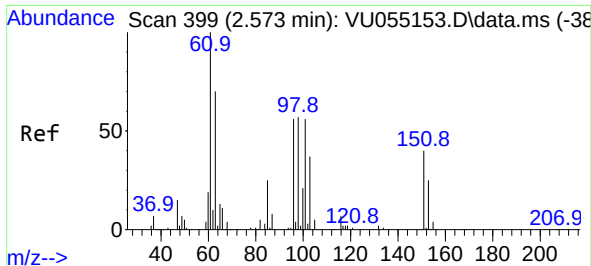


#12
1,1-Dichloroethene
Concen: 0.797 ug/L
RT: 2.573 min Scan# 399
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Instrument :
MSVOA_U
ClientSampleId :



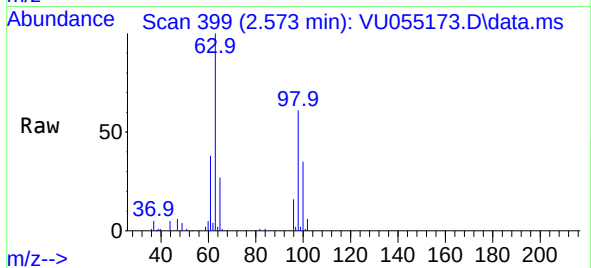



Tgt Ion: 96 Resp: 6179
Ion Ratio Lower Upper
96 100
61 244.2 120.8 224.4#
63 635.3 94.5 175.5#

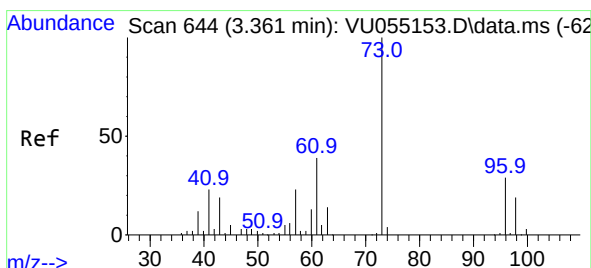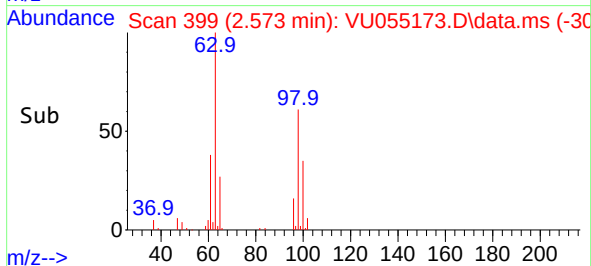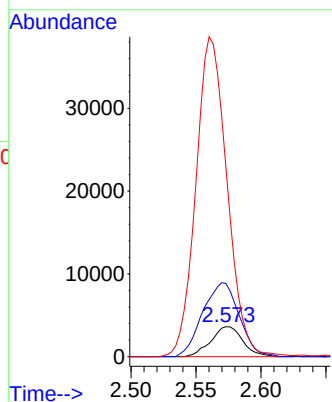

#17
Methyl tert-butyl Ether
Concen: 0.199 ug/L
RT: 3.361 min Scan# 644
Delta R.T. -0.003 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00


Tgt Ion: 73 Resp: 4055
Ion Ratio Lower Upper
73 100
43 9.4 16.2 24.2#
57 3.5 17.4 26.2#

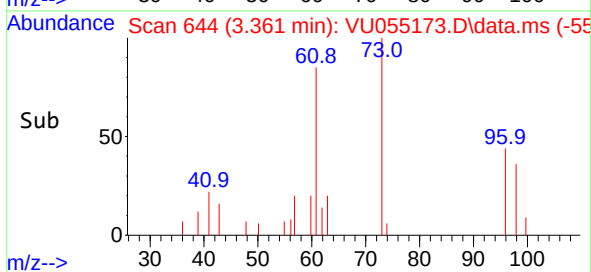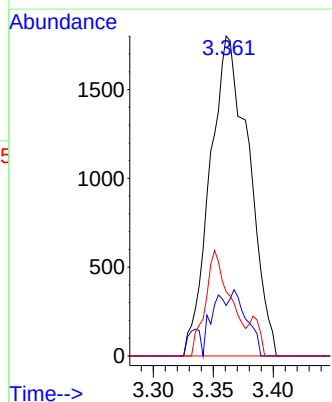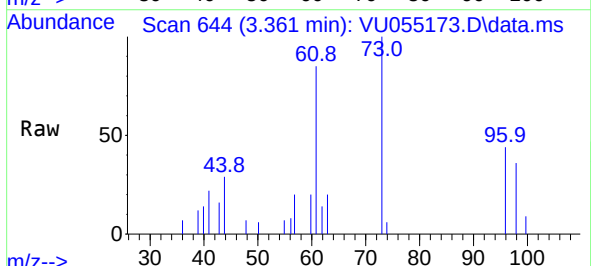



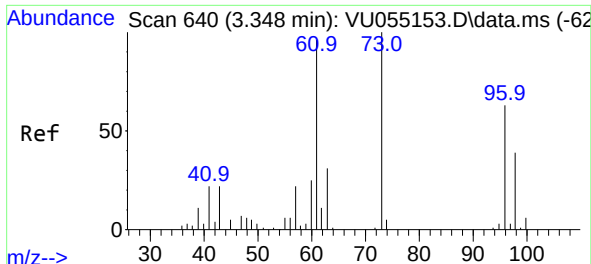


#18
trans-1,2-Dichloroethene
Concen: 0.289 ug/L
RT: 3.351 min Scan# 641
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Instrument :
MSVOA_U
ClientSampleId :



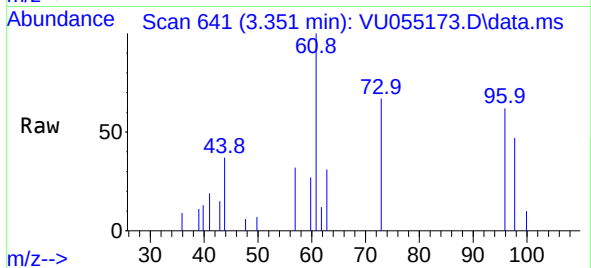



Tgt Ion: 96 Resp: 2274
Ion Ratio Lower Upper
96 100
61 162.1 108.1 200.9
98 76.2 45.4 84.4

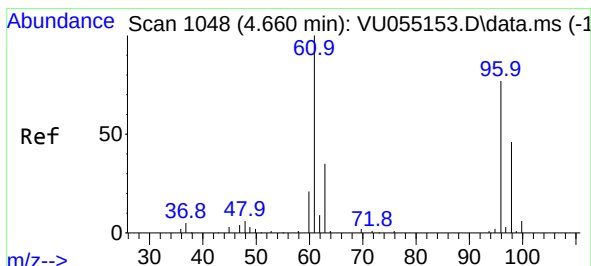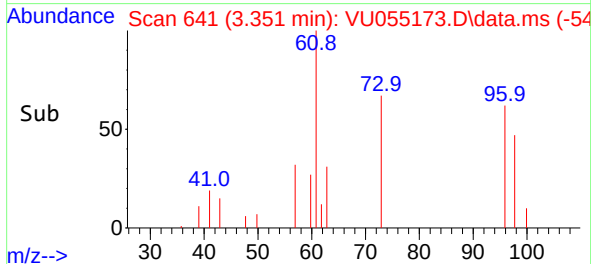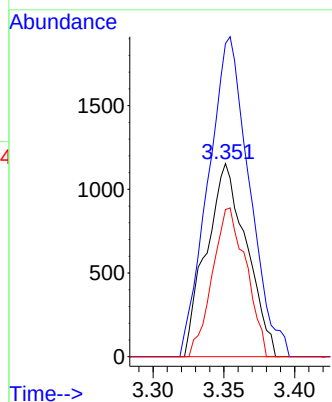

#22
cis-1,2-Dichloroethene
Concen: 45.655 ug/L
RT: 4.663 min Scan# 1049
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Tgt Ion: 96 Resp: 439587
Ion Ratio Lower Upper
96 100
61 132.2 97.2 180.4
98 63.2 46.1 85.7

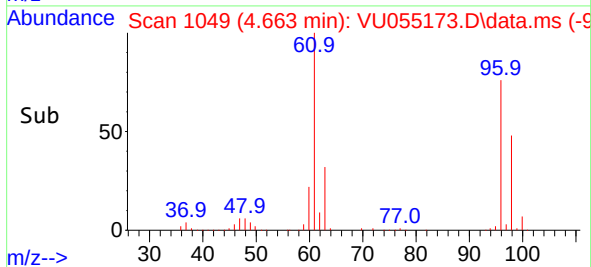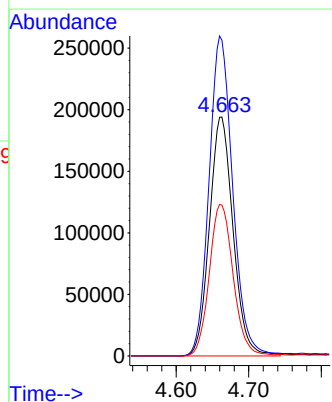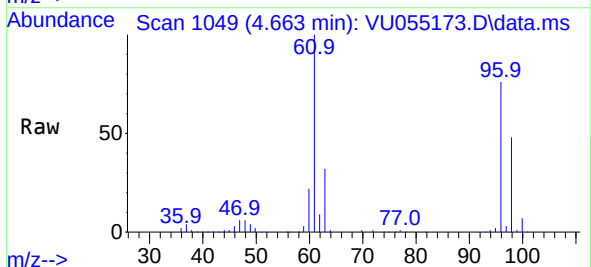




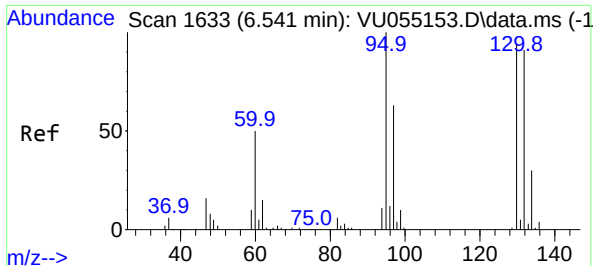


#34
Trichloroethene
Concen: 259.277 ug/L
RT: 6.537 min Scan# 1632
Delta R.T. -0.003 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 95 Resp: 2636563




Ion	Ratio	Lower	Upper
95	100		
97	63.6	44.7	83.1
132	87.8	66.6	123.6
130	92.2	66.5	123.5

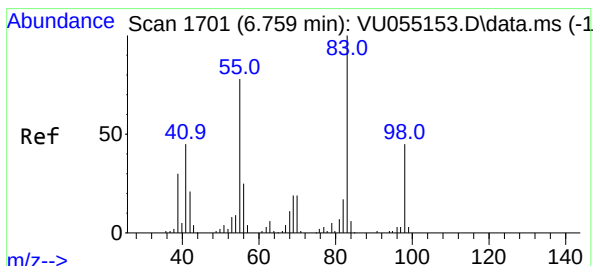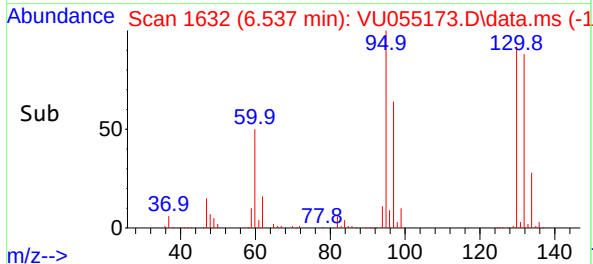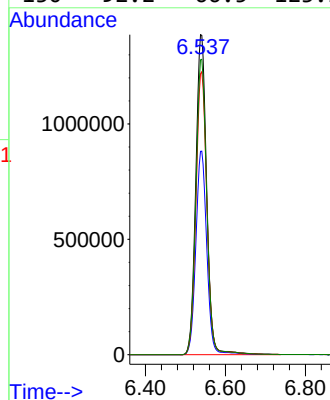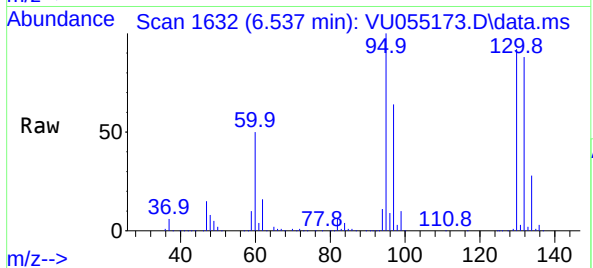


#35
Methylcyclohexane
Concen: 1.060 ug/L
RT: 6.689 min Scan# 1679
Delta R.T. -0.071 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Tgt Ion: 83 Resp: 15117

Ion	Ratio	Lower	Upper
83	100		
55	0.0	60.4	90.6#
98	70.3	35.3	52.9#


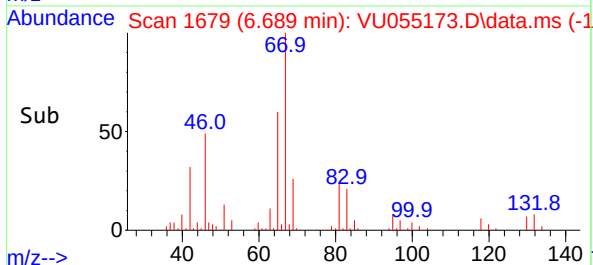
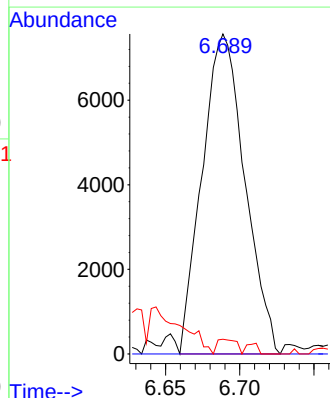
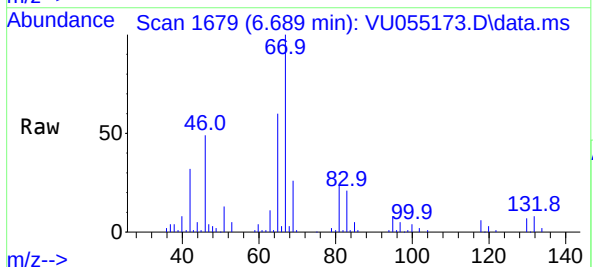


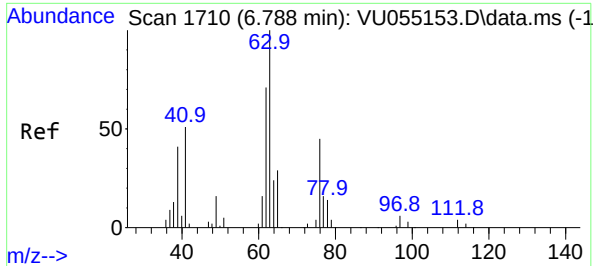

#37
1,2-Dichloropropane
Concen: 0.779 ug/L
RT: 6.689 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 63 Resp: 7764
Ion Ratio Lower Upper
63 100
112 0.0 3.2 4.8#

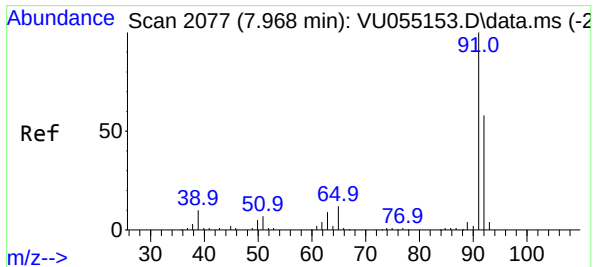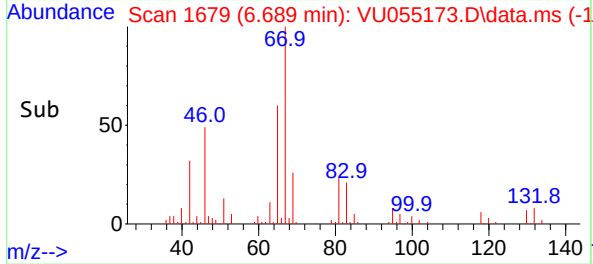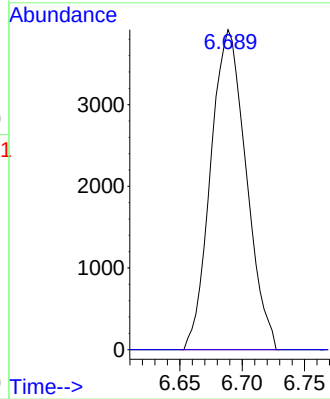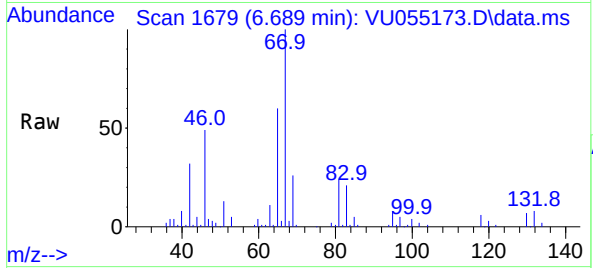

#42
Toluene
Concen: 0.495 ug/L
RT: 7.968 min Scan# 2077
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00


Tgt Ion: 91 Resp: 19299
Ion Ratio Lower Upper
91 100
92 51.3 41.9 77.9

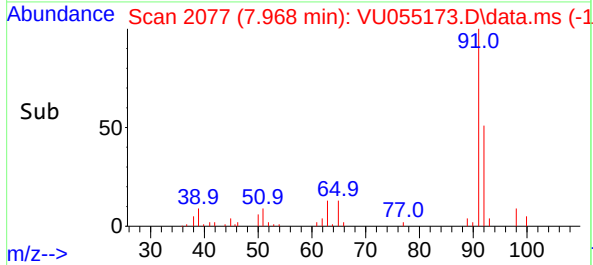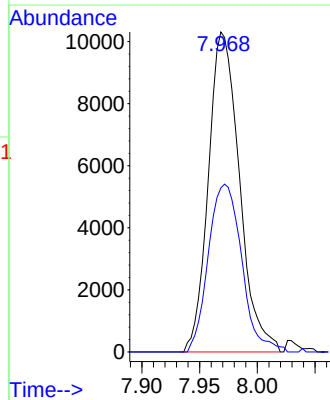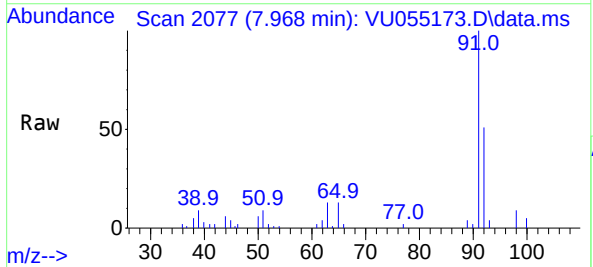

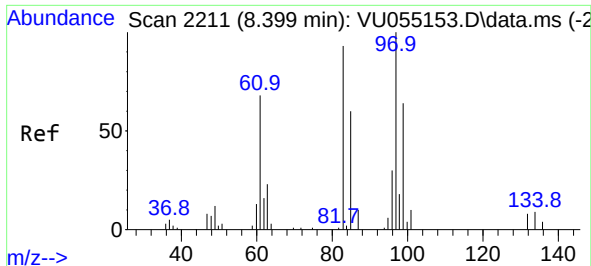




#45
1,1,2-Trichloroethane
Concen: 0.114 ug/L
RT: 8.399 min Scan# 211
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Instrument :
MSVOA_U
ClientSampleId :

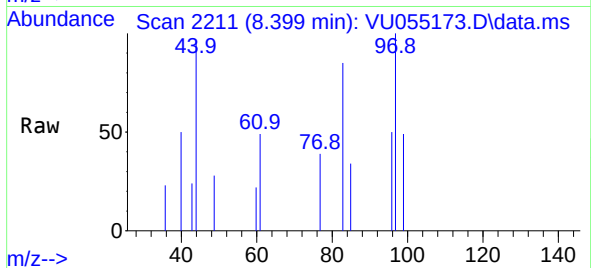

Tgt Ion: 97 Resp: 764




Ion	Ratio	Lower	Upper
97	100		
99	48.6	44.9	83.5
83	85.4	66.9	124.3
85	33.9	42.2	78.4

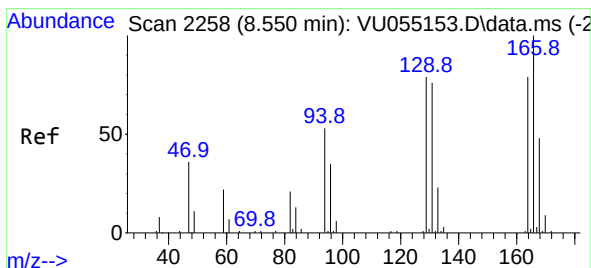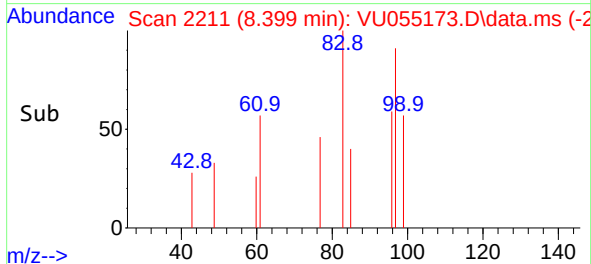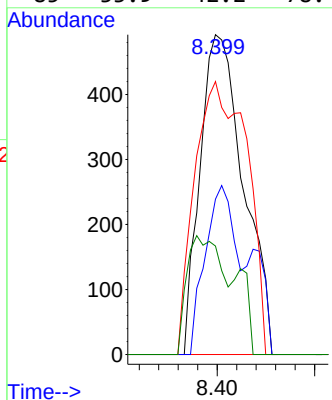


#47
Tetrachloroethene
Concen: 0.426 ug/L
RT: 8.553 min Scan# 2259
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Tgt Ion: 164 Resp: 2994


Ion	Ratio	Lower	Upper
164	100		
129	98.7	69.2	128.6
131	94.6	68.8	127.8
166	115.0	92.3	171.5

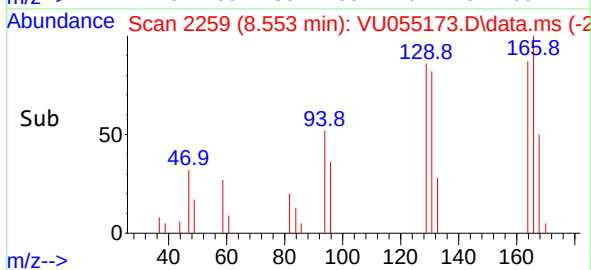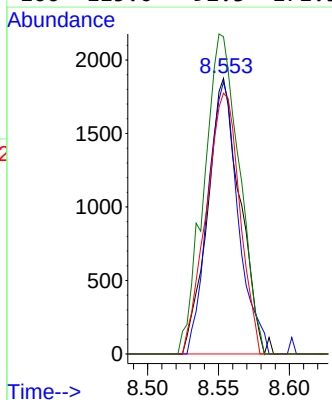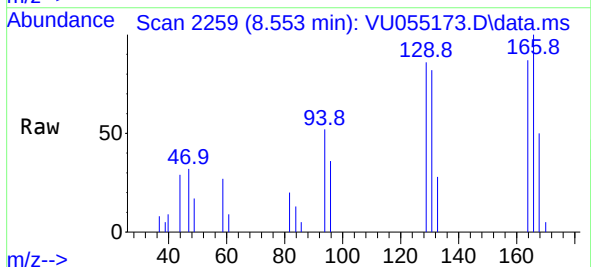



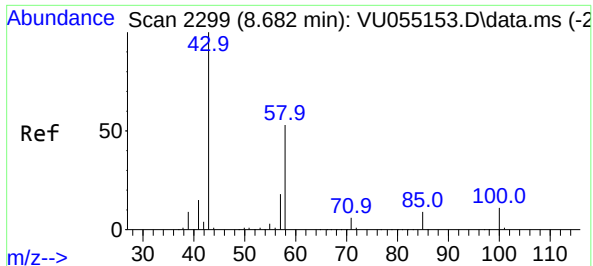


#48
2-Hexanone
Concen: 4.153 ug/L
RT: 8.682 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Instrument :
MSVOA_U
ClientSampleId :



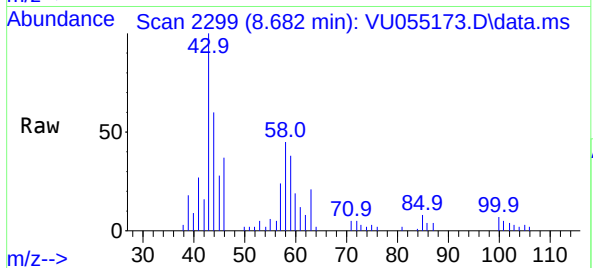



Tgt Ion:	43	Resp:	18483
Ion	Ratio	Lower	Upper
43	100		
58	44.9	44.0	66.0
57	17.5	16.2	24.2
100	9.1	9.0	13.4

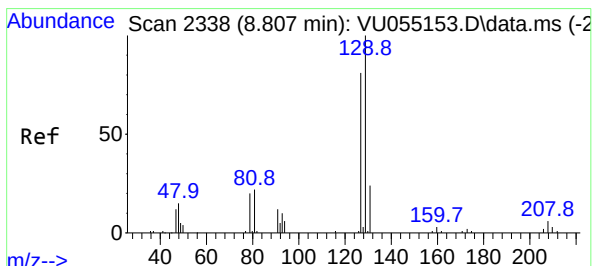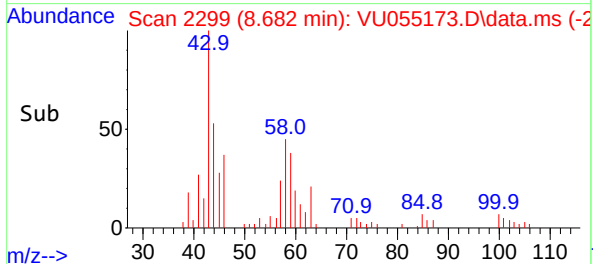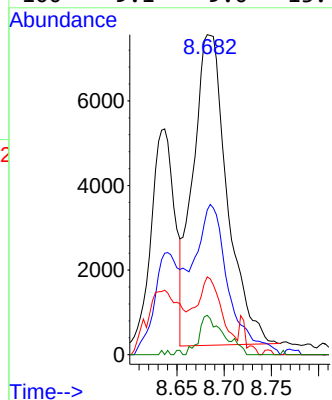

#49
Dibromochloromethane
Concen: 0.378 ug/L
RT: 8.553 min Scan# 2259
Delta R.T. -0.254 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00


Tgt Ion:	129	Resp:	2767
Ion	Ratio	Lower	Upper
129	100		
127	0.0	55.9	103.7#

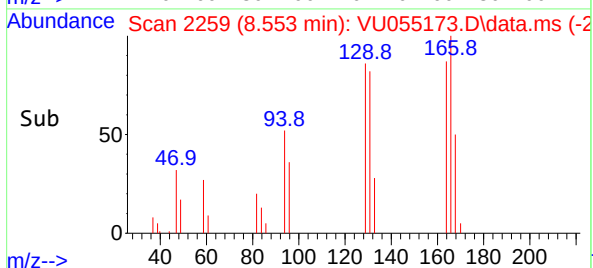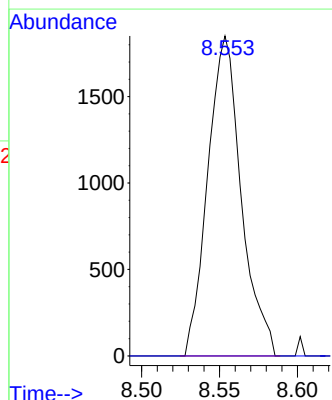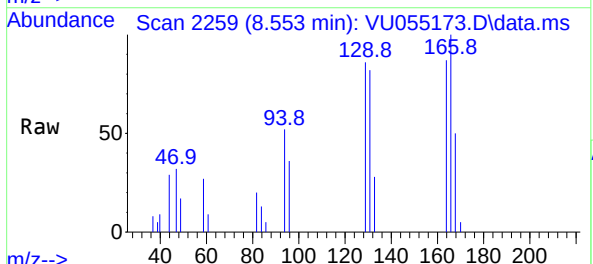



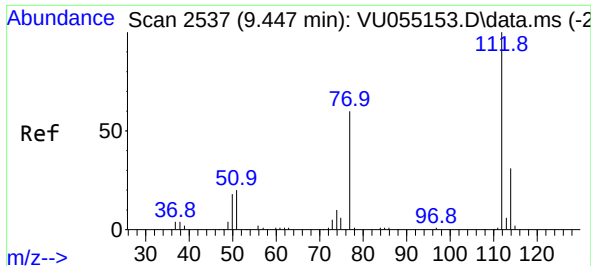


#51
Chlorobenzene
Concen: 0.166 ug/L
RT: 9.451 min Scan# 211
Delta R.T. 0.003 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Instrument :
MSVOA_U
ClientSampleId :



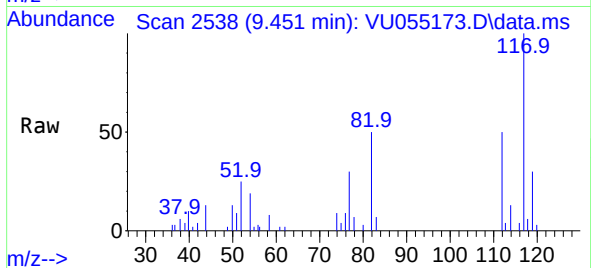



Tgt Ion:112 Resp: 4288
Ion Ratio Lower Upper
112 100
114 24.9 21.7 40.3
77 55.9 48.6 72.8

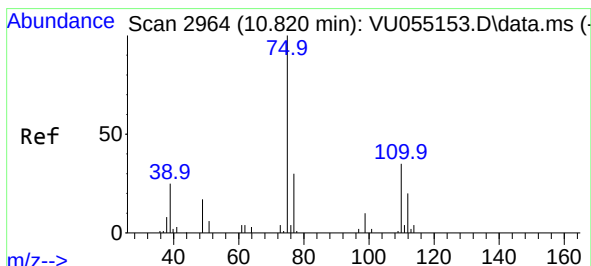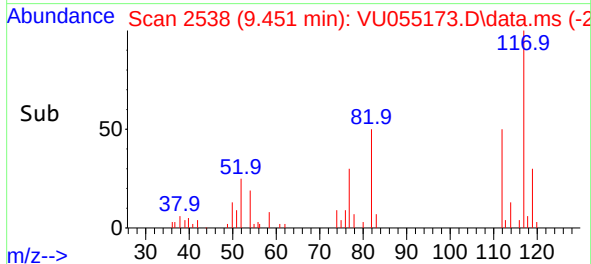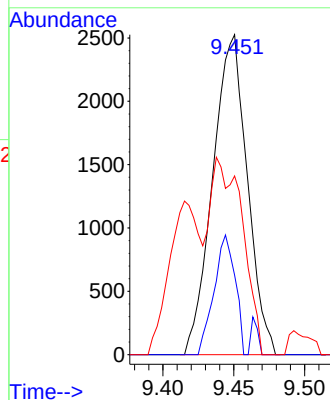

#61
1,2,3-Trichloropropane
Concen: 2.126 ug/L
RT: 11.811 min Scan# 3272
Delta R.T. 0.990 min
Lab File: VU055173.D
Acq: 07 Sep 2023 05:00

Tgt Ion: 75 Resp: 12318
Ion Ratio Lower Upper
75 100
110 2.0 28.2 42.2#
77 33.0 26.2 39.4

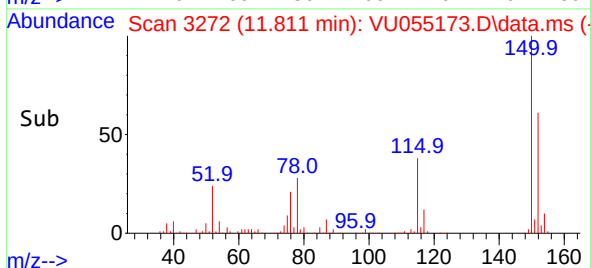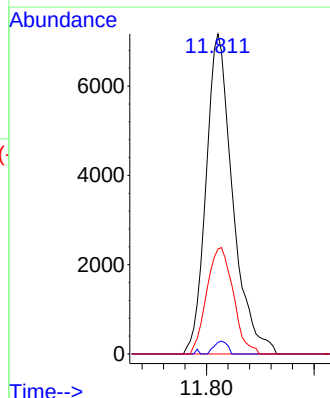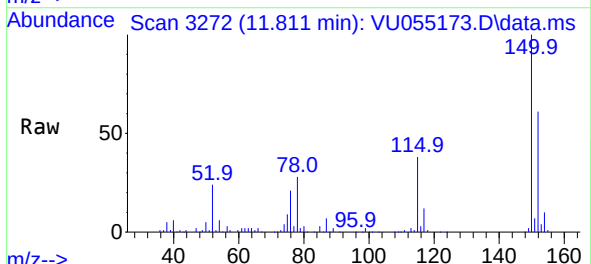

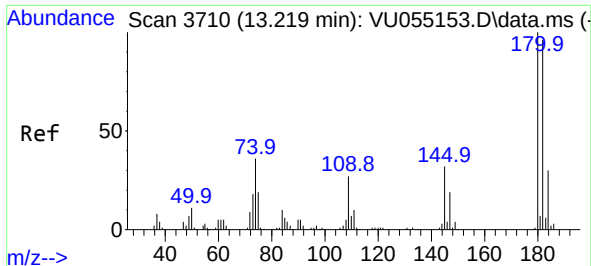

#69

1,3,5-Trichlorobenzene

Concen: 0.774 ug/L

RT: 13.843 min Scan# 3904

Delta R.T. 0.624 min


Lab File: VU055173.D

Acq: 07 Sep 2023 05:00

Instrument :

MSVOA_U

ClientSampleId :

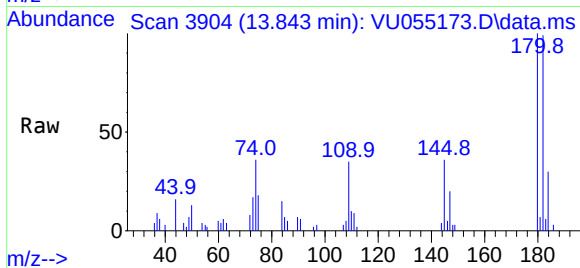

Tgt Ion:180 Resp: 11435




Ion Ratio Lower Upper

180 100

182 93.0 75.8 113.6

184 28.7 24.0 36.0

145 28.7 26.3 39.5

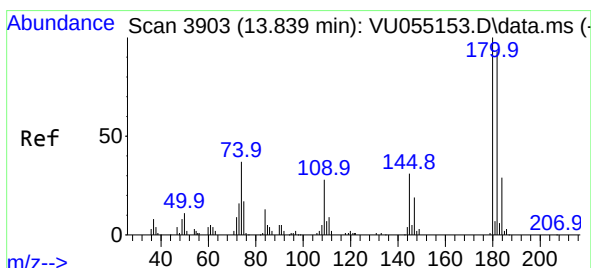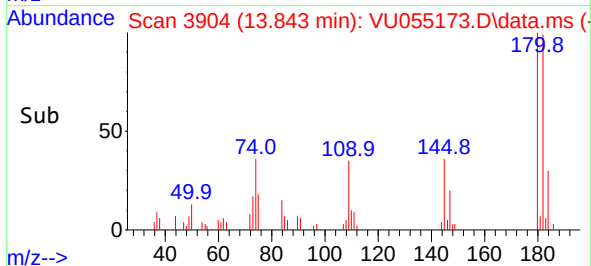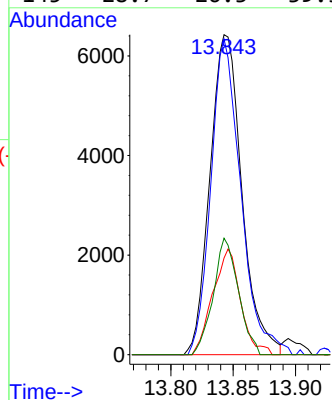

#70

1,2,4-trichlorobenzene

Concen: 0.826 ug/L

RT: 13.843 min Scan# 3904

Delta R.T. 0.003 min

Lab File: VU055173.D

Acq: 07 Sep 2023 05:00

Tgt Ion:180 Resp: 11435

Ion Ratio Lower Upper

180 100

182 93.0 73.6 110.4

145 28.7 25.8 38.8

