

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
 Data File : VU055144.D
 Acq On : 06 Sep 2023 16:45
 Operator : MD/SY
 Sample : 04250-23DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4F2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	107	rBV2	60366	71406	11.81%	1.304%
2	1.779	145	152	162	rVV4	6039	9492	1.57%	0.173%
3	1.908	184	192	206	rBV	59103	77301	12.79%	1.412%
4	2.560	384	395	409	rBV	108926	175291	29.00%	3.201%
5	3.039	533	544	559	rBV3	23648	44317	7.33%	0.809%
6	3.184	574	589	606	rVB	15516	36923	6.11%	0.674%
7	4.631	1022	1039	1044	rBV2	118992	251954	41.69%	4.602%
8	5.062	1159	1173	1197	rBV	114739	259988	43.02%	4.748%
9	5.724	1358	1379	1401	rBV3	226711	590789	97.75%	10.790%
10	6.248	1529	1542	1560	rBV	222122	430103	71.16%	7.855%
11	6.541	1621	1633	1652	rBV3	90919	181532	30.04%	3.315%
12	6.689	1665	1679	1699	rBV	149758	295081	48.82%	5.389%
13	7.566	1936	1952	1973	rBV2	55146	101640	16.82%	1.856%
14	7.898	2043	2055	2074	rBV2	265909	477433	78.99%	8.720%
15	8.181	2133	2143	2159	rBV2	29157	51505	8.52%	0.941%
16	8.634	2273	2284	2325	rBV3	256229	597684	98.89%	10.916%
17	9.418	2514	2528	2550	rBV	335650	588029	97.29%	10.740%
18	10.756	2928	2944	2960	rBV	107646	177686	29.40%	3.245%
19	11.814	3261	3273	3288	rBV	365519	604394	100.00%	11.038%
20	12.193	3379	3391	3410	rBV	267707	452798	74.92%	8.270%




Sum of corrected areas: 5475346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055144.D
Acq On : 06 Sep 2023 16:45
Operator : MD/SY
Sample : 04250-23DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

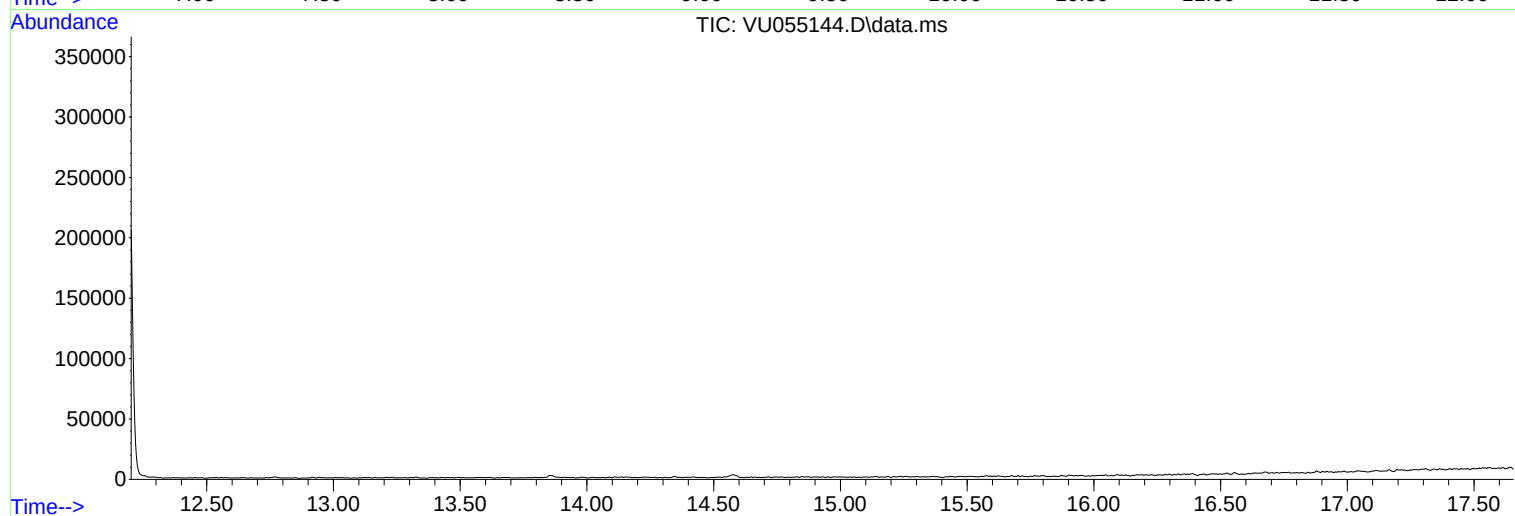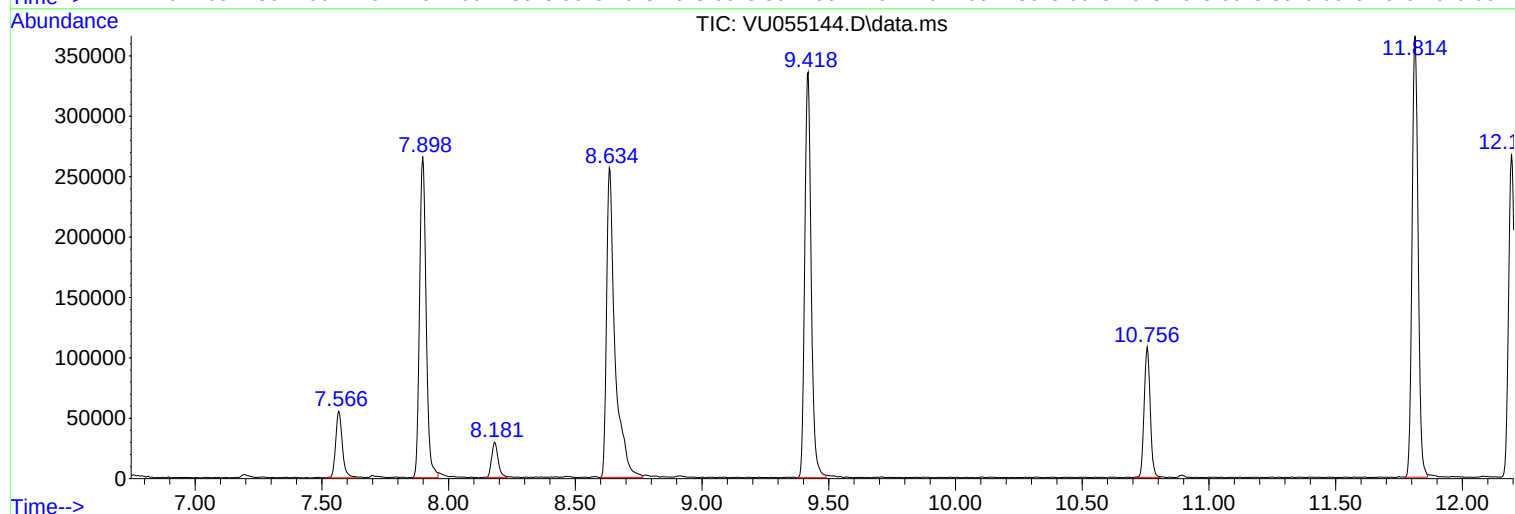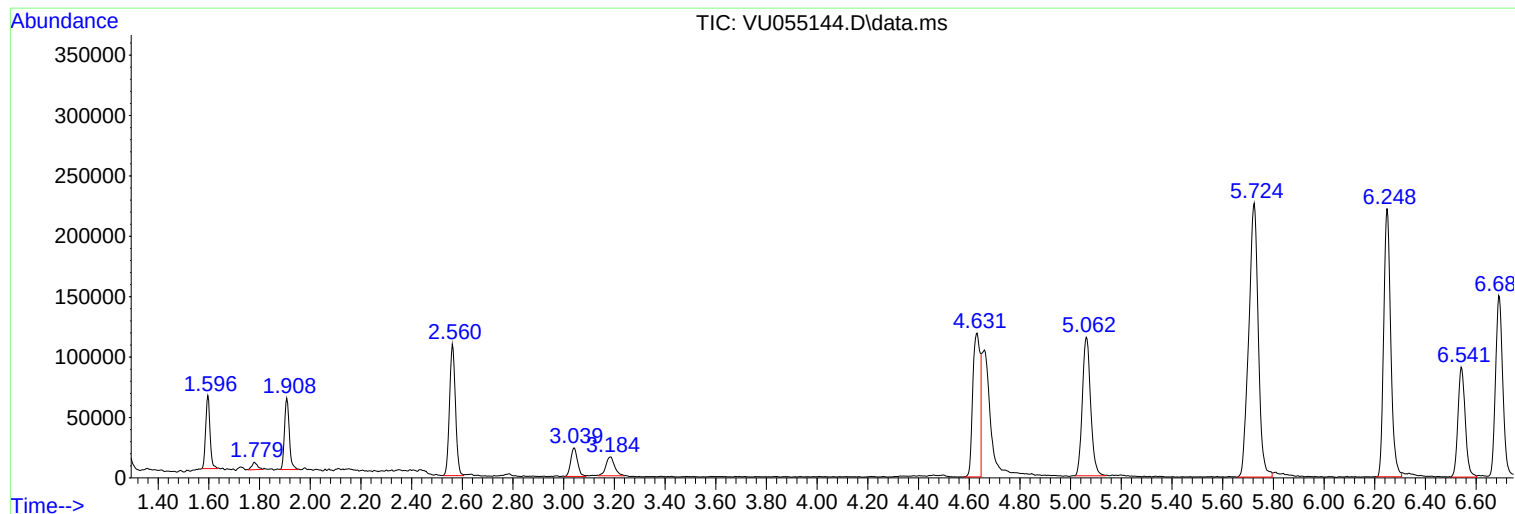

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055144.D
Acq On : 06 Sep 2023 16:45
Operator : MD/SY
Sample : 04250-23DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F2DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.566	1.18 ug/L	101640	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
2			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
3			1,4-Cyclohexadiene	80	C6H8	000628-41-1	23
4			1,3-Cyclohexadiene	80	C6H8	000592-57-4	9
5			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	9

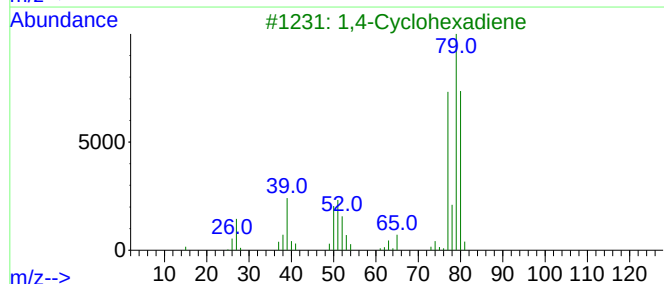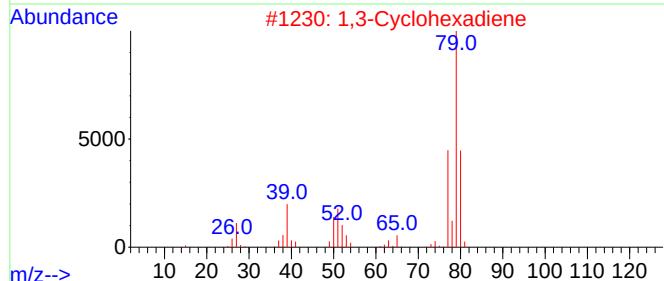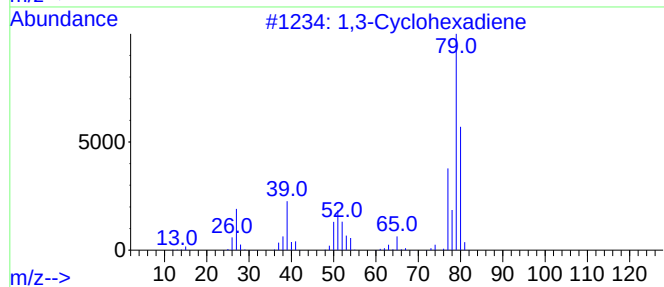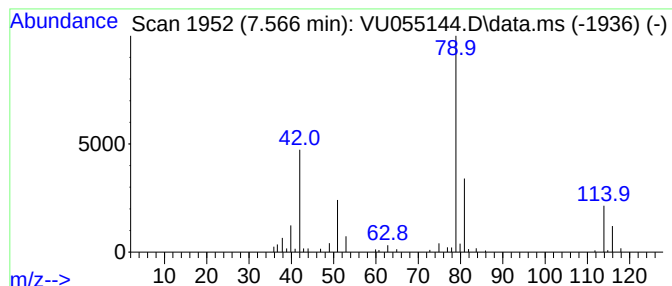

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055144.D
Acq On : 06 Sep 2023 16:45
Operator : MD/SY
Sample : 04250-23DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.566	1.2	ug/L	101640	1	6.248	430103	5.0