

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
 Data File : VU055146.D
 Acq On : 06 Sep 2023 17:34
 Operator : MD/SY
 Sample : 04268-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	109	rBV	44896	56630	9.83%	1.124%
2	1.776	145	151	158	rBV5	4977	5821	1.01%	0.116%
3	1.907	183	192	204	rBV	61361	78177	13.57%	1.551%
4	2.560	380	395	411	rBV	108434	174355	30.27%	3.460%
5	3.039	534	544	556	rBV5	6303	12316	2.14%	0.244%
6	4.628	1026	1038	1065	rBV	90585	235179	40.84%	4.667%
7	5.062	1155	1173	1199	rBV2	114631	268149	46.56%	5.321%
8	5.724	1356	1379	1399	rBV2	220195	575907	100.00%	11.428%
9	6.248	1529	1542	1566	rBV	210944	408487	70.93%	8.105%
10	6.534	1619	1631	1642	rBB7	6733	13649	2.37%	0.271%
11	6.689	1663	1679	1702	rBV2	144386	296141	51.42%	5.876%
12	7.566	1935	1952	1965	rBV2	54164	96663	16.78%	1.918%
13	7.898	2042	2055	2075	rBV	258970	458427	79.60%	9.096%
14	8.184	2132	2144	2164	rBV	30456	54276	9.42%	1.077%
15	8.634	2272	2284	2316	rBV2	245571	574172	99.70%	11.393%
16	9.418	2515	2528	2549	rBV	312825	550207	95.54%	10.918%
17	10.756	2931	2944	2963	rVB	108079	175418	30.46%	3.481%
18	11.814	3261	3273	3296	rBV	347655	570574	99.07%	11.322%
19	12.193	3379	3391	3410	rBV	263794	435085	75.55%	8.633%




Sum of corrected areas: 5039633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055146.D
Acq On : 06 Sep 2023 17:34
Operator : MD/SY
Sample : 04268-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

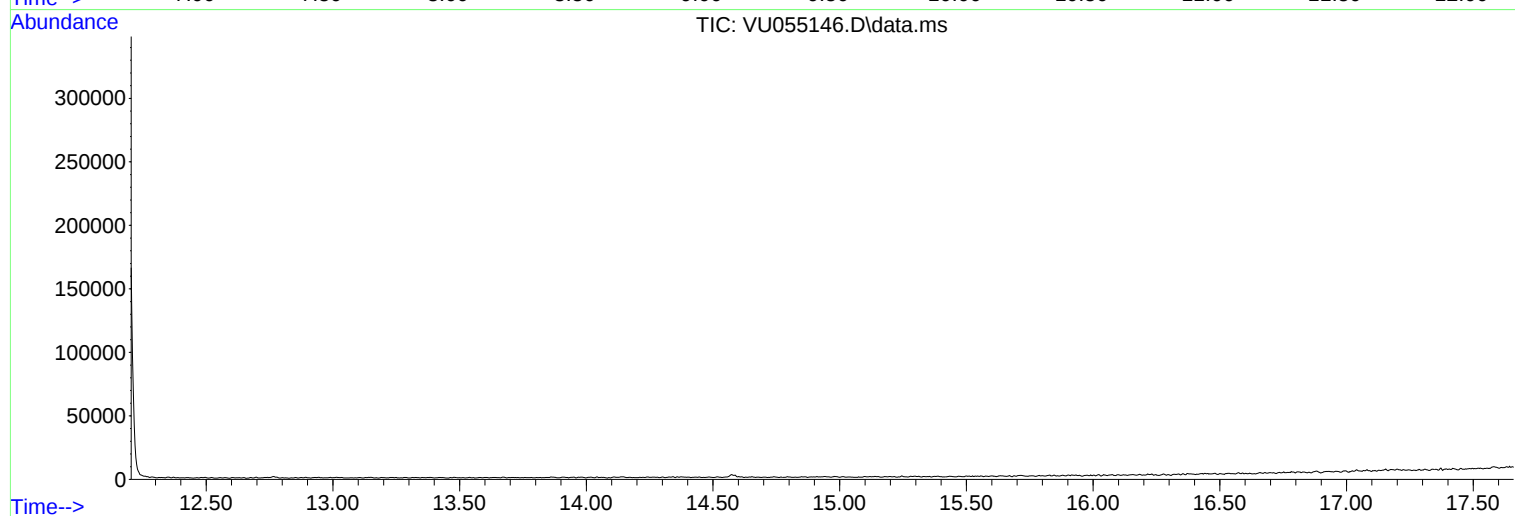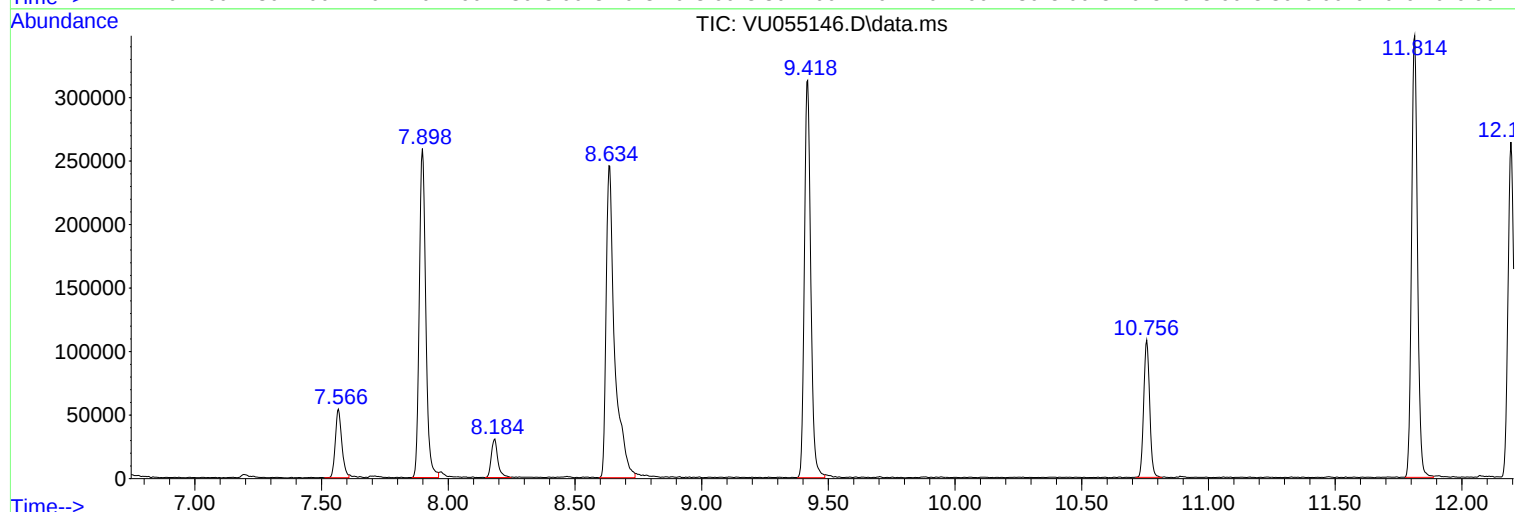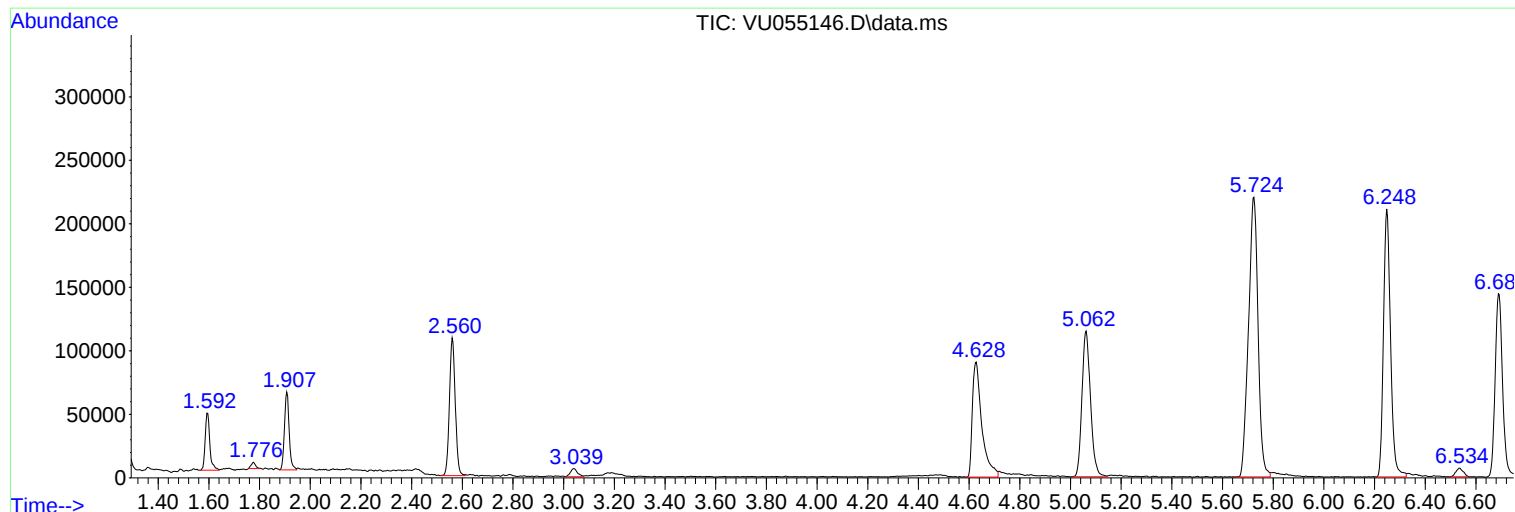

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055146.D
Acq On : 06 Sep 2023 17:34
Operator : MD/SY
Sample : 04268-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.566	1.18 ug/L	96663	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
2			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
3			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
4			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	17
5			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	9

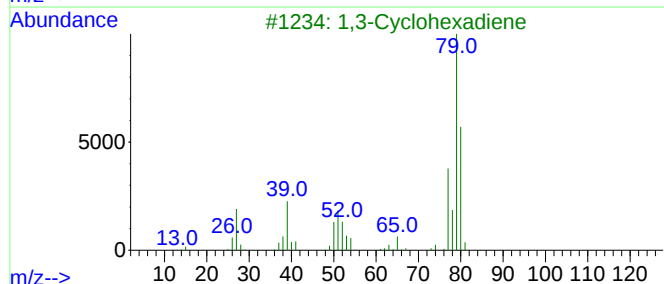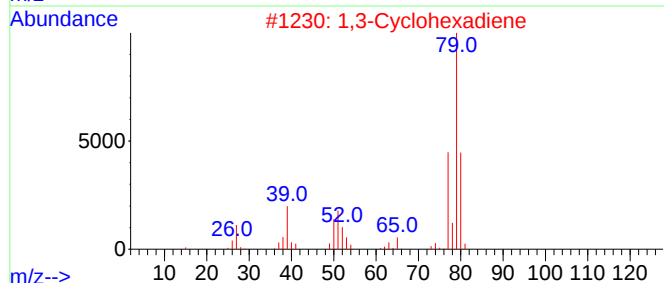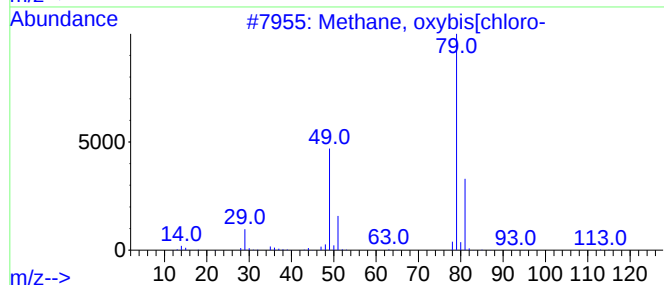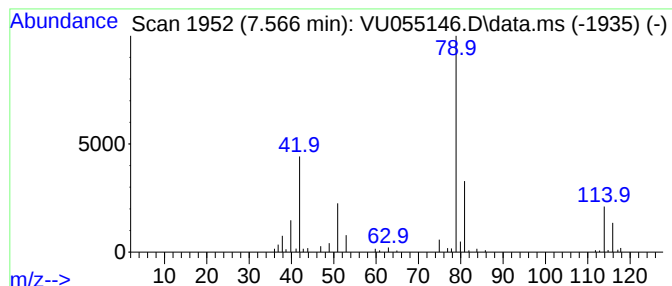

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055146.D
Acq On : 06 Sep 2023 17:34
Operator : MD/SY
Sample : 04268-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.566	1.2	ug/L	96663	1	6.248	408487	5.0