

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
 Data File : VU055160.D
 Acq On : 06 Sep 2023 23:45
 Operator : MD/SY
 Sample : 04286-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4F9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	105	rVB	44390	49473	8.81%	1.027%
2	1.907	184	192	204	rVB	57261	74205	13.21%	1.540%
3	2.560	384	395	410	rBV	99064	163823	29.16%	3.400%
4	4.624	1026	1037	1066	rBV	78714	217093	38.64%	4.506%
5	5.062	1155	1173	1196	rBV	107417	245041	43.61%	5.086%
6	5.724	1359	1379	1400	rBV2	208028	543320	96.70%	11.278%
7	6.248	1529	1542	1560	rBV	212285	404398	71.97%	8.394%
8	6.541	1622	1633	1646	rBV6	9475	19225	3.42%	0.399%
9	6.688	1666	1679	1700	rBV2	135128	272876	48.57%	5.664%
10	7.566	1938	1952	1967	rBV2	46310	84843	15.10%	1.761%
11	7.897	2041	2055	2078	rBV	246018	434574	77.34%	9.020%
12	8.180	2131	2143	2161	rBV3	26456	47448	8.44%	0.985%
13	8.634	2269	2284	2318	rBV4	222805	540761	96.24%	11.224%
14	9.418	2515	2528	2551	rBV	316503	547370	97.42%	11.362%
15	10.756	2932	2944	2961	rBV2	102138	166018	29.55%	3.446%
16	11.814	3261	3273	3291	rBV	340507	561868	100.00%	11.663%
17	12.064	3339	3351	3372	rBV4	11118	27362	4.87%	0.568%
18	12.193	3378	3391	3410	rVB	243839	412010	73.33%	8.552%
19	16.887	4845	4851	4860	rVB7	4375	6019	1.07%	0.125%




Sum of corrected areas: 4817727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055160.D
Acq On : 06 Sep 2023 23:45
Operator : MD/SY
Sample : 04286-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

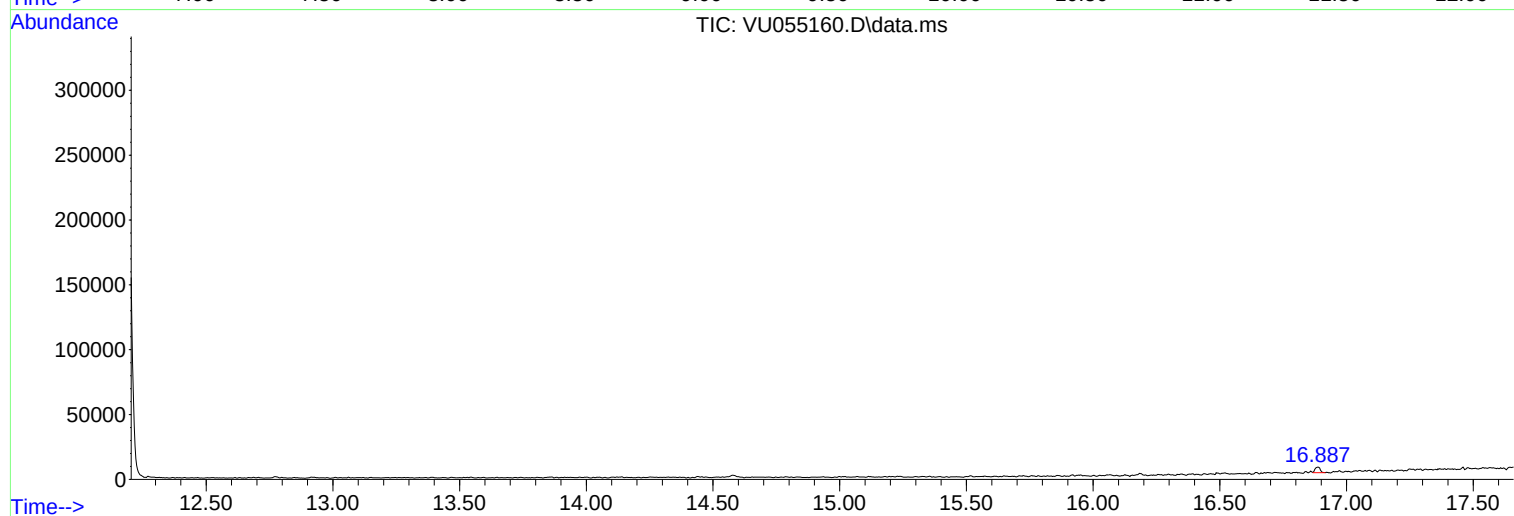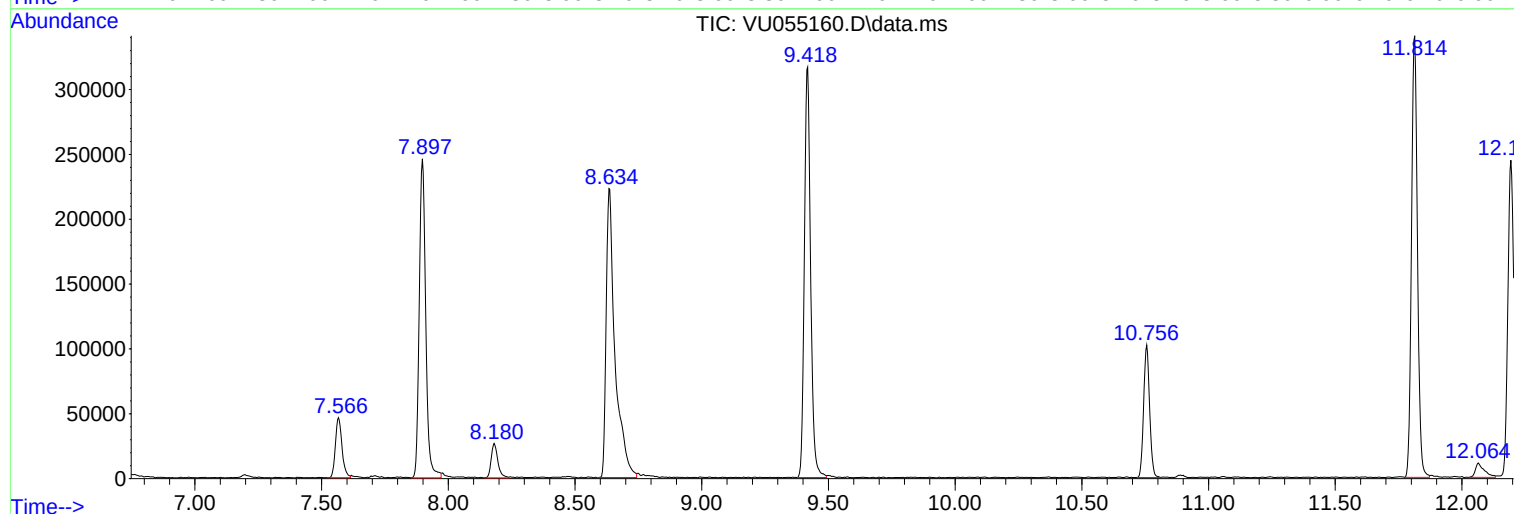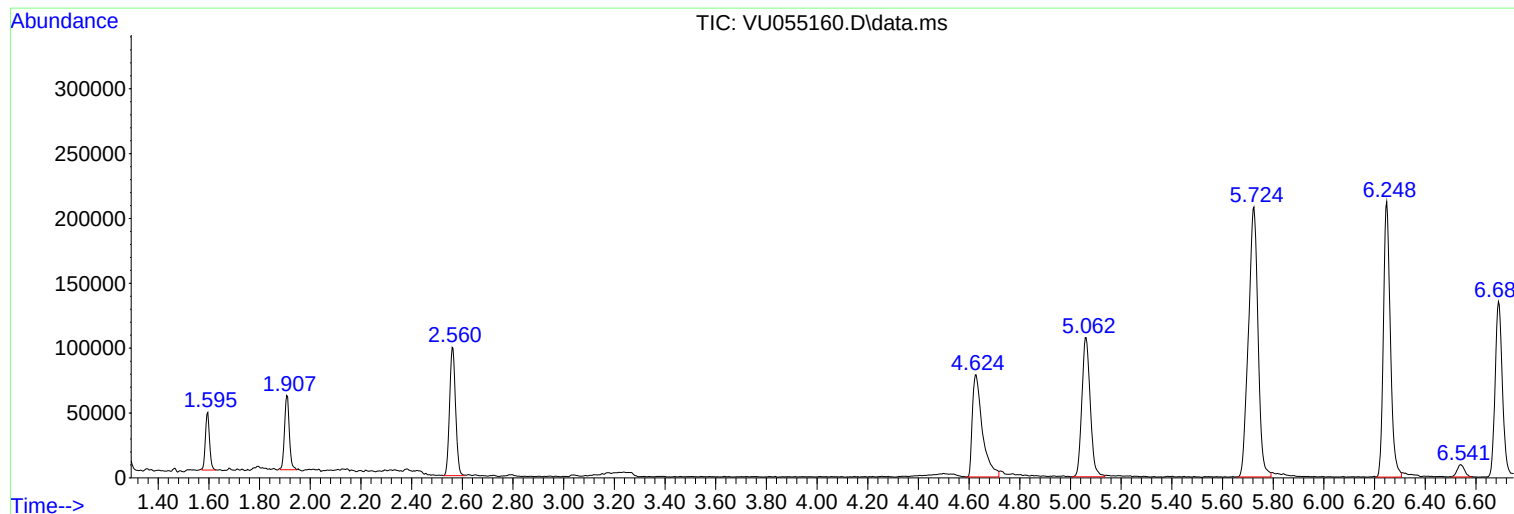

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055160.D
Acq On : 06 Sep 2023 23:45
Operator : MD/SY
Sample : 04286-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
Data File : VU055160.D
Acq On : 06 Sep 2023 23:45
Operator : MD/SY
Sample : 04286-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc