


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090623\
 Data File : VU055131.D
 Acq On : 06 Sep 2023 08:52
 Operator : MD/SY
 Sample : BFB040
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB040

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Sep 08 06:18:43 2023

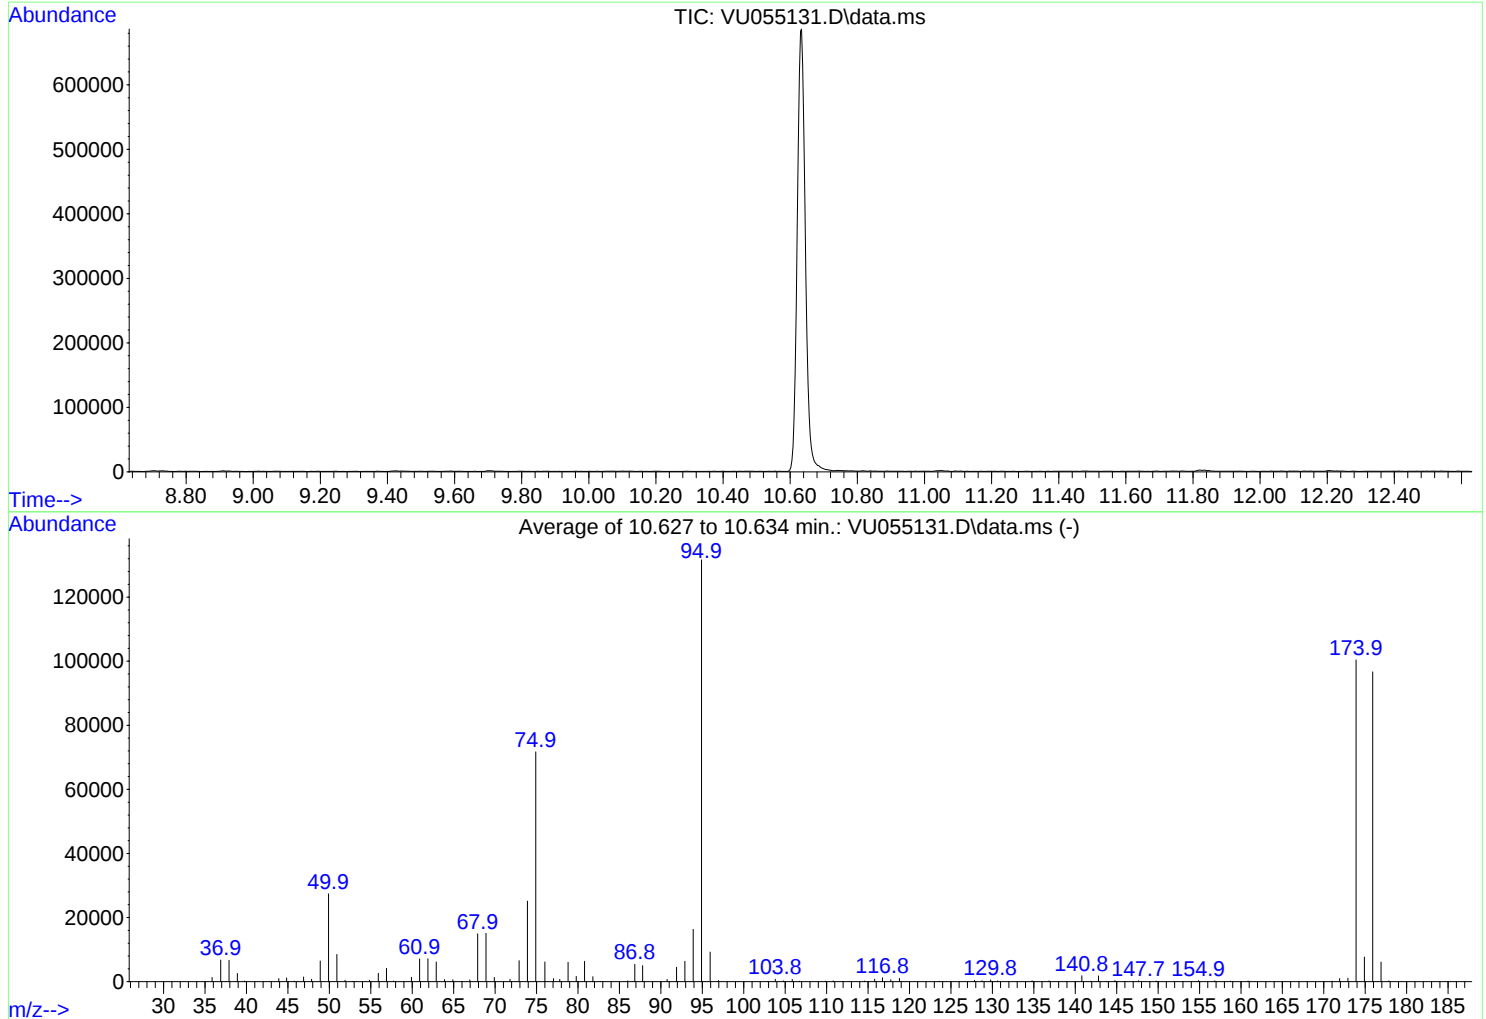

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	27419	PASS
75	95	30	80	54.5	71701	PASS
95	95	100	100	100.0	131640	PASS
96	95	5	9	7.0	9233	PASS
173	174	0.00	2	1.1	1102	PASS
174	95	50	120	76.3	100437	PASS
175	174	5	9	7.7	7711	PASS
176	174	95	101	96.3	96680	PASS
177	176	5	9	6.3	6110	PASS

m/z	Abundance
39.70	122.0
43.90	678.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.80	1265.0
36.90	6298.0
37.90	6315.0
38.90	2231.0
39.80	359.0
42.80	118.0
43.90	1388.0
44.90	1225.0
45.70	150.0
46.90	1467.0
47.80	752.0
48.90	5974.0
49.90	26128.0
50.90	8232.0
51.90	432.0
52.80	194.0
54.80	461.0
55.90	2191.0
56.90	3871.0
57.80	192.0
59.90	1347.0
60.90	6929.0
61.90	6917.0
62.90	5492.0
63.90	658.0
64.90	542.0
66.90	435.0
67.90	14251.0
68.90	14210.0
69.90	1321.0
71.80	772.0
72.90	5901.0
73.90	24024.0
74.90	67440.0
76.00	5970.0
77.10	919.0
77.80	695.0
78.80	5602.0
79.80	1601.0
80.80	6174.0
81.80	1511.0
83.00	133.0
86.00	187.0
86.90	5096.0
87.80	4794.0
90.80	713.0
91.90	4192.0
92.90	5966.0
93.90	15374.0
94.90	124200.0
95.90	8933.0
96.90	385.0
102.90	114.0
103.80	660.0
104.80	232.0
105.90	615.0
106.70	134.0
109.90	147.0
110.80	262.0
112.80	104.0
114.60	193.0
115.80	612.0
116.80	1086.0
117.70	587.0
118.80	930.0
127.80	342.0
128.70	259.0
129.80	543.0
130.60	178.0
134.80	225.0
136.80	251.0
140.80	1675.0
141.90	129.0
142.80	1708.0
143.80	119.0
144.80	382.0
147.70	334.0
149.70	164.0
154.90	299.0
156.90	176.0
158.80	116.0
160.80	189.0
171.00	160.0
171.90	913.0
172.90	868.0
173.90	92256.0
174.90	7184.0
175.90	87480.0
176.90	5665.0
177.80	243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.90	1348.0
36.90	6973.0
37.90	6857.0
38.90	2604.0
39.80	337.0
42.80	118.0
43.90	1607.0
44.80	1135.0
45.70	153.0
46.90	1541.0
47.90	756.0
48.90	6647.0
49.90	28320.0
50.90	8764.0
51.90	437.0
52.80	164.0
54.90	441.0
55.90	2666.0
56.90	4239.0
57.80	243.0
59.90	1400.0
60.90	7163.0
61.90	7398.0
62.90	6292.0
63.90	715.0
64.90	609.0
66.00	106.0
67.00	570.0
67.90	15401.0
68.90	15457.0
69.90	1338.0
71.80	744.0
72.90	6674.0
73.90	25896.0
74.90	74128.0
76.00	6344.0
77.10	983.0
77.80	748.0
78.80	6260.0
79.80	1695.0
80.80	6604.0
81.80	1651.0
82.90	174.0
86.00	236.0
86.80	5547.0
87.80	5242.0
90.80	689.0
91.90	4640.0
92.90	6520.0
93.90	16704.0
94.90	135488.0
96.00	9569.0
96.90	369.0
103.80	739.0
104.80	224.0
105.80	715.0
106.70	172.0
109.80	140.0
110.80	269.0
111.90	112.0
114.60	216.0
115.80	791.0
116.70	1261.0
117.70	665.0
118.80	1039.0
123.60	136.0
127.80	426.0
128.70	288.0
129.80	553.0
130.60	258.0
134.80	336.0
136.90	290.0
140.80	1951.0
141.90	149.0
142.80	1855.0
143.80	138.0
144.80	347.0
146.00	116.0
147.70	311.0
149.80	223.0
153.00	126.0
154.90	346.0
156.90	259.0
158.80	142.0
160.90	220.0
171.00	179.0
171.90	980.0
172.90	1111.0
173.90	103184.0
174.90	8040.0
175.90	99696.0
176.90	6328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

177.80

256.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
35.90	1306.0
36.90	6995.0
37.90	6723.0
38.90	2848.0
39.80	305.0
43.90	1849.0
44.90	1062.0
45.80	127.0
46.90	1402.0
47.90	732.0
48.90	6728.0
49.90	27808.0
50.90	8441.0
51.90	494.0
54.90	416.0
55.90	2894.0
56.90	4278.0
57.70	239.0
59.90	1338.0
60.90	7184.0
61.90	7141.0
62.90	6659.0
63.90	664.0
64.90	581.0
65.90	103.0
67.00	580.0
67.90	15113.0
68.90	15540.0
69.90	1277.0
71.80	673.0
72.90	7086.0
73.90	25496.0
74.90	73536.0
76.00	6148.0
77.00	907.0
77.80	676.0
78.80	6311.0
79.80	1699.0
80.80	6303.0
81.80	1559.0
82.70	201.0
86.00	280.0
86.80	5582.0
87.80	4932.0
90.70	676.0
91.90	4586.0
92.90	6568.0
93.90	16992.0
94.90	135232.0
96.00	9197.0
97.00	282.0
103.80	787.0
104.80	247.0
105.80	793.0
106.70	197.0
109.80	133.0
110.80	220.0
111.90	111.0
114.60	168.0
115.80	816.0
116.80	1272.0
117.80	628.0
118.80	1068.0
123.60	135.0
127.90	467.0
128.80	297.0
129.80	497.0
130.70	312.0
134.80	376.0
136.90	282.0
140.80	2011.0
141.90	124.0
142.80	1829.0
143.80	124.0
144.80	320.0
146.00	136.0
147.60	258.0
149.80	224.0
153.00	178.0
154.90	344.0
156.80	309.0
158.70	176.0
160.90	174.0
171.00	198.0
171.90	975.0
172.90	1328.0
173.90	105872.0
174.90	7909.0
175.90	102864.0
176.90	6337.0
177.90	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040