

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
 Data File : VU060644.D
 Acq On : 06 Sep 2024 16:21
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Sep 07 01:35:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Sat Sep 07 01:24:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.113	96	33762	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	8789	0.711	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	9658	0.780	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	
Target Compounds						
15) Methylene Chloride	3.046	84	3516	0.290	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
Data File : VU060644.D
Acq On : 06 Sep 2024 16:21
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Sep 07 01:35:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Sat Sep 07 01:24:57 2024
Response via : Initial Calibration




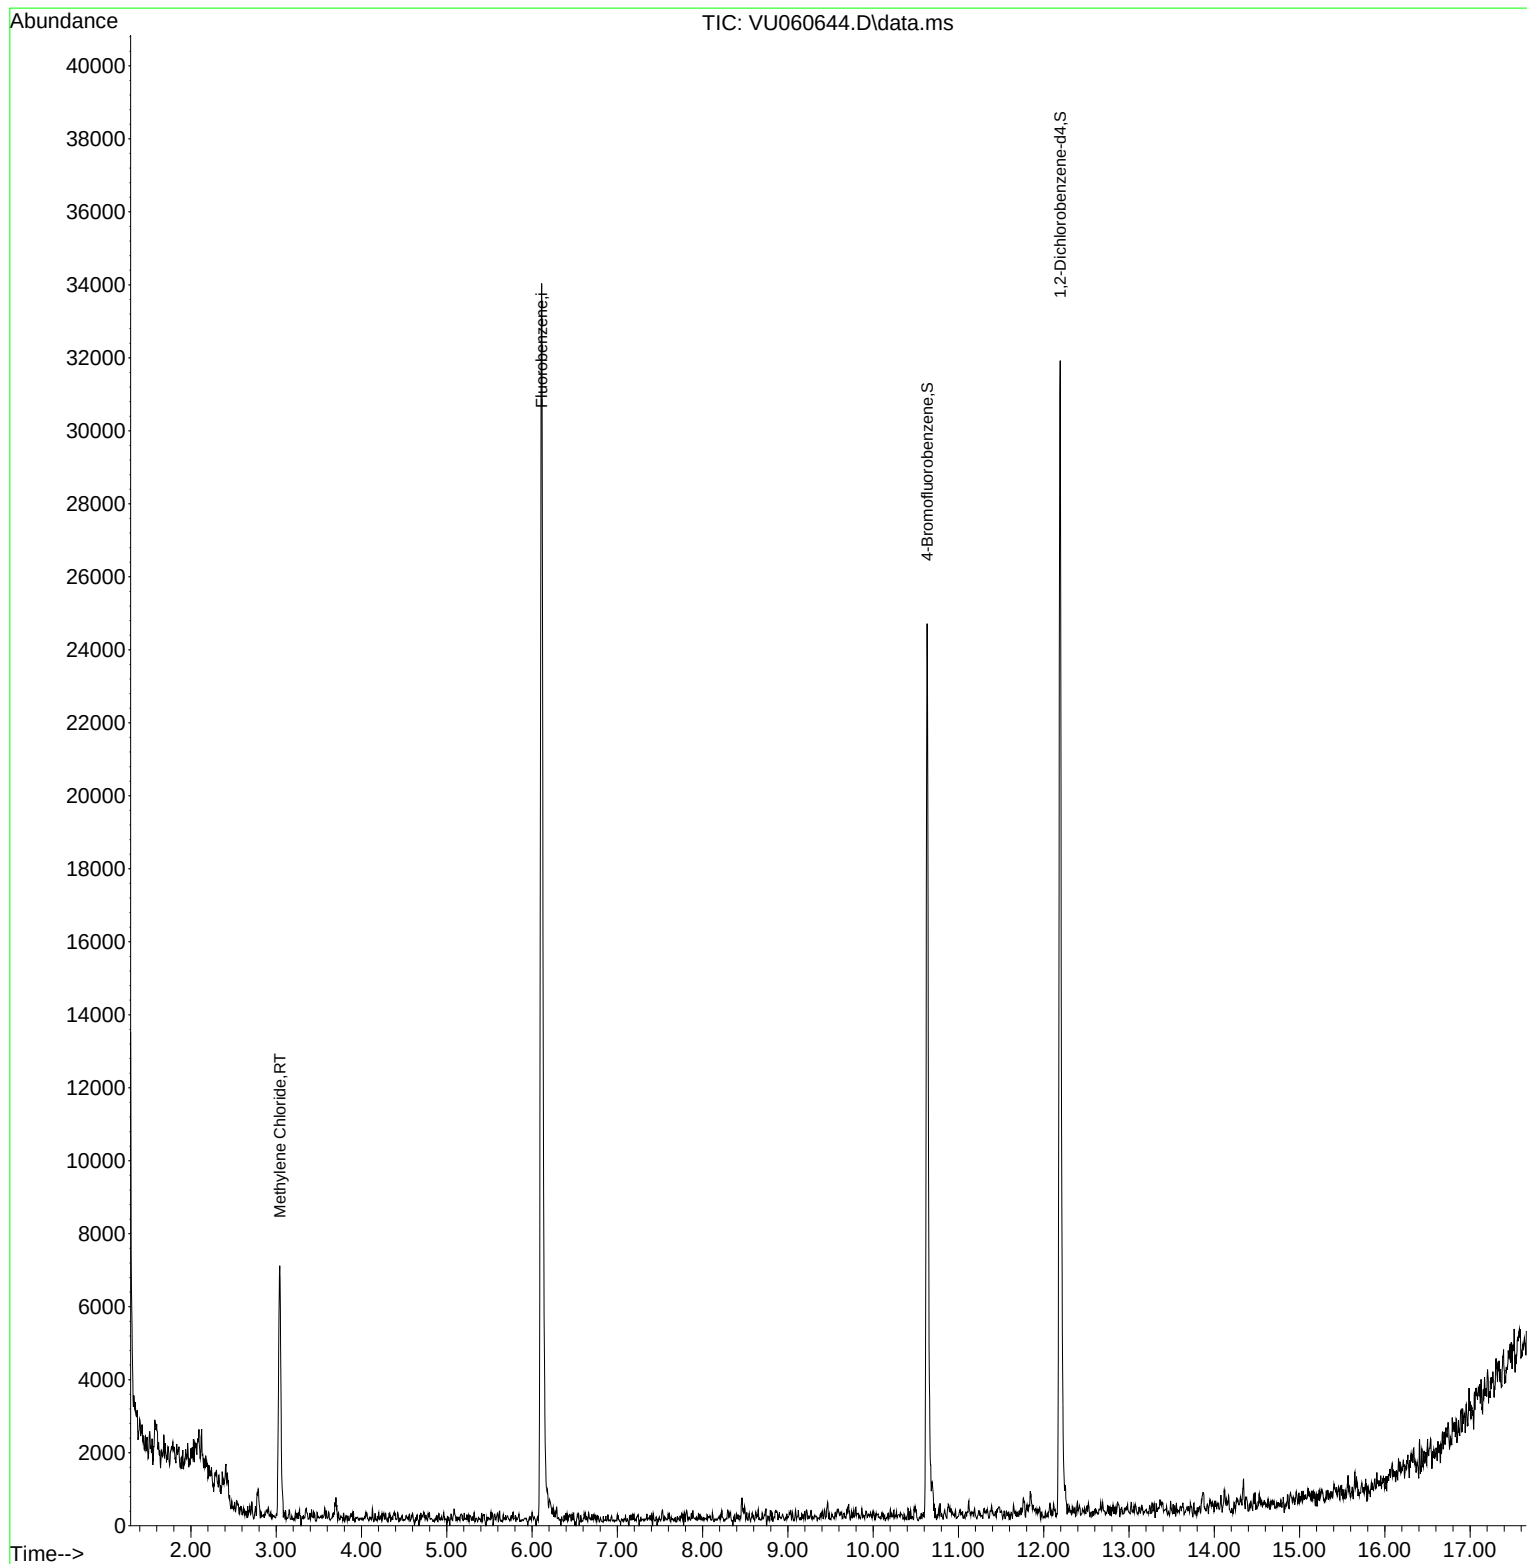


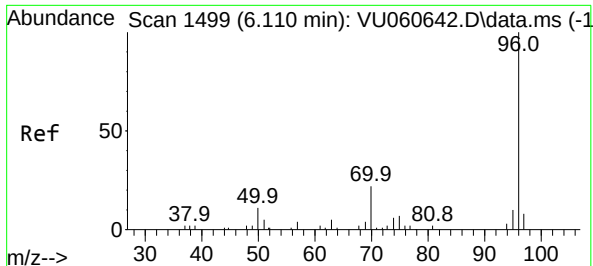

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. 0.003 min
Lab File: VU060644.D
Acq: 06 Sep 2024 16:21




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion: 96	Resp: 33762
Ion Ratio	Lower Upper
96 100	
70 18.7	16.5 24.7
95 8.4	7.7 11.5
97 6.4	0.0 0.0#

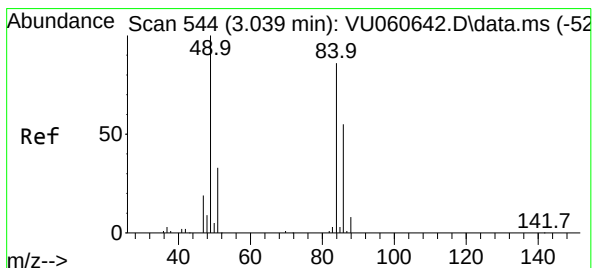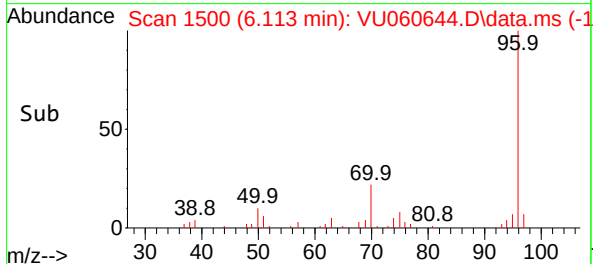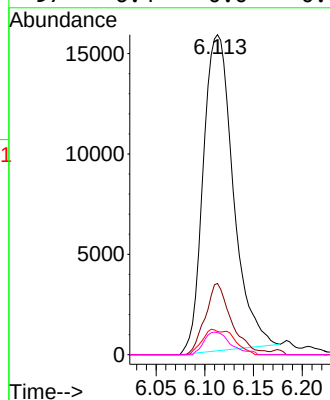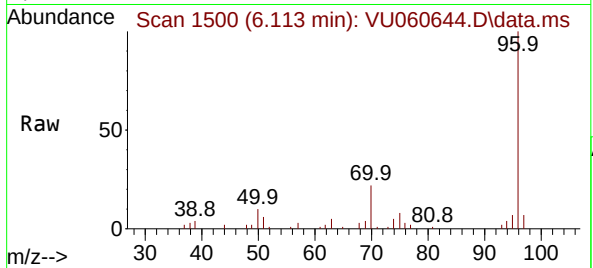

#15
Methylene Chloride
Concen: 0.290 ug/l
RT: 3.046 min Scan# 546
Delta R.T. 0.006 min
Lab File: VU060644.D
Acq: 06 Sep 2024 16:21

Tgt Ion: 84	Resp: 3516
Ion Ratio	Lower Upper
84 100	
49 121.4	92.8 139.2
51 34.5	0.0 75.4
86 72.8	50.6 75.8


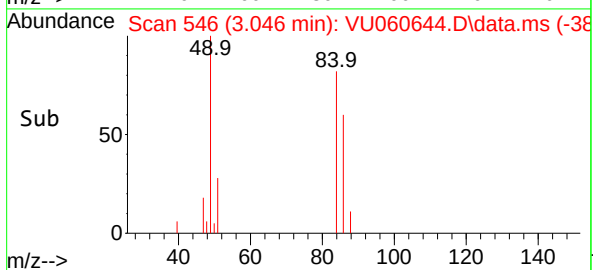
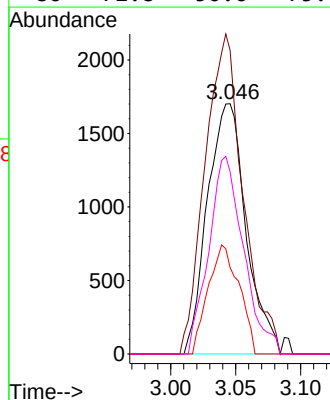
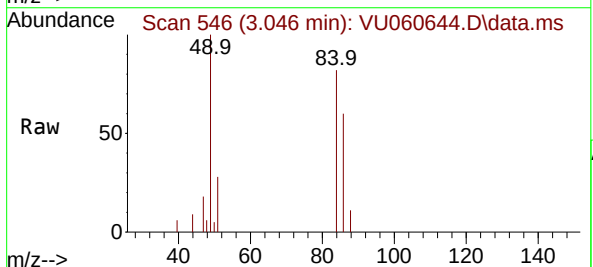


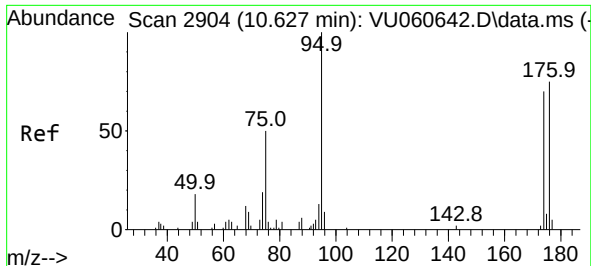

#57
 4-Bromofluorobenzene
 Concen: 0.711 ug/l
 RT: 10.634 min Scan# 2906
 Delta R.T. 0.006 min
 Lab File: VU060644.D
 Acq: 06 Sep 2024 16:21

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Tgt Ion: 95 Resp: 8789
 Ion Ratio Lower Upper
 95 100
 174 95.2 63.2 94.8#
 176 90.2 62.8 94.2

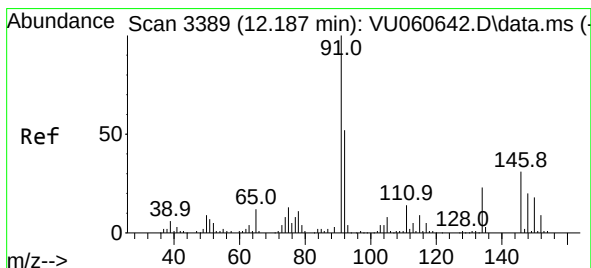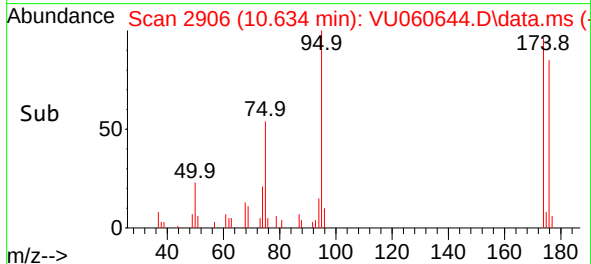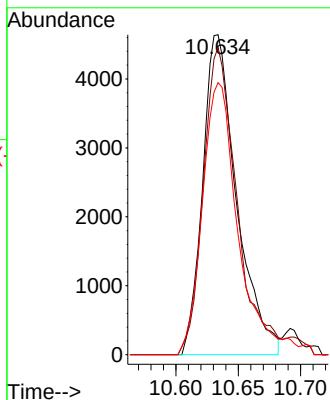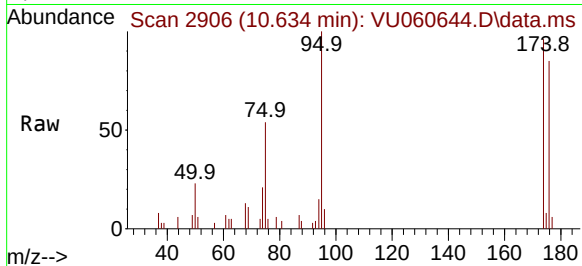

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.780 ug/l
 RT: 12.193 min Scan# 3391
 Delta R.T. 0.006 min
 Lab File: VU060644.D
 Acq: 06 Sep 2024 16:21

Tgt Ion:152 Resp: 9658
 Ion Ratio Lower Upper
 152 100
 115 66.0 0.0 300.4
 150 163.9 0.0 669.4

