

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
Data File : VU060644.D
Acq On : 06 Sep 2024 16:21
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU060644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.042	534	545	558	rVB3	6898	13314	18.81%	7.025%
2	6.113	1488	1500	1520	rBV	33911	70777	100.00%	37.347%
3	10.634	2895	2906	2921	rBV2	24481	43067	60.85%	22.725%
4	10.692	2921	2924	2930	rVB3	805	984	1.39%	0.519%
5	12.193	3380	3391	3407	rBV2	31609	56378	79.66%	29.749%
6	12.251	3407	3409	3416	rVB5	794	821	1.16%	0.433%
7	13.868	3903	3912	3917	rBV4	564	1022	1.44%	0.539%
8	14.122	3982	3991	3994	rBV3	613	811	1.15%	0.428%
9	14.344	4054	4060	4066	rVB4	806	912	1.29%	0.481%
10	14.894	4226	4231	4238	rBV3	439	719	1.02%	0.379%
11	16.408	4699	4702	4705	rBV3	1063	708	1.00%	0.374%




Sum of corrected areas: 189513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
Data File : VU060644.D
Acq On : 06 Sep 2024 16:21
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

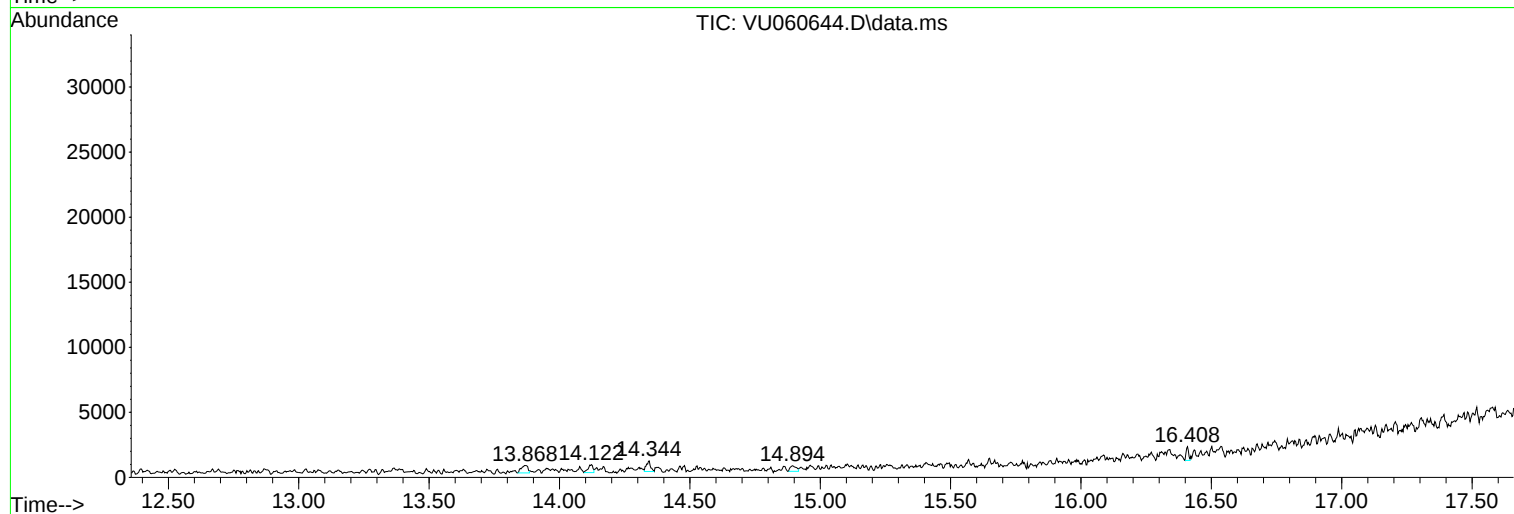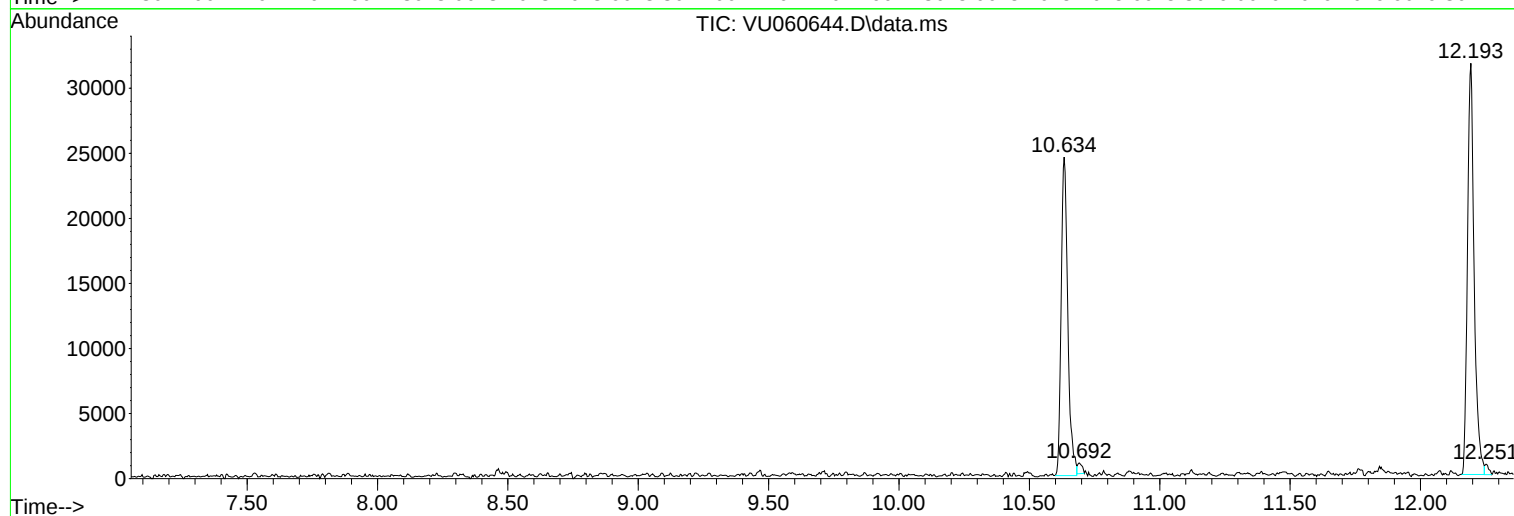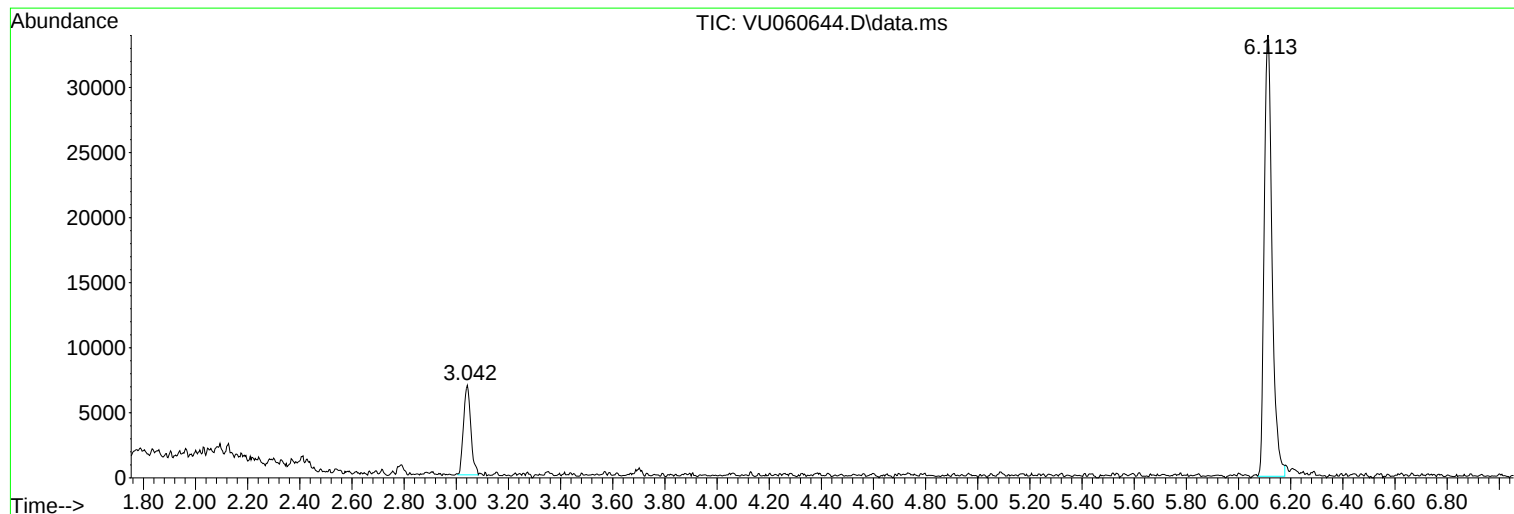

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
Data File : VU060644.D
Acq On : 06 Sep 2024 16:21
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
Data File : VU060644.D
Acq On : 06 Sep 2024 16:21
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------