


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090624\
Data File : VU060637.D
Acq On : 06 Sep 2024 11:24
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U090624DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Sep 09 08:13:33 2024

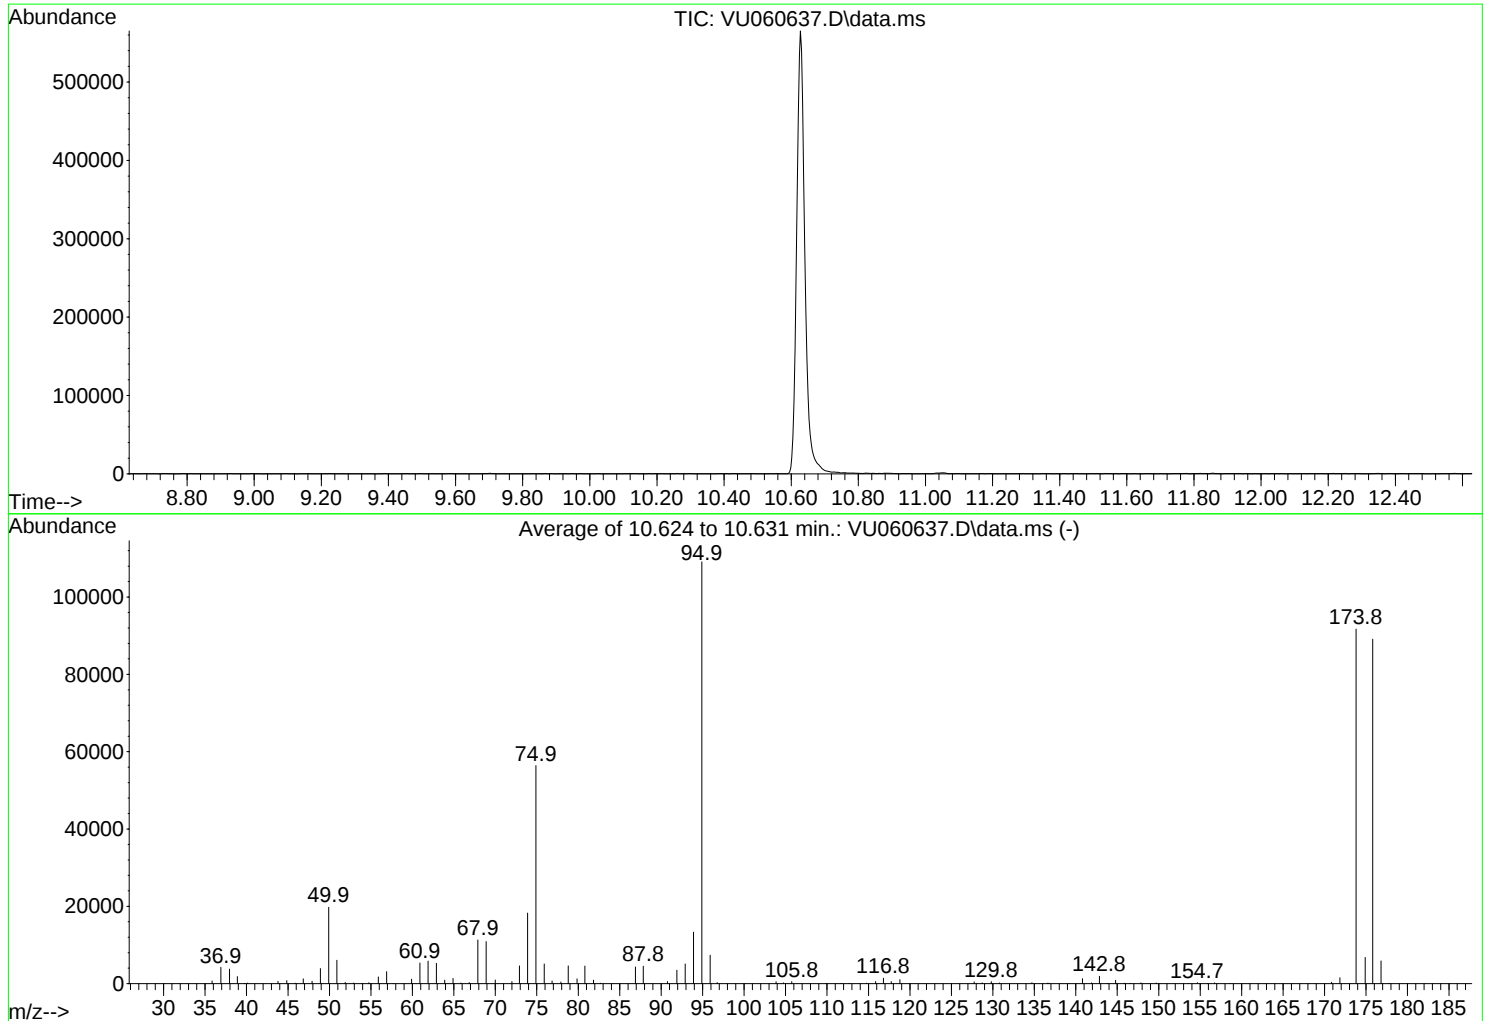

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	19757	PASS
75	95	30	60	51.7	56408	PASS
95	95	100	100	100.0	109107	PASS
96	95	5	9	6.8	7383	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.1	91709	PASS
175	174	5	9	7.4	6784	PASS
176	174	95	101	97.2	89115	PASS
177	176	5	9	6.6	5882	PASS