

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU090718\
 Data File : VU026611.D
 Acq On : 07 Sep 2018 09:33
 Operator : MD/SY
 Sample : VU0907WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0907WBL01

Quant Time: Sep 07 12:19:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U082018DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Mon Aug 20 13:35:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.75	96	24240	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	6559	0.75	ug/l	0.00
Spiked Amount 1.000			Recovery	=	75.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	7909	0.78	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU090718\
Data File : VU026611.D
Acq On : 07 Sep 2018 09:33
Operator : MD/SY
Sample : VU0907WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0907WBL01

Quant Time: Sep 07 12:19:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U082018DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Mon Aug 20 13:35:41 2018
Response via : Initial Calibration

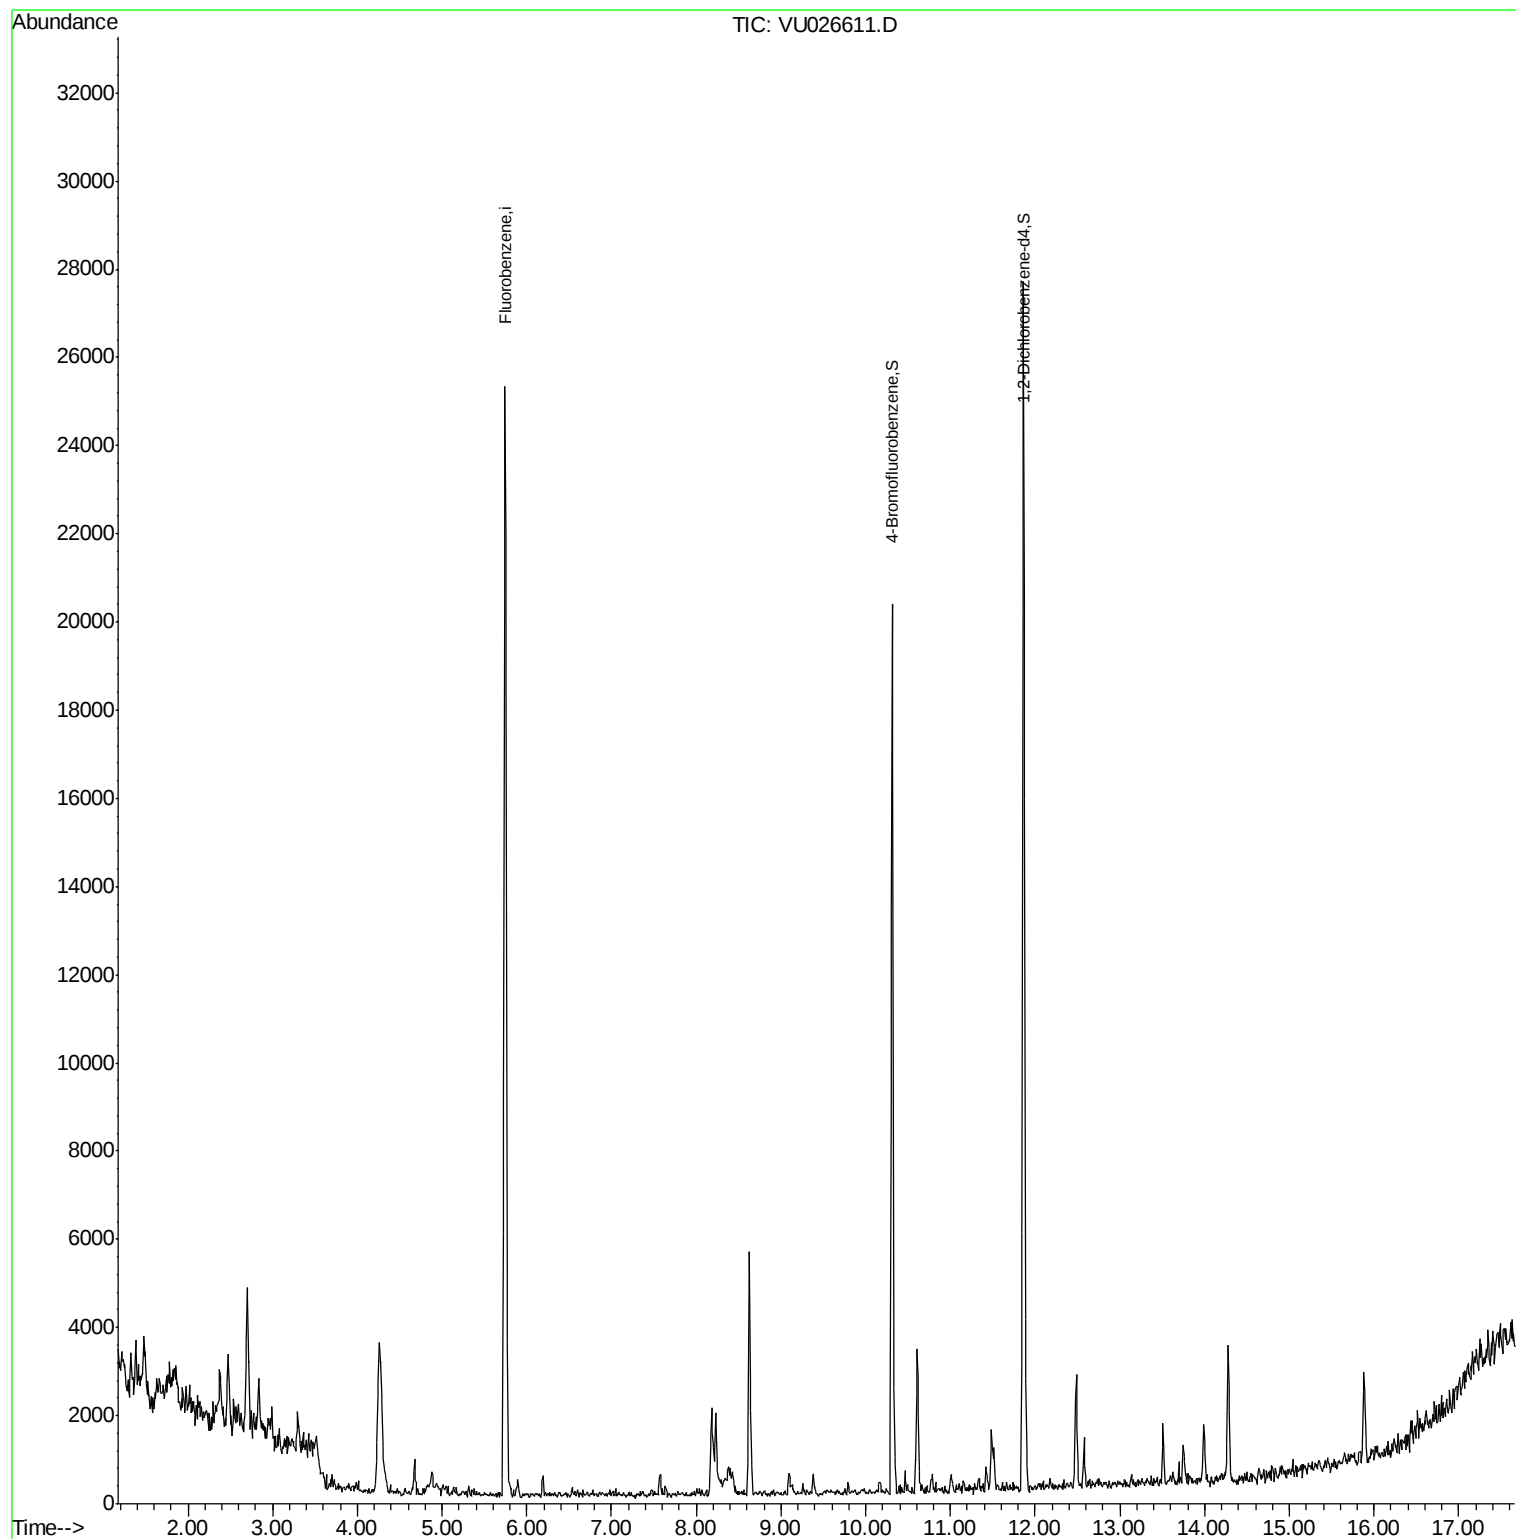

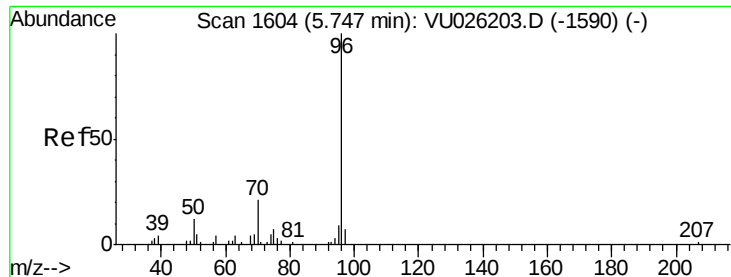

#1

Fluorobenzene

Concen: 1.00 ug/l

RT: 5.75 min Scan# 1422

Delta R.T. -0.00 min

Lab File: VU026611.D

Acq: 07 Sep 2018 09:33

Instrument :

MSVOA_U

ClientSampleId :

VU0907WBL01

Tot Ion: 96 Resp: 24240





Ion Ratio Lower Upper

96 100

70 20.6 16.2 24.4

95 9.4 6.9 10.3

97 5.9 0.0 0.0#

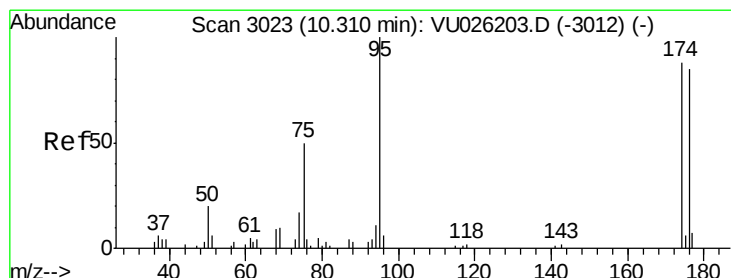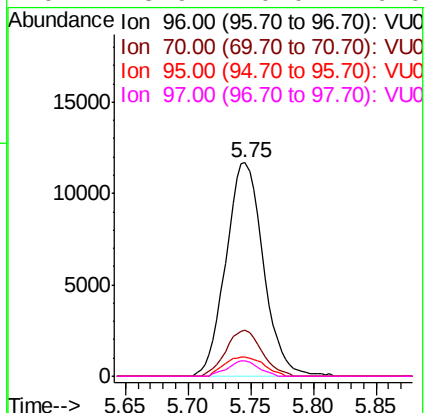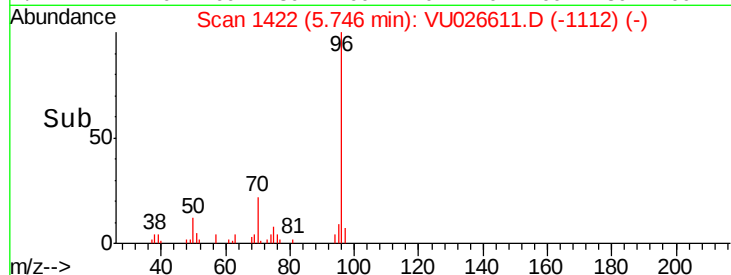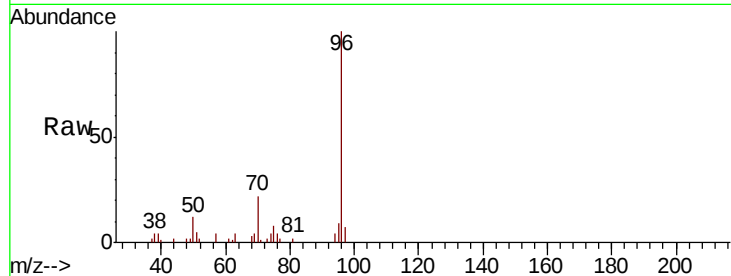

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2841

Delta R.T. -0.00 min

Lab File: VU026611.D

Acq: 07 Sep 2018 09:33




Tgt Ion: 95 Resp: 6559


Ion Ratio Lower Upper

95 100

174 91.6 65.6 98.4

176 86.9 62.0 93.0

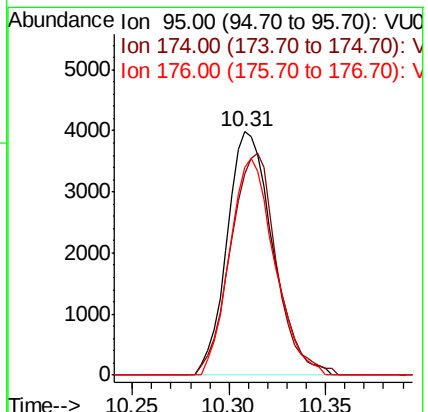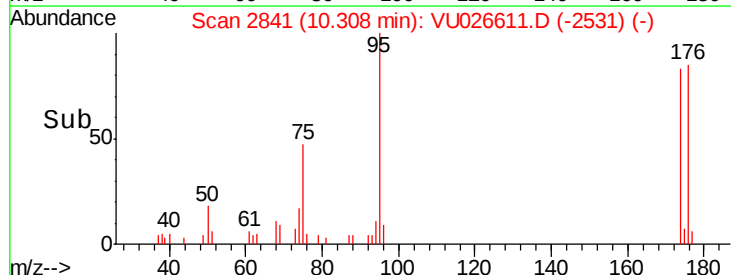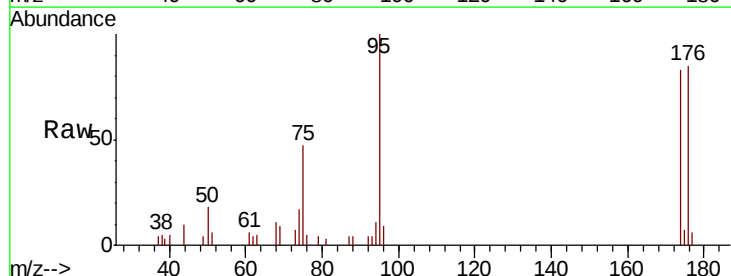

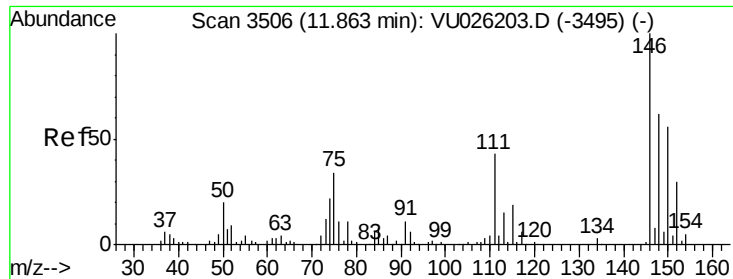

#68

1,2-Dichlorobenzene-d4

Concen: N.D. ug/l

RT: 11.86 min Scan# 3325

Delta R.T. 0.00 min

Lab File: VU026611.D

Acq: 07 Sep 2018 09:33

Instrument :

MSVOA_U

ClientSampleId :

VU0907WBL01


Tot Ion:152 Resp: 7909

Ion Ratio Lower Upper

152 100

115 60.8 0.0 118.8

150 152.3 0.0 0.0#

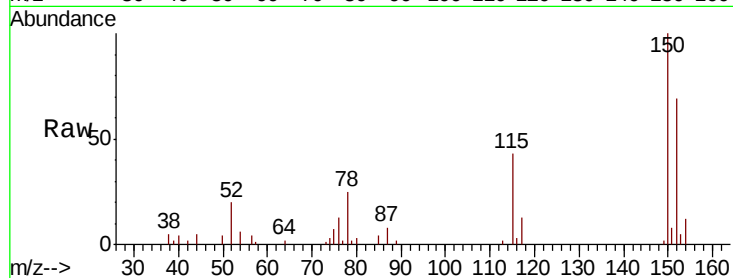

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

