


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU090718\
Data File : VU026609.D
Acq On : 07 Sep 2018 08:01
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U082018DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Aug 20 13:35:41 2018

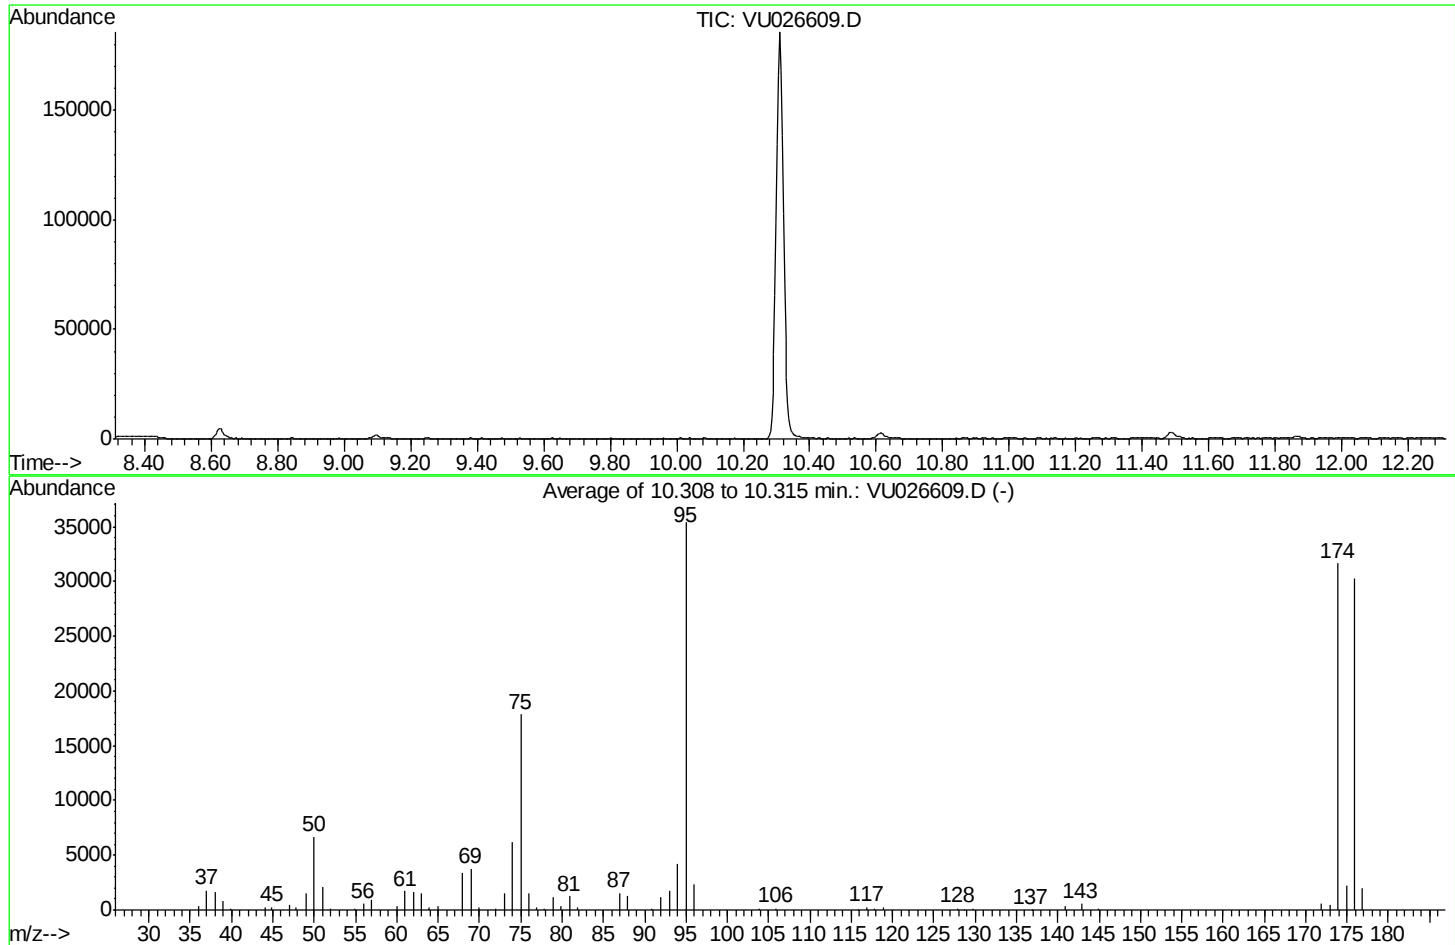

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	6699	PASS
75	95	30	60	50.4	17834	PASS
95	95	100	100	100.0	35400	PASS
96	95	5	9	6.5	2285	PASS
173	174	0.00	2	1.6	516	PASS
174	95	50	100	89.4	31645	PASS
175	174	5	9	7.2	2263	PASS
176	174	95	101	95.8	30312	PASS
177	176	5	9	6.6	1998	PASS