

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
 Data File : VU044586.D
 Acq On : 07 Sep 2021 16:14
 Operator : SY/MD
 Sample : M3647-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W33

Quant Time: Sep 08 02:37:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Sep 08 02:31:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	111002	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	114110	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	59228	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	34624	3.857	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.200%
7) Chloroethane-d5	1.919	69	36668	4.700	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.000%
11) 1,1-Dichloroethene-d2	2.575	65	15215	3.984	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.600%
20) 2-Butanone-d5	4.642	46	102609	41.327	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.660%
24) Chloroform-d	5.070	84	67432	4.248	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.000%
26) 1,2-Dichloroethane-d4	5.710	65	37977	4.387	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
32) Benzene-d6	5.735	84	140061	4.359	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	6.697	67	43656	4.247	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.000%
41) Toluene-d8	7.903	98	122840	4.311	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.200%
43) trans-1,3-Dichloroprop...	8.186	79	14740	3.993	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.645	63	90327	45.246	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.500%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	38342	4.429	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	12.198	152	49360	4.933	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.600%
Target Compounds						Qvalue
3) Chloromethane	1.523	50	5669	0.379	ug/L	98
13) Acetone	2.652	43	23064	11.187	ug/L	76
14) Carbon disulfide	2.800	76	2020	0.073	ug/L #	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044586.D
Acq On : 07 Sep 2021 16:14
Operator : SY/MD
Sample : M3647-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W33

Quant Time: Sep 08 02:37:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 08 02:31:37 2021
Response via : Initial Calibration

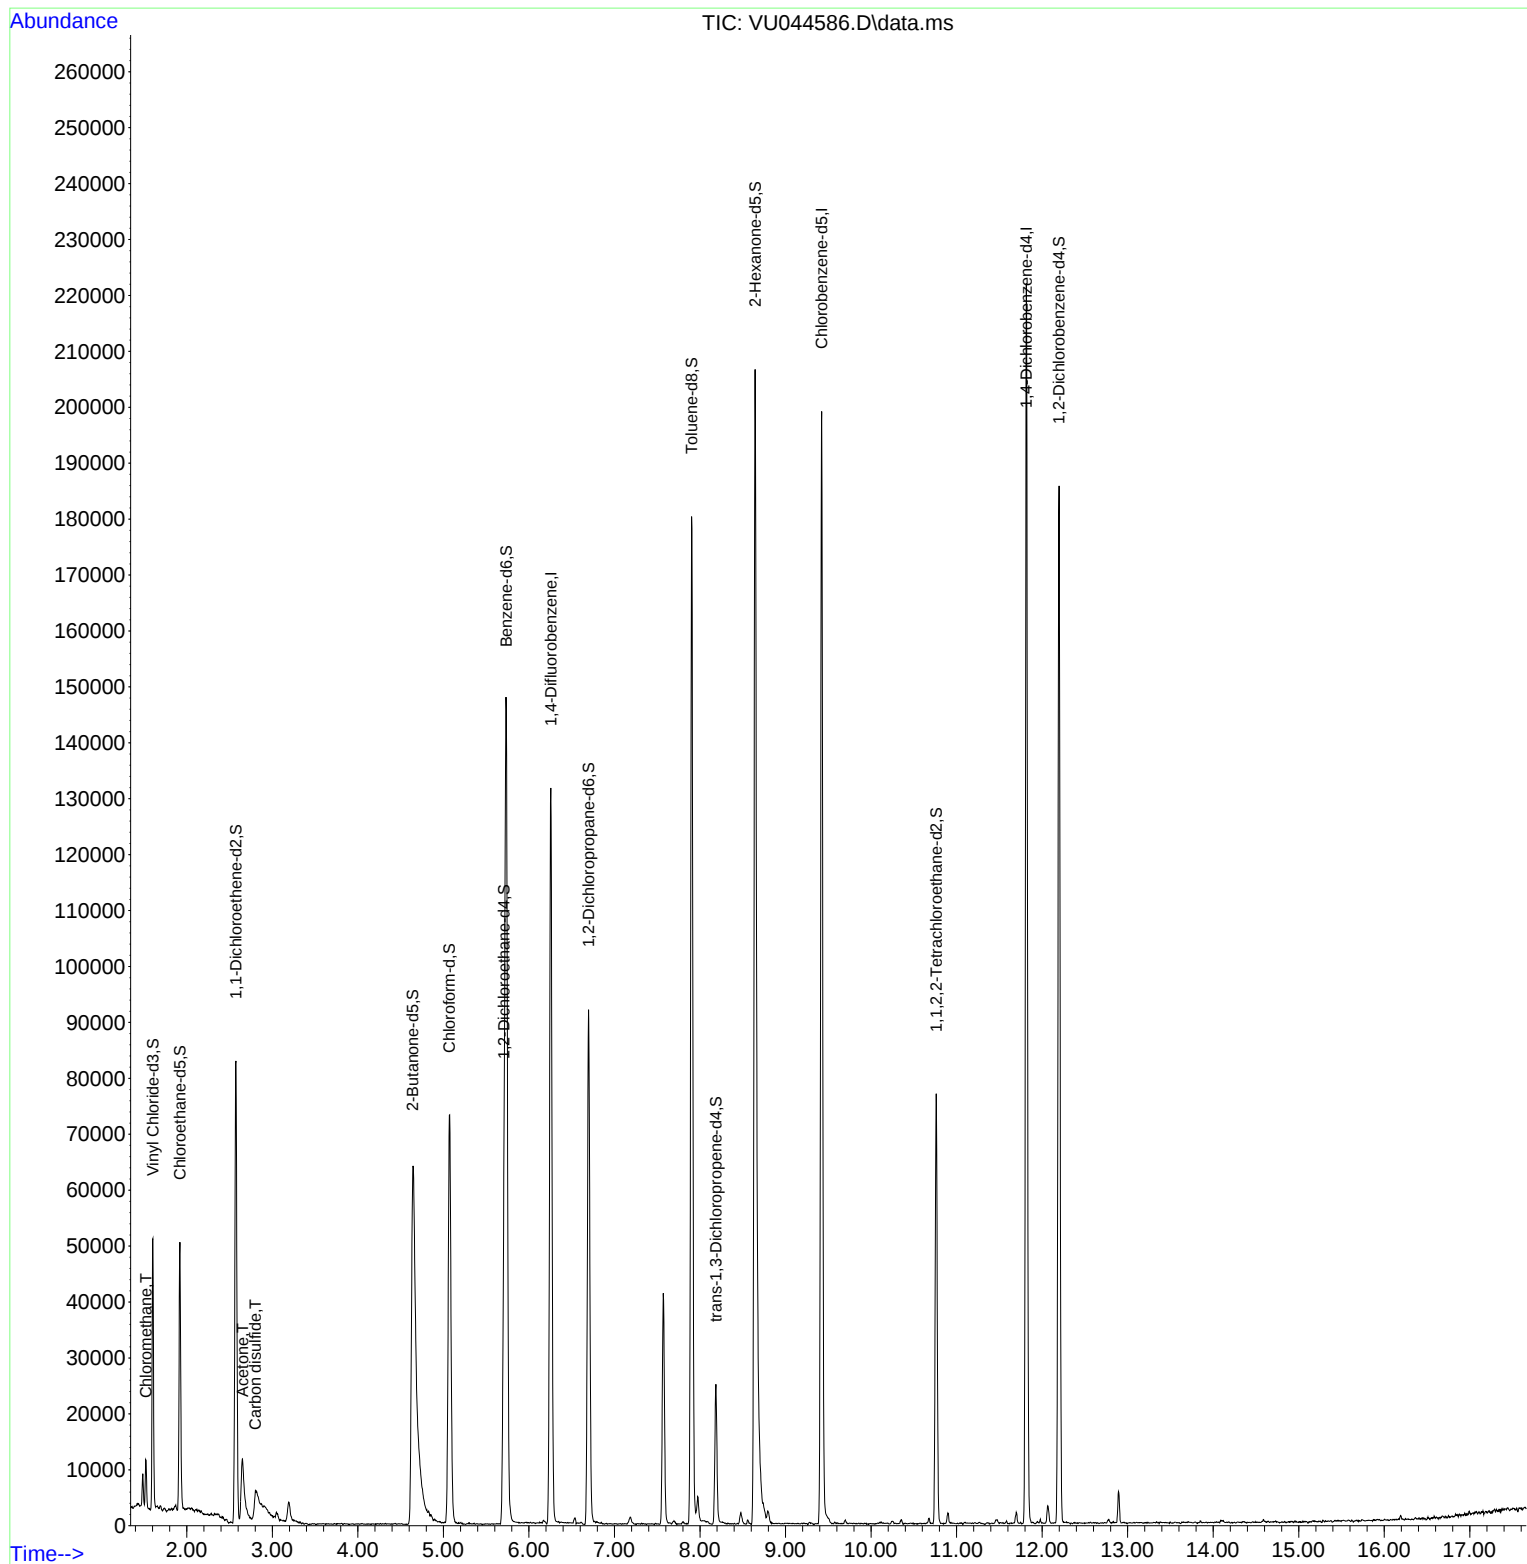

Abundance Scan 56 (1.520 min): VU044576.D\data.ms (-48)


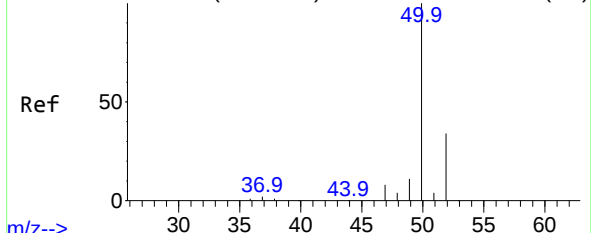


#3
Chloromethane
Concen: 0.379 ug/L
RT: 1.523 min Scan# 57
Delta R.T. 0.003 min
Lab File: VU044586.D
Acq: 07 Sep 2021 16:14


Tgt Ion: 50 Resp: 5669
Ion Ratio Lower Upper
50 100
52 31.5 22.8 42.4

Instrument :
MSVOA_U
ClientSampled :
F3W33


Abundance Scan 57 (1.523 min): VU044586.D\data.ms

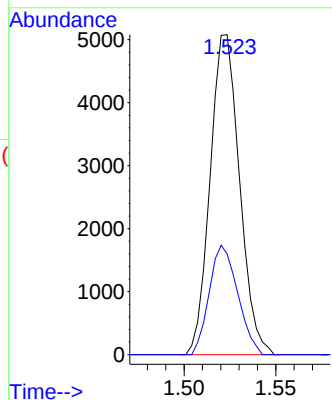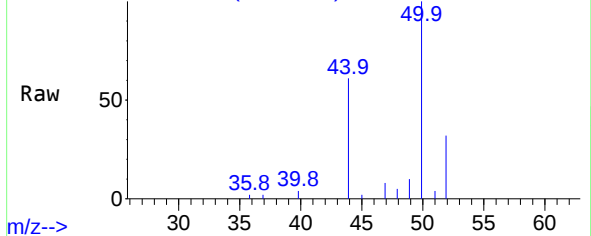

Abundance Scan 57 (1.523 min): VU044586.D\data.ms (-1)

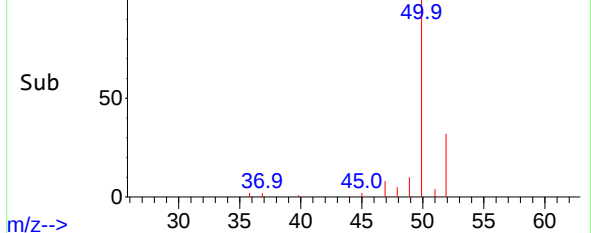



Abundance Scan 407 (2.649 min): VU044576.D\data.ms (-39)

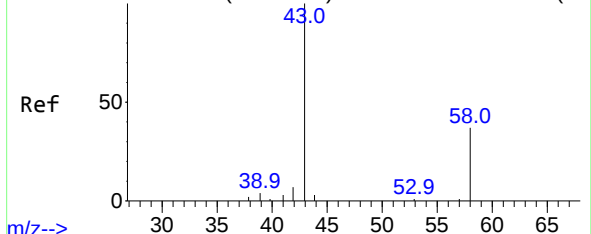


#13
Acetone
Concen: 11.187 ug/L
RT: 2.652 min Scan# 408
Delta R.T. 0.003 min
Lab File: VU044586.D
Acq: 07 Sep 2021 16:14


Tgt Ion: 43 Resp: 23064
Ion Ratio Lower Upper
43 100
58 34.1 0.0 45.4

Abundance Scan 408 (2.652 min): VU044586.D\data.ms

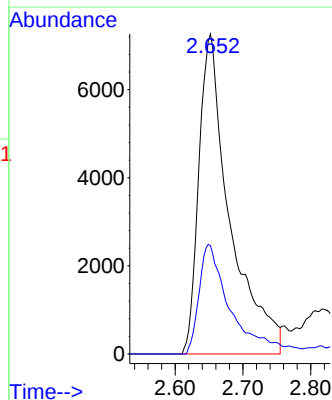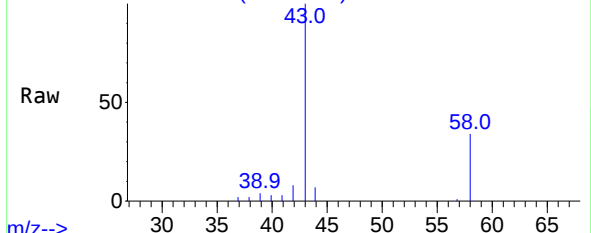


Abundance Scan 408 (2.652 min): VU044586.D\data.ms (-31)

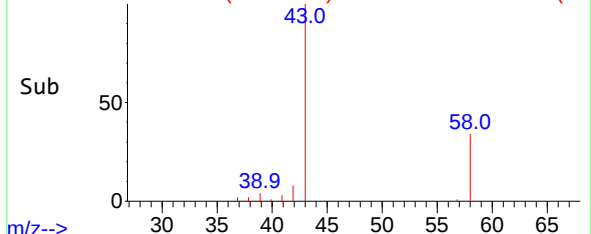

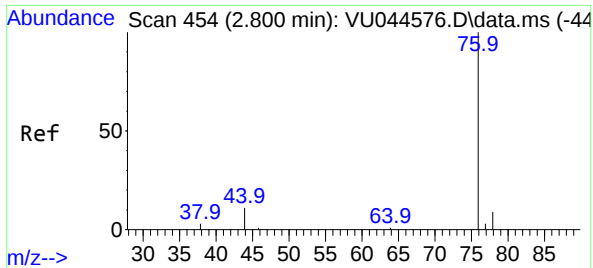

#14
Carbon disulfide
Concen: 0.073 ug/L
RT: 2.800 min Scan# 454
Delta R.T. 0.000 min
Lab File: VU044586.D
Acq: 07 Sep 2021 16:14

Instrument :
MSVOA_U
ClientSampleId :
F3W33

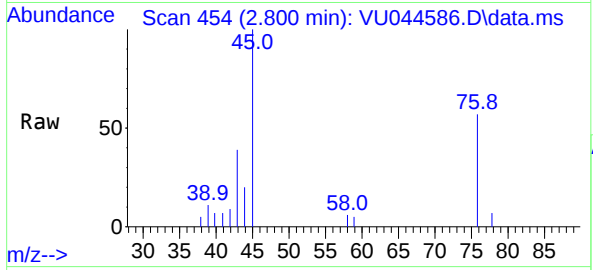

Tgt Ion: 76 Resp: 2020
Ion Ratio Lower Upper
76 100
78 11.5 7.2 10.8#

