

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
 Data File : VU044578.D
 Acq On : 07 Sep 2021 13:00
 Operator : SY/MD
 Sample : M3596-06DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W07DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	52	rVB	28362	27232	5.06%	0.634%
2	1.600	73	81	95	rBV	59793	68627	12.75%	1.598%
3	1.919	171	180	192	rBV	55830	73310	13.62%	1.707%
4	2.571	371	383	401	rBV	100774	161968	30.10%	3.771%
5	3.054	521	533	552	rVB	23305	44002	8.18%	1.024%
6	4.645	1010	1028	1063	rBV	48118	183693	34.14%	4.276%
7	5.070	1145	1160	1184	rBV	107621	255993	47.58%	5.959%
8	5.732	1345	1366	1387	rBV2	175132	454300	84.43%	10.576%
9	6.256	1514	1529	1544	rBV	139615	262077	48.71%	6.101%
10	6.546	1610	1619	1628	rVB6	3782	7115	1.32%	0.166%
11	6.697	1652	1666	1692	rBV	108420	211774	39.36%	4.930%
12	7.571	1925	1938	1964	rBV	49225	89170	16.57%	2.076%
13	7.902	2028	2041	2056	rBV	217023	376330	69.94%	8.761%
14	7.973	2059	2063	2073	rVB	4220	6327	1.18%	0.147%
15	8.185	2118	2129	2145	rBV	30415	53534	9.95%	1.246%
16	8.558	2233	2245	2260	rBV	150418	257657	47.89%	5.998%
17	8.645	2260	2272	2315	rVB	218890	538074	100.00%	12.526%
18	9.423	2496	2514	2554	rVB	207518	354400	65.86%	8.250%
19	10.761	2919	2930	2948	rVB	90203	147102	27.34%	3.424%
20	11.815	3247	3258	3279	rBV	232132	367019	68.21%	8.544%
21	12.198	3365	3377	3395	rBV	222163	355926	66.15%	8.286%




Sum of corrected areas: 4295630

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044578.D
Acq On : 07 Sep 2021 13:00
Operator : SY/MD
Sample : M3596-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W07DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

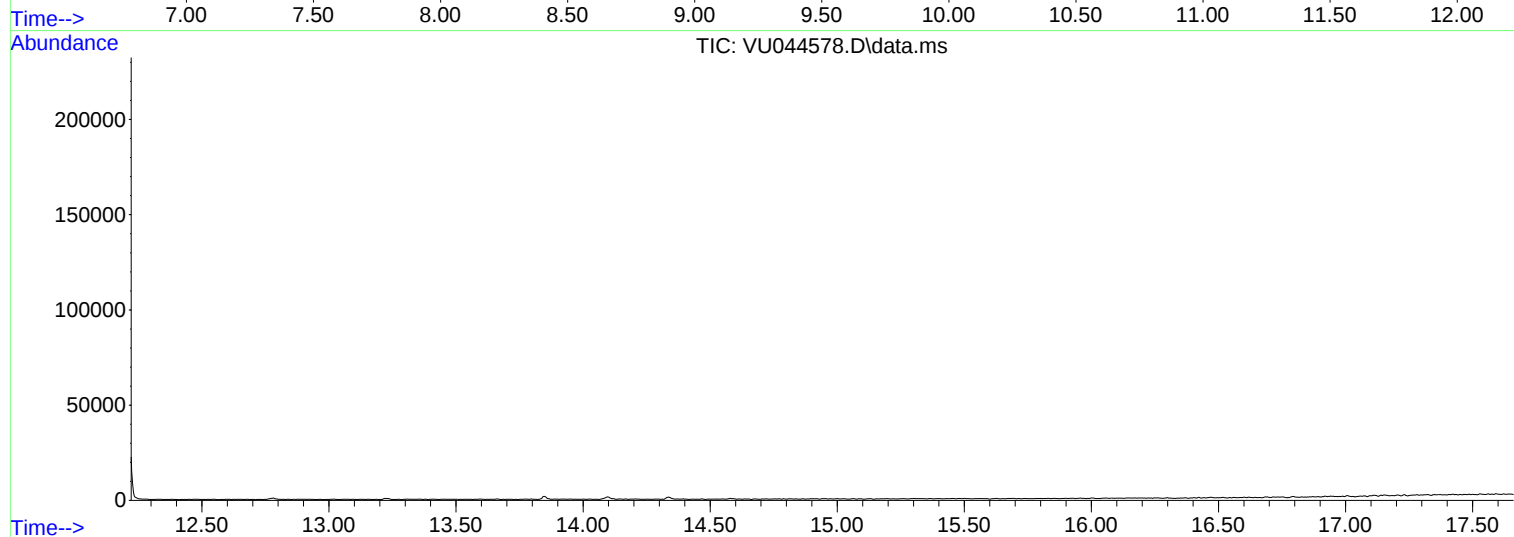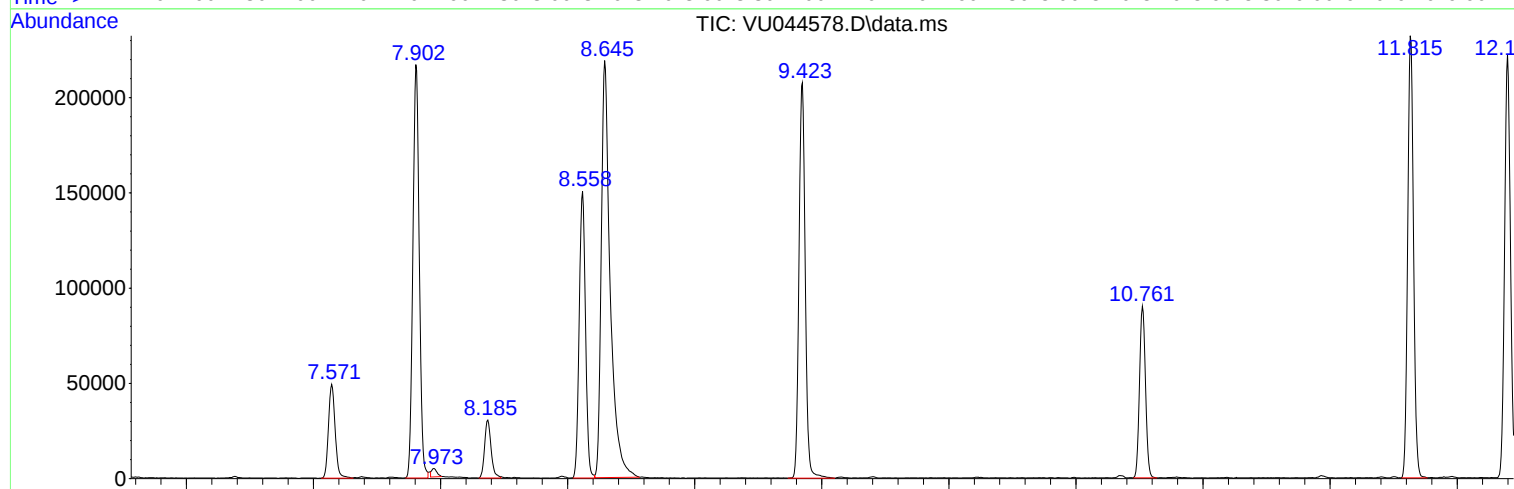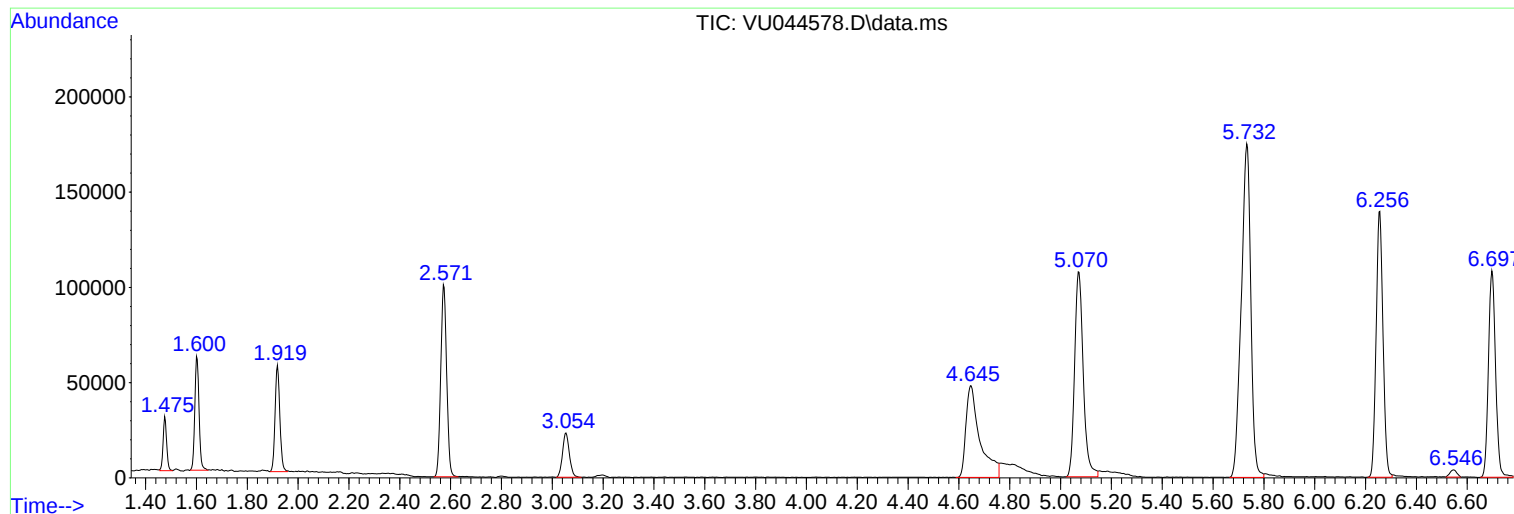

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044578.D
Acq On : 07 Sep 2021 13:00
Operator : SY/MD
Sample : M3596-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W07DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.475	0.52 ug/L	27232	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Trifluoroguanidine	113	CH2F3N3	037950-72-4	4
4			Formamidoxime	60	CH4N2O	000624-82-8	4
5			Methyl formate	60	C2H4O2	000107-31-3	3

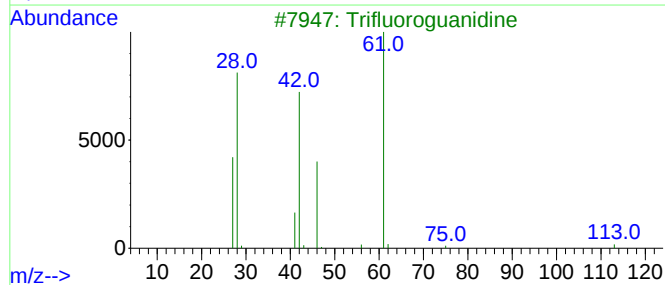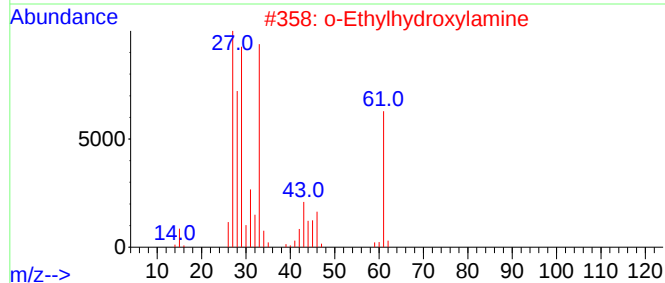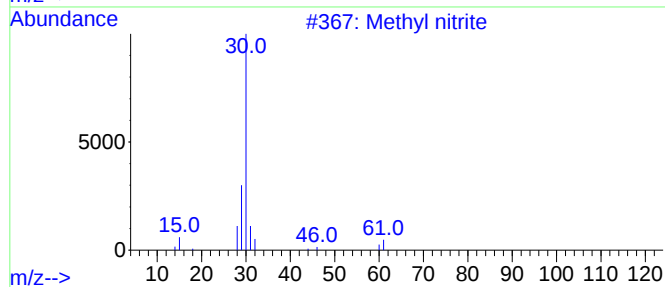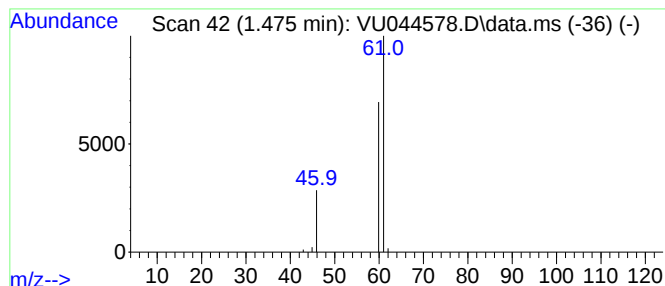

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044578.D
Acq On : 07 Sep 2021 13:00
Operator : SY/MD
Sample : M3596-06DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W07DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.475	0.5	ug/L	27232	1	6.256	262077	5.0