

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
 Data File : VU044580.D
 Acq On : 07 Sep 2021 13:49
 Operator : SY/MD
 Sample : M3622-01DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044580.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	35	42	52	rVB	36914	35079	6.93%	0.821%
2	1.601	73	81	97	rVB	59677	68869	13.61%	1.612%
3	1.919	171	180	195	rBV	53526	70482	13.93%	1.649%
4	2.144	240	250	263	rVB	53008	76195	15.06%	1.783%
5	2.572	371	383	402	rBV	97278	158586	31.34%	3.711%
6	3.054	521	533	551	rBV	24451	47029	9.29%	1.100%
7	4.645	1012	1028	1055	rBV	42424	145937	28.84%	3.415%
8	5.070	1145	1160	1179	rBV	83046	184910	36.54%	4.327%
9	5.732	1345	1366	1392	rBV2	166480	437239	86.41%	10.231%
10	6.256	1515	1529	1551	rBV	125387	239453	47.32%	5.603%
11	6.546	1609	1619	1629	rVB7	4397	8482	1.68%	0.198%
12	6.697	1653	1666	1685	rBV	101491	200522	39.63%	4.692%
13	7.571	1926	1938	1960	rBV	48057	85709	16.94%	2.006%
14	7.903	2025	2041	2057	rBV	210619	361262	71.40%	8.454%
15	8.186	2118	2129	2146	rBV	29517	50591	10.00%	1.184%
16	8.559	2232	2245	2259	rBV	274107	463644	91.63%	10.849%
17	8.645	2260	2272	2315	rVB	203476	506003	100.00%	11.841%
18	9.423	2501	2514	2534	rBV	191226	320598	63.36%	7.502%
19	10.761	2919	2930	2948	rVB	86869	140131	27.69%	3.279%
20	11.816	3245	3258	3278	rBV	208603	331318	65.48%	7.753%
21	12.198	3363	3377	3395	rBV	211541	341446	67.48%	7.990%




Sum of corrected areas: 4273485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044580.D
Acq On : 07 Sep 2021 13:49
Operator : SY/MD
Sample : M3622-01DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

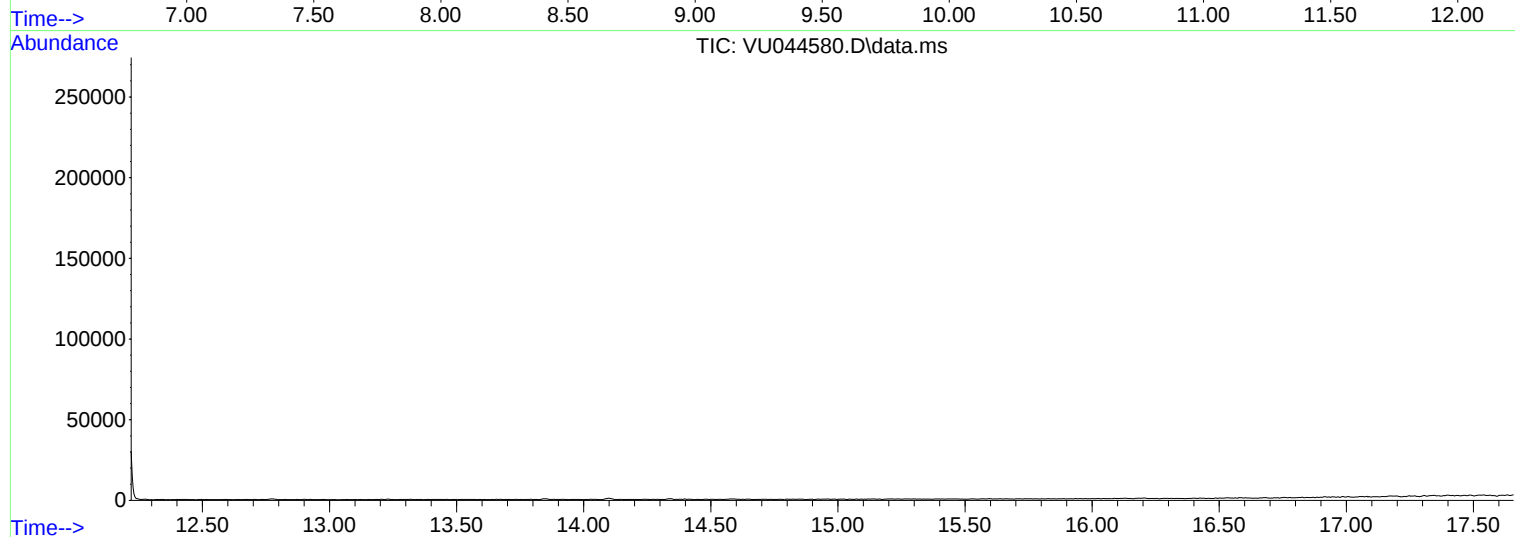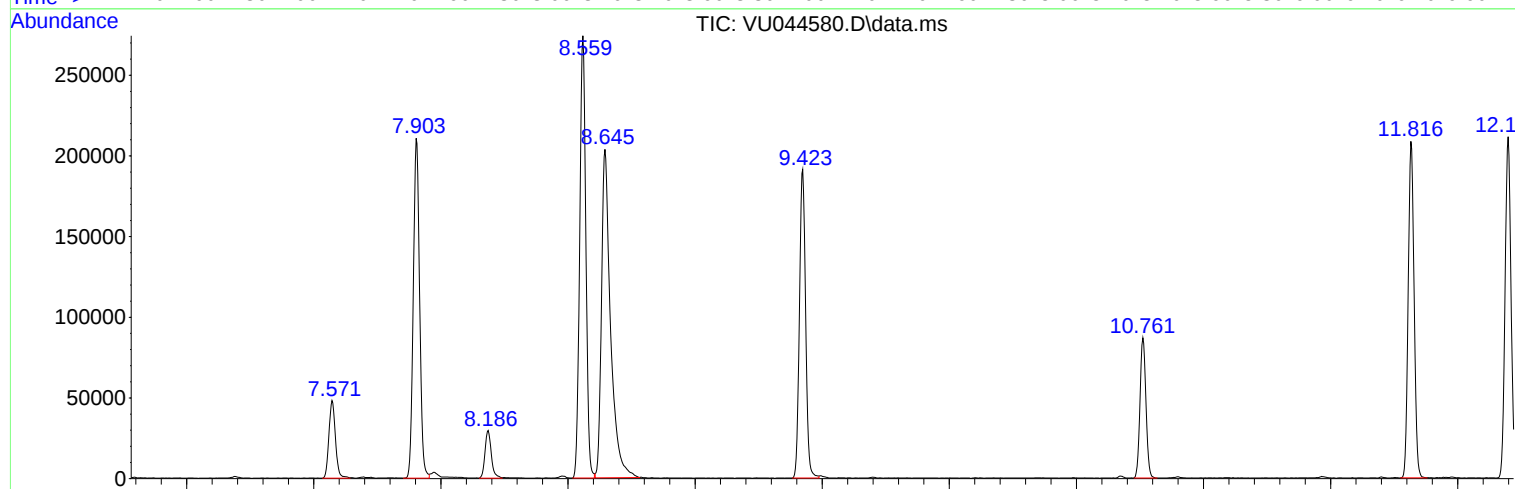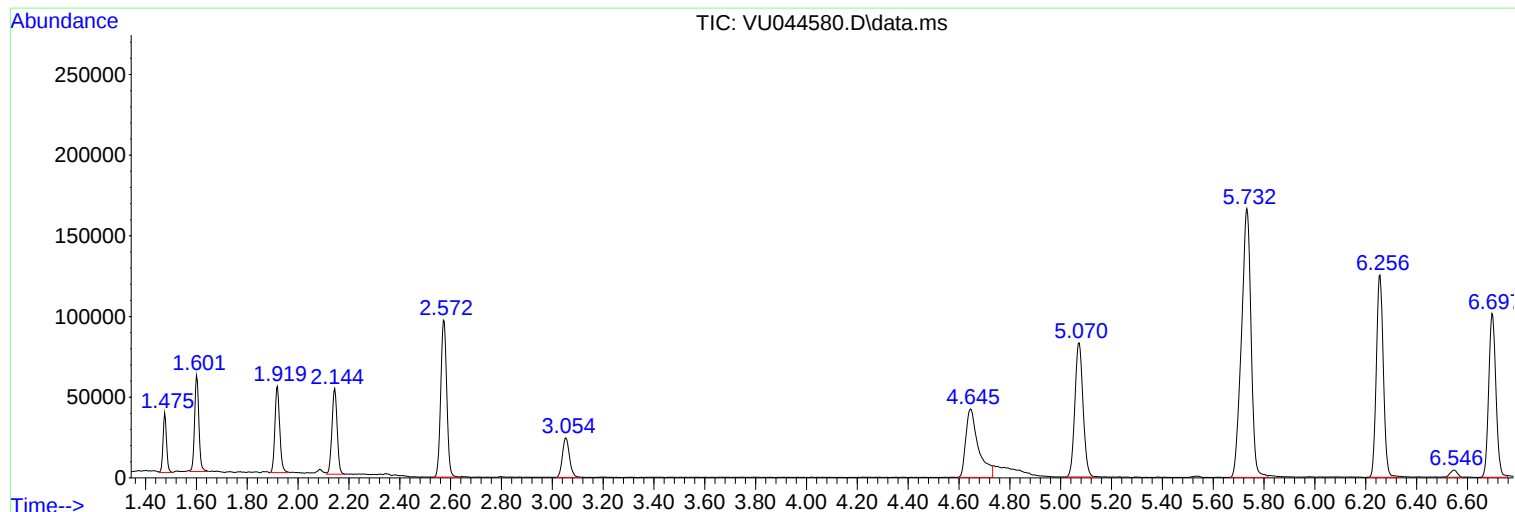

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044580.D
Acq On : 07 Sep 2021 13:49
Operator : SY/MD
Sample : M3622-01DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY3DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.475	0.73 ug/L	35079	1,4-Difluorobenzene	6.256

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Cyanogen chloride	61	CClN	000506-77-4	4
4			Cyanogen chloride	61	CClN	000506-77-4	4
5			Methyl formate	60	C2H4O2	000107-31-3	3

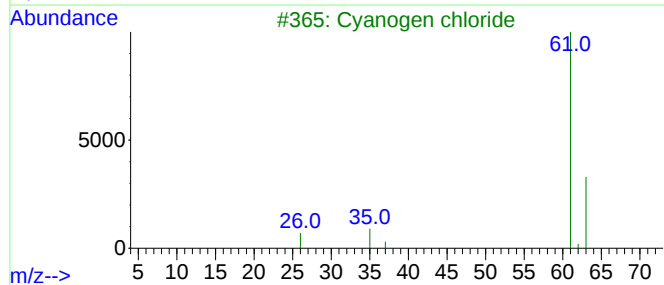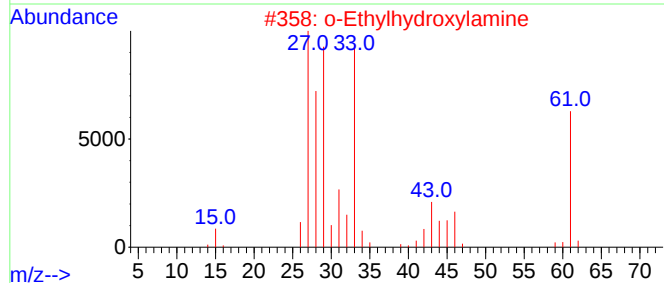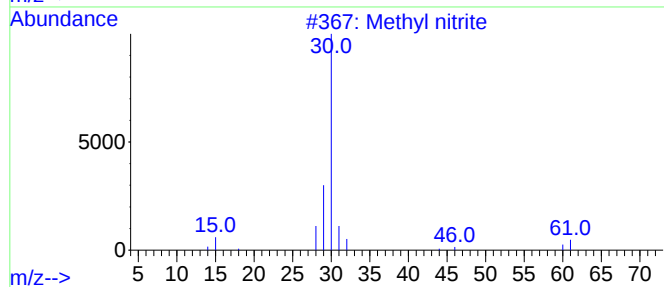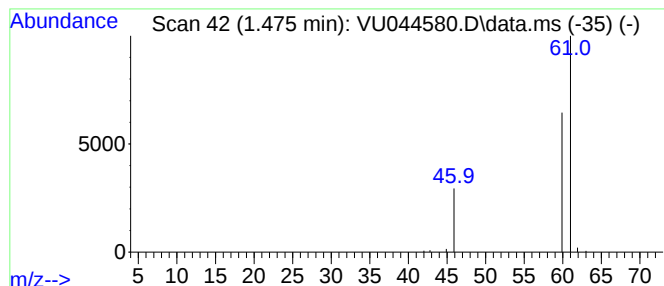

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044580.D
Acq On : 07 Sep 2021 13:49
Operator : SY/MD
Sample : M3622-01DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard---			
					#	RT	Resp	Conc
unknown-01	1.475	0.7	ug/L	35079	1	6.256	239453	5.0