

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
 Data File : VU044588.D
 Acq On : 07 Sep 2021 17:03
 Operator : SY/MD
 Sample : M3647-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.520	51	56	65	rVB	5186	5622	1.29%	0.167%
2	1.600	74	81	93	rBV	49467	56295	12.92%	1.670%
3	1.736	116	123	136	rVB	11384	14083	3.23%	0.418%
4	1.919	171	180	193	rBV	47252	63145	14.50%	1.874%
5	2.571	371	383	397	rBV	80654	130709	30.01%	3.878%
6	3.192	563	576	588	rBV2	1967	4504	1.03%	0.134%
7	4.645	1013	1028	1074	rBV2	58218	216119	49.62%	6.412%
8	5.073	1144	1161	1179	rBV	70658	155488	35.70%	4.613%
9	5.732	1346	1366	1384	rBV2	142289	367898	84.46%	10.916%
10	6.256	1513	1529	1550	rBV	131954	250291	57.46%	7.426%
11	6.697	1652	1666	1684	rBV	87862	172148	39.52%	5.108%
12	7.571	1925	1938	1955	rBV	41047	71538	16.42%	2.123%
13	7.902	2022	2041	2058	rBV	176809	302202	69.38%	8.966%
14	8.185	2116	2129	2141	rBV	23623	40442	9.28%	1.200%
15	8.478	2210	2220	2230	rVB3	2906	5147	1.18%	0.153%
16	8.645	2258	2272	2310	rBV	202461	435577	100.00%	12.924%
17	9.423	2500	2514	2535	rBV	196372	331606	76.13%	9.839%
18	10.761	2918	2930	2946	rBV	74065	118848	27.29%	3.526%
19	10.896	2962	2972	2981	rBV3	3051	4751	1.09%	0.141%
20	11.815	3247	3258	3277	rBV	212289	338154	77.63%	10.033%
21	12.198	3365	3377	3396	rBV	177328	285794	65.61%	8.480%




Sum of corrected areas: 3370361

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044588.D
Acq On : 07 Sep 2021 17:03
Operator : SY/MD
Sample : M3647-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

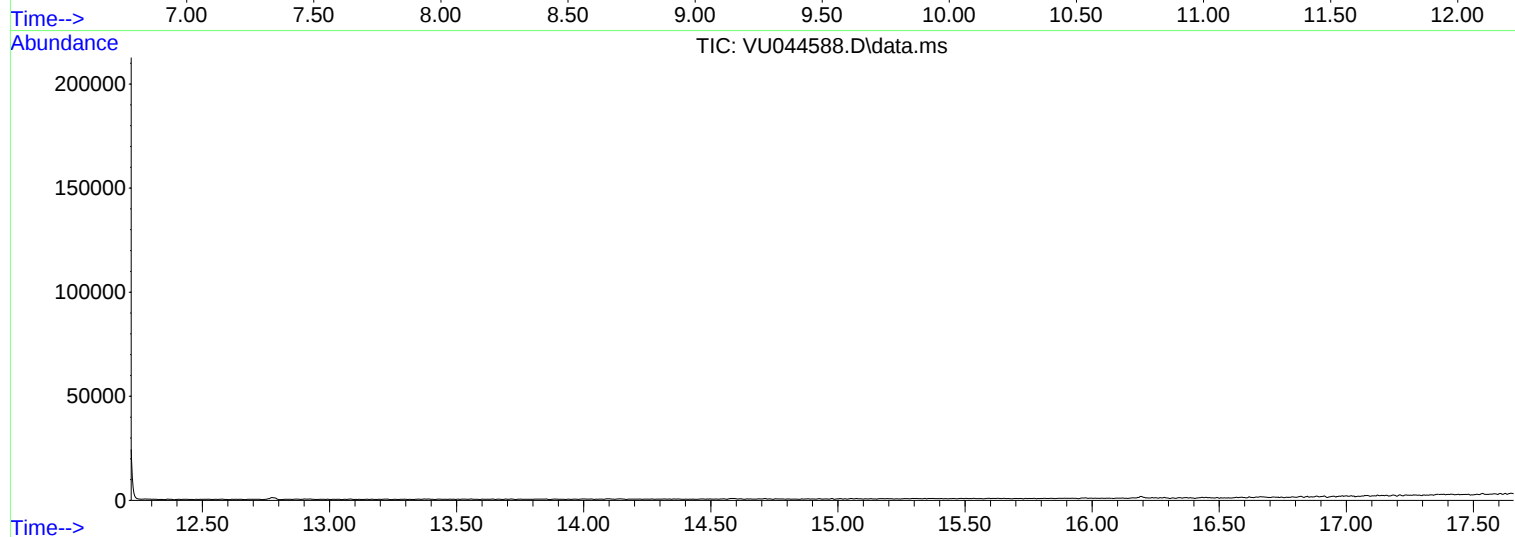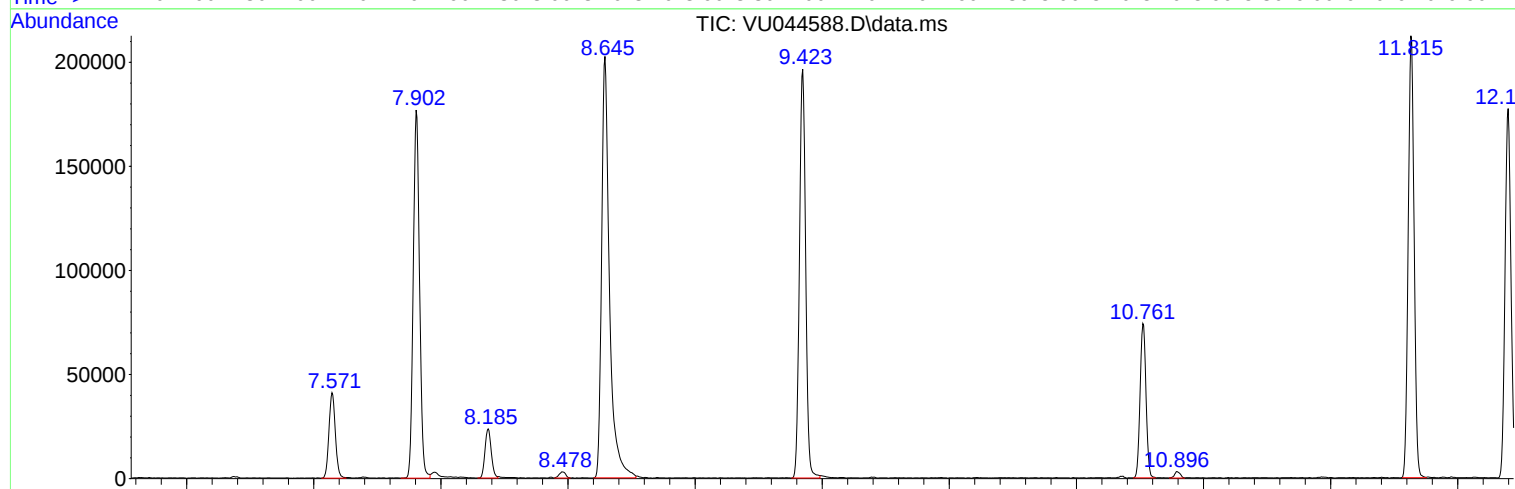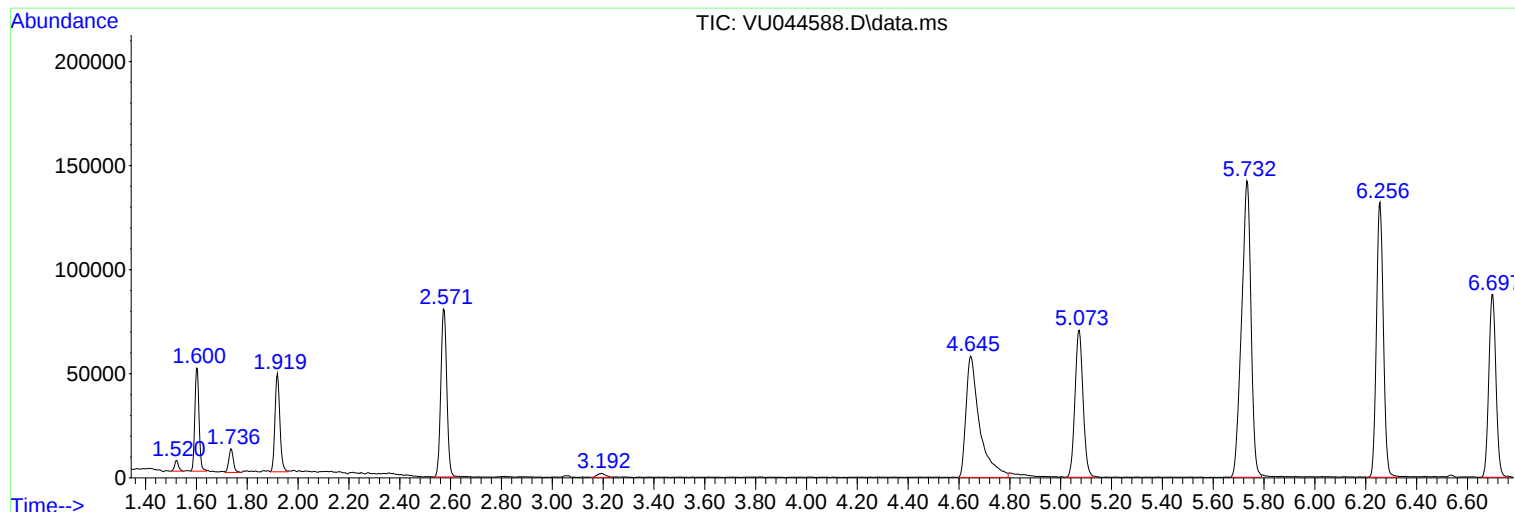

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044588.D
Acq On : 07 Sep 2021 17:03
Operator : SY/MD
Sample : M3647-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044588.D
Acq On : 07 Sep 2021 17:03
Operator : SY/MD
Sample : M3647-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
