

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
 Data File : VU044589.D
 Acq On : 07 Sep 2021 17:27
 Operator : SY/MD
 Sample : M3647-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU044589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	20	rVB3	3740	4690	1.04%	0.124%
2	1.601	73	81	91	rBV	52379	59733	13.26%	1.581%
3	1.919	171	180	193	rVB	49644	64180	14.25%	1.698%
4	2.575	372	384	400	rBV	79970	129936	28.84%	3.438%
5	4.642	1012	1027	1068	rBV2	53518	182823	40.58%	4.838%
6	5.070	1145	1160	1184	rBV	72093	158132	35.10%	4.184%
7	5.732	1346	1366	1392	rBV2	147608	379179	84.17%	10.033%
8	6.256	1514	1529	1545	rBV	124818	236392	52.47%	6.255%
9	6.697	1653	1666	1683	rBV	90110	174854	38.81%	4.627%
10	7.571	1924	1938	1955	rBV	40492	71458	15.86%	1.891%
11	7.903	2028	2041	2057	rBV	175416	305213	67.75%	8.076%
12	7.973	2057	2063	2074	rVB2	4925	8293	1.84%	0.219%
13	8.185	2114	2129	2141	rBV	25246	41767	9.27%	1.105%
14	8.558	2233	2245	2256	rBV2	25372	42248	9.38%	1.118%
15	8.642	2259	2271	2302	rBV	218283	450508	100.00%	11.921%
16	9.423	2500	2514	2533	rBV	184479	313061	69.49%	8.284%
17	9.700	2591	2600	2609	rVB2	3952	5752	1.28%	0.152%
18	10.761	2919	2930	2946	rBV	77363	122069	27.10%	3.230%
19	10.899	2961	2973	2986	rVB4	2764	4582	1.02%	0.121%
20	11.472	3142	3151	3160	rVB3	3730	5909	1.31%	0.156%
21	11.816	3246	3258	3276	rBV	203064	321527	71.37%	8.508%
22	12.198	3364	3377	3392	rBV	179720	291983	64.81%	7.726%
23	13.626	3817	3821	3834	rVB5	5676	8050	1.79%	0.213%
24	14.195	3990	3998	4008	rVB4	3524	5088	1.13%	0.135%
25	14.291	4018	4028	4036	rBV8	2631	4791	1.06%	0.127%
26	14.690	4138	4152	4161	rBV10	7379	14789	3.28%	0.391%
27	14.815	4182	4191	4199	rBV10	2852	4794	1.06%	0.127%
28	14.886	4205	4213	4221	rVB5	2835	4691	1.04%	0.124%
29	15.021	4246	4255	4268	rBV6	7316	12835	2.85%	0.340%
30	15.201	4303	4311	4324	rBV5	12037	25244	5.60%	0.668%
31	15.275	4326	4334	4343	rVB3	12497	19554	4.34%	0.517%
32	15.346	4350	4356	4364	rBV5	3518	5395	1.20%	0.143%
33	15.426	4375	4381	4389	rVV9	3439	5530	1.23%	0.146%
34	15.471	4389	4395	4400	rVV7	4470	6720	1.49%	0.178%
35	15.507	4400	4406	4416	rVB7	8320	12759	2.83%	0.338%
36	15.600	4424	4435	4445	rVB8	5320	9456	2.10%	0.250%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
 Data File : VU044589.D
 Acq On : 07 Sep 2021 17:27
 Operator : SY/MD
 Sample : M3647-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F3W03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M

Title : TRACE VOA SFAM1.0

37	15.764	4474	4486	4494	rBV7	4922	10396	2.31%	0.275%
38	15.928	4525	4537	4545	rBV6	11970	25169	5.59%	0.666%
39	16.095	4584	4589	4599	rVB6	4436	7671	1.70%	0.203%
40	16.156	4599	4608	4614	rBV7	9697	15386	3.42%	0.407%
41	16.192	4615	4619	4627	rVB6	6784	8788	1.95%	0.233%
42	16.269	4636	4643	4651	rBV6	8194	12582	2.79%	0.333%
43	16.362	4653	4672	4679	rVV5	18899	40512	8.99%	1.072%
44	16.410	4682	4687	4695	rVB6	12956	18834	4.18%	0.498%
45	16.529	4716	4724	4738	rBV	13770	30178	6.70%	0.799%
46	16.648	4756	4761	4777	rBV	7269	15611	3.47%	0.413%
47	16.893	4828	4837	4850	rBV2	51583	80039	17.77%	2.118%




Sum of corrected areas: 3779151

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044589.D
Acq On : 07 Sep 2021 17:27
Operator : SY/MD
Sample : M3647-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

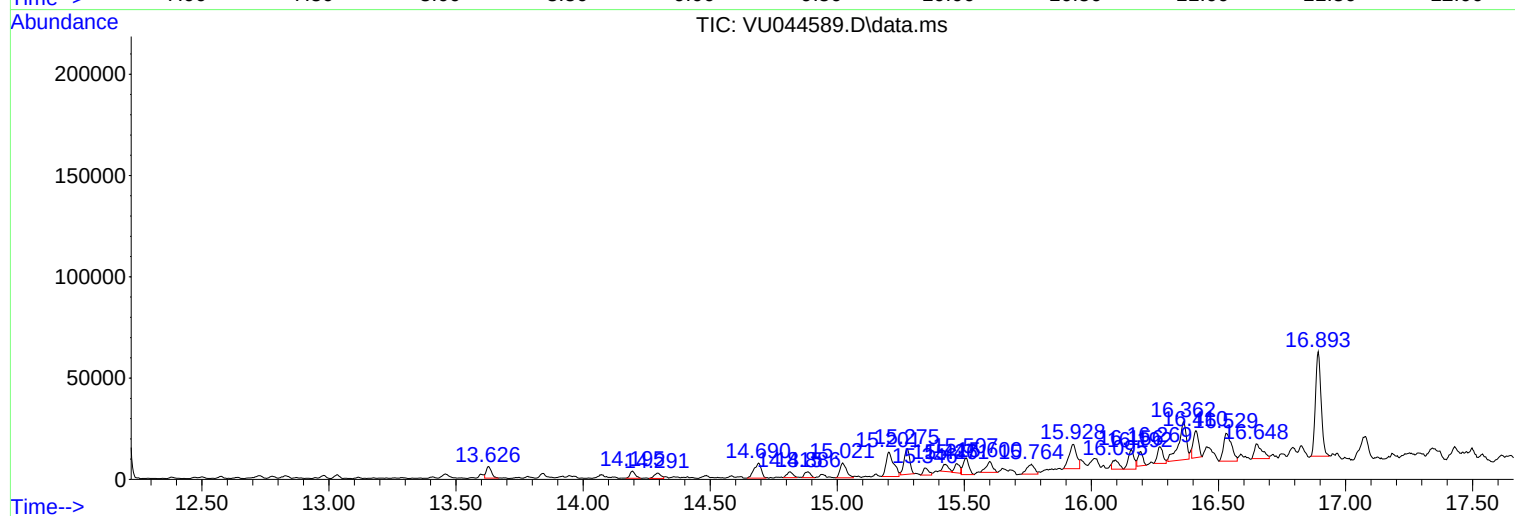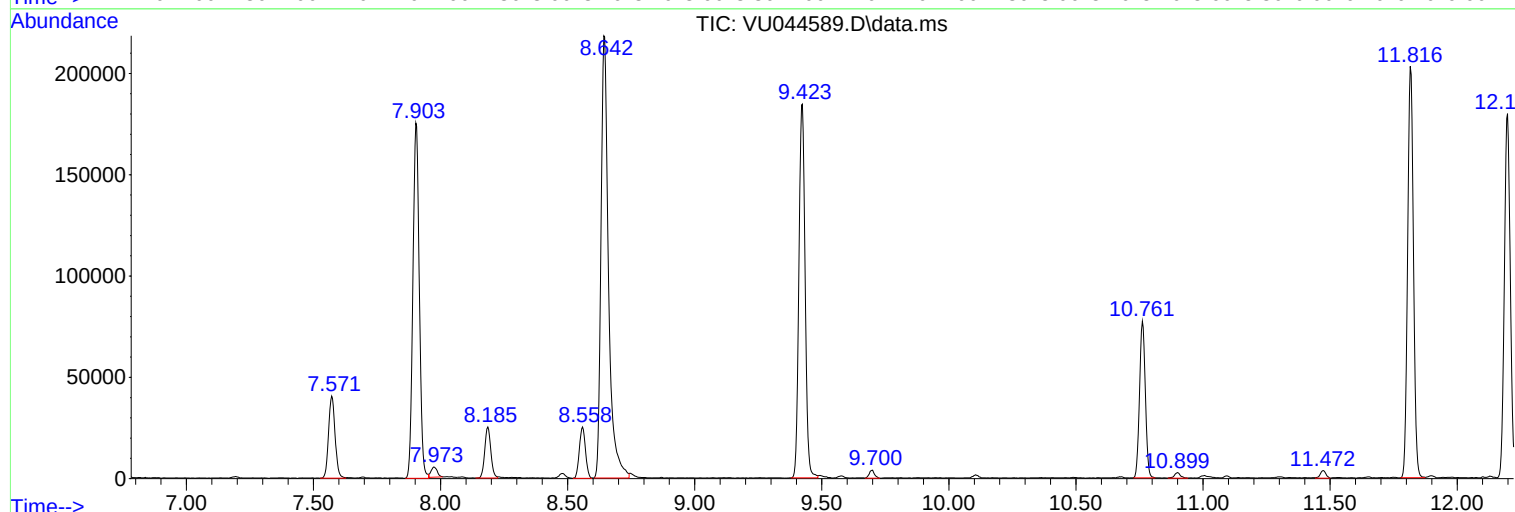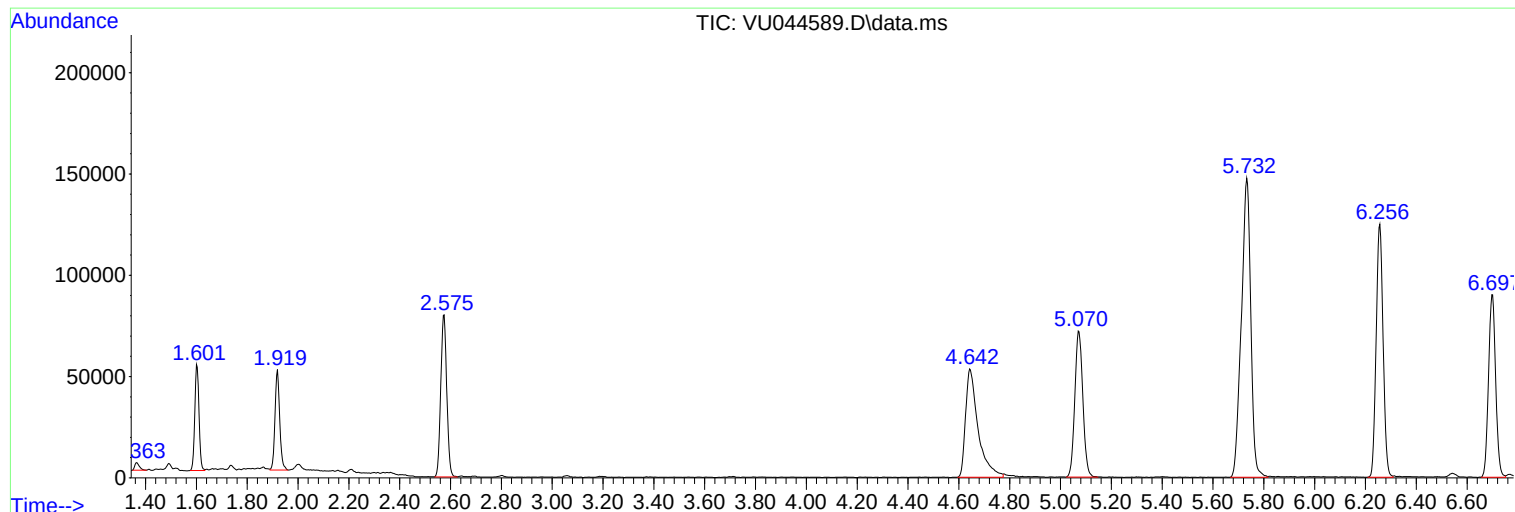

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044589.D
Acq On : 07 Sep 2021 17:27
Operator : SY/MD
Sample : M3647-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044589.D
Acq On : 07 Sep 2021 17:27
Operator : SY/MD
Sample : M3647-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F3W03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
