


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090721\
Data File : VU044575.D
Acq On : 07 Sep 2021 10:08
Operator : SY/MD
Sample : BFB013
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB013

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR081821WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 09 07:35:45 2021

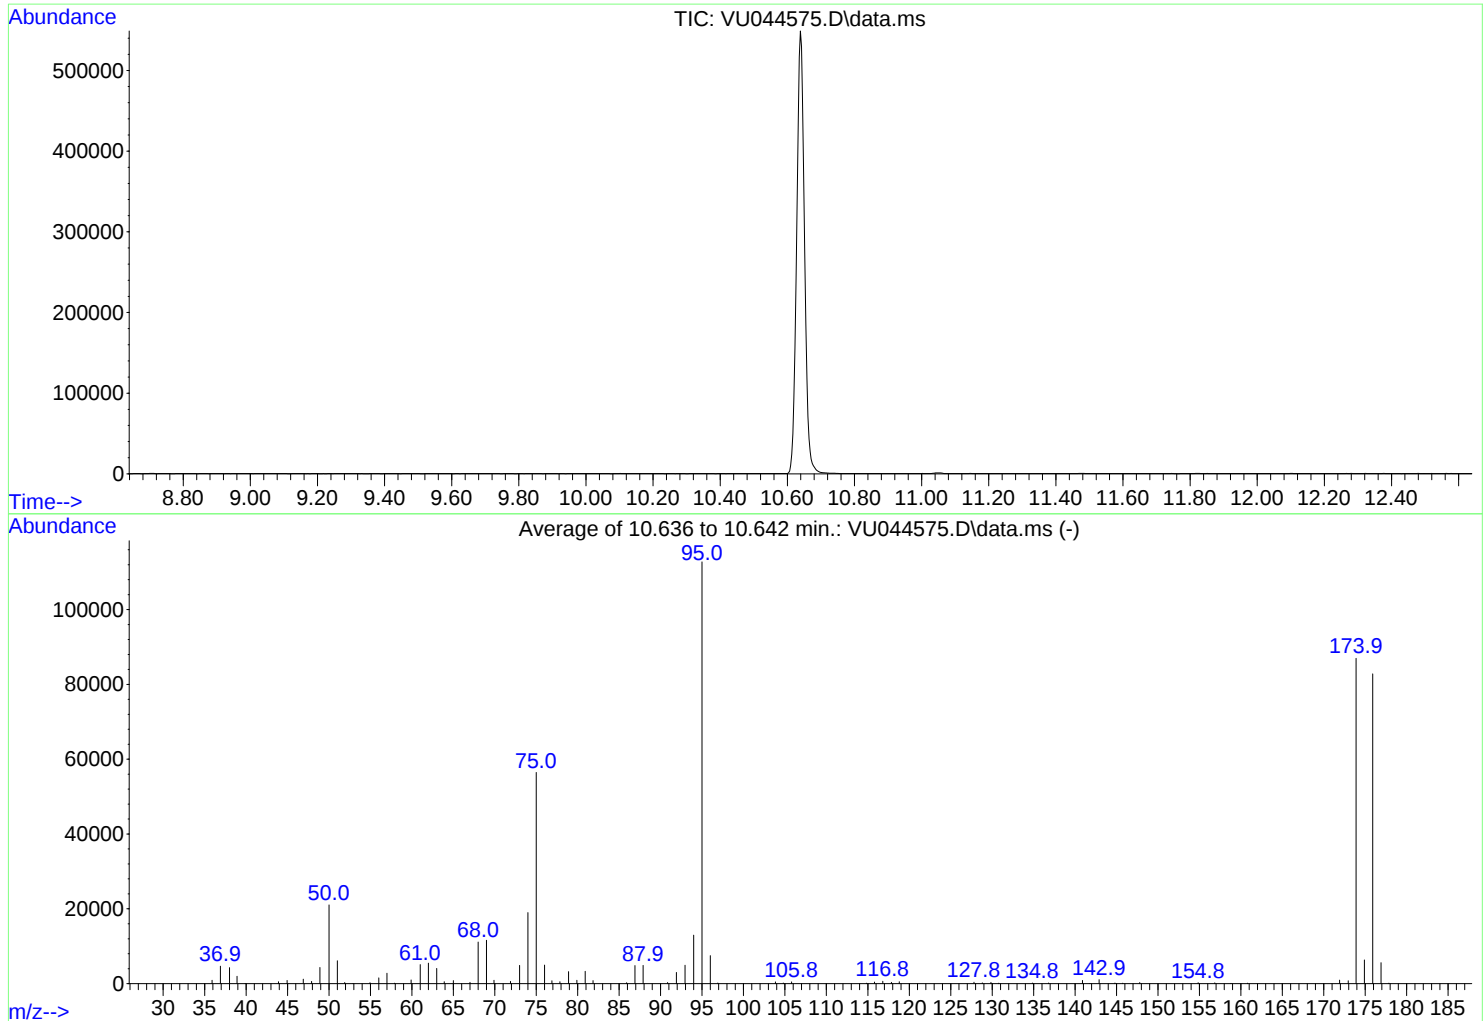

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	21048	PASS
75	95	30	80	50.1	56453	PASS
95	95	100	100	100.0	112768	PASS
96	95	5	9	6.7	7501	PASS
173	174	0.00	2	0.9	772	PASS
174	95	50	120	77.1	86965	PASS
175	174	5	9	7.3	6340	PASS
176	174	95	101	95.2	82813	PASS
177	176	5	9	6.8	5620	PASS

m/z	Abundance
35.90	979.0
36.90	4837.0
38.00	4413.0
38.90	2069.0
39.90	204.0
44.00	812.0
45.00	919.0
46.90	1262.0
47.90	637.0
48.90	4415.0
50.00	21856.0
51.00	6310.0
51.90	334.0
55.00	275.0
56.00	1610.0
57.00	2898.0
57.90	122.0
59.90	1017.0
61.00	5272.0
62.00	5684.0
63.00	4167.0
63.90	544.0
65.00	843.0
67.00	371.0
68.00	11509.0
69.00	11960.0
69.90	946.0
71.90	634.0
73.00	5040.0
74.00	19656.0
75.00	58304.0
76.00	5146.0
76.90	796.0
77.80	523.0
78.90	3334.0
79.90	904.0
80.90	3418.0
81.80	849.0
85.90	254.0
86.90	4929.0
87.90	5063.0
90.90	308.0
91.90	3102.0
92.90	5095.0
94.00	13391.0
95.00	116328.0
96.00	7707.0
96.90	178.0
103.90	512.0
104.80	207.0
105.80	516.0
114.80	124.0
115.80	434.0
116.80	653.0
117.80	359.0
118.80	549.0
127.80	391.0
128.80	218.0
129.80	355.0
130.80	135.0
134.80	158.0
136.80	171.0
140.90	885.0
142.90	1103.0
144.80	184.0
145.70	130.0
147.80	322.0
154.80	241.0
156.90	191.0
158.80	122.0
160.80	133.0
171.90	976.0
173.00	768.0
173.90	89768.0
174.90	6576.0
175.90	85488.0
176.90	5826.0
177.80	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	868.0
36.90	4722.0
38.00	4311.0
38.90	1979.0
40.00	209.0
44.00	755.0
44.90	844.0
46.90	1204.0
47.90	562.0
48.90	4328.0
50.00	20808.0
51.00	6064.0
51.90	327.0
55.00	235.0
56.00	1471.0
57.00	2760.0
57.90	130.0
59.90	990.0
61.00	5043.0
62.00	5394.0
63.00	4024.0
63.90	524.0
65.00	740.0
67.00	378.0
68.00	10925.0
69.00	11387.0
69.90	870.0
71.90	605.0
73.00	4725.0
74.00	18576.0
75.00	55496.0
76.00	4859.0
76.90	771.0
77.80	530.0
78.90	3129.0
79.90	893.0
80.90	3223.0
81.80	823.0
85.90	269.0
86.90	4997.0
87.90	4729.0
90.80	320.0
91.90	3021.0
93.00	4883.0
94.00	12520.0
95.00	109720.0
96.00	7439.0
96.90	236.0
103.80	453.0
104.80	201.0
105.80	502.0
114.80	132.0
115.80	360.0
116.80	645.0
117.90	361.0
118.80	501.0
127.80	390.0
128.80	194.0
129.90	338.0
130.80	130.0
134.90	105.0
136.80	139.0
140.90	823.0
142.90	1098.0
144.80	239.0
145.80	152.0
147.80	298.0
154.80	258.0
156.90	144.0
158.80	102.0
160.80	123.0
171.90	959.0
172.90	737.0
173.90	82968.0
174.90	6111.0
175.90	78816.0
176.90	5427.0
177.90	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

Scan 2878 (10.594 min): VU044575.D\data.ms
BFB013

m/z	Abundance
39.90	162.0
43.80	270.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	917.0
36.90	4491.0
38.00	4099.0
38.90	1859.0
39.80	203.0
43.90	816.0
45.00	865.0
46.90	1195.0
47.90	637.0
48.90	4169.0
50.00	20480.0
51.00	5986.0
51.90	285.0
52.90	105.0
54.90	267.0
56.00	1530.0
57.00	2711.0
57.90	102.0
59.90	949.0
61.00	4946.0
62.00	5373.0
63.00	3991.0
63.90	513.0
65.00	889.0
67.00	322.0
68.00	10985.0
69.00	11475.0
69.90	931.0
71.90	602.0
73.00	4831.0
74.00	18808.0
75.00	55560.0
76.00	4885.0
76.90	723.0
77.90	482.0
78.90	3230.0
79.90	880.0
80.90	3303.0
81.90	779.0
85.90	203.0
86.90	4559.0
87.90	4841.0
90.80	305.0
91.90	2886.0
92.90	4811.0
94.00	12987.0
95.00	112256.0
96.00	7357.0
96.90	142.0
103.90	509.0
104.80	175.0
105.80	464.0
114.90	108.0
115.80	450.0
116.80	598.0
117.80	360.0
118.80	527.0
127.80	356.0
128.80	205.0
129.80	326.0
130.80	134.0
134.80	201.0
136.80	194.0
140.90	861.0
141.80	108.0
142.90	1022.0
144.80	126.0
145.70	102.0
147.80	301.0
154.90	244.0
156.80	259.0
158.80	107.0
160.80	109.0
171.90	939.0
173.00	810.0
173.90	88160.0
174.90	6333.0
175.90	84136.0
176.90	5608.0
177.80	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013