

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050661.D
 Acq On : 07 Sep 2022 15:27
 Operator : SY/MD
 Sample : N4482-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW350

Quant Time: Sep 08 05:43:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 07 01:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	289631	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	289150	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	107155	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	91153	36.796	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.600%
7) Chloroethane-d5	1.906	69	72135	43.060	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.120%
11) 1,1-Dichloroethene-d2	2.562	63	139142	31.785	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.560%
21) 2-Butanone-d5	4.629	46	167311	92.313	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.310%
24) Chloroform-d	5.060	84	231867	49.385	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.780%
26) 1,2-Dichloroethane-d4	5.700	65	155205	54.096	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.200%
32) Benzene-d6	5.726	84	449828	47.075	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.160%
36) 1,2-Dichloropropane-d6	6.690	67	150034	47.823	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.640%
41) Toluene-d8	7.896	98	376612	46.089	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.180%
43) trans-1,3-Dichloroprop...	8.179	79	65283	50.293	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.580%
47) 2-Hexanone-d5	8.636	63	64630	81.900	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.900%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	224258	47.237	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.480%
66) 1,2-Dichlorobenzene-d4	12.192	152	125750	50.131	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.260%
Target Compounds						
13) Acetone	2.636	43	11527	8.431	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050661.D
Acq On : 07 Sep 2022 15:27
Operator : SY/MD
Sample : N4482-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW350

Quant Time: Sep 08 05:43:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 07 01:37:50 2022
Response via : Initial Calibration

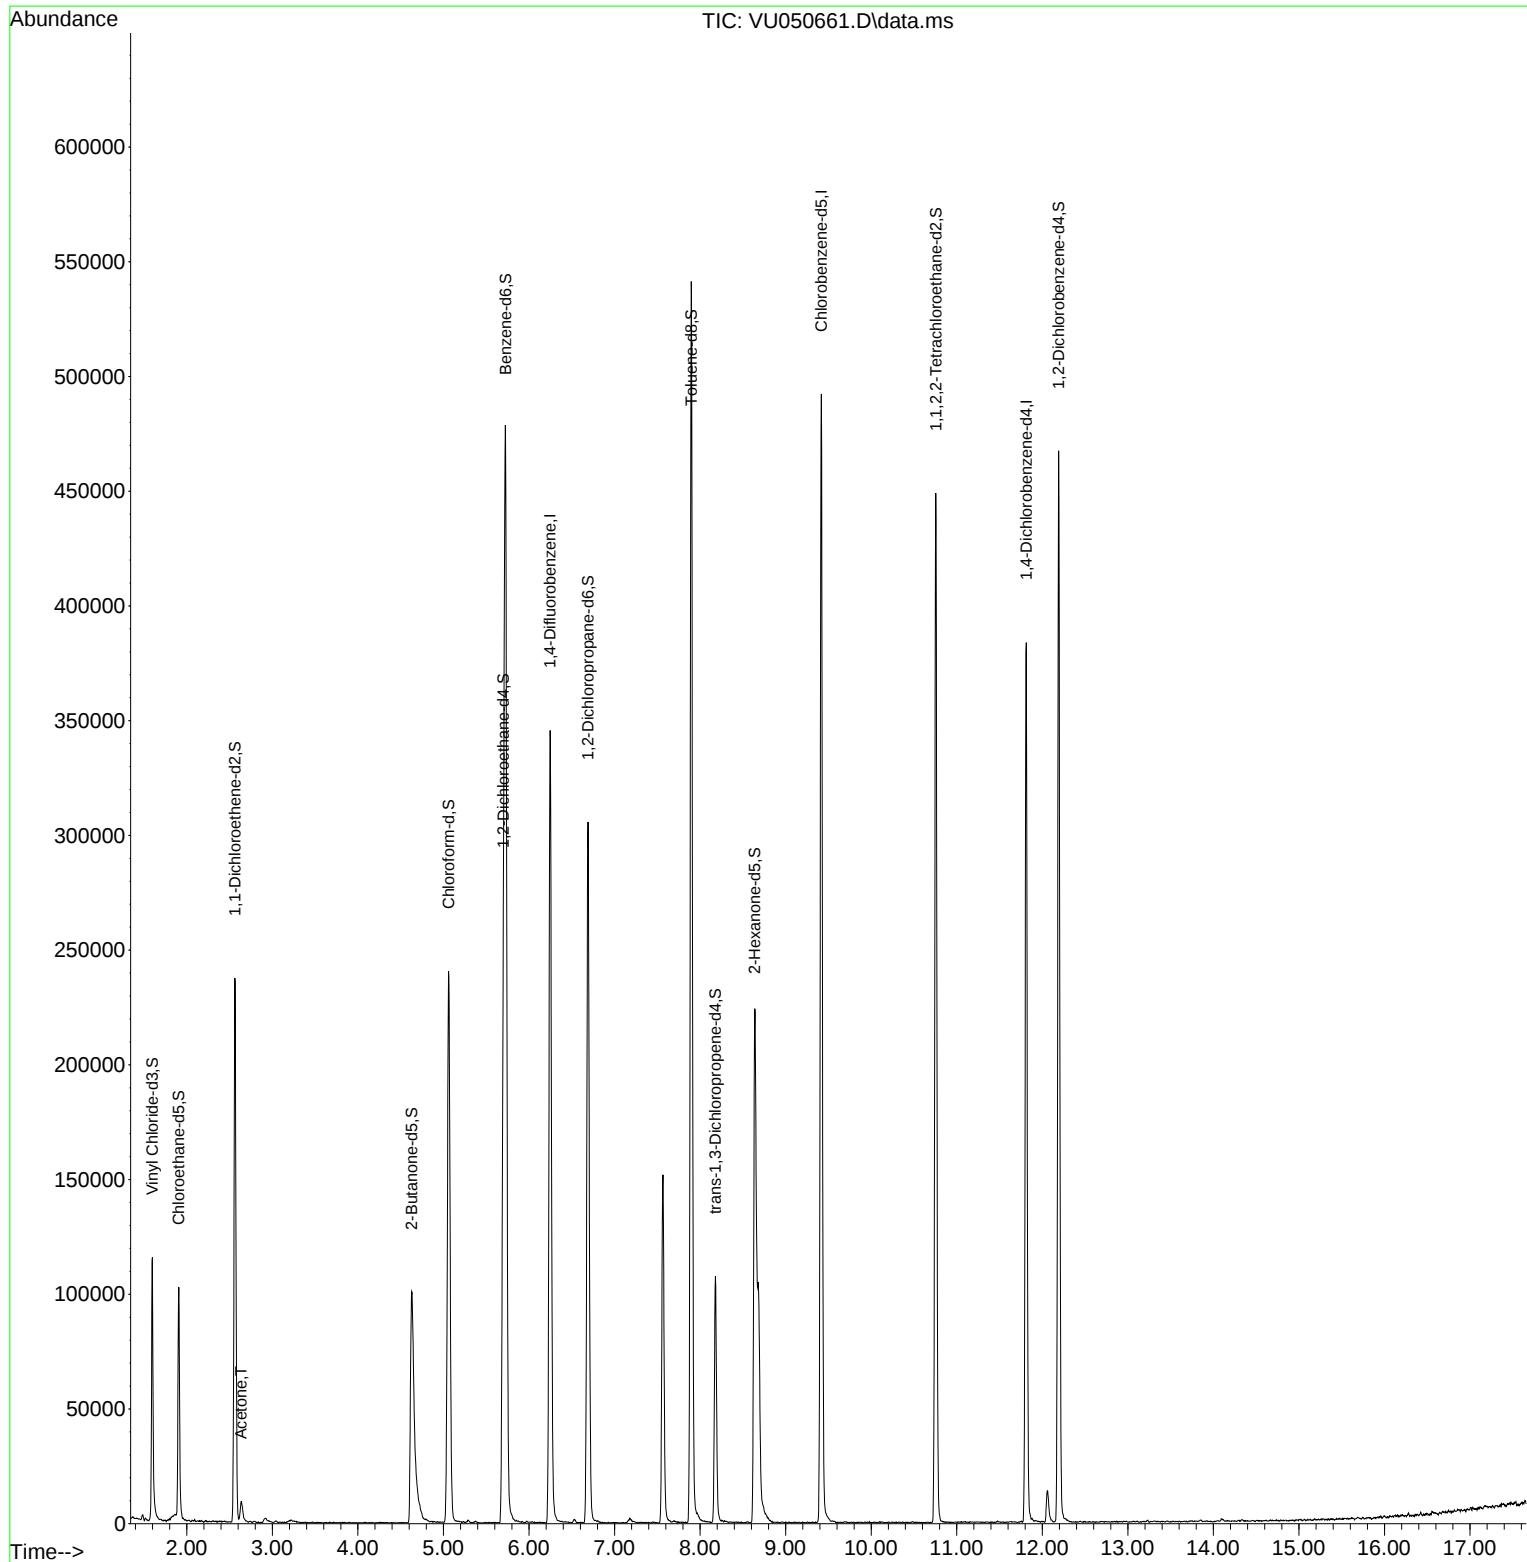

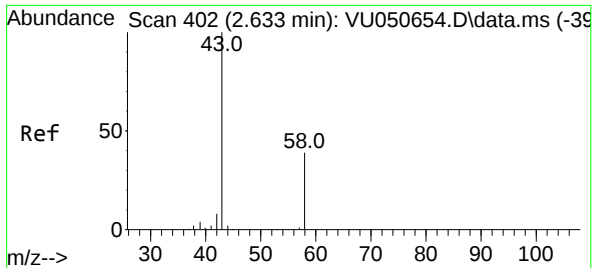

#13
 Acetone
 Concen: 8.431 ug/L
 RT: 2.636 min Scan# 40
 Delta R.T. 0.013 min
 Lab File: VU050661.D
 Acq: 07 Sep 2022 15:27

Instrument :
 MSVOA_U
 ClientSampleId :
 EW350

Tgt Ion: 43 Resp: 11527
 Ion Ratio Lower Upper
 43 100
 58 37.5 0.0 76.2

