

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050671.D
 Acq On : 07 Sep 2022 19:26
 Operator : SY/MD
 Sample : N4482-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Quant Time: Sep 08 05:44:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 07 01:37:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	643178	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	614058	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	239620	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	203903	37.065	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	74.140%	
7) Chloroethane-d5	1.899	69	156137	41.971	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	83.940%	
11) 1,1-Dichloroethene-d2	2.562	63	299140	30.771	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	61.540%	
21) 2-Butanone-d5	4.616	46	315888	78.485	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	78.480%	
24) Chloroform-d	5.060	84	467529	44.842	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.680%	
26) 1,2-Dichloroethane-d4	5.700	65	300196	47.117	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.240%	
32) Benzene-d6	5.726	84	928508	45.756	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.520%	
36) 1,2-Dichloropropane-d6	6.690	67	299869	45.009	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	90.020%	
41) Toluene-d8	7.896	98	809823	46.667	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.340%	
43) trans-1,3-Dichloroprop...	8.179	79	128104	46.471	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.940%	
47) 2-Hexanone-d5	8.632	63	128591	76.731	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	76.730%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	451779	44.810	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	89.620%	
66) 1,2-Dichlorobenzene-d4	12.192	152	274769	48.984	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.960%	
Target Compounds						
13) Acetone	2.626	43	9597	3.161	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050671.D
Acq On : 07 Sep 2022 19:26
Operator : SY/MD
Sample : N4482-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW348

Quant Time: Sep 08 05:44:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 07 01:37:50 2022
Response via : Initial Calibration

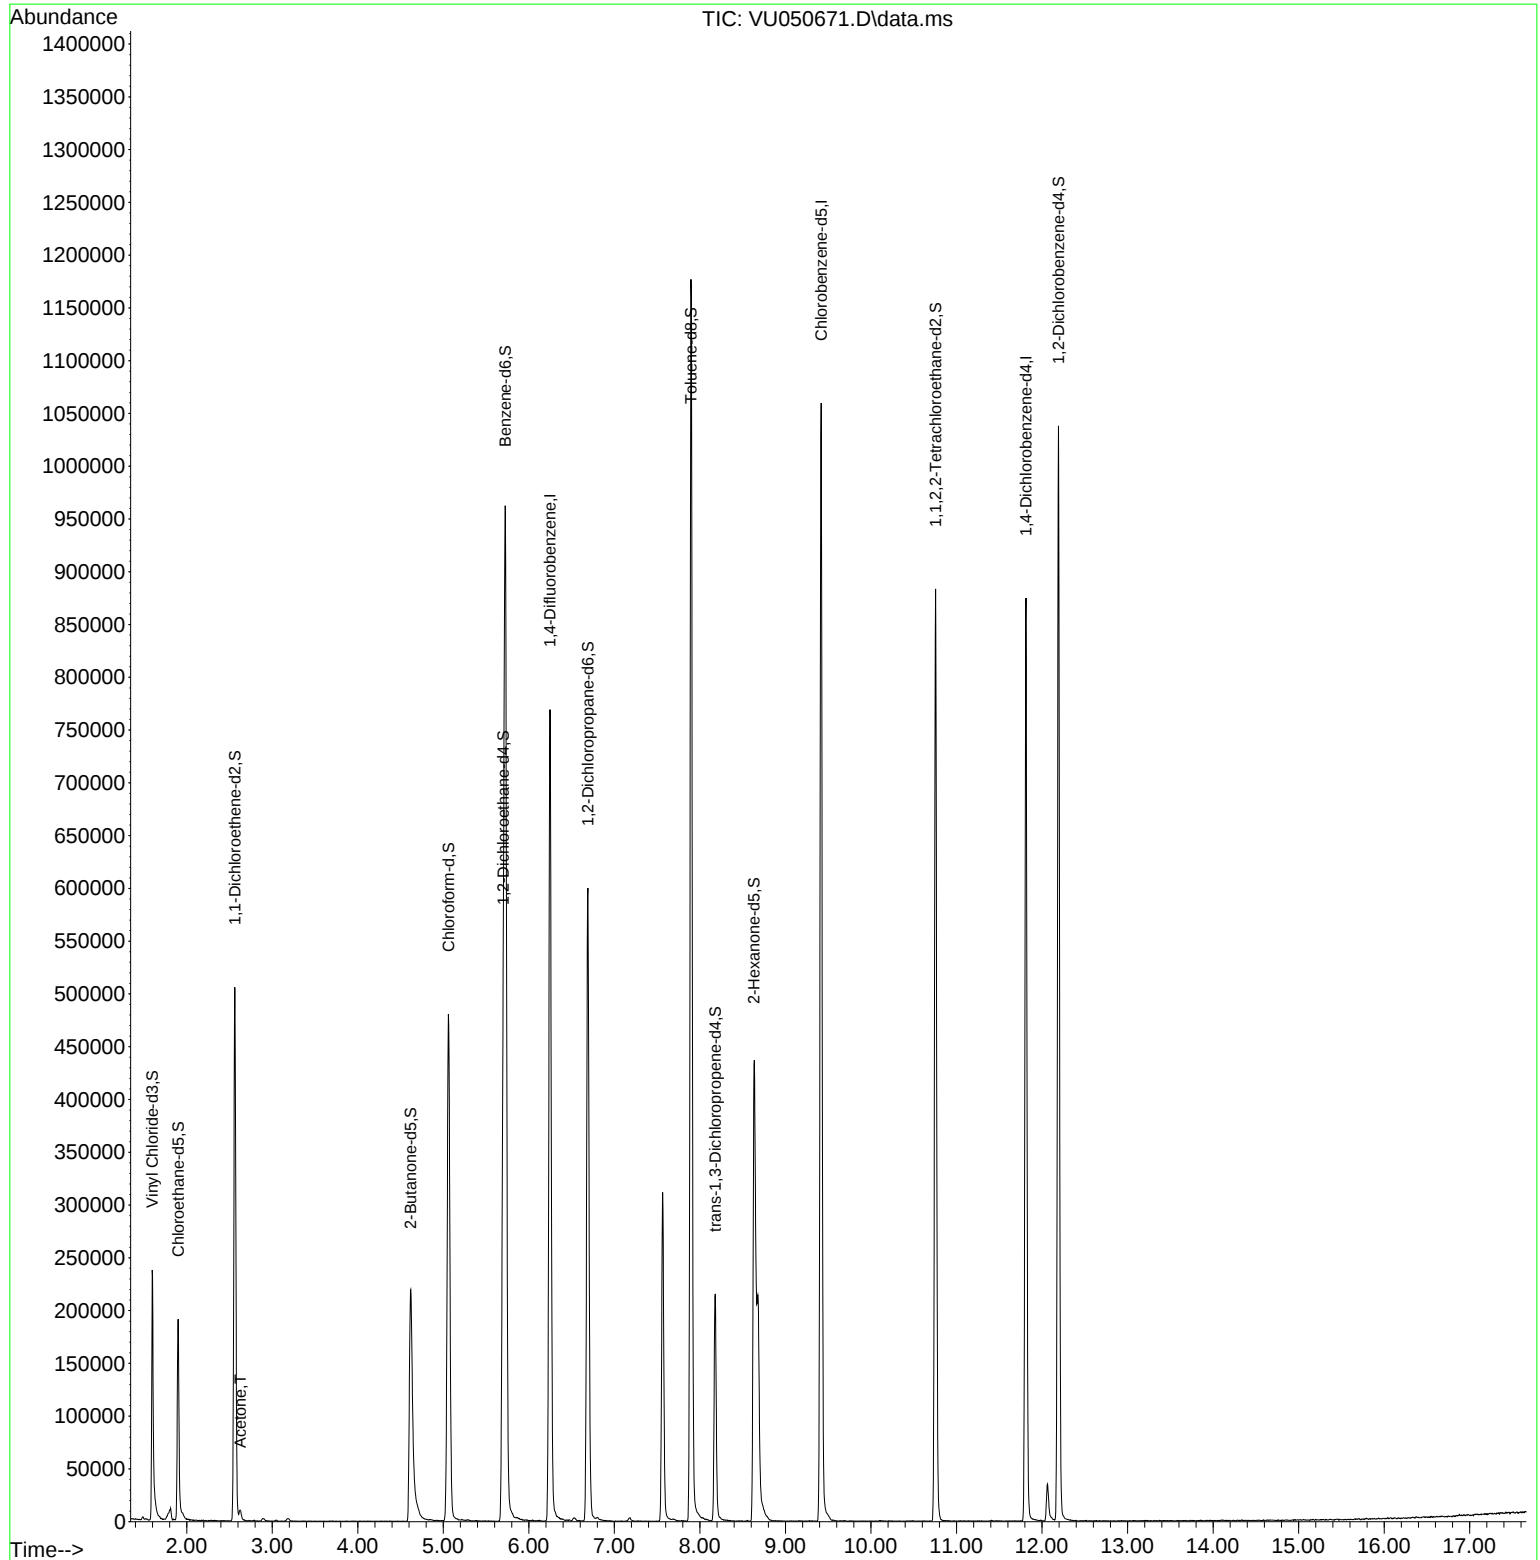

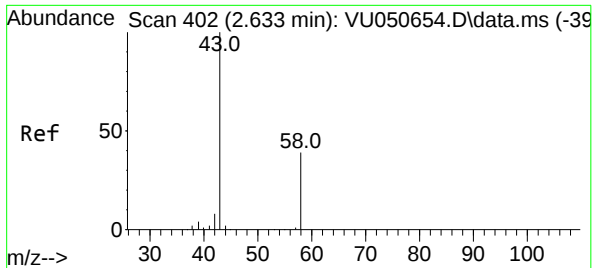

#13
 Acetone
 Concen: 3.161 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU050671.D
 Acq: 07 Sep 2022 19:26

Instrument :
 MSVOA_U
 ClientSampleId :
 EW348

Tgt Ion: 43 Resp: 9597
 Ion Ratio Lower Upper
 43 100
 58 40.3 0.0 76.2

