

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050657.D
 Acq On : 07 Sep 2022 13:55
 Operator : SY/MD
 Sample : N4481-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rVB5	3069	3507	0.24%	0.034%
2	1.597	72	80	103	rBV	155185	187437	12.80%	1.807%
3	1.909	169	177	196	rVB	123648	160642	10.97%	1.548%
4	2.025	209	213	217	rVB4	628	555	0.04%	0.005%
5	2.063	223	225	228	rVB2	751	343	0.02%	0.003%
6	2.115	239	241	244	rVB2	374	200	0.01%	0.002%
7	2.141	247	249	252	rBV3	465	276	0.02%	0.003%
8	2.179	258	261	263	rBV	393	242	0.02%	0.002%
9	2.234	276	278	281	rVB2	353	225	0.02%	0.002%
10	2.295	292	297	298	rBV2	365	310	0.02%	0.003%
11	2.398	327	329	334	rVB3	411	316	0.02%	0.003%
12	2.565	369	381	397	rBV	309042	501709	34.26%	4.836%
13	2.732	431	433	437	rVB2	426	219	0.01%	0.002%
14	2.774	443	446	447	rVV	460	269	0.02%	0.003%
15	2.787	447	450	461	rVB2	1220	1509	0.10%	0.015%
16	2.906	485	487	492	rVB3	429	294	0.02%	0.003%
17	2.973	505	508	511	rVV2	293	198	0.01%	0.002%
18	3.047	524	531	537	rBV3	789	1122	0.08%	0.011%
19	3.125	552	555	559	rBV2	241	227	0.02%	0.002%
20	3.179	563	572	584	rVV3	2037	4182	0.29%	0.040%
21	3.568	690	693	702	rVB2	376	496	0.03%	0.005%
22	3.607	702	705	707	rBV	368	197	0.01%	0.002%
23	3.909	796	799	802	rVB2	301	221	0.02%	0.002%
24	4.051	839	843	848	rBV2	252	220	0.02%	0.002%
25	4.343	928	934	938	rBV2	221	214	0.01%	0.002%
26	4.427	954	960	963	rBV2	273	365	0.02%	0.004%
27	4.629	1010	1023	1064	rBV	104606	339177	23.16%	3.269%
28	4.819	1080	1082	1087	rVB3	610	375	0.03%	0.004%
29	4.999	1135	1138	1141	rBV3	338	289	0.02%	0.003%
30	5.063	1141	1158	1186	rBV	266441	585443	39.98%	5.643%
31	5.179	1192	1194	1198	rBV2	389	250	0.02%	0.002%
32	5.231	1207	1210	1212	rBV2	279	200	0.01%	0.002%
33	5.272	1219	1223	1224	rBV2	666	339	0.02%	0.003%
34	5.372	1248	1254	1255	rBV3	441	478	0.03%	0.005%
35	5.726	1341	1364	1400	rVV2	548156	1464207	100.00%	14.113%
36	5.996	1445	1448	1453	rBV2	222	233	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050657.D
 Acq On : 07 Sep 2022 13:55
 Operator : SY/MD
 Sample : N4481-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.041	1458	1462	1464	rBV3	397	340	0.02%	0.003%
38	6.118	1480	1486	1490	rVB4	378	472	0.03%	0.005%
39	6.250	1510	1527	1551	rBV	391324	752066	51.36%	7.249%
40	6.536	1604	1616	1625	rBV9	2394	5166	0.35%	0.050%
41	6.690	1647	1664	1692	rBV	331954	651593	44.50%	6.281%
42	6.832	1707	1708	1713	rVB	510	271	0.02%	0.003%
43	6.858	1713	1716	1718	rBV	352	193	0.01%	0.002%
44	7.144	1802	1805	1808	rBV	328	235	0.02%	0.002%
45	7.185	1812	1818	1819	rBV2	787	654	0.04%	0.006%
46	7.375	1871	1877	1881	rBV2	337	457	0.03%	0.004%
47	7.414	1881	1889	1894	rVB2	317	508	0.03%	0.005%
48	7.501	1912	1916	1920	rBV2	448	371	0.03%	0.004%
49	7.565	1924	1936	1956	rBV	167745	302913	20.69%	2.920%
50	7.748	1991	1993	1998	rVB	375	257	0.02%	0.002%
51	7.800	2004	2009	2013	rVV2	541	608	0.04%	0.006%
52	7.819	2013	2015	2020	rVB3	444	268	0.02%	0.003%
53	7.899	2025	2040	2066	rBV	654902	1144405	78.16%	11.031%
54	8.179	2115	2127	2148	rBV	116591	206103	14.08%	1.987%
55	8.292	2159	2162	2166	rBV4	372	235	0.02%	0.002%
56	8.430	2203	2205	2212	rVB2	265	243	0.02%	0.002%
57	8.555	2234	2244	2254	rBV7	7480	12241	0.84%	0.118%
58	8.642	2257	2271	2316	rBV7	222483	704166	48.09%	6.787%
59	8.854	2332	2337	2343	rBV2	628	736	0.05%	0.007%
60	8.944	2363	2365	2372	rVB	262	191	0.01%	0.002%
61	8.986	2375	2378	2382	rBV2	337	264	0.02%	0.003%
62	9.028	2389	2391	2394	rBV2	353	249	0.02%	0.002%
63	9.263	2461	2464	2468	rBV2	238	213	0.01%	0.002%
64	9.417	2499	2512	2546	rBV	537446	914182	62.44%	8.812%
65	9.645	2582	2583	2589	rVB	322	210	0.01%	0.002%
66	9.703	2599	2601	2604	rVB2	543	292	0.02%	0.003%
67	10.034	2702	2704	2710	rVB2	253	214	0.01%	0.002%
68	10.073	2710	2716	2719	rBV	252	249	0.02%	0.002%
69	10.095	2719	2723	2727	rBV3	428	425	0.03%	0.004%
70	10.378	2808	2811	2820	rVB2	270	297	0.02%	0.003%
71	10.481	2840	2843	2846	rBV3	326	220	0.02%	0.002%
72	10.648	2892	2895	2901	rBV2	224	214	0.01%	0.002%
73	10.754	2915	2928	2952	rBV	468523	757318	51.72%	7.300%
74	10.877	2964	2966	2970	rVB2	426	238	0.02%	0.002%
75	10.915	2970	2978	2982	rBV	417	477	0.03%	0.005%
76	11.034	3012	3015	3024	rVB2	353	362	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050657.D
 Acq On : 07 Sep 2022 13:55
 Operator : SY/MD
 Sample : N4481-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBVF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.137	3044	3047	3053	rVB2	250	214	0.01%	0.002%
78	11.224	3071	3074	3077	rBV	383	316	0.02%	0.003%
79	11.404	3124	3130	3132	rBV2	213	247	0.02%	0.002%
80	11.475	3145	3152	3161	rVB4	571	879	0.06%	0.008%
81	11.607	3190	3193	3197	rBV	274	212	0.01%	0.002%
82	11.745	3233	3236	3238	rBV2	698	416	0.03%	0.004%
83	11.812	3244	3257	3280	rBV	457451	734354	50.15%	7.078%
84	12.192	3361	3375	3393	rBV	548587	903216	61.69%	8.706%
85	12.349	3421	3424	3426	rVB2	787	463	0.03%	0.004%
86	12.555	3485	3488	3492	rBV	344	215	0.01%	0.002%
87	12.616	3502	3507	3510	rBV3	304	361	0.02%	0.003%
88	12.652	3515	3518	3523	rBV2	220	199	0.01%	0.002%
89	12.848	3577	3579	3583	rVB2	304	195	0.01%	0.002%
90	13.143	3668	3671	3678	rVB2	467	563	0.04%	0.005%
91	13.221	3689	3695	3697	rBV3	1349	1293	0.09%	0.012%
92	13.278	3710	3713	3719	rBV3	372	356	0.02%	0.003%
93	13.304	3719	3721	3727	rBV2	295	306	0.02%	0.003%
94	13.851	3883	3891	3899	rVB5	2529	3792	0.26%	0.037%
95	14.095	3961	3967	3977	rBV4	3056	5207	0.36%	0.050%
96	14.256	4015	4017	4021	rBV2	405	349	0.02%	0.003%
97	14.336	4036	4042	4052	rVB5	2416	3986	0.27%	0.038%
98	14.375	4052	4054	4058	rVB2	454	283	0.02%	0.003%
99	14.645	4136	4138	4141	rBV	552	458	0.03%	0.004%
100	14.886	4210	4213	4214	rBV	512	329	0.02%	0.003%




Sum of corrected areas: 10374811

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050657.D
Acq On : 07 Sep 2022 13:55
Operator : SY/MD
Sample : N4481-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

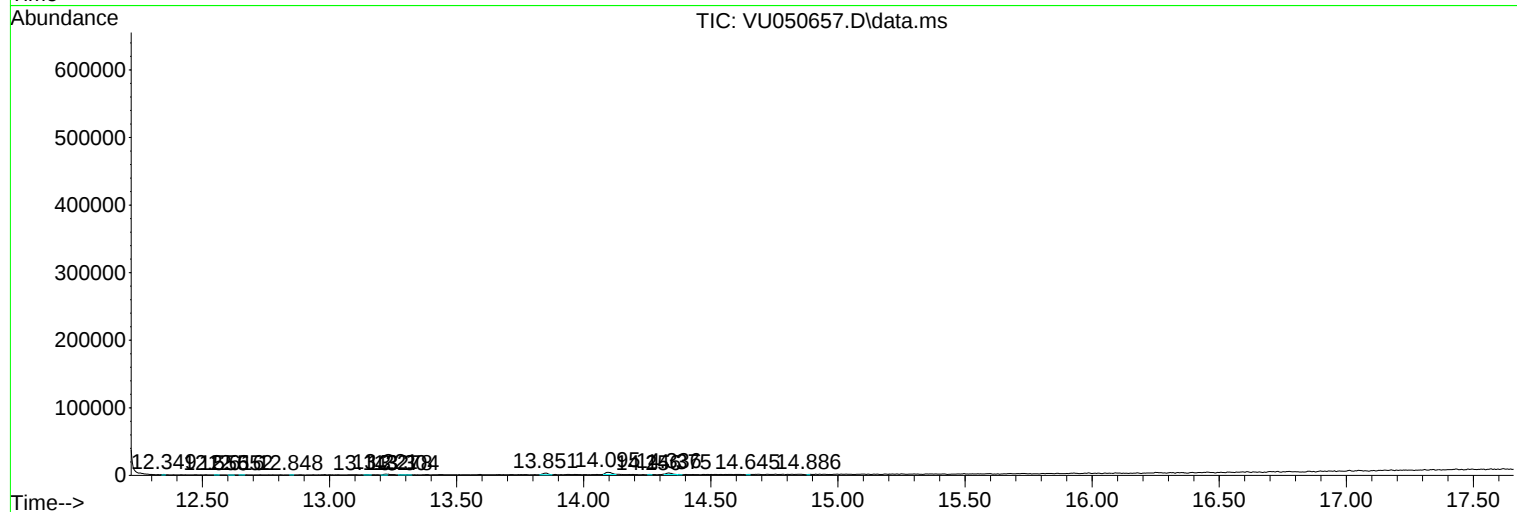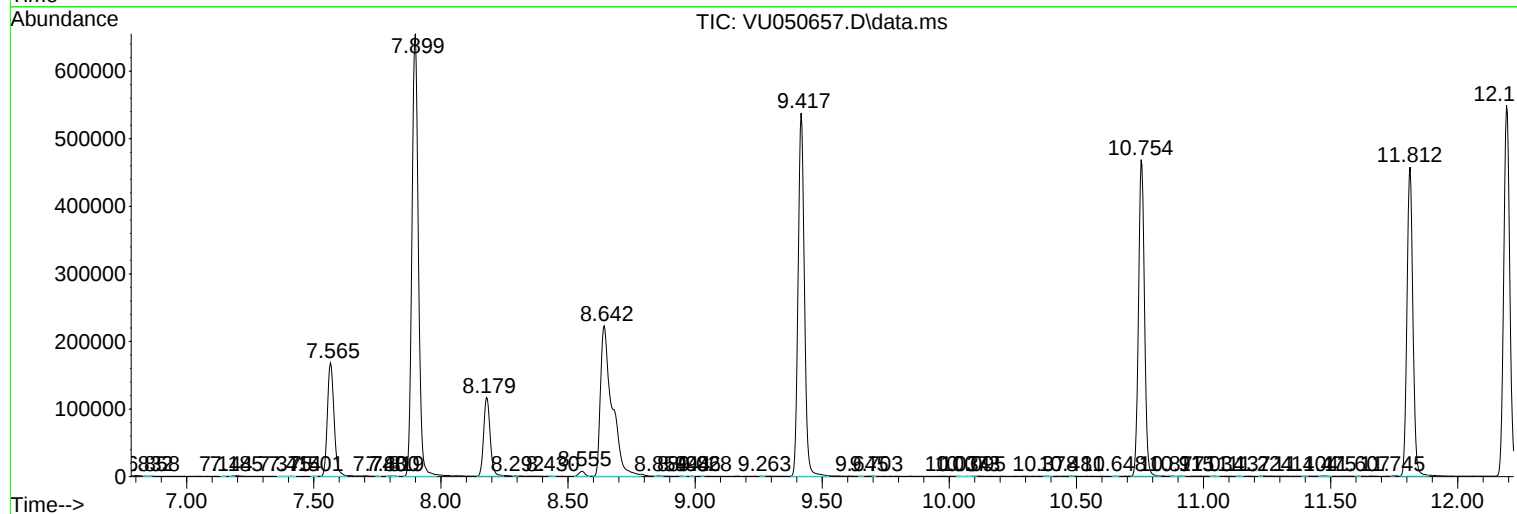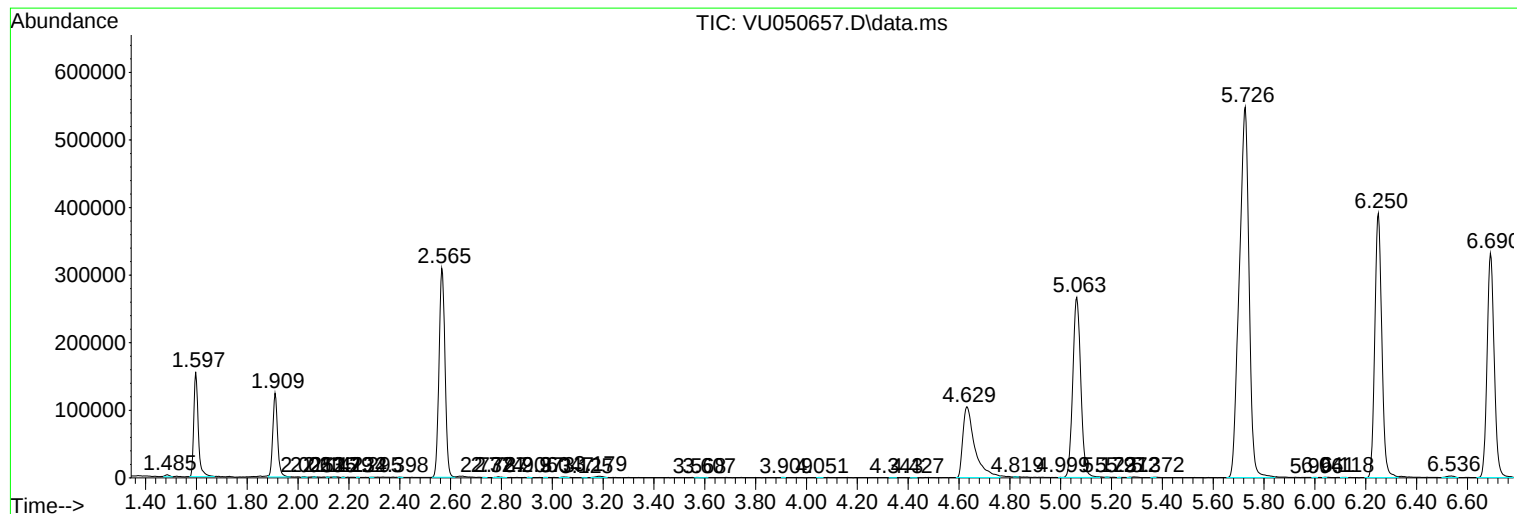

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050657.D
Acq On : 07 Sep 2022 13:55
Operator : SY/MD
Sample : N4481-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050657.D
Acq On : 07 Sep 2022 13:55
Operator : SY/MD
Sample : N4481-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBVF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------