

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050658.D
 Acq On : 07 Sep 2022 14:18
 Operator : SY/MD
 Sample : N4481-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	110	rVB	151118	184547	12.64%	1.785%
2	1.909	169	177	203	rVB	121032	162145	11.10%	1.568%
3	2.279	289	292	293	rBV2	387	210	0.01%	0.002%
4	2.565	368	381	399	rBV	310406	504398	34.53%	4.878%
5	2.710	423	426	432	rBV3	265	255	0.02%	0.002%
6	2.974	505	508	513	rBV	302	260	0.02%	0.003%
7	3.453	655	657	660	rBV	130	95	0.01%	0.001%
8	3.694	729	732	734	rBV	217	140	0.01%	0.001%
9	3.755	749	751	755	rBV2	76	49	0.00%	0.000%
10	3.787	758	761	765	rBV	236	195	0.01%	0.002%
11	3.832	771	775	781	rBV	305	362	0.02%	0.004%
12	4.018	827	833	837	rBV2	128	173	0.01%	0.002%
13	4.035	837	838	839	rBV	285	82	0.01%	0.001%
14	4.154	873	875	879	rBV	226	96	0.01%	0.001%
15	4.215	892	894	896	rBV	116	56	0.00%	0.001%
16	4.237	896	901	904	rVV2	166	163	0.01%	0.002%
17	4.443	962	965	969	rVB	185	160	0.01%	0.002%
18	4.469	969	973	976	rBV2	148	98	0.01%	0.001%
19	4.485	976	978	982	rVV	122	77	0.01%	0.001%
20	4.629	1010	1023	1067	rBV2	106680	340712	23.33%	3.295%
21	5.063	1141	1158	1181	rBV	264679	587346	40.21%	5.680%
22	5.289	1220	1228	1229	rBV3	1024	1126	0.08%	0.011%
23	5.353	1245	1248	1249	rBV	151	71	0.00%	0.001%
24	5.417	1265	1268	1269	rBV	156	94	0.01%	0.001%
25	5.726	1341	1364	1386	rBV2	540894	1460601	100.00%	14.124%
26	5.970	1438	1440	1442	rBV	282	170	0.01%	0.002%
27	6.076	1470	1473	1475	rBV2	513	233	0.02%	0.002%
28	6.150	1495	1496	1497	rBV	182	58	0.00%	0.001%
29	6.247	1512	1526	1551	rBV	405355	783468	53.64%	7.576%
30	6.530	1606	1614	1624	rVB5	2382	4370	0.30%	0.042%
31	6.575	1624	1628	1630	rBV	257	160	0.01%	0.002%
32	6.600	1635	1636	1637	rVB	238	46	0.00%	0.000%
33	6.690	1648	1664	1694	rBV	328751	651547	44.61%	6.301%
34	6.893	1724	1727	1730	rVB2	262	135	0.01%	0.001%
35	6.977	1750	1753	1759	rVB2	306	293	0.02%	0.003%
36	7.031	1767	1770	1773	rBV	123	80	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050658.D
 Acq On : 07 Sep 2022 14:18
 Operator : SY/MD
 Sample : N4481-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	7.051	1773	1776	1778	rBV	196	118	0.01%	0.001%
38	7.362	1870	1873	1876	rBV	283	219	0.01%	0.002%
39	7.417	1888	1890	1893	rVB2	223	126	0.01%	0.001%
40	7.469	1903	1906	1909	rBB	205	99	0.01%	0.001%
41	7.488	1909	1912	1913	rBV	172	106	0.01%	0.001%
42	7.565	1922	1936	1954	rBV	168732	300184	20.55%	2.903%
43	7.694	1973	1976	1978	rBV	620	468	0.03%	0.005%
44	7.735	1988	1989	1992	rBV	218	141	0.01%	0.001%
45	7.803	2009	2010	2011	rBV	199	65	0.00%	0.001%
46	7.896	2025	2039	2062	rBV	632068	1125024	77.02%	10.879%
47	8.179	2116	2127	2144	rBV2	114221	199271	13.64%	1.927%
48	8.462	2213	2215	2218	rVB2	315	179	0.01%	0.002%
49	8.478	2218	2220	2223	rBV	288	214	0.01%	0.002%
50	8.507	2227	2229	2230	rVV	176	50	0.00%	0.000%
51	8.571	2246	2249	2254	rBV2	204	154	0.01%	0.001%
52	8.639	2257	2270	2309	rBV7	223944	710772	48.66%	6.873%
53	8.954	2365	2368	2371	rBV2	316	186	0.01%	0.002%
54	9.173	2434	2436	2438	rVB	409	176	0.01%	0.002%
55	9.189	2438	2441	2443	rBV2	350	219	0.01%	0.002%
56	9.247	2456	2459	2461	rBV2	265	122	0.01%	0.001%
57	9.417	2498	2512	2535	rBV	545270	930941	63.74%	9.002%
58	9.645	2577	2583	2586	rBV3	544	485	0.03%	0.005%
59	9.809	2632	2634	2636	rBV2	187	107	0.01%	0.001%
60	9.864	2648	2651	2653	rVB	223	108	0.01%	0.001%
61	10.047	2705	2708	2714	rBV2	282	274	0.02%	0.003%
62	10.102	2723	2725	2729	rBV2	221	138	0.01%	0.001%
63	10.121	2729	2731	2735	rVB2	432	248	0.02%	0.002%
64	10.456	2832	2835	2838	rBV	281	166	0.01%	0.002%
65	10.587	2873	2876	2880	rBV2	220	200	0.01%	0.002%
66	10.755	2916	2928	2949	rBV	464156	759146	51.97%	7.341%
67	11.407	3128	3131	3135	rBV2	559	422	0.03%	0.004%
68	11.468	3147	3150	3152	rBV2	500	393	0.03%	0.004%
69	11.539	3169	3172	3174	rBV2	220	140	0.01%	0.001%
70	11.597	3188	3190	3196	rVB	318	221	0.02%	0.002%
71	11.745	3232	3236	3238	rBV	593	528	0.04%	0.005%
72	11.812	3244	3257	3277	rBV	457190	740291	50.68%	7.159%
73	12.044	3327	3329	3330	rBV	194	78	0.01%	0.001%
74	12.192	3362	3375	3406	rBV	538314	883131	60.46%	8.540%
75	12.382	3432	3434	3435	rBV	381	106	0.01%	0.001%
76	12.783	3554	3559	3561	rBV2	501	434	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050658.D
Acq On : 07 Sep 2022 14:18
Operator : SY/MD
Sample : N4481-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Title : VOC Analysis

77	13.025	3628	3634	3638	rBV	567	723	0.05%	0.007%
78	13.401	3745	3751	3756	rBV3	503	787	0.05%	0.008%




Sum of corrected areas: 10341031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050658.D
Acq On : 07 Sep 2022 14:18
Operator : SY/MD
Sample : N4481-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

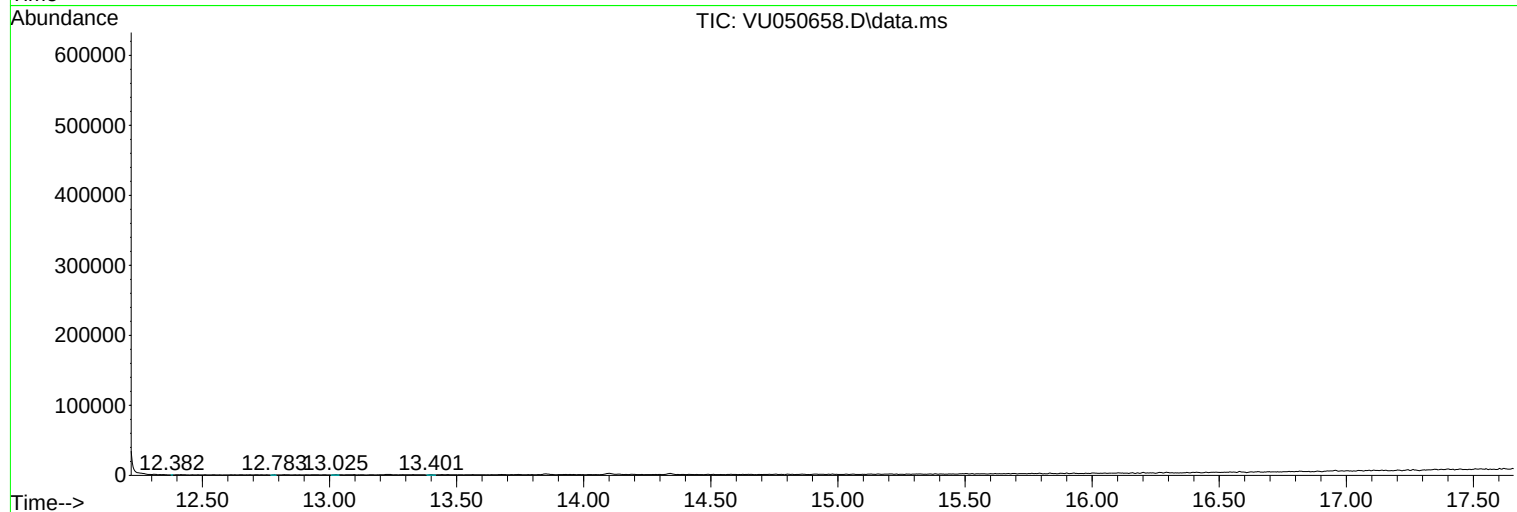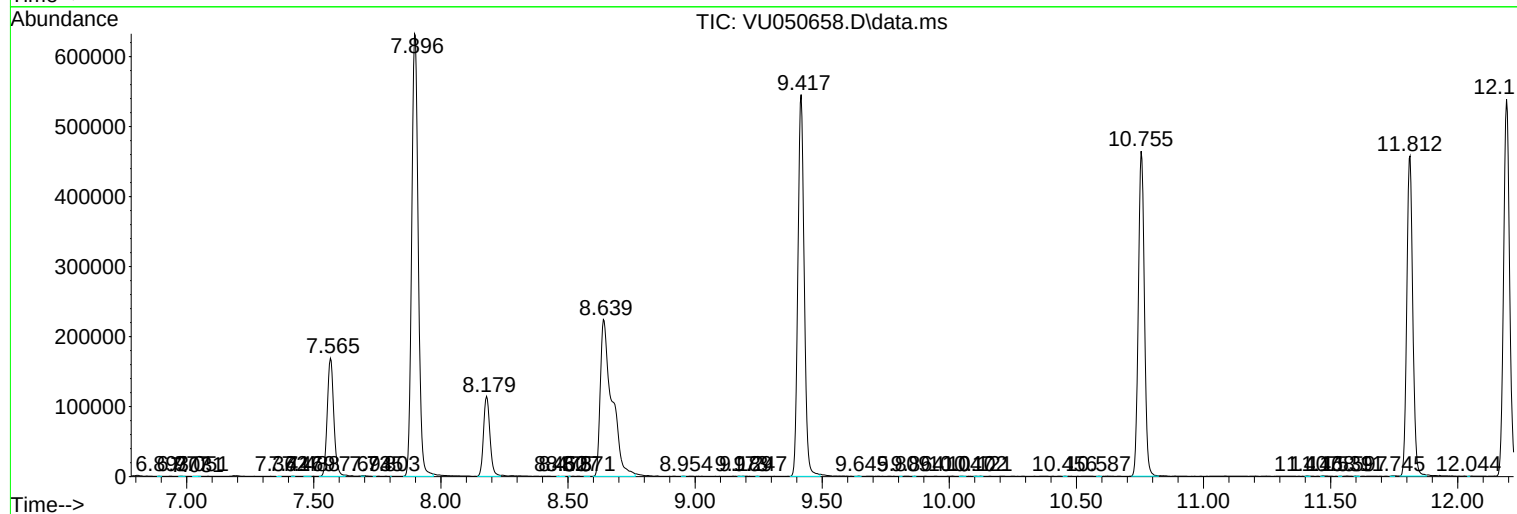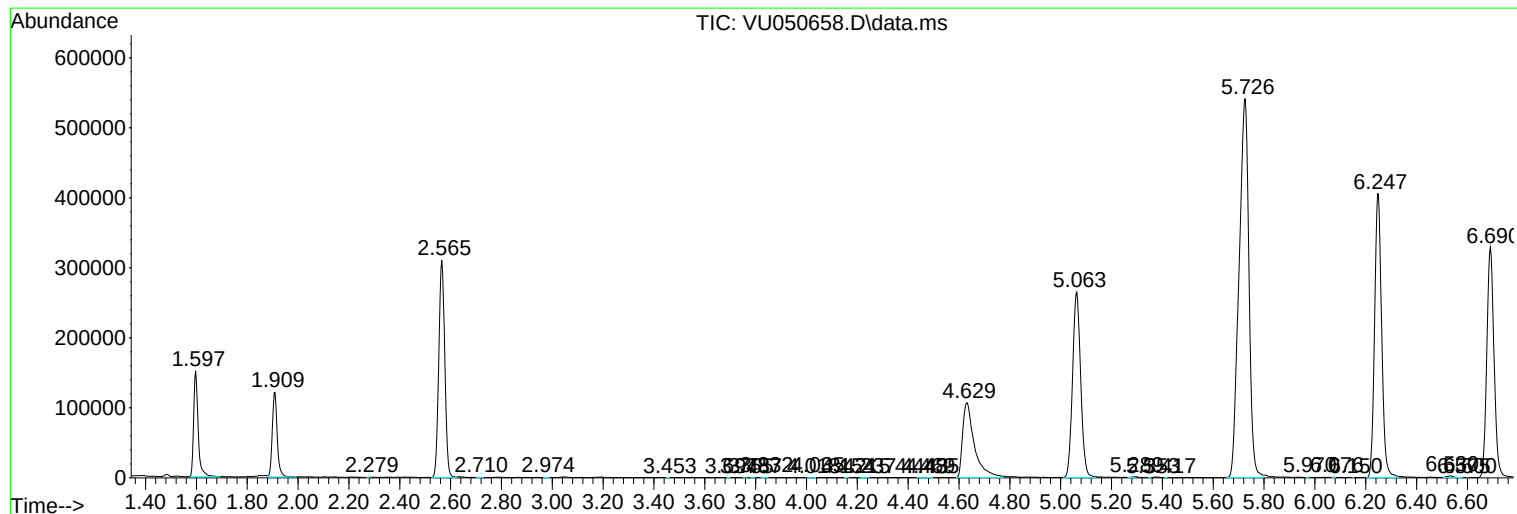

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050658.D
Acq On : 07 Sep 2022 14:18
Operator : SY/MD
Sample : N4481-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050658.D
Acq On : 07 Sep 2022 14:18
Operator : SY/MD
Sample : N4481-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------