

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050665.D
 Acq On : 07 Sep 2022 17:02
 Operator : SY/MD
 Sample : N4372-01DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY183DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

Signal : TIC: VU050665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	53	rVB5	2668	2986	0.22%	0.031%
2	1.600	72	81	103	rBV	134662	174099	12.64%	1.778%
3	1.732	117	122	128	rVB2	2432	2486	0.18%	0.025%
4	1.906	166	176	200	rBV	104837	148139	10.75%	1.513%
5	2.195	262	266	270	rVB4	517	457	0.03%	0.005%
6	2.317	302	304	307	rBV2	462	335	0.02%	0.003%
7	2.404	328	331	334	rBV3	540	483	0.04%	0.005%
8	2.565	368	381	401	rBV	278116	453781	32.94%	4.635%
9	2.674	413	415	419	rVB3	436	259	0.02%	0.003%
10	2.755	435	440	443	rBV2	605	579	0.04%	0.006%
11	2.957	499	503	507	rVB2	349	266	0.02%	0.003%
12	3.047	523	531	539	rBV3	2102	3285	0.24%	0.034%
13	3.182	558	573	598	rBV	16194	37735	2.74%	0.385%
14	3.356	620	627	630	rBV4	1061	1450	0.11%	0.015%
15	3.565	686	692	697	rBV2	253	328	0.02%	0.003%
16	3.604	700	704	707	rVV2	341	241	0.02%	0.002%
17	3.861	775	784	787	rBV4	1622	2067	0.15%	0.021%
18	4.102	855	859	861	rBV2	335	317	0.02%	0.003%
19	4.288	913	917	920	rVB2	336	282	0.02%	0.003%
20	4.308	920	923	926	rBV	331	224	0.02%	0.002%
21	4.388	944	948	960	rVB2	336	487	0.04%	0.005%
22	4.620	1007	1020	1047	rBV	117033	333764	24.23%	3.409%
23	4.925	1112	1115	1119	rBV2	543	417	0.03%	0.004%
24	5.063	1141	1158	1180	rBV	252109	554996	40.28%	5.669%
25	5.298	1229	1231	1234	rBV2	457	270	0.02%	0.003%
26	5.359	1246	1250	1253	rBV2	372	319	0.02%	0.003%
27	5.385	1256	1258	1266	rVV2	498	523	0.04%	0.005%
28	5.517	1296	1299	1302	rBV2	523	242	0.02%	0.002%
29	5.726	1342	1364	1398	rBV2	503351	1377713	100.00%	14.073%
30	6.112	1478	1484	1488	rBV3	442	538	0.04%	0.005%
31	6.250	1512	1527	1553	rBV	368675	723006	52.48%	7.386%
32	6.417	1577	1579	1583	rVB3	484	225	0.02%	0.002%
33	6.542	1605	1618	1633	rBV2	110494	211223	15.33%	2.158%
34	6.626	1642	1644	1650	rVB4	560	470	0.03%	0.005%
35	6.690	1650	1664	1689	rBV	309581	616420	44.74%	6.297%
36	6.870	1718	1720	1725	rVB4	495	398	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050665.D
 Acq On : 07 Sep 2022 17:02
 Operator : SY/MD
 Sample : N4372-01DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY183DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.938	1737	1741	1745	rVB2	325	322	0.02%	0.003%
38	7.079	1782	1785	1789	rBV	292	225	0.02%	0.002%
39	7.144	1801	1805	1810	rBV2	346	294	0.02%	0.003%
40	7.185	1810	1818	1819	rBV3	1246	1040	0.08%	0.011%
41	7.285	1845	1849	1852	rBV	276	262	0.02%	0.003%
42	7.456	1898	1902	1904	rBV2	277	221	0.02%	0.002%
43	7.565	1921	1936	1957	rBV	156356	282224	20.48%	2.883%
44	7.681	1968	1972	1973	rBV3	574	359	0.03%	0.004%
45	7.726	1984	1986	1990	rBV2	428	280	0.02%	0.003%
46	7.783	2000	2004	2008	rBV2	220	227	0.02%	0.002%
47	7.896	2025	2039	2072	rBV	579574	1049297	76.16%	10.719%
48	8.179	2114	2127	2143	rBV2	106172	186329	13.52%	1.903%
49	8.427	2201	2204	2210	rBV2	294	234	0.02%	0.002%
50	8.636	2257	2269	2278	rBV4	202063	439874	31.93%	4.493%
51	8.925	2356	2359	2365	rBV	252	226	0.02%	0.002%
52	9.002	2379	2383	2387	rBV2	248	240	0.02%	0.002%
53	9.211	2446	2448	2455	rVB	448	315	0.02%	0.003%
54	9.417	2499	2512	2554	rBV	515178	882102	64.03%	9.011%
55	9.565	2554	2558	2559	rBV2	437	257	0.02%	0.003%
56	9.693	2594	2598	2601	rBV2	568	469	0.03%	0.005%
57	9.787	2623	2627	2632	rVB2	285	244	0.02%	0.002%
58	9.870	2647	2653	2658	rBV2	251	277	0.02%	0.003%
59	10.008	2692	2696	2699	rBV2	319	292	0.02%	0.003%
60	10.095	2718	2723	2726	rBV2	407	405	0.03%	0.004%
61	10.118	2728	2730	2736	rVB2	412	312	0.02%	0.003%
62	10.182	2744	2750	2754	rVB2	364	429	0.03%	0.004%
63	10.205	2754	2757	2763	rBV2	258	227	0.02%	0.002%
64	10.237	2764	2767	2772	rBV2	323	306	0.02%	0.003%
65	10.320	2790	2793	2799	rVB2	282	268	0.02%	0.003%
66	10.404	2816	2819	2824	rBV2	224	229	0.02%	0.002%
67	10.430	2824	2827	2833	rVV2	250	244	0.02%	0.002%
68	10.484	2839	2844	2847	rBV	467	549	0.04%	0.006%
69	10.754	2916	2928	2947	rBV	453790	747124	54.23%	7.632%
70	10.918	2976	2979	2984	rVB	378	230	0.02%	0.002%
71	11.050	3016	3020	3023	rBV3	304	263	0.02%	0.003%
72	11.269	3085	3088	3096	rVB2	263	295	0.02%	0.003%
73	11.475	3148	3152	3155	rBV2	567	387	0.03%	0.004%
74	11.497	3155	3159	3166	rVB2	354	353	0.03%	0.004%
75	11.661	3206	3210	3215	rVV	318	308	0.02%	0.003%
76	11.812	3244	3257	3279	rBV	421142	692057	50.23%	7.069%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050665.D
 Acq On : 07 Sep 2022 17:02
 Operator : SY/MD
 Sample : N4372-01DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY183DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.928	3291	3293	3296	rVB2	601	333	0.02%	0.003%
78	11.954	3296	3301	3304	rVV2	405	379	0.03%	0.004%
79	12.073	3329	3338	3339	rBV3	1788	2259	0.16%	0.023%
80	12.131	3353	3356	3359	rBV3	265	241	0.02%	0.002%
81	12.192	3361	3375	3406	rVV	498157	838887	60.89%	8.569%
82	12.410	3440	3443	3446	rVV2	293	228	0.02%	0.002%
83	12.446	3450	3454	3458	rBV2	325	311	0.02%	0.003%
84	12.687	3527	3529	3534	rVB2	462	339	0.02%	0.003%
85	12.832	3571	3574	3578	rVB2	420	264	0.02%	0.003%
86	12.880	3586	3589	3590	rBV	484	244	0.02%	0.002%
87	13.131	3664	3667	3670	rVB2	350	283	0.02%	0.003%
88	13.468	3767	3772	3777	rBV3	359	457	0.03%	0.005%
89	13.581	3802	3807	3810	rBV	439	514	0.04%	0.005%
90	13.651	3824	3829	3832	rBV3	396	449	0.03%	0.005%
91	13.703	3843	3845	3850	rBV2	324	310	0.02%	0.003%
92	13.854	3889	3892	3896	rVV3	695	561	0.04%	0.006%
93	13.873	3896	3898	3905	rVB3	418	310	0.02%	0.003%
94	14.066	3955	3958	3960	rBV2	595	369	0.03%	0.004%
95	14.105	3965	3970	3972	rBV2	590	567	0.04%	0.006%
96	14.169	3987	3990	3993	rBV3	370	239	0.02%	0.002%
97	14.230	4006	4009	4013	rBV2	394	278	0.02%	0.003%
98	14.825	4191	4194	4197	rVB3	555	365	0.03%	0.004%
99	14.867	4204	4207	4209	rBV2	748	440	0.03%	0.004%
100	15.285	4334	4337	4339	rBV2	661	465	0.03%	0.005%




Sum of corrected areas: 9789498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050665.D
Acq On : 07 Sep 2022 17:02
Operator : SY/MD
Sample : N4372-01DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY183DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

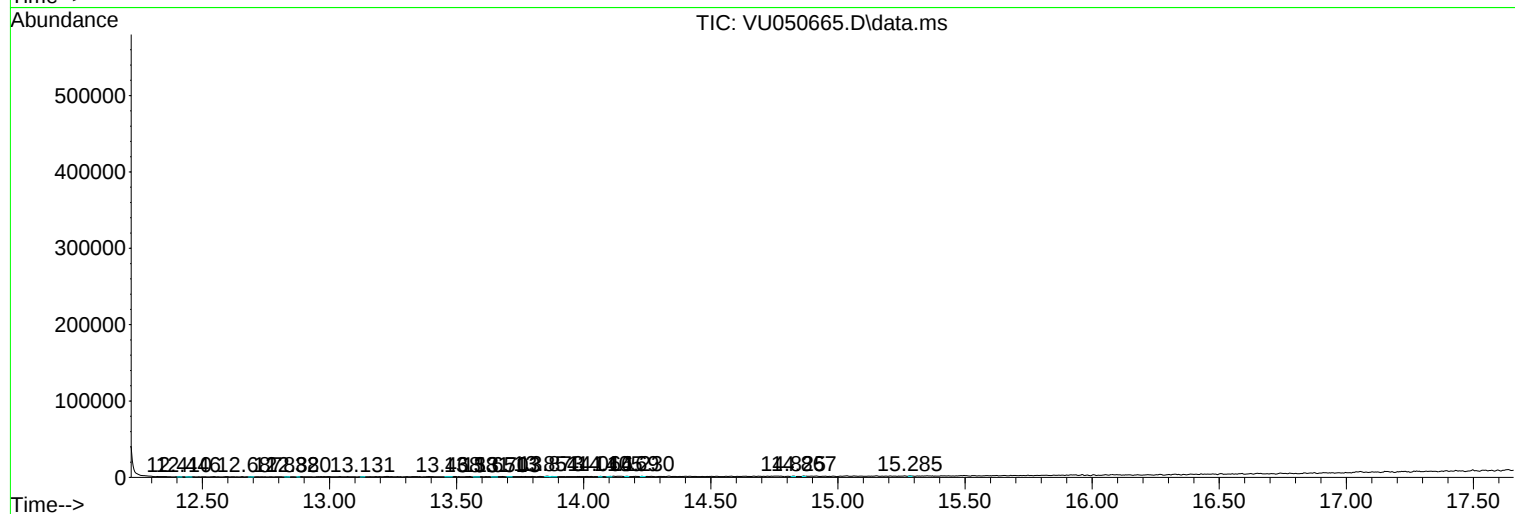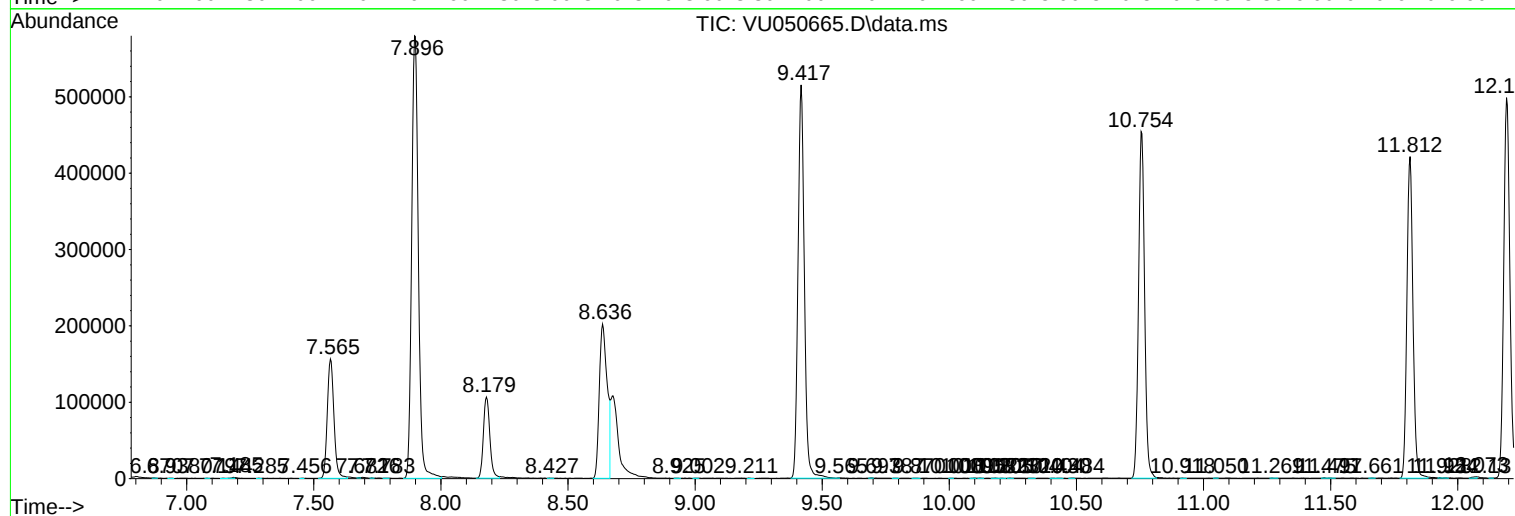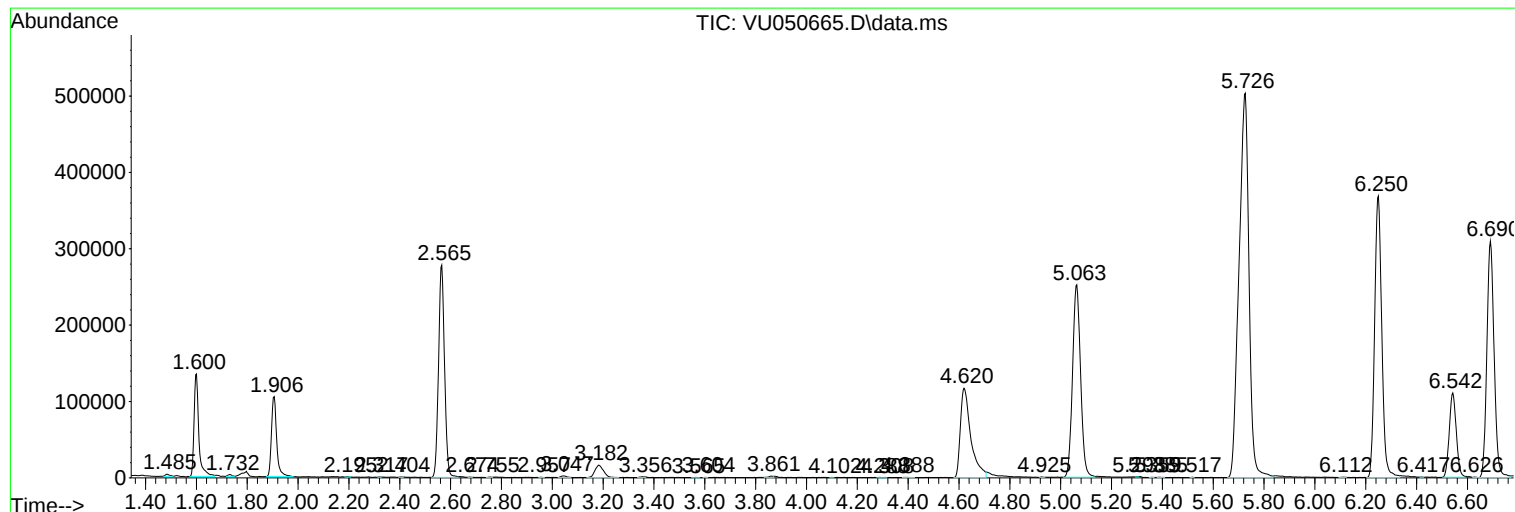

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050665.D
Acq On : 07 Sep 2022 17:02
Operator : SY/MD
Sample : N4372-01DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY183DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050665.D
Acq On : 07 Sep 2022 17:02
Operator : SY/MD
Sample : N4372-01DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY183DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------