

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050667.D
 Acq On : 07 Sep 2022 17:50
 Operator : SY/MD
 Sample : N4372-01DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY183DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

Signal : TIC: VU050667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	108	rBV	127629	159910	12.32%	1.544%
2	1.906	168	176	196	rVB	98948	136994	10.56%	1.322%
3	2.211	269	271	272	rBV	409	182	0.01%	0.002%
4	2.565	368	381	398	rBV	261369	426188	32.85%	4.114%
5	2.755	438	440	443	rBV2	380	247	0.02%	0.002%
6	2.777	446	447	449	rBV	395	201	0.02%	0.002%
7	2.822	459	461	464	rBB2	251	108	0.01%	0.001%
8	2.871	473	476	478	rBV	157	113	0.01%	0.001%
9	3.044	522	530	539	rBV3	2355	3621	0.28%	0.035%
10	3.186	560	574	591	rBV	8192	18520	1.43%	0.179%
11	3.356	618	627	642	rVB4	3603	7512	0.58%	0.073%
12	3.437	650	652	655	rBV2	201	148	0.01%	0.001%
13	3.478	663	665	668	rVB2	230	114	0.01%	0.001%
14	3.498	668	671	673	rBV2	151	92	0.01%	0.001%
15	3.530	680	681	682	rBV	228	66	0.01%	0.001%
16	3.581	694	697	701	rVB	231	145	0.01%	0.001%
17	3.604	701	704	712	rBV2	231	278	0.02%	0.003%
18	3.636	712	714	717	rBV2	142	77	0.01%	0.001%
19	3.729	741	743	744	rBV2	235	60	0.00%	0.001%
20	3.787	756	761	765	rBV2	208	228	0.02%	0.002%
21	3.871	771	787	805	rBV	11174	24995	1.93%	0.241%
22	4.012	824	831	833	rBV	244	267	0.02%	0.003%
23	4.192	883	887	888	rBV	354	181	0.01%	0.002%
24	4.227	895	898	900	rBV	111	85	0.01%	0.001%
25	4.321	923	927	928	rBV2	101	77	0.01%	0.001%
26	4.350	934	936	939	rBV	119	57	0.00%	0.001%
27	4.520	986	989	991	rBV2	171	108	0.01%	0.001%
28	4.565	1001	1003	1006	rVB2	159	80	0.01%	0.001%
29	4.620	1006	1020	1062	rBV	112018	360281	27.77%	3.478%
30	5.063	1142	1158	1181	rBV	236818	523925	40.38%	5.057%
31	5.440	1273	1275	1278	rBV	232	139	0.01%	0.001%
32	5.472	1283	1285	1286	rBV	203	66	0.01%	0.001%
33	5.520	1295	1300	1301	rBV	360	250	0.02%	0.002%
34	5.726	1342	1364	1394	rBV2	469807	1297492	100.00%	12.524%
35	6.137	1490	1492	1496	rBV2	206	115	0.01%	0.001%
36	6.198	1509	1511	1513	rBV	197	86	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050667.D
 Acq On : 07 Sep 2022 17:50
 Operator : SY/MD
 Sample : N4372-01DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY183DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1554	rBV	374204	737424	56.83%	7.118%
38	6.543	1603	1618	1642	rBV	584943	1124236	86.65%	10.852%
39	6.690	1651	1664	1694	rVB	295313	577984	44.55%	5.579%
40	6.896	1727	1728	1731	rBV2	186	75	0.01%	0.001%
41	6.925	1731	1737	1740	rBV	388	404	0.03%	0.004%
42	6.980	1752	1754	1755	rBV	203	91	0.01%	0.001%
43	7.025	1766	1768	1771	rBV2	192	129	0.01%	0.001%
44	7.067	1779	1781	1782	rBV	239	106	0.01%	0.001%
45	7.105	1790	1793	1798	rVB3	478	351	0.03%	0.003%
46	7.131	1798	1801	1804	rBV2	174	109	0.01%	0.001%
47	7.189	1812	1819	1823	rBV3	1091	1264	0.10%	0.012%
48	7.243	1831	1836	1837	rBV	238	181	0.01%	0.002%
49	7.253	1837	1839	1844	rVB2	340	259	0.02%	0.003%
50	7.285	1844	1849	1851	rBV2	206	132	0.01%	0.001%
51	7.311	1855	1857	1860	rVB	318	142	0.01%	0.001%
52	7.340	1860	1866	1870	rBV2	267	311	0.02%	0.003%
53	7.475	1905	1908	1911	rVV	203	113	0.01%	0.001%
54	7.488	1911	1912	1915	rVB	160	60	0.00%	0.001%
55	7.565	1922	1936	1960	rBV	148532	270165	20.82%	2.608%
56	7.780	1999	2003	2004	rBV2	272	145	0.01%	0.001%
57	7.790	2004	2006	2009	rBV4	413	280	0.02%	0.003%
58	7.899	2025	2040	2067	rBV	546946	976996	75.30%	9.431%
59	8.179	2116	2127	2147	rBV	99155	173798	13.39%	1.678%
60	8.427	2201	2204	2207	rBV2	186	134	0.01%	0.001%
61	8.452	2208	2212	2214	rBV	278	209	0.02%	0.002%
62	8.491	2222	2224	2228	rVB	145	66	0.01%	0.001%
63	8.513	2228	2231	2234	rBV2	348	229	0.02%	0.002%
64	8.555	2241	2244	2247	rVB2	480	239	0.02%	0.002%
65	8.636	2256	2269	2278	rBV3	194650	425922	32.83%	4.111%
66	8.893	2346	2349	2351	rVB	386	156	0.01%	0.002%
67	8.915	2354	2356	2362	rBV	309	283	0.02%	0.003%
68	9.115	2415	2418	2423	rBV	471	362	0.03%	0.003%
69	9.269	2463	2466	2468	rBV2	311	194	0.01%	0.002%
70	9.298	2472	2475	2478	rBV	186	125	0.01%	0.001%
71	9.346	2488	2490	2496	rBV2	220	184	0.01%	0.002%
72	9.369	2496	2497	2498	rVB	261	50	0.00%	0.000%
73	9.417	2498	2512	2541	rBV	520684	903672	69.65%	8.723%
74	9.645	2581	2583	2590	rVB3	454	276	0.02%	0.003%
75	9.748	2611	2615	2616	rBV3	473	306	0.02%	0.003%
76	9.925	2667	2670	2672	rBV	183	108	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050667.D
 Acq On : 07 Sep 2022 17:50
 Operator : SY/MD
 Sample : N4372-01DL 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY183DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M

Title : VOC Analysis

77	9.960	2677	2681	2687	rVV2	256	267	0.02%	0.003%
78	10.063	2710	2713	2717	rVB	389	250	0.02%	0.002%
79	10.102	2719	2725	2727	rBV3	819	765	0.06%	0.007%
80	10.340	2797	2799	2804	rBV	229	184	0.01%	0.002%
81	10.481	2839	2843	2851	rBV4	610	798	0.06%	0.008%
82	10.620	2882	2886	2892	rVB2	454	348	0.03%	0.003%
83	10.755	2916	2928	2955	rBV	433917	716945	55.26%	6.920%
84	11.417	3131	3134	3136	rBV	335	223	0.02%	0.002%
85	11.812	3244	3257	3283	rBV	420627	695332	53.59%	6.712%
86	12.192	3362	3375	3400	rBV	466261	784022	60.43%	7.568%
87	13.375	3740	3743	3744	rBV2	320	200	0.02%	0.002%
88	13.607	3811	3815	3816	rBV2	383	268	0.02%	0.003%




Sum of corrected areas: 10359880

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050667.D
Acq On : 07 Sep 2022 17:50
Operator : SY/MD
Sample : N4372-01DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY183DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

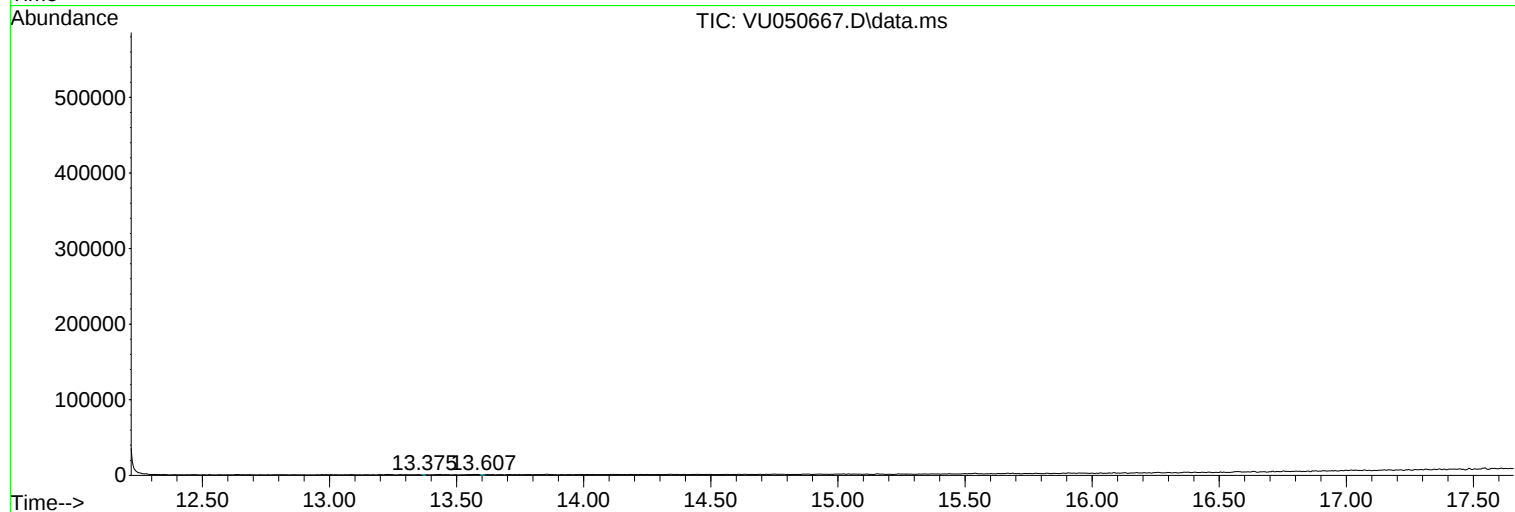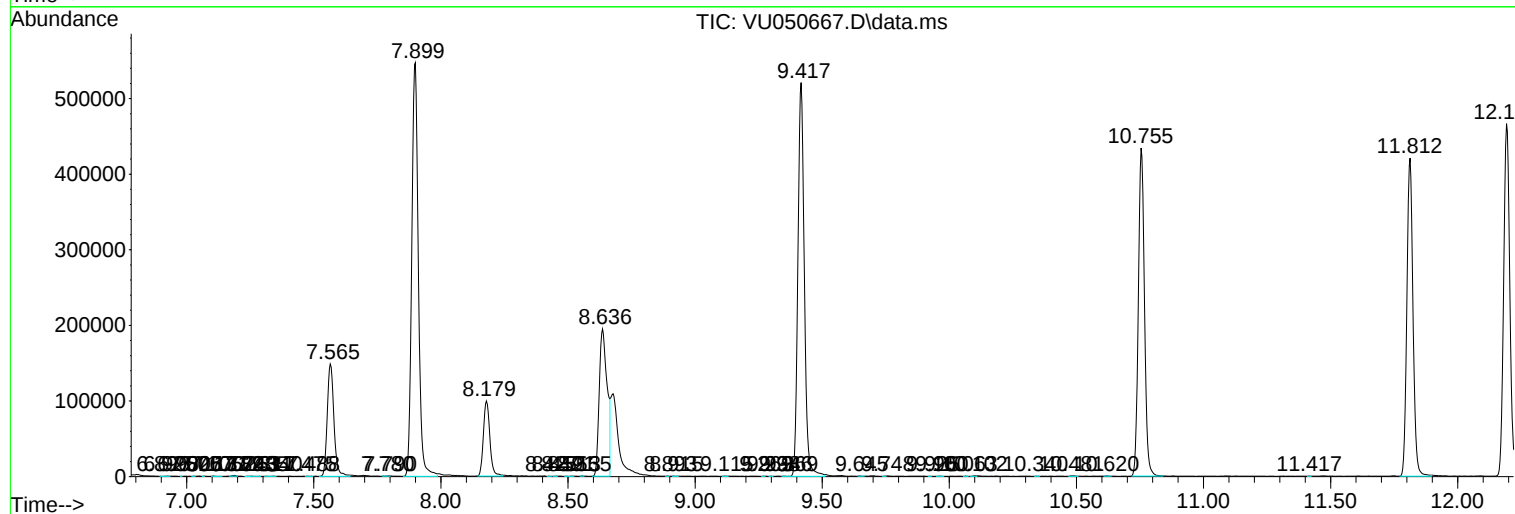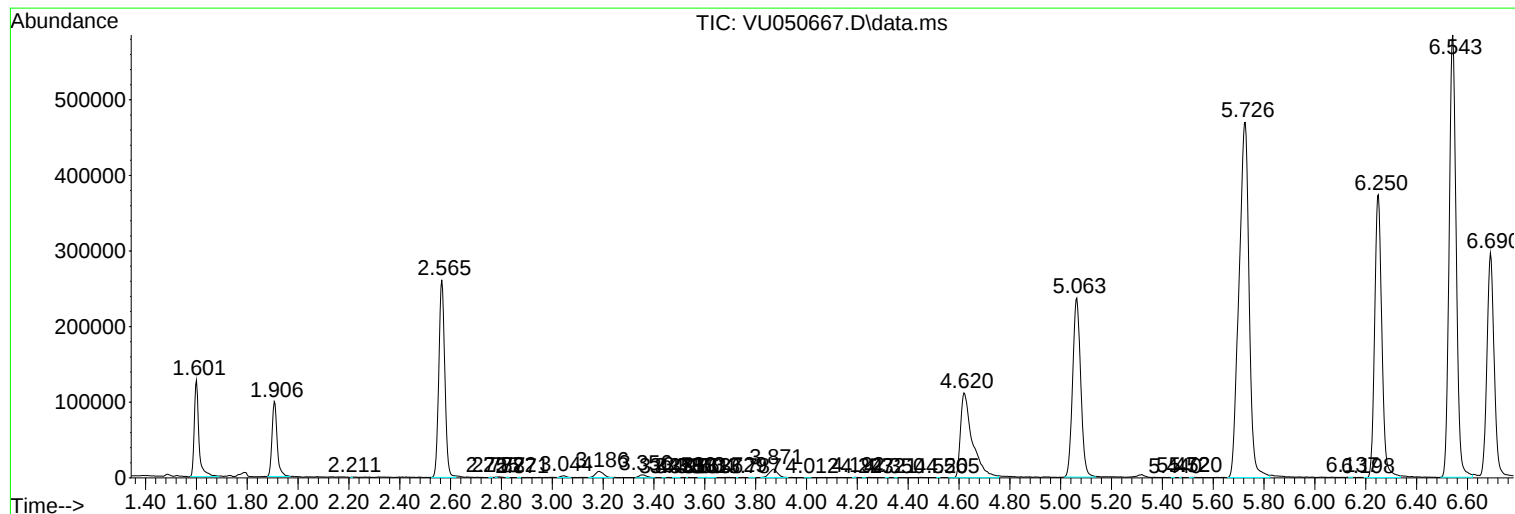

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050667.D
Acq On : 07 Sep 2022 17:50
Operator : SY/MD
Sample : N4372-01DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY183DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050667.D
Acq On : 07 Sep 2022 17:50
Operator : SY/MD
Sample : N4372-01DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY183DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------