

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050669.D
 Acq On : 07 Sep 2022 18:38
 Operator : SY/MD
 Sample : N4482-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

Signal : TIC: VU050669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rVB4	2100	2549	0.19%	0.028%
2	1.597	71	80	105	rBV	115285	151432	11.41%	1.674%
3	1.771	127	134	135	rBV5	4193	4187	0.32%	0.046%
4	1.903	165	175	197	rBV	95043	132753	10.00%	1.468%
5	2.154	250	253	257	rBV2	726	613	0.05%	0.007%
6	2.228	273	276	280	rBV3	520	462	0.03%	0.005%
7	2.266	286	288	294	rVB3	485	423	0.03%	0.005%
8	2.562	368	380	393	rBV	235684	380947	28.70%	4.211%
9	2.626	394	400	412	rVB2	8728	15625	1.18%	0.173%
10	2.739	429	435	437	rBV	346	313	0.02%	0.003%
11	2.755	437	440	445	rVV3	276	249	0.02%	0.003%
12	2.777	445	447	449	rBV	332	210	0.02%	0.002%
13	2.906	472	487	505	rVV4	3718	10673	0.80%	0.118%
14	3.044	523	530	535	rBV4	695	950	0.07%	0.011%
15	3.131	554	557	561	rVB2	288	213	0.02%	0.002%
16	3.182	561	573	575	rBV2	1757	2588	0.20%	0.029%
17	3.668	719	724	726	rBV2	199	198	0.01%	0.002%
18	3.990	818	824	828	rVB2	187	206	0.02%	0.002%
19	4.038	836	839	843	rVB2	266	212	0.02%	0.002%
20	4.080	847	852	857	rBV2	435	433	0.03%	0.005%
21	4.224	887	897	902	rBV2	343	613	0.05%	0.007%
22	4.317	922	926	931	rBV2	213	212	0.02%	0.002%
23	4.481	971	977	981	rBV	205	198	0.01%	0.002%
24	4.510	981	986	988	rBV	210	199	0.01%	0.002%
25	4.620	1008	1020	1063	rBV	113453	329909	24.86%	3.647%
26	4.870	1096	1098	1101	rBV3	391	238	0.02%	0.003%
27	4.986	1132	1134	1138	rVB2	367	245	0.02%	0.003%
28	5.060	1141	1157	1183	rBV	241510	539202	40.63%	5.961%
29	5.247	1211	1215	1220	rVB5	406	386	0.03%	0.004%
30	5.272	1220	1223	1224	rBV	426	247	0.02%	0.003%
31	5.375	1249	1255	1262	rVV2	699	1008	0.08%	0.011%
32	5.446	1267	1277	1279	rBV2	256	357	0.03%	0.004%
33	5.504	1291	1295	1299	rBV	281	228	0.02%	0.003%
34	5.723	1342	1363	1391	rBV2	481589	1327167	100.00%	14.672%
35	5.980	1440	1443	1445	rBV2	453	240	0.02%	0.003%
36	6.051	1458	1465	1469	rBV3	519	625	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050669.D
 Acq On : 07 Sep 2022 18:38
 Operator : SY/MD
 Sample : N4482-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

37	6.121	1484	1487	1491	rVB2	649	461	0.03%	0.005%
38	6.160	1495	1499	1505	rVB3	328	361	0.03%	0.004%
39	6.195	1505	1510	1512	rBV2	341	321	0.02%	0.004%
40	6.247	1512	1526	1551	rBV	339797	661823	49.87%	7.316%
41	6.533	1607	1615	1628	rVB7	3455	6194	0.47%	0.068%
42	6.690	1650	1664	1695	rBV	308504	611102	46.05%	6.756%
43	6.851	1712	1714	1717	rVB2	637	319	0.02%	0.004%
44	6.874	1717	1721	1724	rVB3	296	241	0.02%	0.003%
45	6.964	1745	1749	1757	rVB2	293	392	0.03%	0.004%
46	7.163	1805	1811	1812	rBV	1389	1079	0.08%	0.012%
47	7.224	1829	1830	1839	rVB3	358	327	0.02%	0.004%
48	7.263	1839	1842	1849	rVB2	302	419	0.03%	0.005%
49	7.295	1849	1852	1855	rBV	351	301	0.02%	0.003%
50	7.378	1874	1878	1885	rVB2	203	218	0.02%	0.002%
51	7.420	1885	1891	1892	rBV	240	202	0.02%	0.002%
52	7.449	1898	1900	1903	rVB	377	217	0.02%	0.002%
53	7.565	1923	1936	1956	rBV	151156	271116	20.43%	2.997%
54	7.896	2026	2039	2071	rBV	543744	973799	73.37%	10.765%
55	8.179	2113	2127	2140	rBV2	104324	177295	13.36%	1.960%
56	8.636	2257	2269	2278	rBV3	205803	448260	33.78%	4.955%
57	8.890	2344	2348	2352	rVB	435	414	0.03%	0.005%
58	8.960	2366	2370	2375	rBV2	246	250	0.02%	0.003%
59	9.314	2474	2480	2484	rVV2	403	388	0.03%	0.004%
60	9.417	2498	2512	2535	rBV	489120	823563	62.05%	9.104%
61	9.584	2560	2564	2568	rBV2	305	207	0.02%	0.002%
62	9.610	2568	2572	2575	rVB2	287	232	0.02%	0.003%
63	9.636	2575	2580	2582	rBV	399	336	0.03%	0.004%
64	9.693	2594	2598	2602	rVV	323	275	0.02%	0.003%
65	9.719	2604	2606	2611	rVV	283	211	0.02%	0.002%
66	9.780	2620	2625	2630	rBV2	264	294	0.02%	0.003%
67	9.819	2631	2637	2640	rBV2	406	520	0.04%	0.006%
68	9.960	2675	2681	2684	rBV	332	355	0.03%	0.004%
69	9.980	2684	2687	2691	rVB2	244	229	0.02%	0.003%
70	10.021	2697	2700	2703	rBV	343	248	0.02%	0.003%
71	10.041	2703	2706	2710	rVV	231	225	0.02%	0.002%
72	10.118	2726	2730	2734	rBV2	479	546	0.04%	0.006%
73	10.494	2842	2847	2849	rBV2	371	307	0.02%	0.003%
74	10.755	2915	2928	2953	rBV	462646	757977	57.11%	8.379%
75	11.201	3063	3067	3073	rBV2	478	444	0.03%	0.005%
76	11.472	3148	3151	3154	rBV	470	334	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
 Data File : VU050669.D
 Acq On : 07 Sep 2022 18:38
 Operator : SY/MD
 Sample : N4482-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
 Title : VOC Analysis

77	11.488	3154	3156	3159	rVB2	379	202	0.02%	0.002%
78	11.812	3244	3257	3277	rBV	370754	611928	46.11%	6.765%
79	12.050	3327	3331	3333	rBV2	555	387	0.03%	0.004%
80	12.192	3362	3375	3396	rBV	466132	778406	58.65%	8.605%
81	12.423	3443	3447	3449	rBV	329	279	0.02%	0.003%
82	12.455	3455	3457	3461	rVB3	560	343	0.03%	0.004%
83	12.481	3461	3465	3468	rBV	312	276	0.02%	0.003%
84	12.555	3485	3488	3491	rBV2	363	231	0.02%	0.003%
85	12.706	3532	3535	3543	rVB2	401	387	0.03%	0.004%
86	12.780	3554	3558	3562	rBV2	406	451	0.03%	0.005%
87	12.873	3584	3587	3590	rVB3	537	315	0.02%	0.003%
88	13.185	3681	3684	3686	rBV2	280	227	0.02%	0.003%
89	13.230	3695	3698	3701	rBV2	311	241	0.02%	0.003%
90	13.369	3738	3741	3747	rBV2	328	355	0.03%	0.004%
91	13.565	3800	3802	3808	rVB	396	312	0.02%	0.003%
92	13.597	3808	3812	3814	rBV	337	310	0.02%	0.003%
93	13.713	3845	3848	3851	rBV	514	348	0.03%	0.004%
94	14.102	3965	3969	3971	rBV3	447	370	0.03%	0.004%
95	14.343	4041	4044	4046	rBV2	376	253	0.02%	0.003%
96	14.587	4117	4120	4123	rBV3	673	448	0.03%	0.005%
97	14.844	4197	4200	4202	rBV2	539	326	0.02%	0.004%
98	14.931	4225	4227	4230	rBV3	563	297	0.02%	0.003%
99	15.131	4287	4289	4290	rBV	458	221	0.02%	0.002%
100	15.674	4455	4458	4462	rBV4	897	801	0.06%	0.009%




Sum of corrected areas: 9045826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050669.D
Acq On : 07 Sep 2022 18:38
Operator : SY/MD
Sample : N4482-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

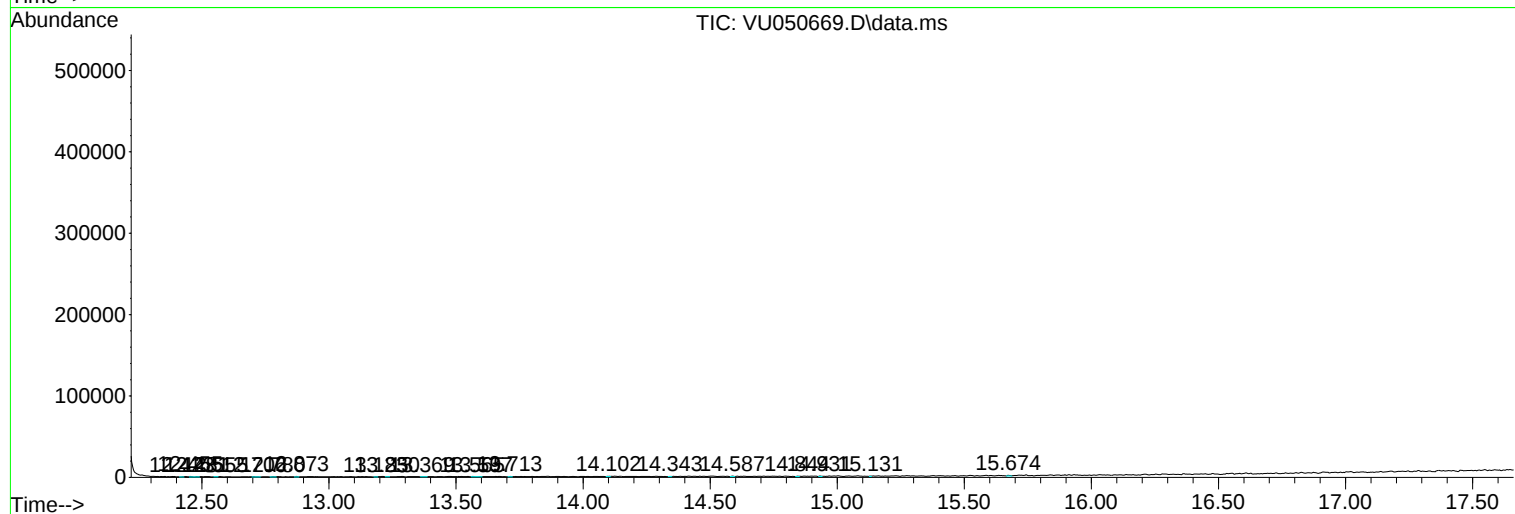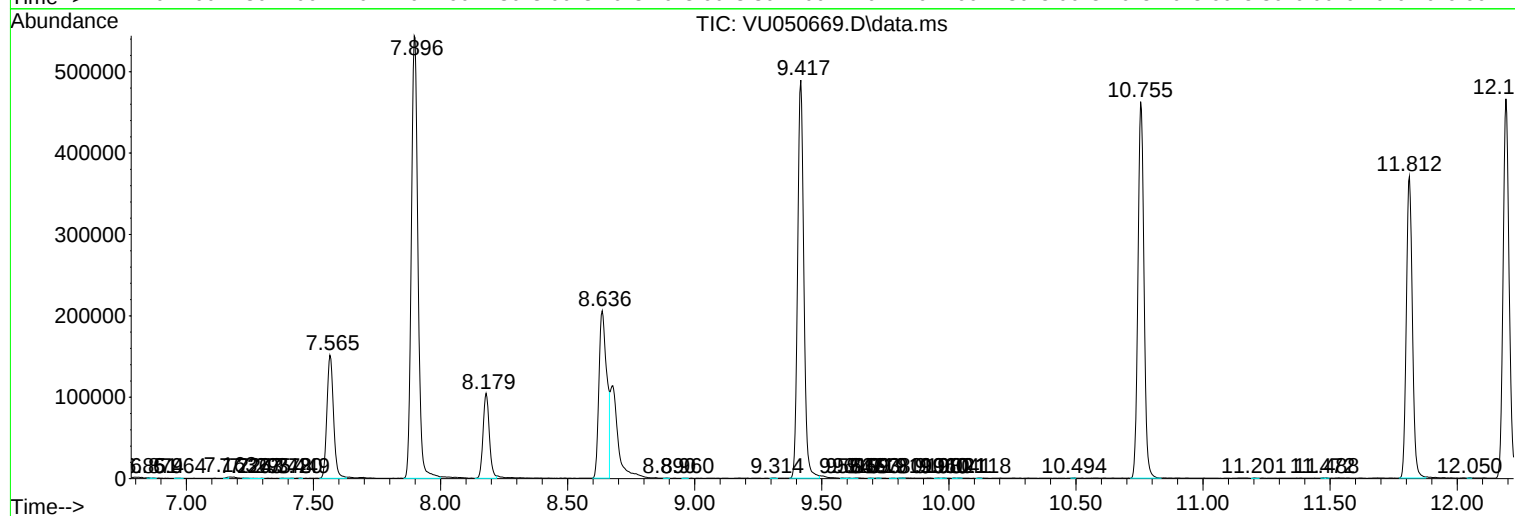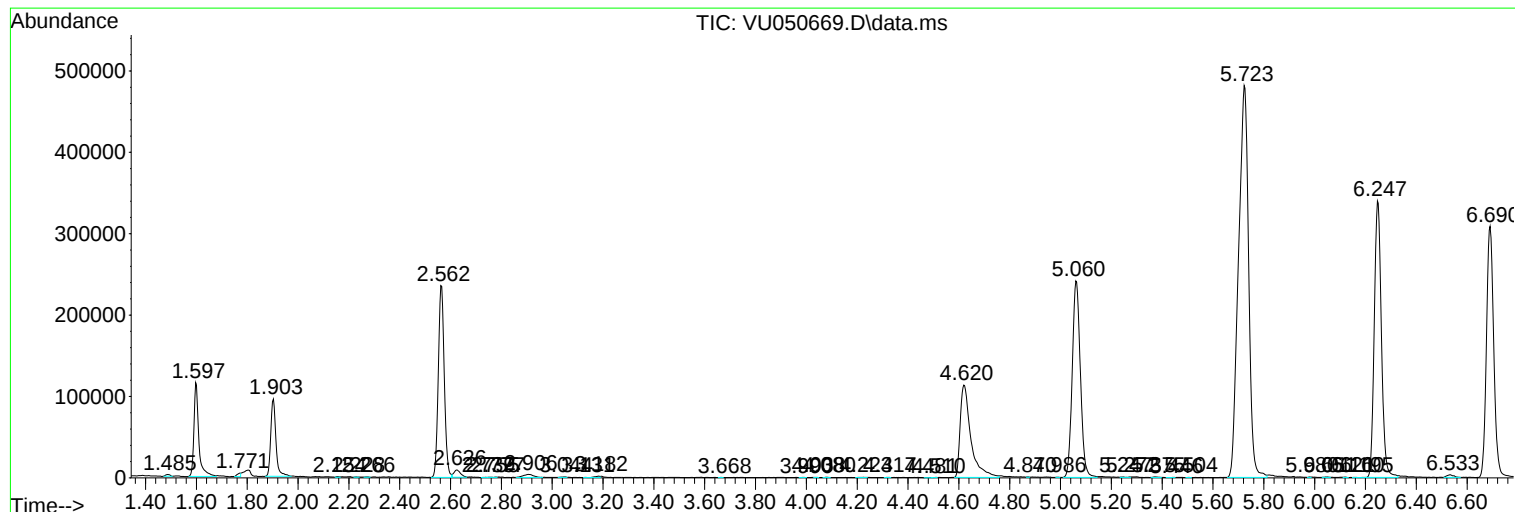

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050669.D
Acq On : 07 Sep 2022 18:38
Operator : SY/MD
Sample : N4482-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050669.D
Acq On : 07 Sep 2022 18:38
Operator : SY/MD
Sample : N4482-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc