


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090722\
Data File : VU050653.D
Acq On : 07 Sep 2022 10:05
Operator : SY/MD
Sample : BFB121
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB121

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM090222WMA.M
Title : VOC Analysis
Last Update : Thu Sep 08 22:51:50 2022

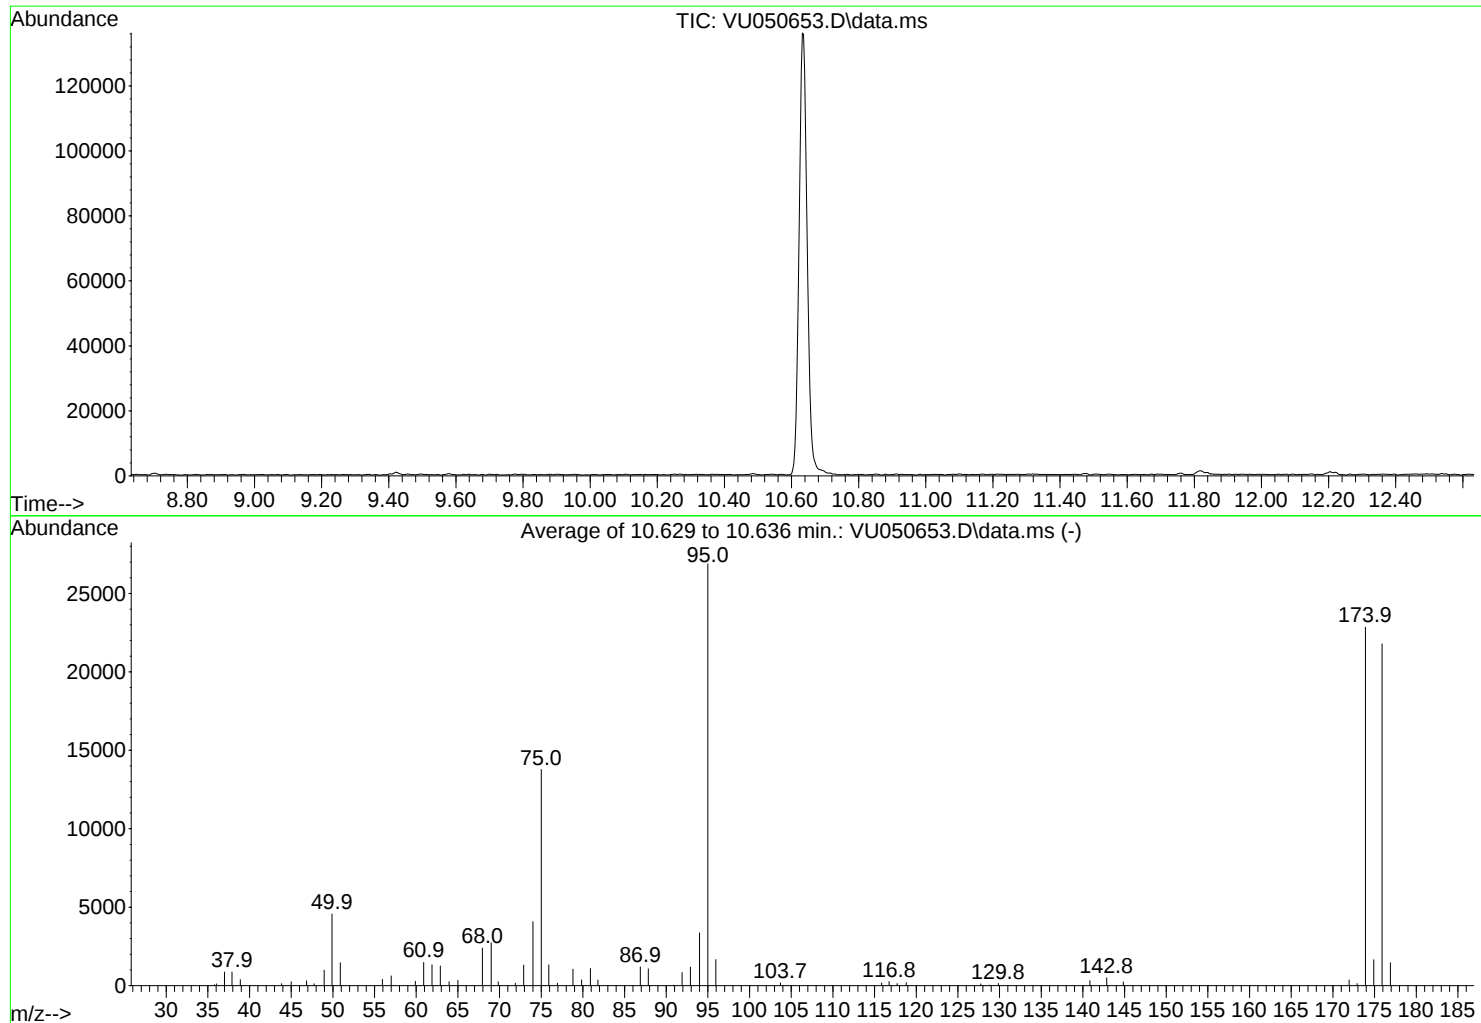

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	4567	PASS
75	95	30	80	51.3	13779	PASS
95	95	100	100	100.0	26885	PASS
96	95	5	9	6.2	1664	PASS
173	174	0.00	2	0.6	137	PASS
174	95	50	120	85.0	22840	PASS
175	174	5	9	7.2	1653	PASS
176	174	95	101	95.4	21789	PASS
177	176	5	9	6.7	1462	PASS

Scan 2878 (10.594 min): VU050653.D\data.ms
BFB121

m/z	Abundance
39.80	186.0
43.90	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB121

m/z	Abundance
36.10	157.0
37.00	788.0
37.90	936.0
38.90	396.0
39.80	168.0
43.80	252.0
45.00	184.0
46.90	266.0
47.80	100.0
49.00	945.0
49.90	4435.0
50.90	1446.0
56.00	396.0
57.00	575.0
59.90	218.0
60.90	1393.0
61.90	1365.0
62.90	1206.0
63.90	249.0
65.00	338.0
68.00	2374.0
69.00	2663.0
69.90	235.0
71.90	120.0
72.90	1254.0
74.00	3875.0
75.00	13084.0
75.90	1270.0
76.90	152.0
78.80	1093.0
79.90	307.0
80.90	1050.0
81.80	337.0
86.90	1003.0
87.80	932.0
91.90	754.0
92.90	1136.0
94.00	3014.0
95.00	25872.0
95.90	1706.0
103.70	147.0
115.90	167.0
116.80	265.0
117.70	137.0
118.80	181.0
127.70	100.0
129.80	133.0
140.90	273.0
142.90	489.0
144.80	188.0
172.00	356.0
173.90	20752.0
174.90	1552.0
175.90	20168.0
176.90	1437.0

Instrument :
MSVOA_U
ClientSampleId :
BFB121

m/z	Abundance
36.00	175.0
37.00	917.0
37.90	903.0
38.90	396.0
39.80	133.0
43.80	279.0
45.00	264.0
46.80	325.0
47.70	132.0
48.90	1004.0
49.90	4735.0
50.90	1526.0
56.00	410.0
57.00	679.0
59.90	283.0
60.90	1535.0
61.90	1394.0
62.90	1275.0
64.00	257.0
65.00	358.0
67.90	2397.0
69.00	2851.0
69.90	228.0
71.70	112.0
72.00	118.0
72.90	1381.0
74.00	4153.0
75.00	14195.0
75.90	1408.0
76.90	148.0
78.80	1073.0
79.90	392.0
80.90	1118.0
81.80	379.0
86.90	1251.0
87.80	1055.0
91.90	848.0
92.90	1221.0
94.00	3536.0
95.00	27696.0
96.00	1672.0
103.70	182.0
115.80	177.0
116.80	294.0
117.70	155.0
118.80	198.0
127.80	117.0
128.80	100.0
129.80	157.0
140.80	318.0
142.80	506.0
144.80	247.0
172.00	342.0
173.00	231.0
173.90	23432.0
174.90	1666.0
175.90	22424.0
176.90	1499.0

Instrument :
MSVOA_U
ClientSampleId :
BFB121

m/z	Abundance
35.80	181.0
37.00	892.0
37.90	775.0
38.90	370.0
39.80	134.0
43.90	340.0
45.00	294.0
46.80	317.0
47.80	145.0
48.90	1021.0
49.90	4531.0
50.90	1417.0
55.90	374.0
57.00	622.0
59.90	333.0
60.90	1517.0
61.90	1224.0
62.90	1290.0
64.00	254.0
65.00	312.0
67.90	2414.0
69.00	2700.0
69.80	256.0
72.00	121.0
72.90	1269.0
74.00	4198.0
75.00	14059.0
75.90	1314.0
77.00	146.0
78.80	996.0
79.80	408.0
80.90	1093.0
81.80	352.0
86.90	1324.0
87.90	1226.0
90.90	105.0
91.90	920.0
92.90	1179.0
94.00	3545.0
95.00	27088.0
96.00	1615.0
103.70	185.0
115.80	164.0
116.70	251.0
117.70	116.0
118.80	215.0
127.80	107.0
129.90	120.0
140.90	345.0
142.80	512.0
144.90	261.0
171.90	373.0
172.80	180.0
173.90	24336.0
174.90	1741.0
175.90	22776.0
176.90	1451.0

Instrument :
MSVOA_U
ClientSampleId :
BFB121