

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055220.D
 Acq On : 08 Sep 2023 05:19
 Operator : MD/SY
 Sample : 04307-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Sep 08 06:41:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	161105	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	171703	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.814	152	84517	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	31802	4.212	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	84.200%	
7) Chloroethane-d5	1.910	69	39534	4.523	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	2.563	65	20748	4.823	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.400%	
20) 2-Butanone-d5	4.631	46	132786	60.601	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	121.200%	
24) Chloroform-d	5.061	84	100773	5.030	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.600%	
26) 1,2-Dichloroethane-d4	5.701	65	53363	5.323	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.400%	
32) Benzene-d6	5.727	84	188905	4.457	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.200%	
36) 1,2-Dichloropropane-d6	6.688	67	66681	4.947	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.000%	
41) Toluene-d8	7.897	98	163620	4.191	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
43) trans-1,3-Dichloroprop...	8.180	79	14476	3.899	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.634	63	66809	44.328	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.660%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	48675	5.134	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	102.600%	
66) 1,2-Dichlorobenzene-d4	12.193	152	56695	4.596	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.000%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.515	50	1998	0.210	ug/L	94
22) cis-1,2-Dichloroethene	4.663	96	49261	5.325	ug/L	96
34) Trichloroethene	6.541	95	52823	5.201	ug/L	97
35) Methylcyclohexane	6.688	83	15140	1.062	ug/L #	19
37) 1,2-Dichloropropane	6.688	63	7411	0.745	ug/L #	88
48) 2-Hexanone	8.682	43	24040	5.408	ug/L #	93
61) 1,2,3-Trichloropropane	11.810	75	12986	2.315	ug/L #	70
69) 1,3,5-Trichlorobenzene	13.842	180	6318	0.442	ug/L	92
70) 1,2,4-trichlorobenzene	13.842	180	6318	0.471	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055220.D
Acq On : 08 Sep 2023 05:19
Operator : MD/SY
Sample : 04307-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Sep 08 06:41:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration




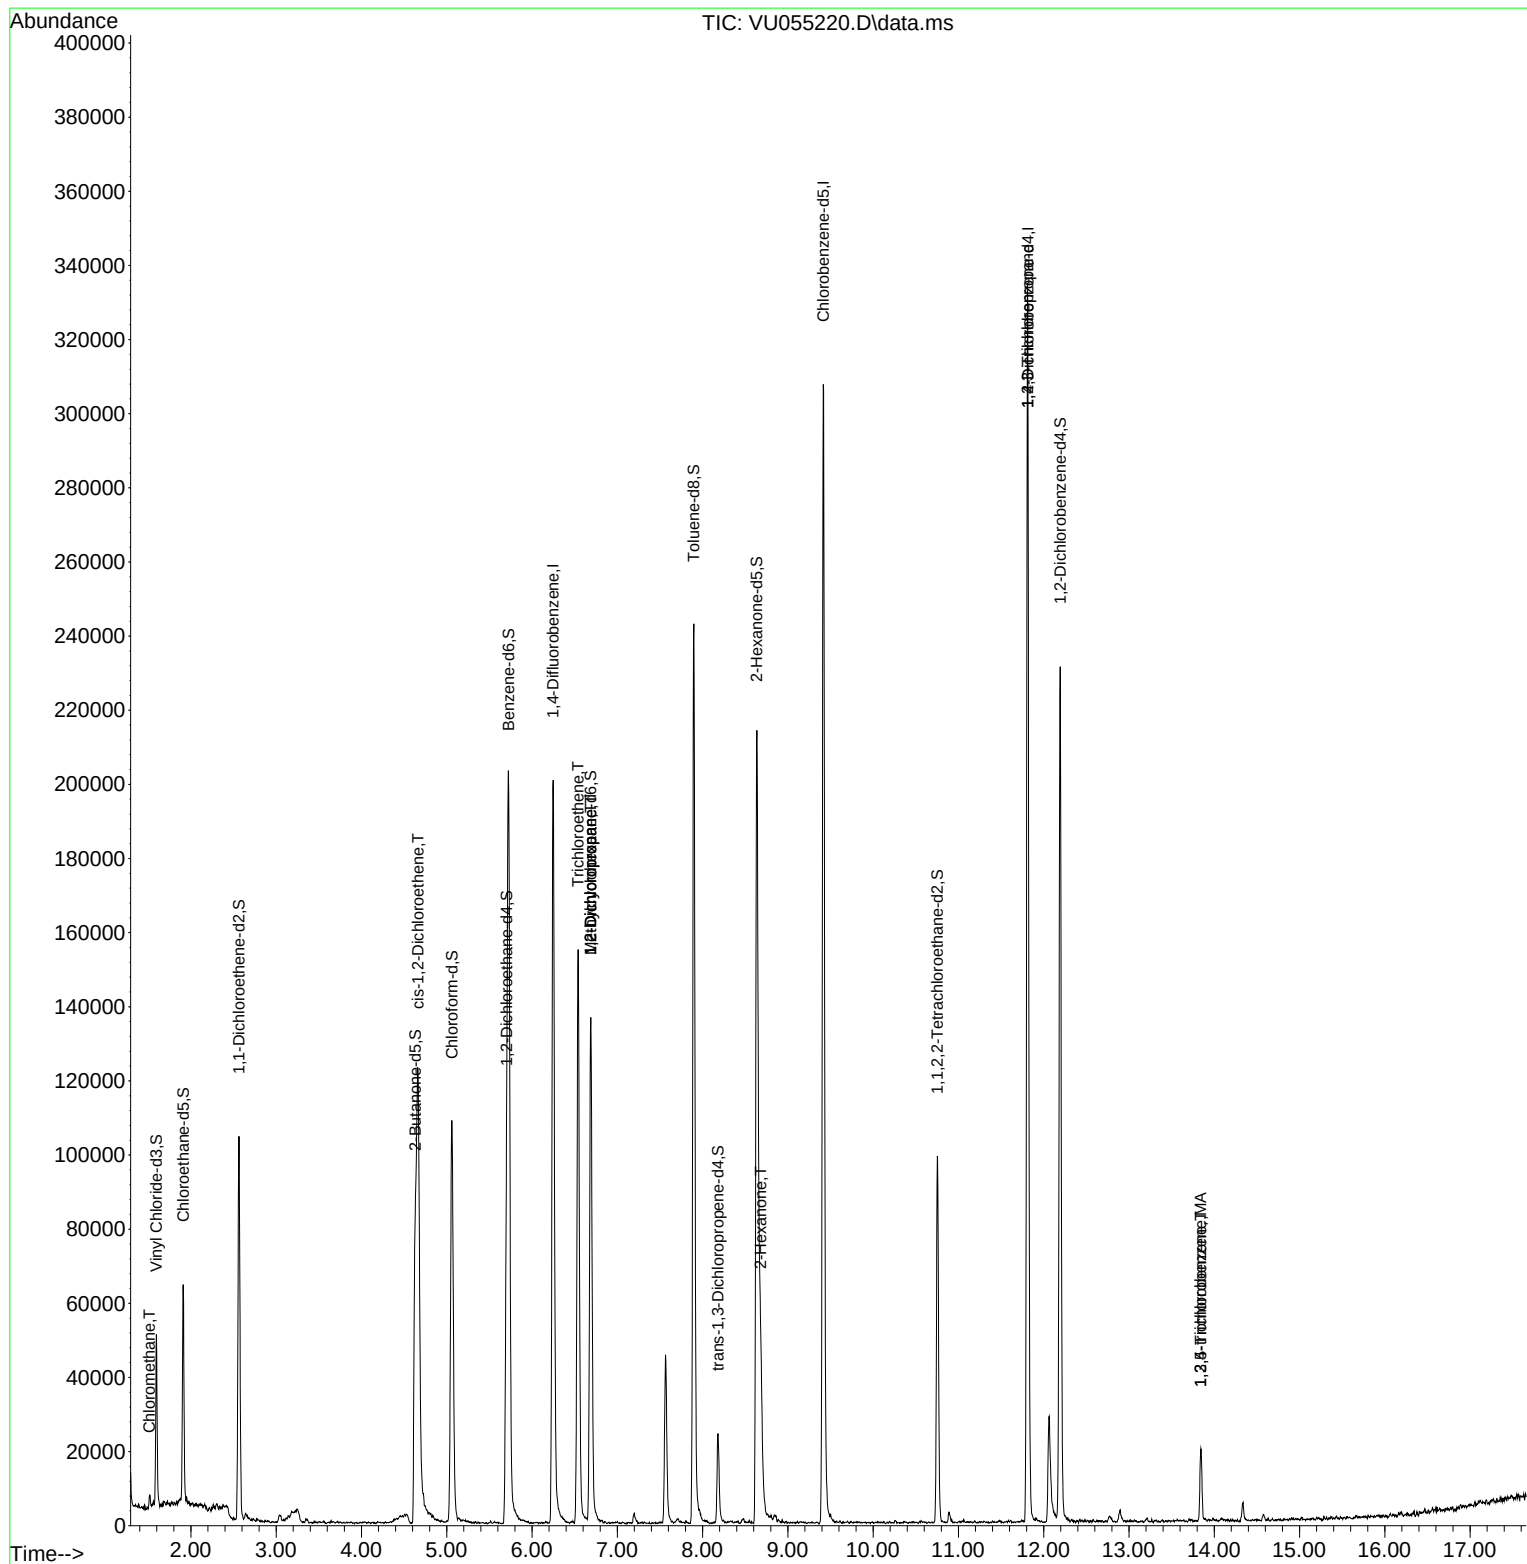


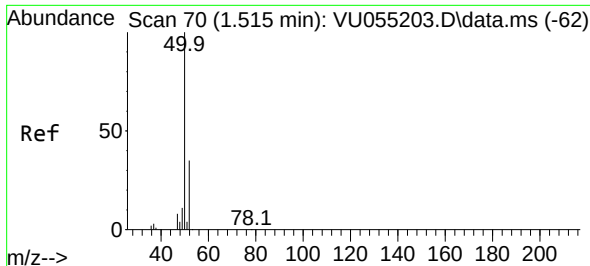

#3
Chloromethane
Concen: 0.210 ug/L
RT: 1.515 min Scan# 70
Delta R.T. -0.000 min
Lab File: VU055220.D
Acq: 08 Sep 2023 05:19




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 50 Resp: 1998
Ion Ratio Lower Upper
50 100
52 28.5 22.5 41.7

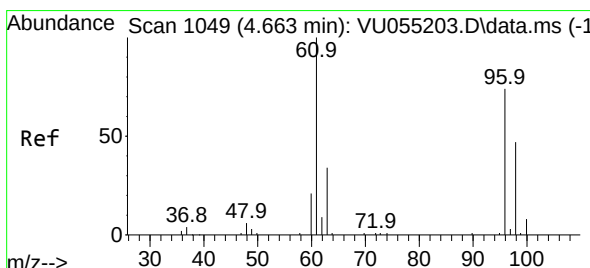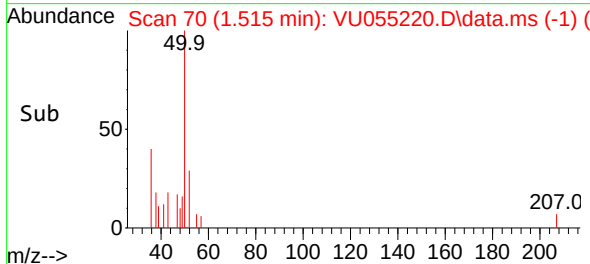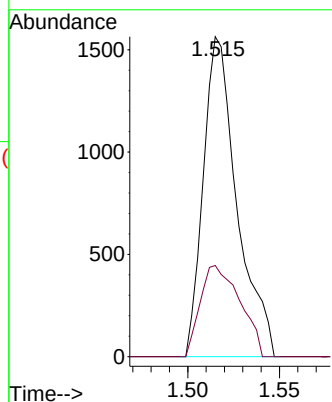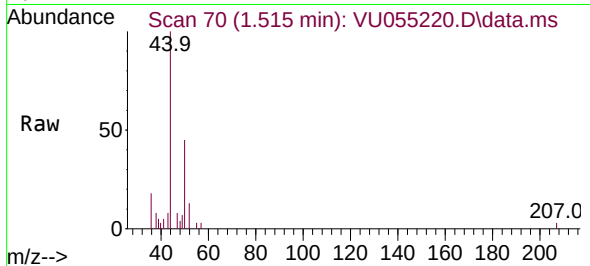

#22
cis-1,2-Dichloroethene
Concen: 5.325 ug/L
RT: 4.663 min Scan# 1049
Delta R.T. -0.000 min
Lab File: VU055220.D
Acq: 08 Sep 2023 05:19

Tgt Ion: 96 Resp: 49261
Ion Ratio Lower Upper
96 100
61 133.9 97.2 180.4
98 63.9 46.1 85.7


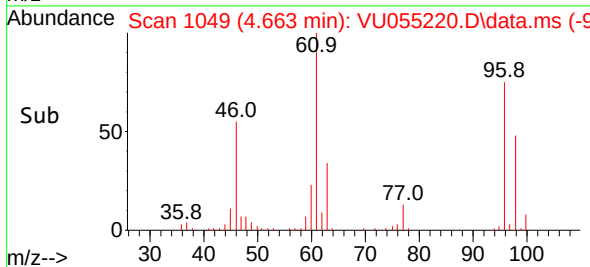
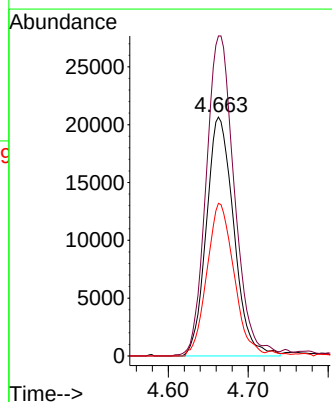
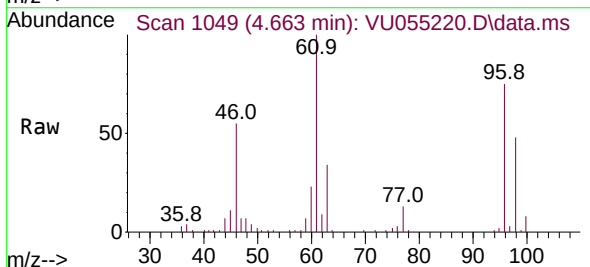


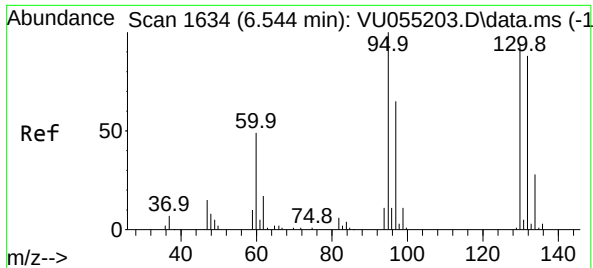

#34
Trichloroethene
Concen: 5.201 ug/L
RT: 6.541 min Scan# 1634
Delta R.T. -0.003 min
Lab File: VU055220.D
Acq: 08 Sep 2023 05:19




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 95 Resp: 52823
Ion Ratio Lower Upper
95 100
97 65.3 44.7 83.1
132 90.5 66.6 123.6
130 92.7 66.5 123.5

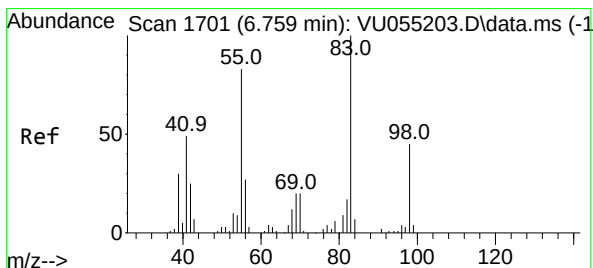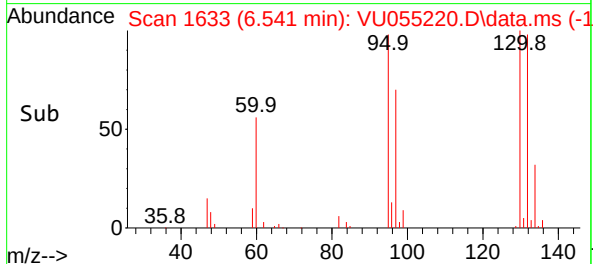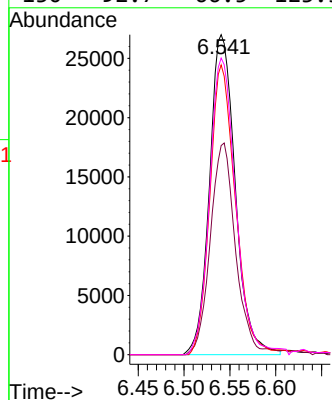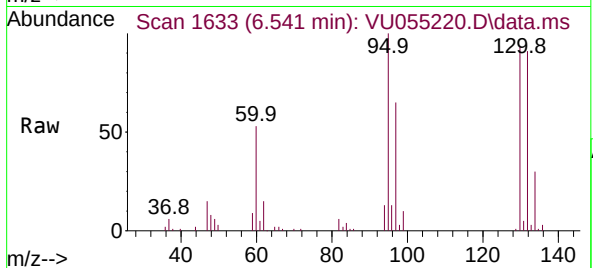

#35
Methylcyclohexane
Concen: 1.062 ug/L
RT: 6.688 min Scan# 1679
Delta R.T. -0.071 min
Lab File: VU055220.D
Acq: 08 Sep 2023 05:19

Tgt Ion: 83 Resp: 15140
Ion Ratio Lower Upper
83 100
55 0.3 60.4 90.6#
98 0.0 35.3 52.9#


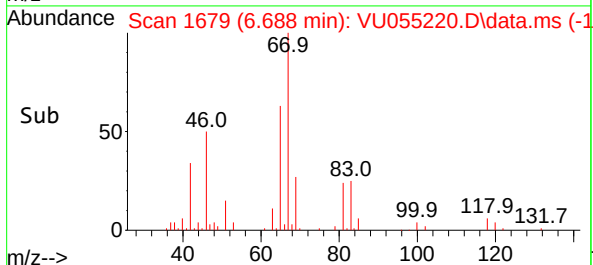
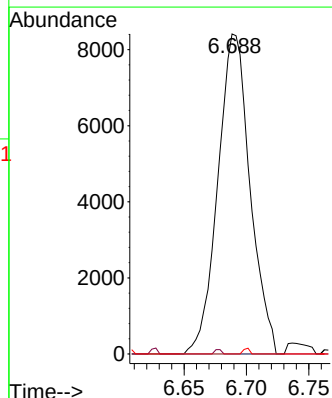
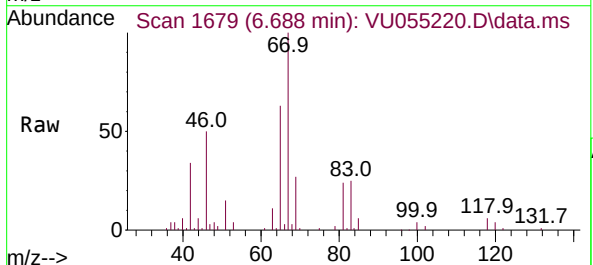


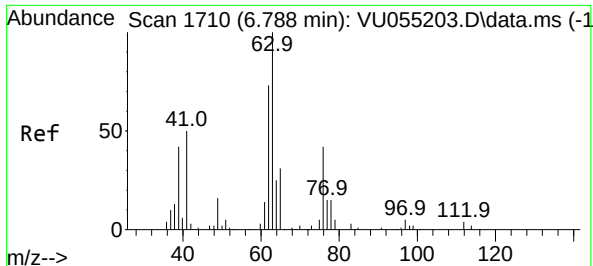

#37
1,2-Dichloropropane
Concen: 0.745 ug/L
RT: 6.688 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU055220.D
Acq: 08 Sep 2023 05:19




Instrument :
MSVOA_U
ClientSampleId :


Tgt Ion: 63 Resp: 7411
Ion Ratio Lower Upper
63 100
112 0.0 3.2 4.8#

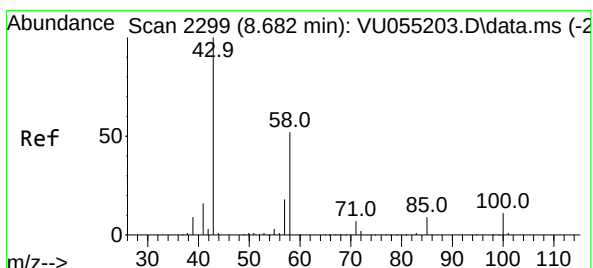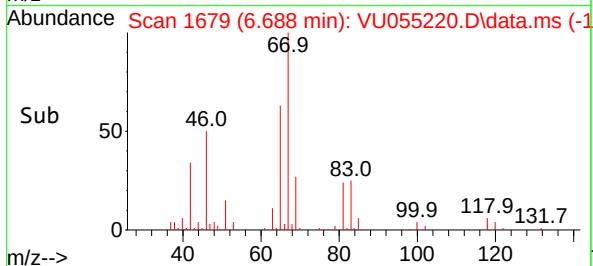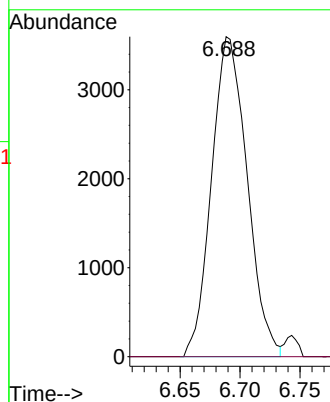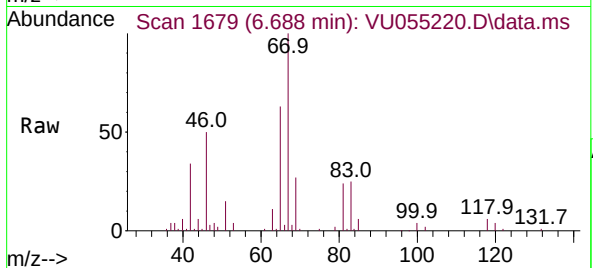

#48
2-Hexanone
Concen: 5.408 ug/L
RT: 8.682 min Scan# 2299
Delta R.T. -0.000 min
Lab File: VU055220.D
Acq: 08 Sep 2023 05:19

Tgt Ion: 43 Resp: 24040
Ion Ratio Lower Upper
43 100
58 48.8 44.0 66.0
57 19.8 16.2 24.2
100 8.3 9.0 13.4#

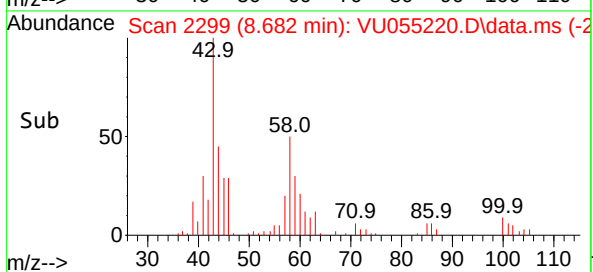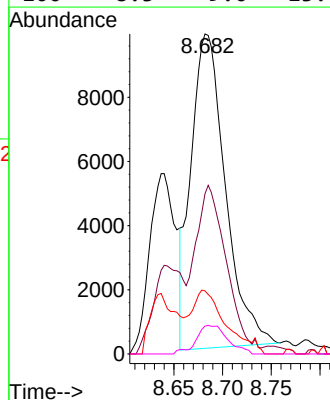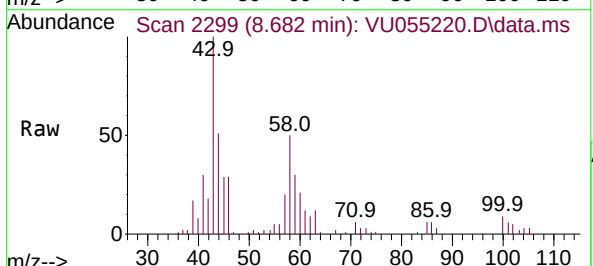

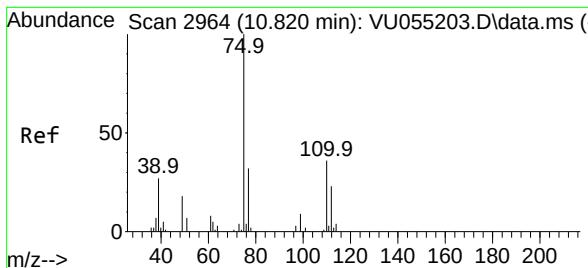

#61

1,2,3-Trichloropropane

Concen: 2.315 ug/L

RT: 11.810 min Scan# 31

Delta R.T. 0.990 min

Lab File: VU055220.D





Acq: 08 Sep 2023 05:19

Instrument :

MSVOA_U

ClientSampleId :

Tgt Ion:	75	Resp:	12986
Ion	Ratio	Lower	Upper
75	100		
110	3.2	28.2	42.2#
77	31.2	26.2	39.4

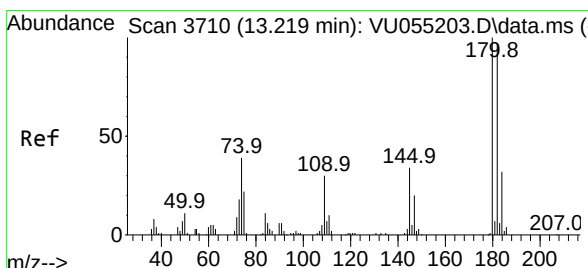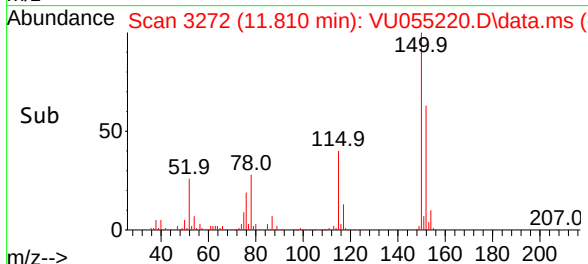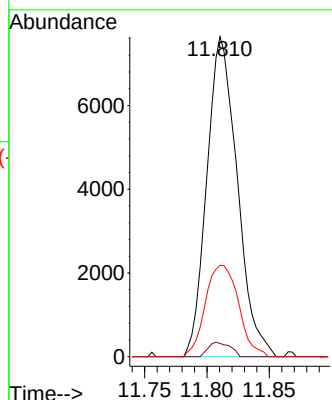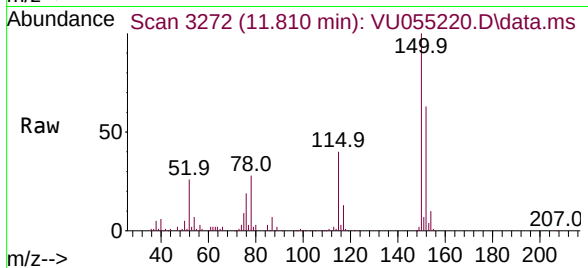

#69

1,3,5-Trichlorobenzene

Concen: 0.442 ug/L




RT: 13.842 min Scan# 3904


Delta R.T. 0.624 min

Lab File: VU055220.D

Acq: 08 Sep 2023 05:19

Tgt Ion:	180	Resp:	6318
Ion	Ratio	Lower	Upper
180	100		
182	86.7	75.8	113.6
184	26.2	24.0	36.0
145	28.5	26.3	39.5

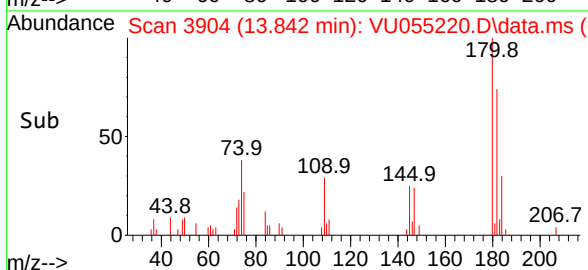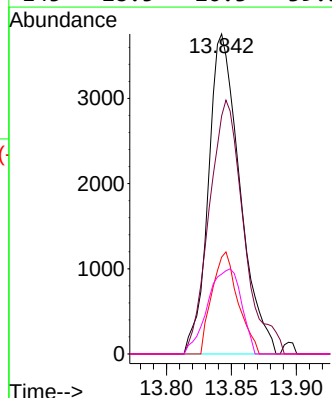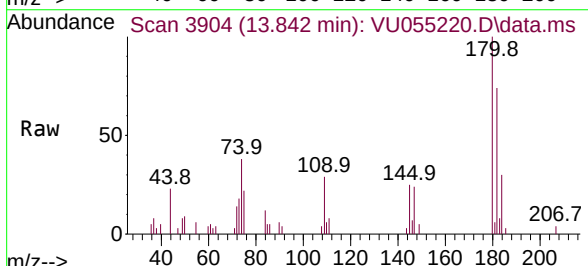

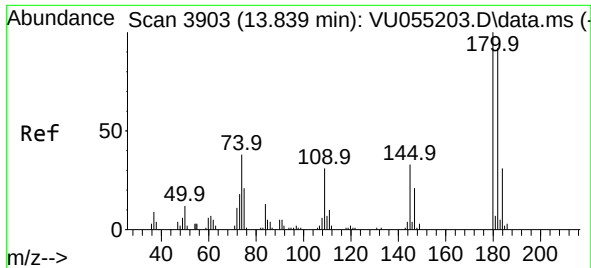

#70

1,2,4-trichlorobenzene

Concen: 0.471 ug/L

RT: 13.842 min Scan# 3904

Delta R.T. 0.003 min


Lab File: VU055220.D

Acq: 08 Sep 2023 05:19

Instrument :

MSVOA_U

ClientSampleId :

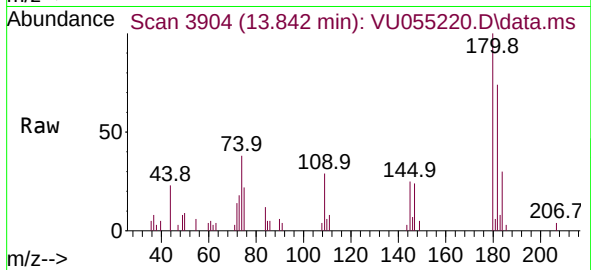

Tgt Ion:180 Resp: 6318

Ion Ratio Lower Upper

180 100

182 86.7 73.6 110.4

145 28.5 25.8 38.8

