




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

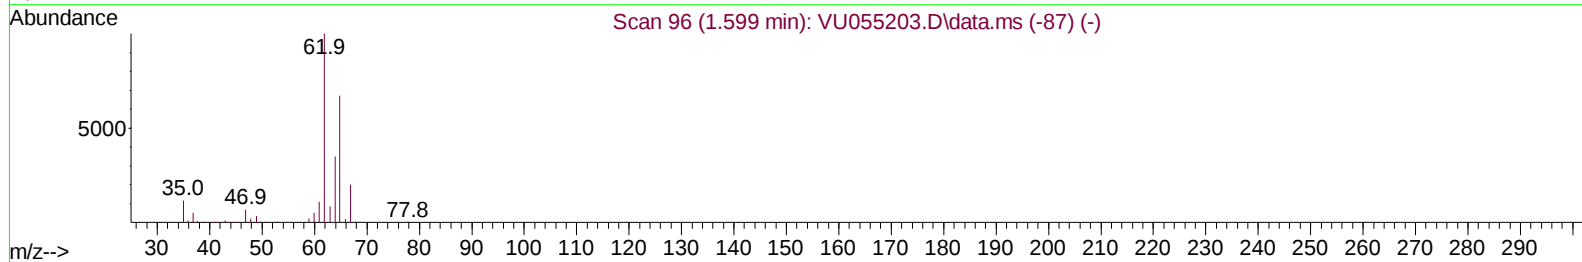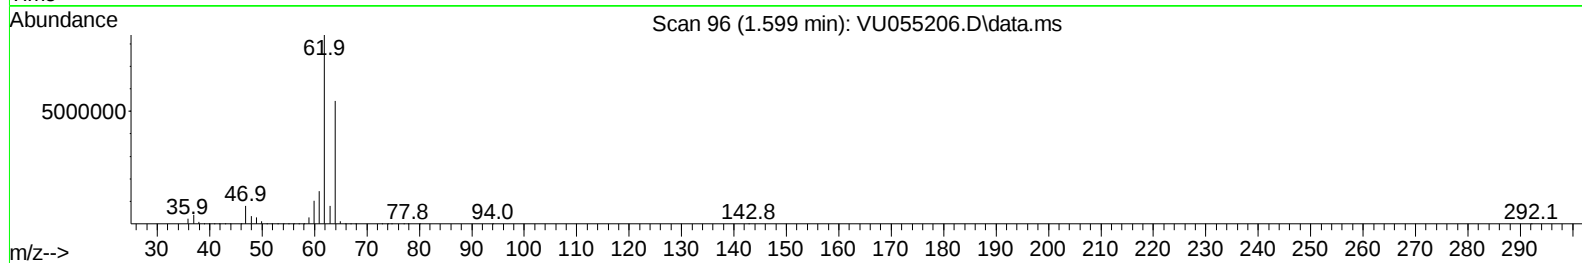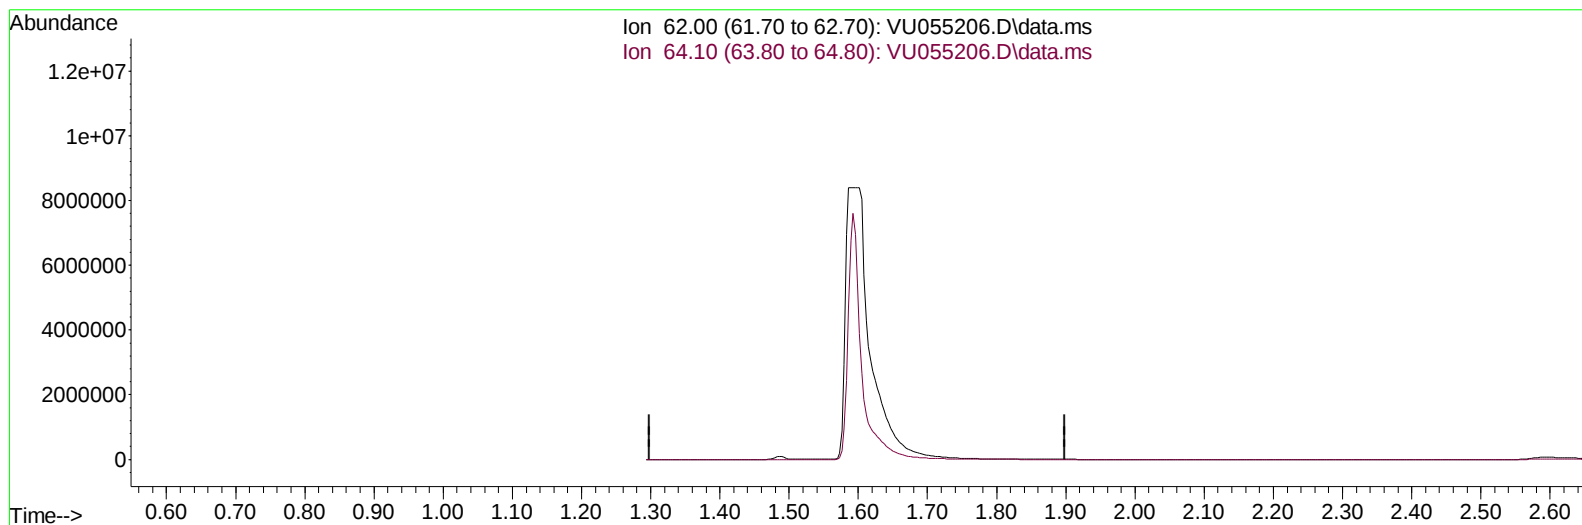

TIC: VU055206.D\data.ms

(5) Vinyl chloride (T)

1.599min (-1.599) 0.00 ug/L

response 0

Ion	Exp%	Act%
62.00	100.00	0.00
64.10	34.60	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

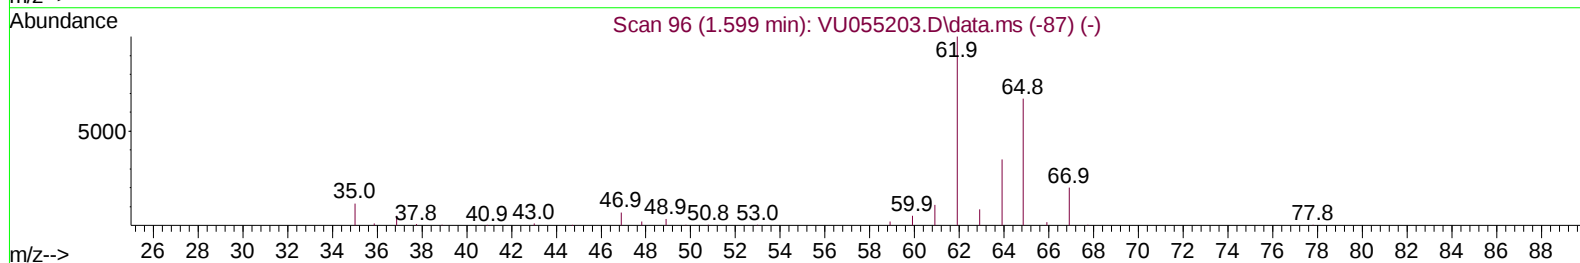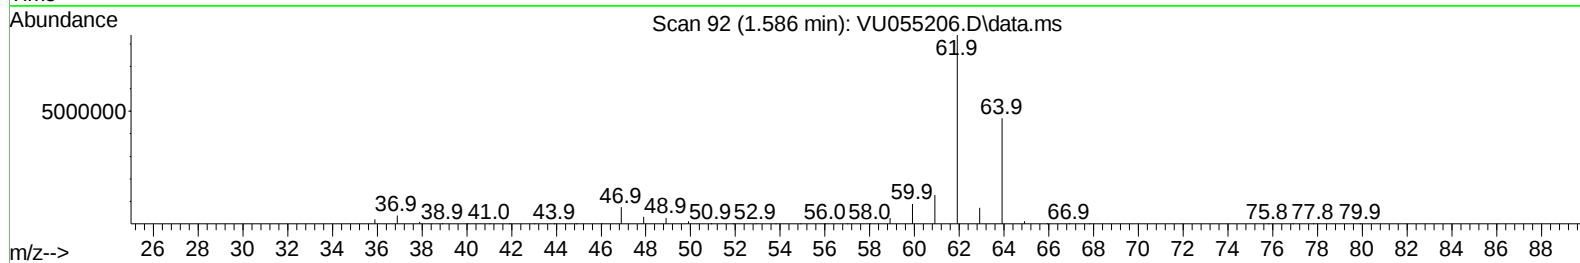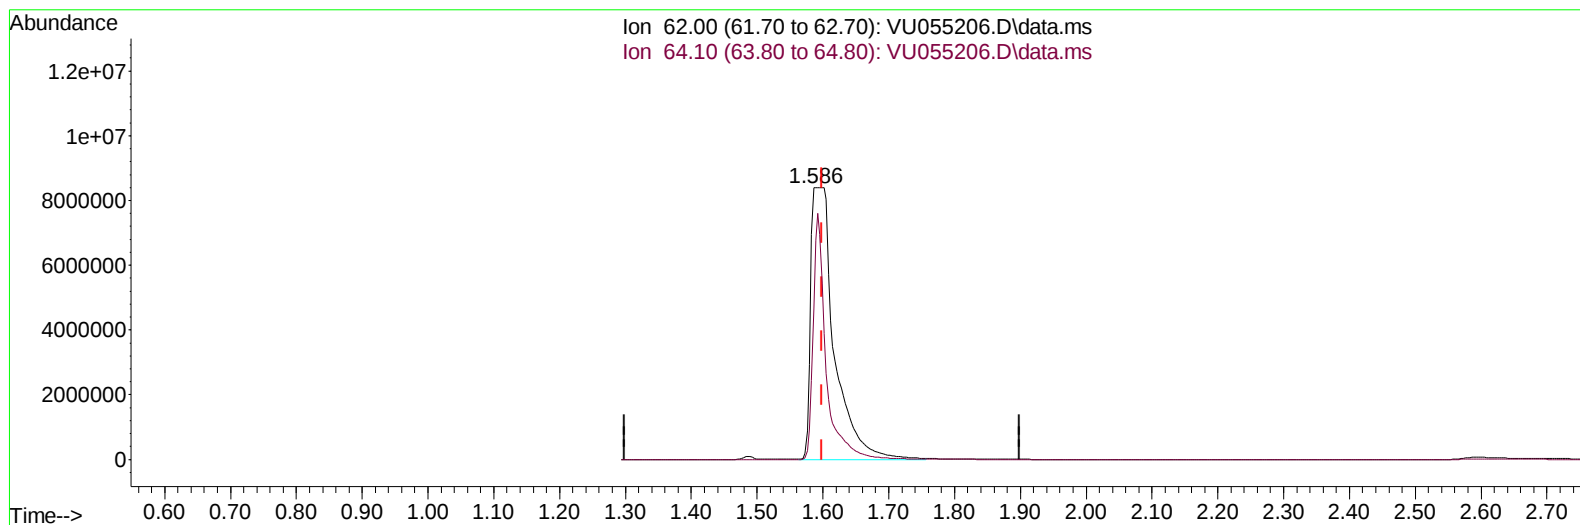

TIC: VU055206.D\data.ms

(5) Vinyl chloride (T)

1.586min (-0.013) 1530.09 ug/L m

response 20995863

Ion	Exp%	Act%
62.00	100.00	100.00
64.10	34.60	55.81#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

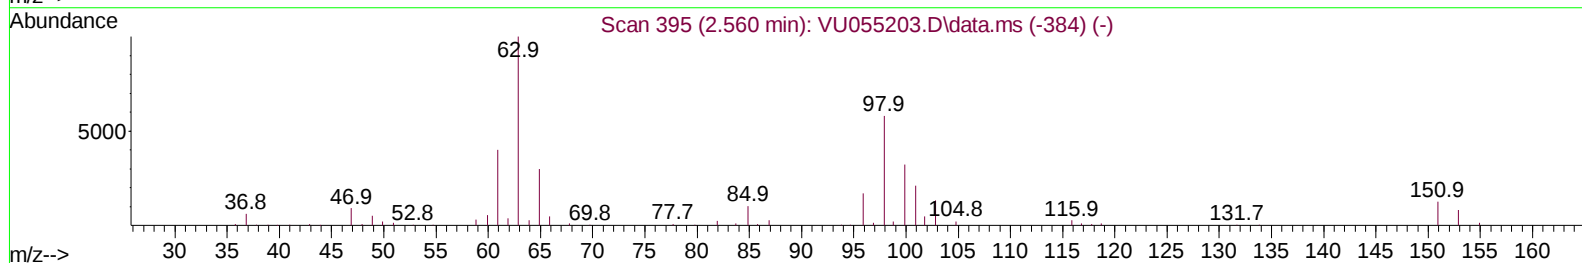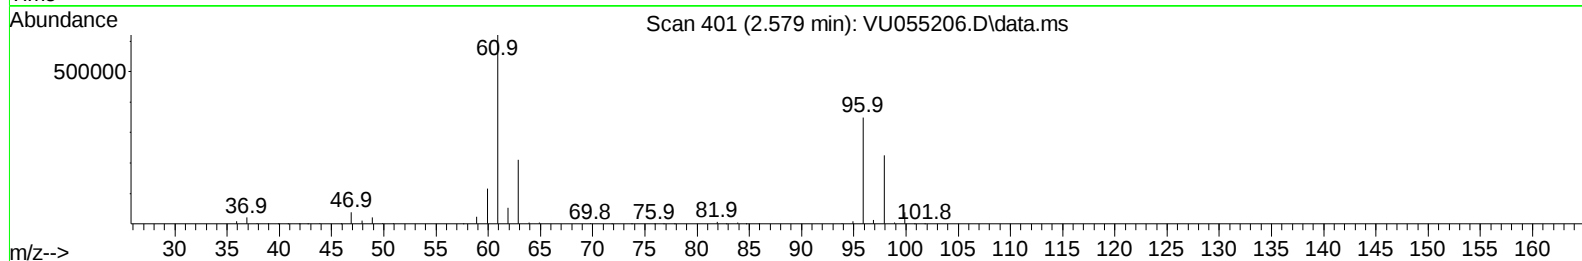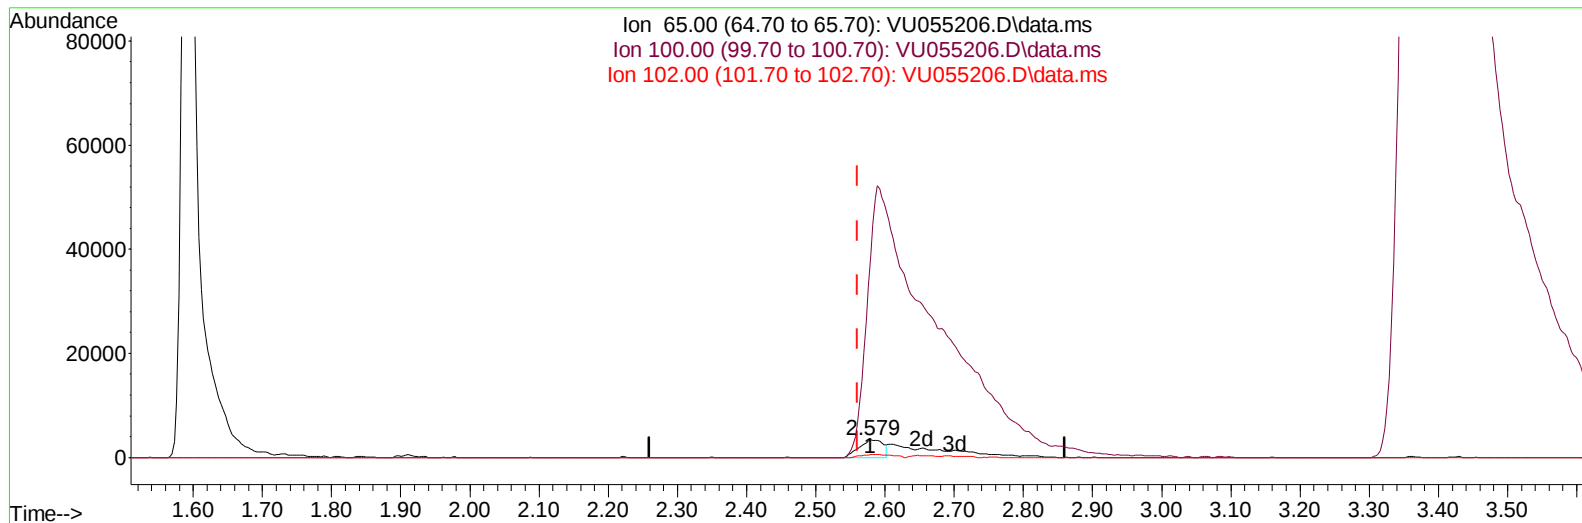

TIC: VU055206.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.579min (+ 0.019) 1.40 ug/L

response 8228

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	132.40	4385.10#
102.00	20.30	21.01
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

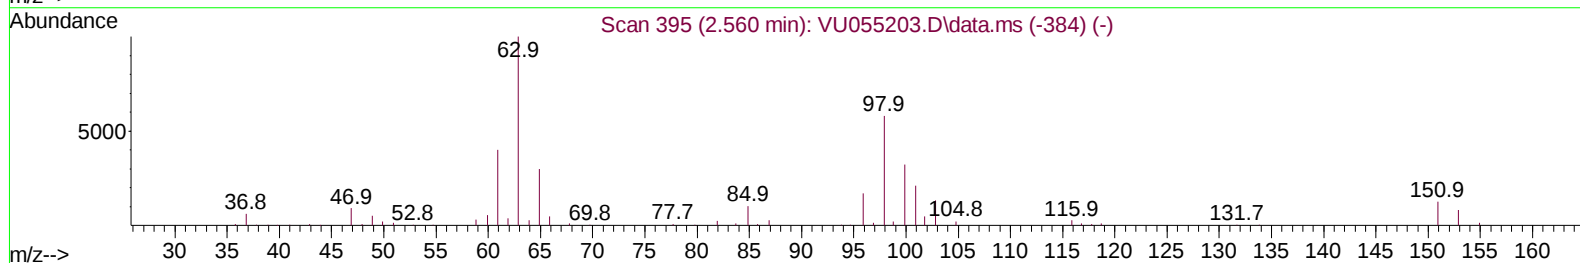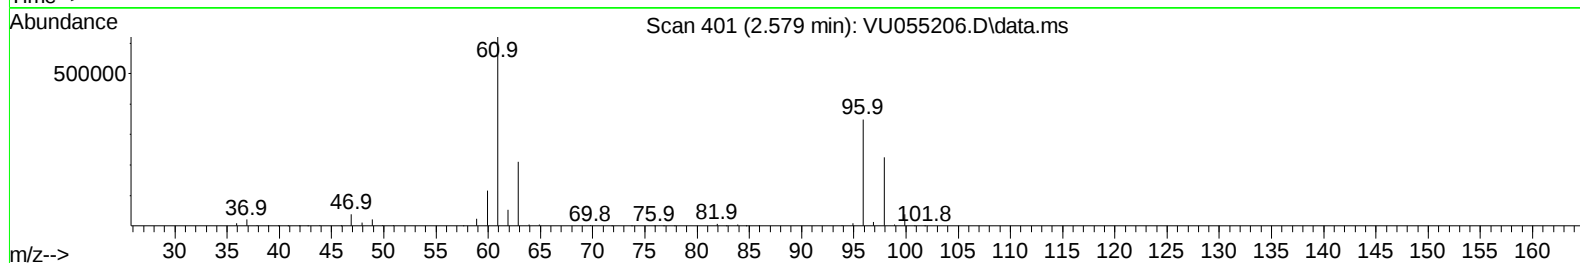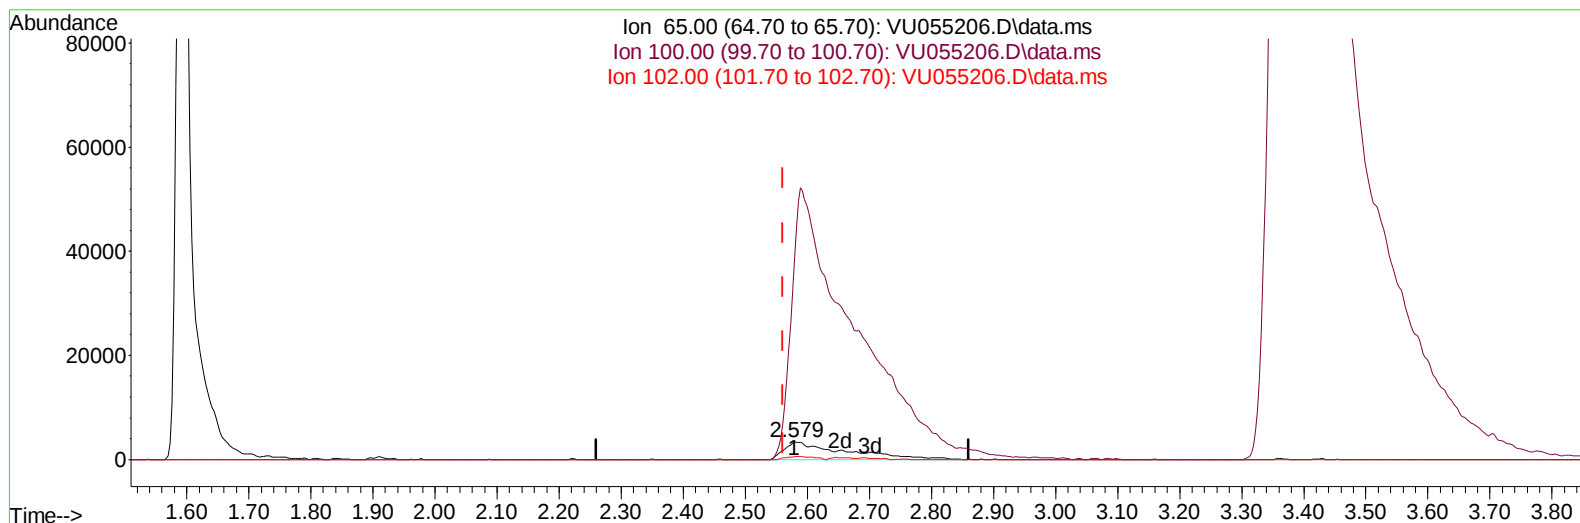

TIC: VU055206.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.579min (+ 0.019) 3.93 ug/L m

response 23101

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	132.40	1561.86#
102.00	20.30	7.48#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

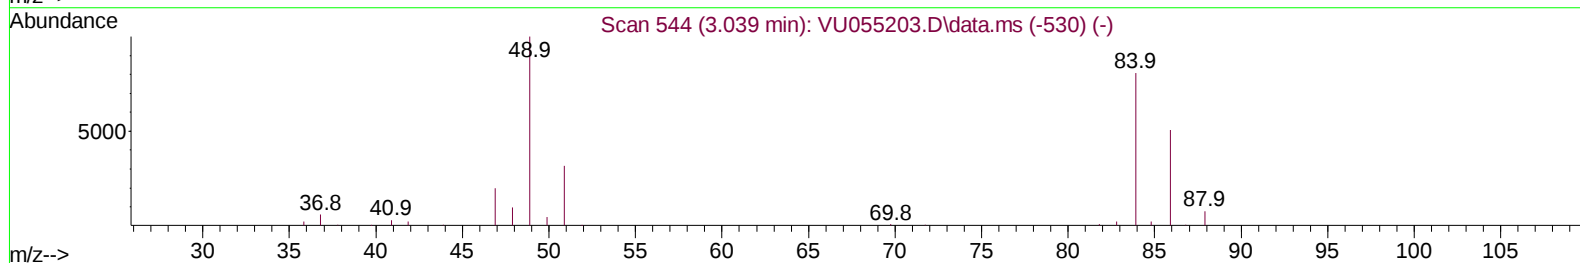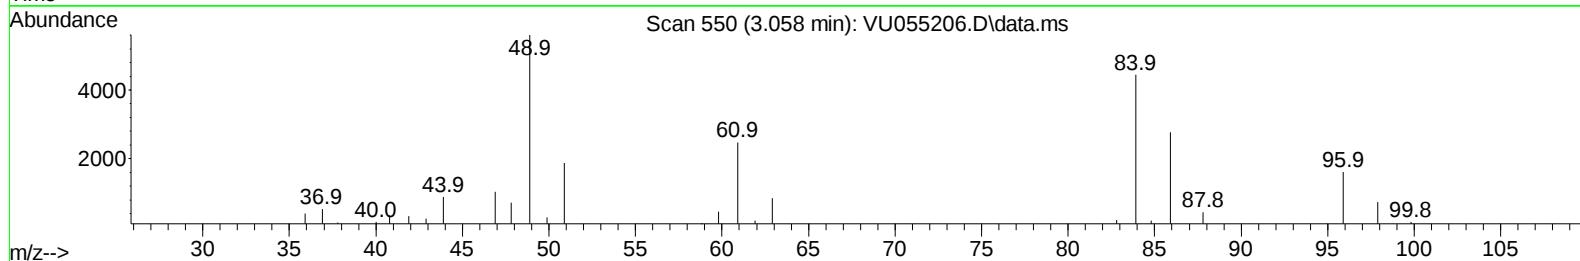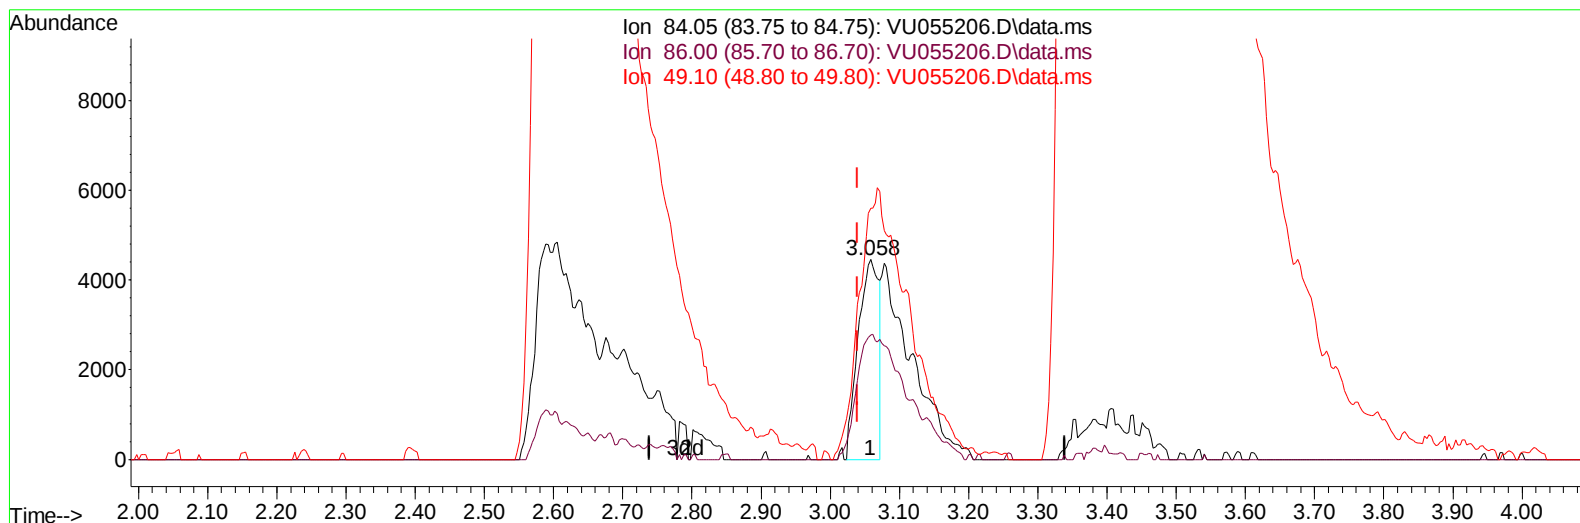

TIC: VU055206.D\data.ms

(16) Methylene chloride (T)

3.058min (+ 0.019) 0.59 ug/L

response 9186

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	62.00	62.39
49.10	125.30	125.80
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

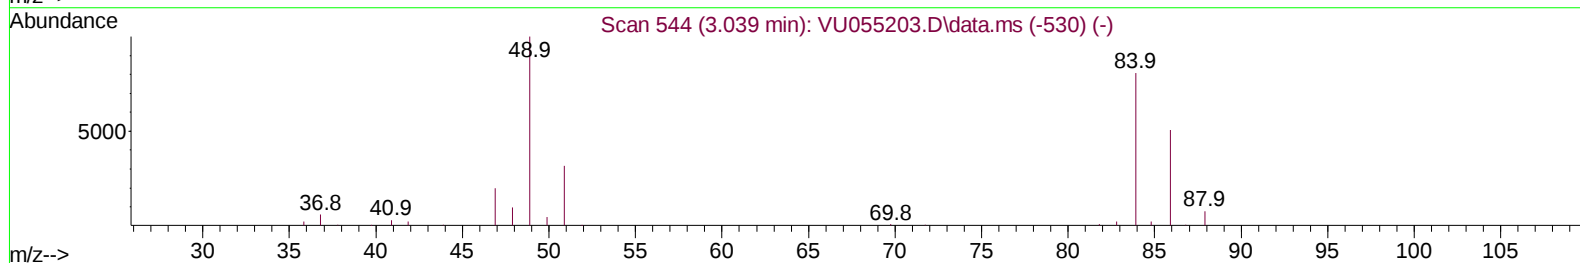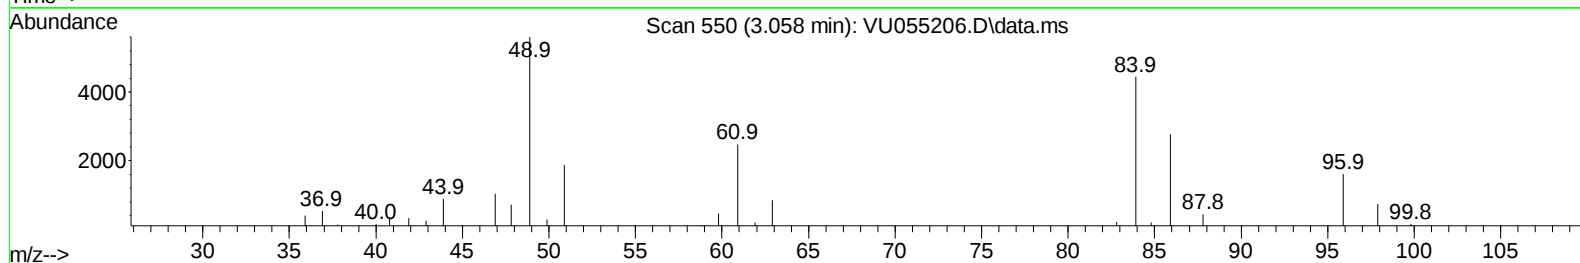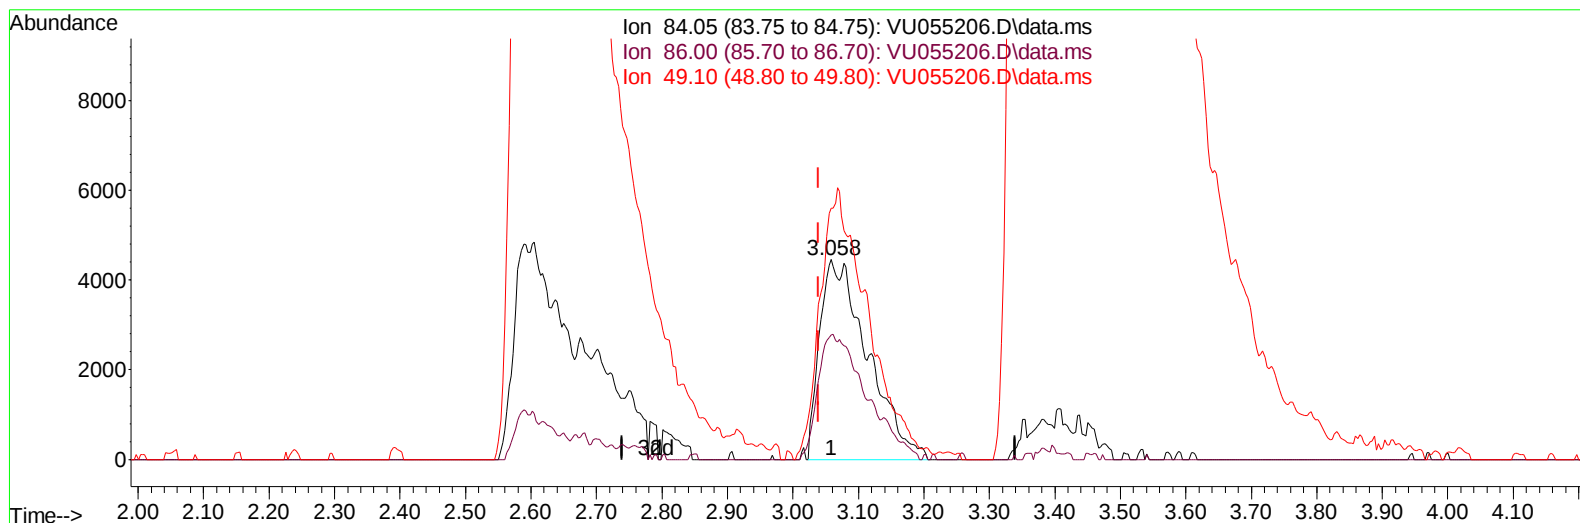

TIC: VU055206.D\data.ms

(16) Methylene chloride (T)

3.058min (+ 0.019) 1.46 ug/L m

response 22606

Ion	Exp%	Act%
84.05	100.00	100.00
86.00	62.00	62.39
49.10	125.30	125.80
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

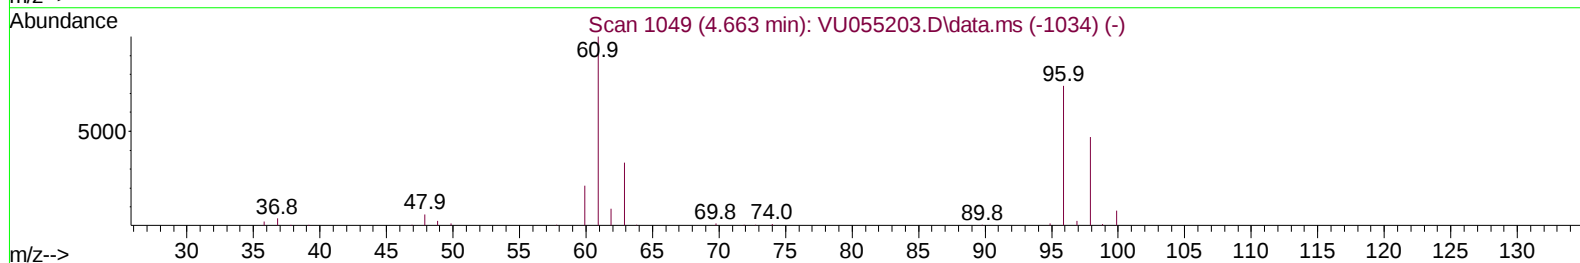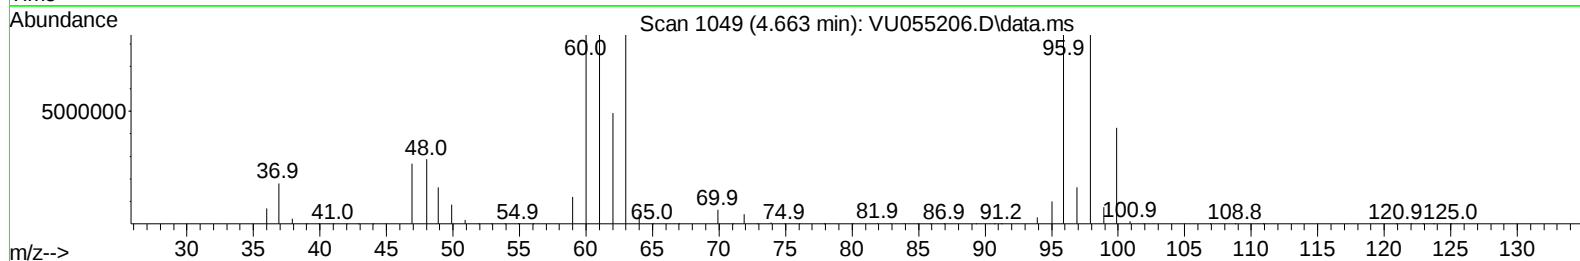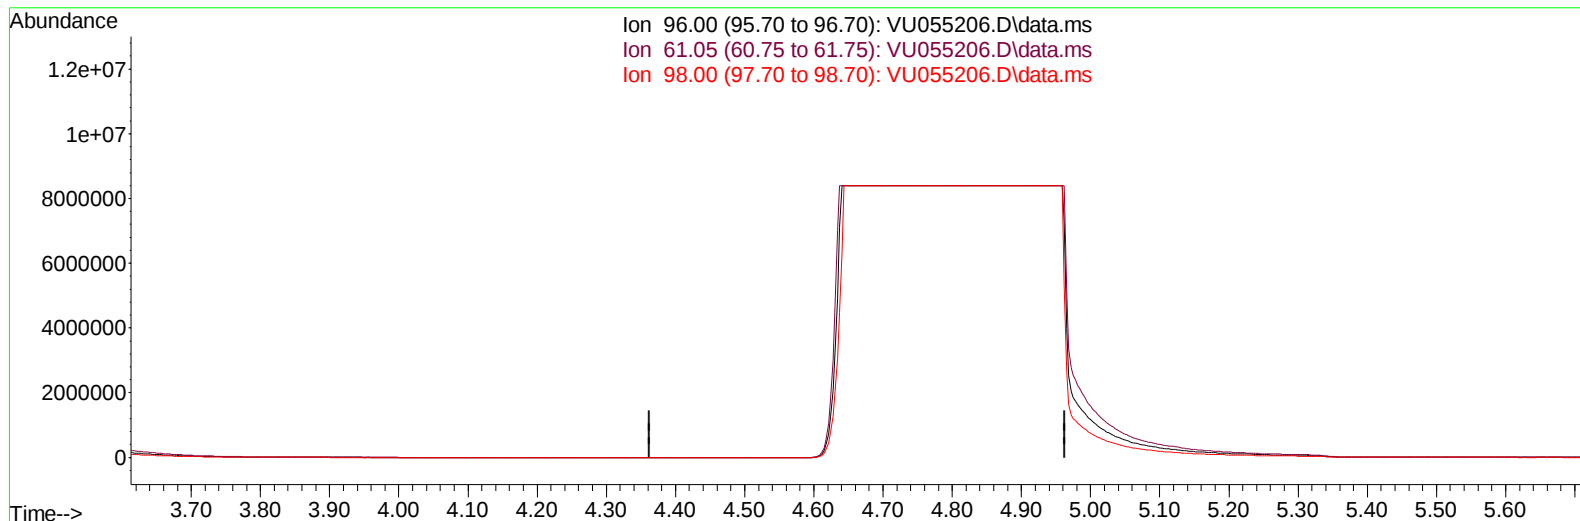

TIC: VU055206.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.663min (-4.663) 0.00 ug/L

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
61.05	138.80	0.00#
98.00	65.90	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

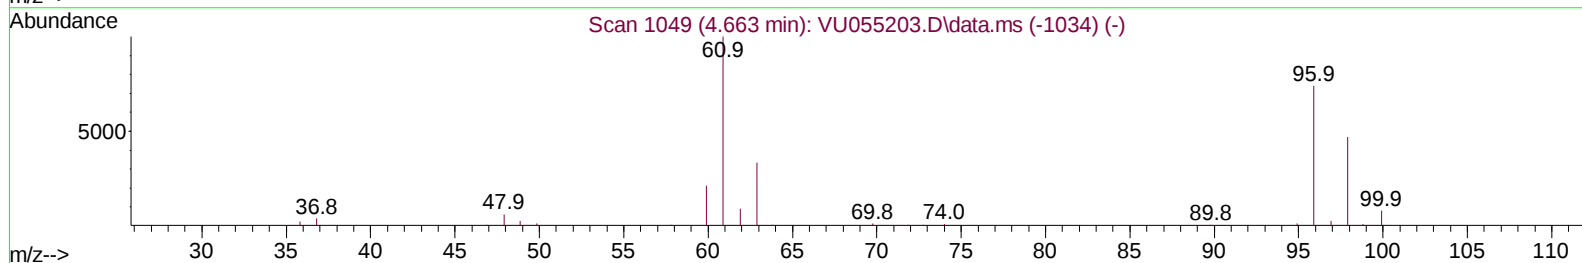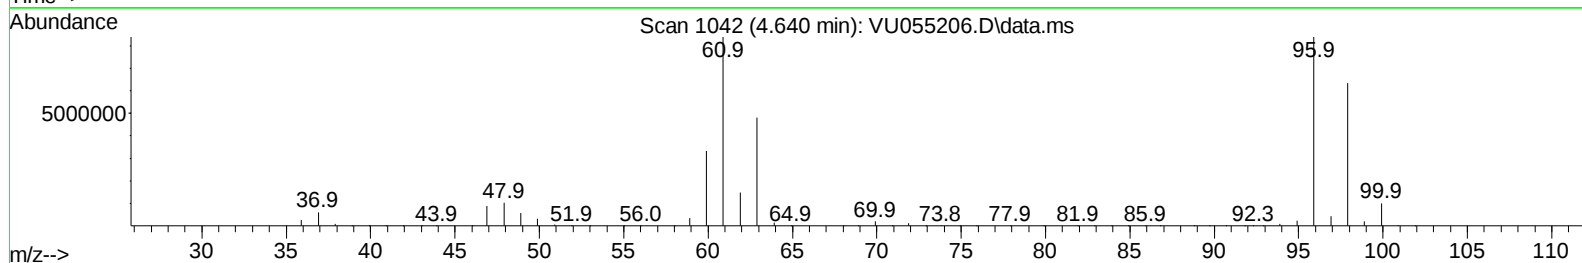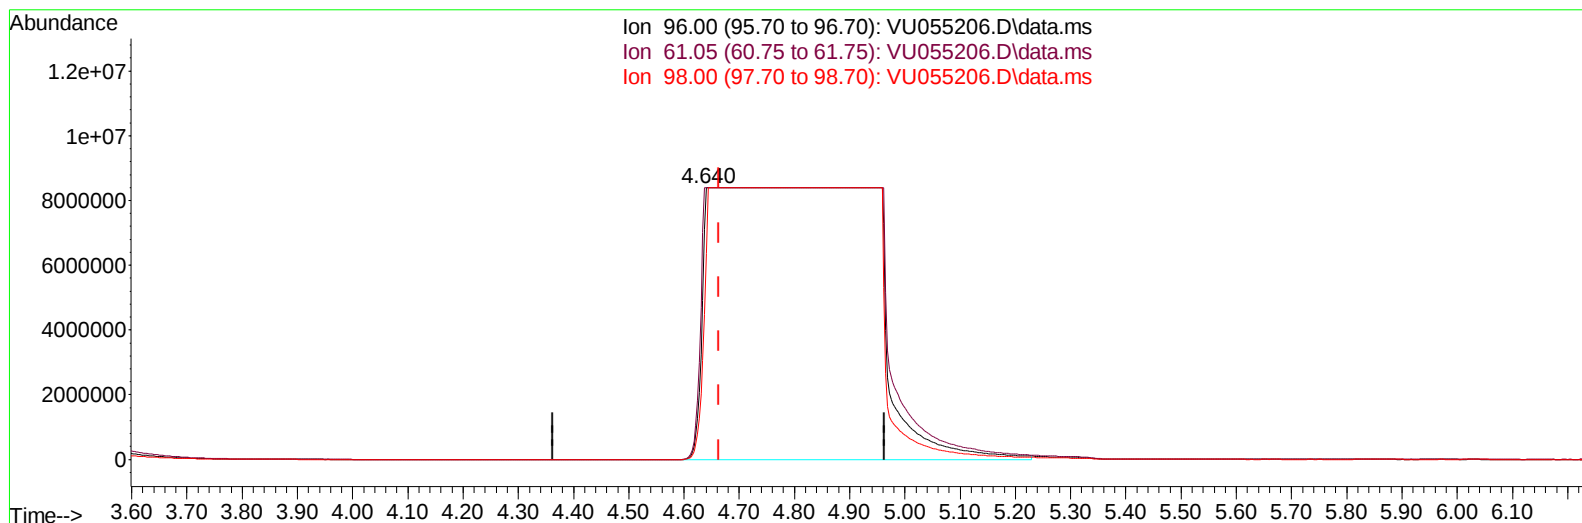

TIC: VU055206.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.640min (-0.023) 13951.15 ug/L m

response 176124367

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	138.80	100.00
98.00	65.90	75.76
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

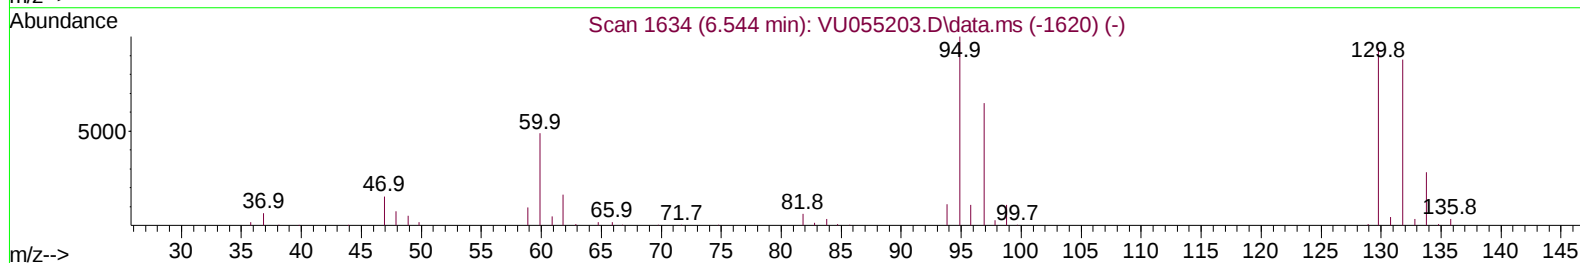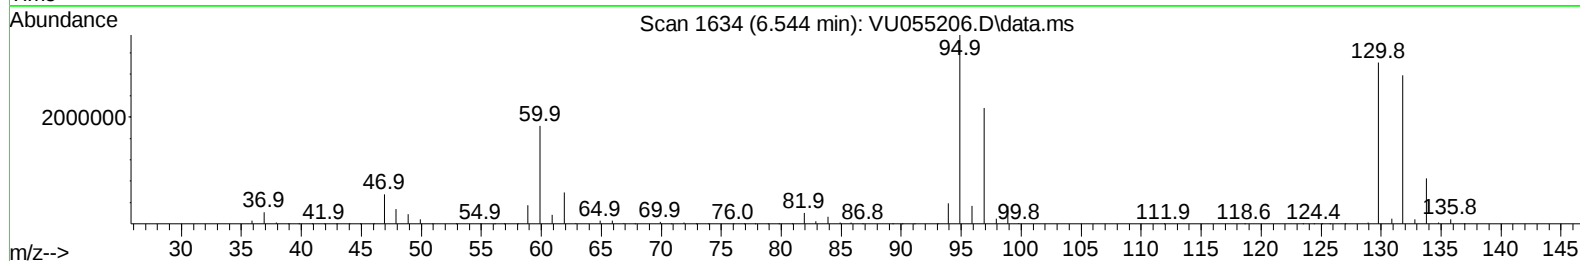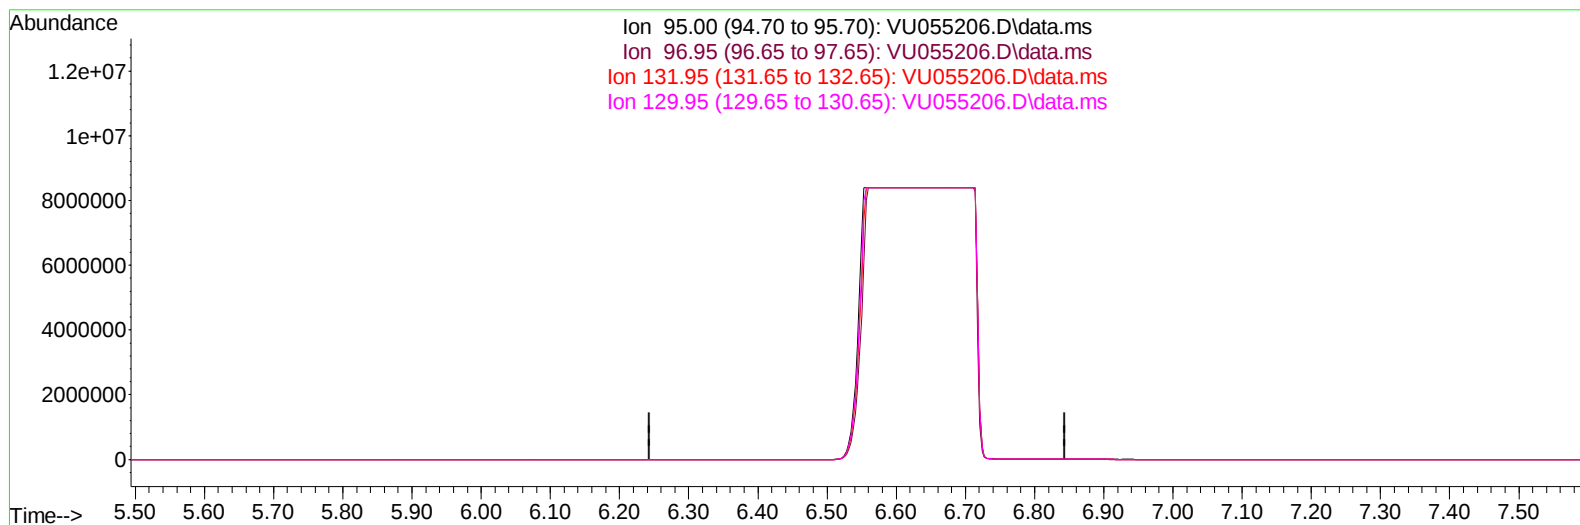

TIC: VU055206.D\data.ms

(34) Trichloroethene (T)

6.544min (-6.544) 0.00 ug/L

response 0

Ion	Exp%	Act%
95.00	100.00	0.00
96.95	63.90	0.00#
131.95	95.10	0.00#
129.95	95.00	0.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

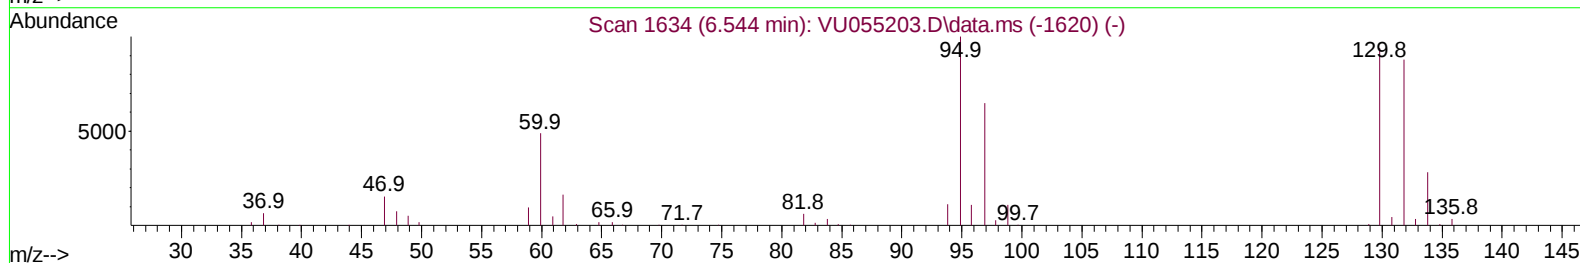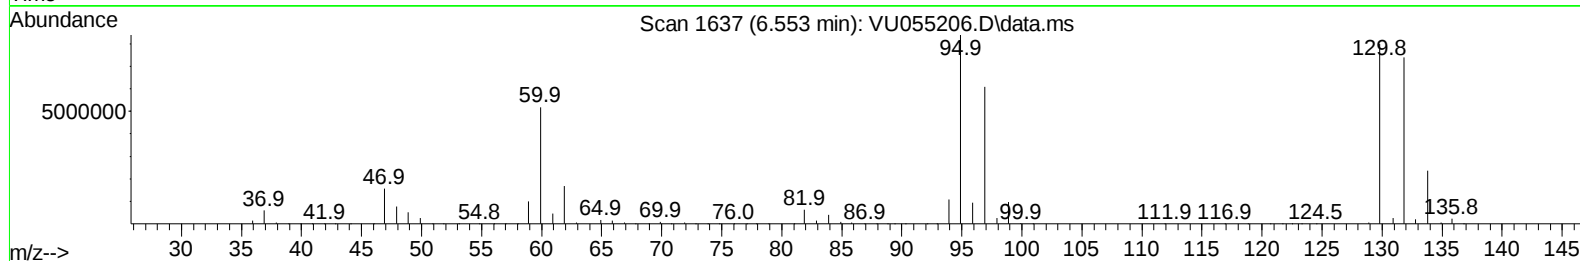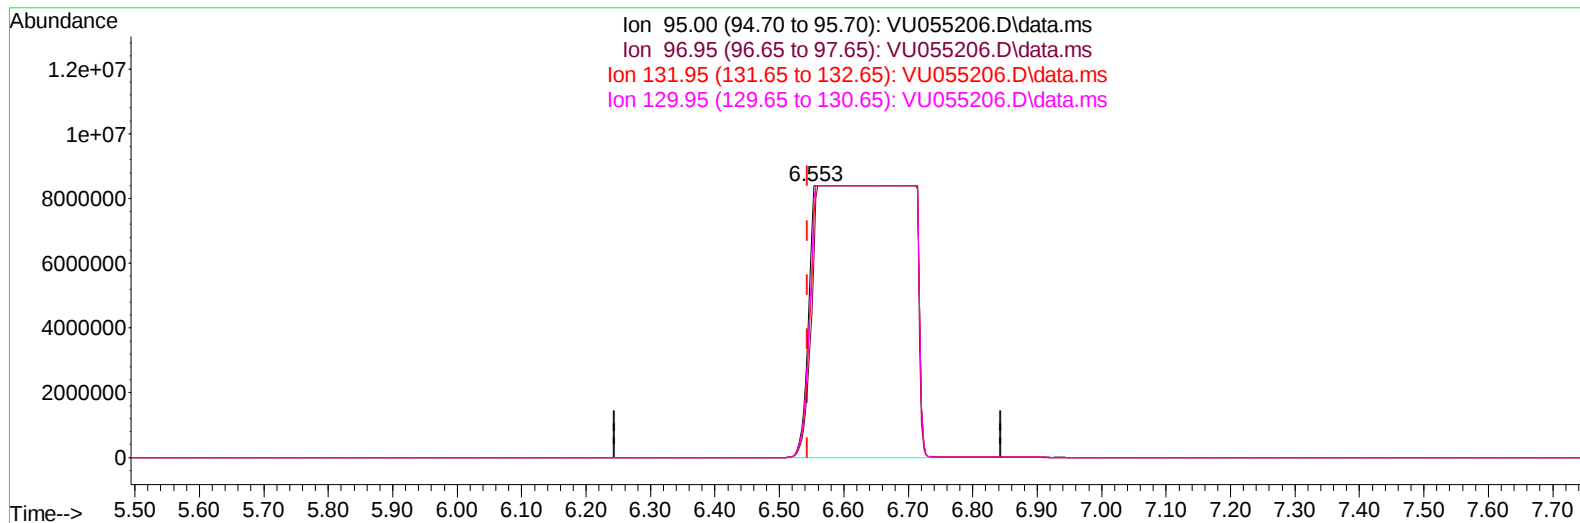

TIC: VU055206.D\data.ms

(34) Trichloroethene (T)

6.553min (+ 0.010) 6396.59 ug/L m

response 87969932

Ion	Exp%	Act%
95.00	100.00	100.00
96.95	63.90	72.47
131.95	95.10	88.02
129.95	95.00	95.10




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

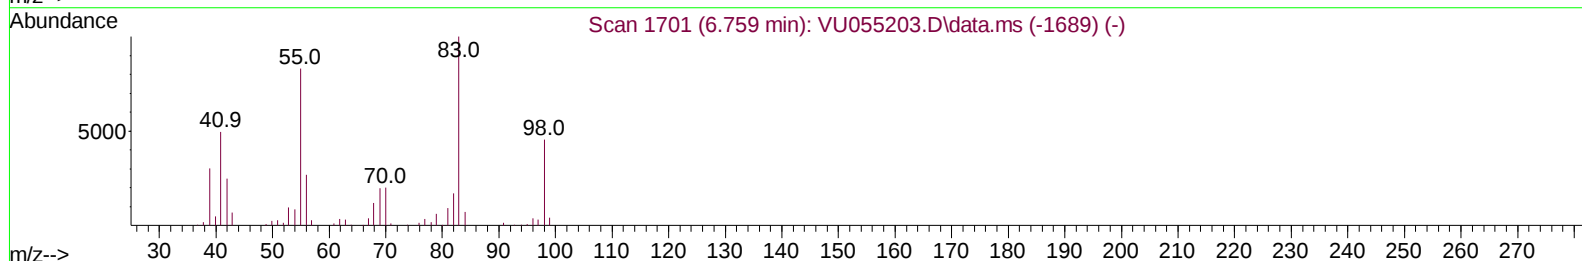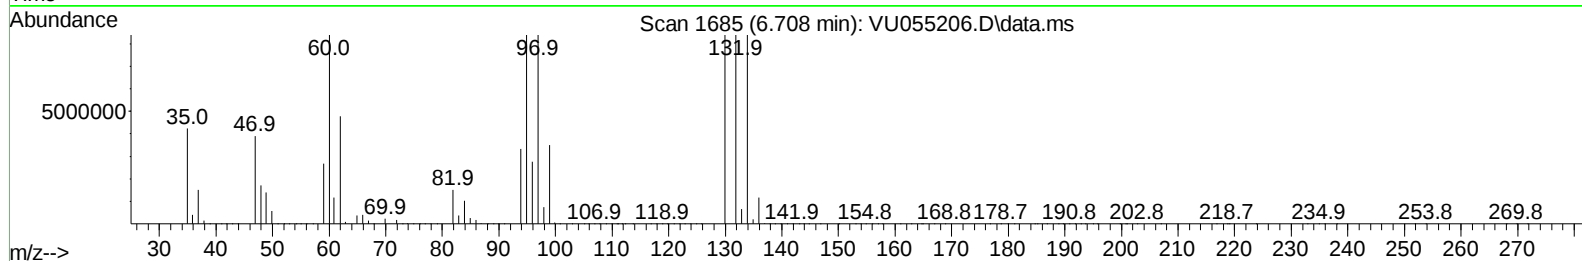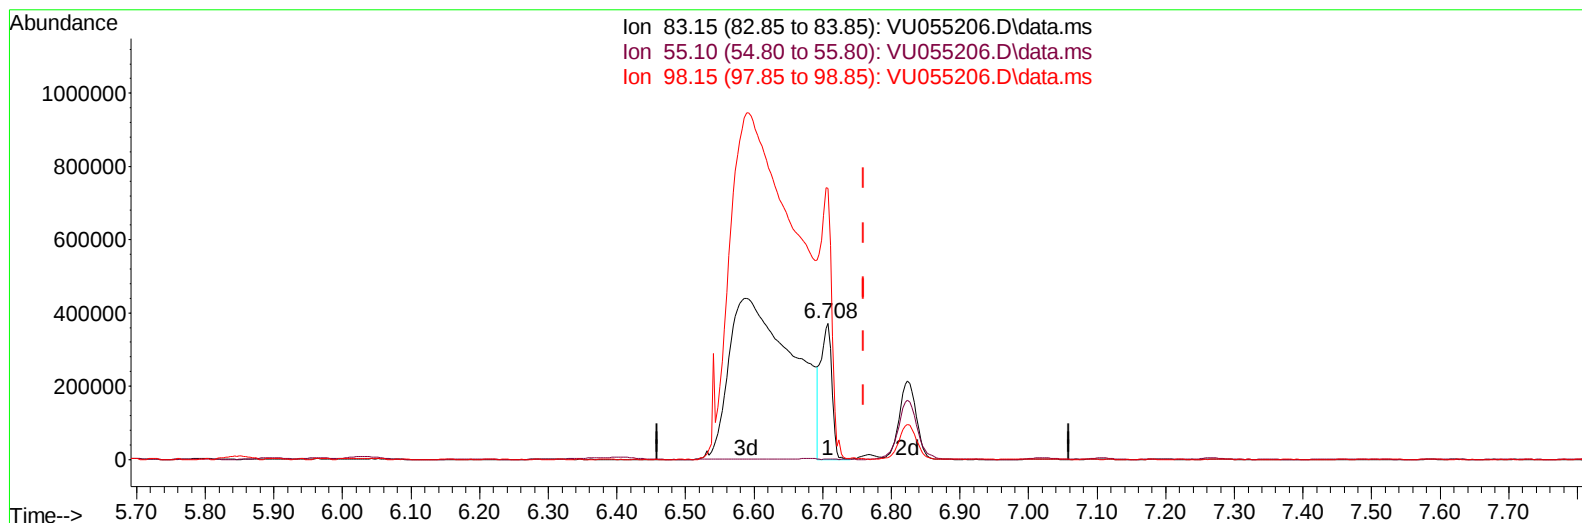

TIC: VU055206.D\data.ms

(35) Methylcyclohexane (T)

6.708min (-0.051) 21.55 ug/L

response 415859

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	75.50	0.00#
98.15	44.10	205.96#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055206.D
Acq On : 07 Sep 2023 23:44
Operator : MD/SY
Sample : 04306-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 06:18:43 2023
Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
Supervised By :Mahesh Dadoda 09/14/2023

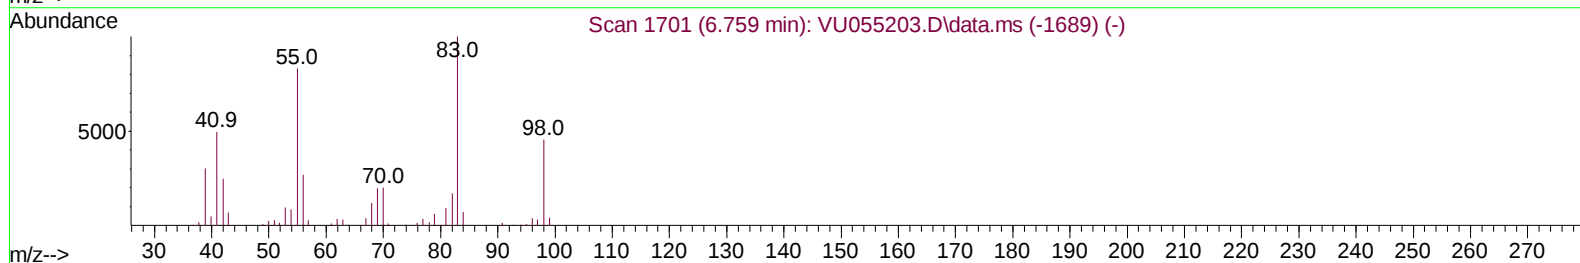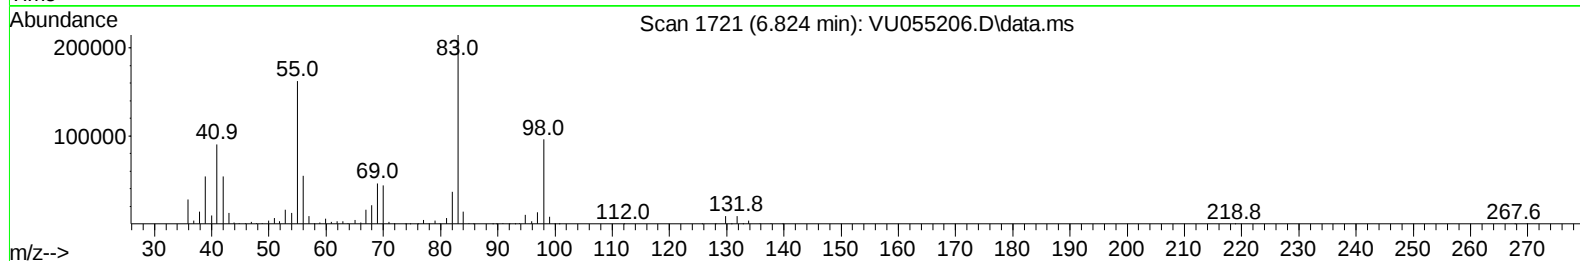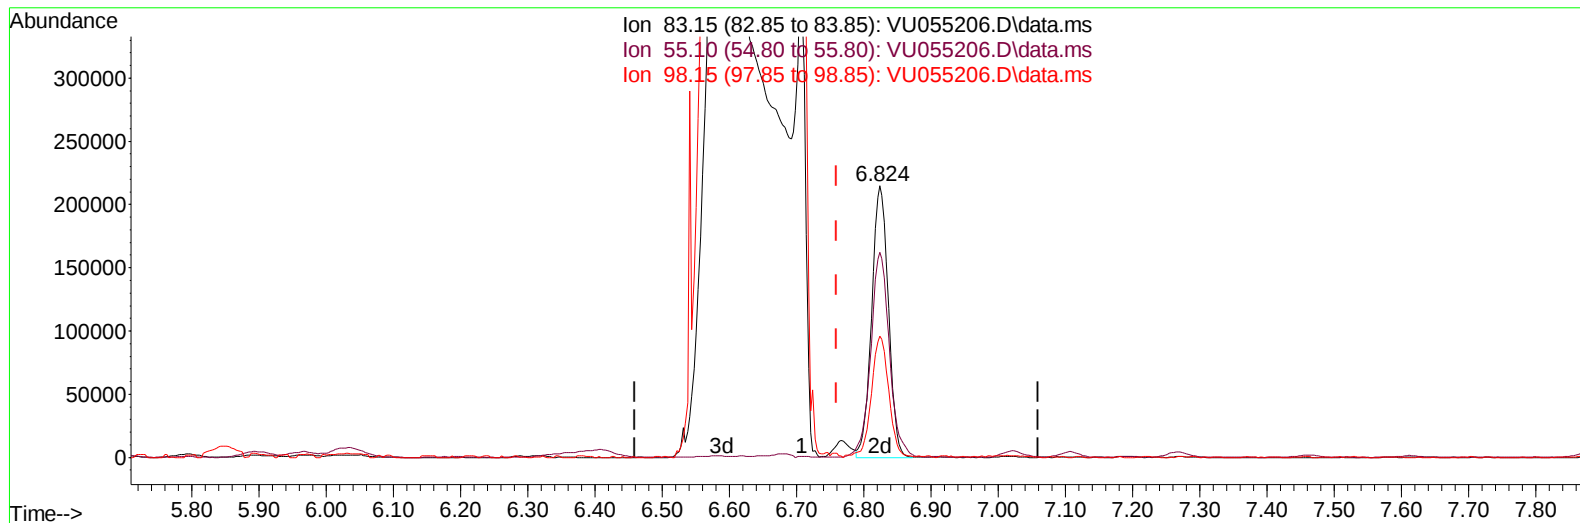

TIC: VU055206.D\data.ms

(35) Methylcyclohexane (T)

6.824min (+ 0.064) 19.21 ug/L m

response 370661

Ion	Exp%	Act%
83.15	100.00	100.00
55.10	75.50	0.00#
98.15	44.10	231.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.306	114	219870	5.000	ug/L	0.06
28) Chlorobenzene-d5	9.425	117	232507	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.814	152	135004	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	256373	24.879	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	497.600%#	
7) Chloroethane-d5	1.911	69	36459	3.057	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	61.200%#	
11) 1,1-Dichloroethene-d2	2.579	65	23101m	3.934	ug/L	0.02
Spiked Amount 5.000	Range 60	- 125	Recovery	=	78.600%	
20) 2-Butanone-d5	0.000	46	0d	0.000	ug/L	
Spiked Amount 50.000	Range 40	- 130	Recovery	=	0.000%#	
24) Chloroform-d	5.155	84	131739	4.818	ug/L	0.09
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	5.759	65	65194	4.765	ug/L	0.06
Spiked Amount 5.000	Range 70	- 130	Recovery	=	95.400%	
32) Benzene-d6	5.788	84	242897	4.232	ug/L	0.06
Spiked Amount 5.000	Range 70	- 125	Recovery	=	84.600%	
36) 1,2-Dichloropropane-d6	6.708	67	142730	7.819	ug/L	0.02
Spiked Amount 5.000	Range 60	- 140	Recovery	=	156.400%#	
41) Toluene-d8	7.920	98	229815	4.347	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	=	87.000%	
43) trans-1,3-Dichloroprop...	8.196	79	27046	5.380	ug/L	0.02
Spiked Amount 5.000	Range 55	- 130	Recovery	=	107.600%	
46) 2-Hexanone-d5	8.647	63	113458	55.594	ug/L	0.02
Spiked Amount 50.000	Range 45	- 130	Recovery	=	111.180%	
56) 1,1,2,2-Tetrachloroeth...	10.759	84	69759	5.434	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	108.600%	
66) 1,2-Dichlorobenzene-d4	12.193	152	85638	4.346	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	87.000%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.586	62	20995863m	1530.089	ug/L	
12) 1,1-Dichloroethene	2.595	96	3318933	326.507	ug/L #	71
16) Methylene chloride	3.058	84	22606m	1.455	ug/L	
18) trans-1,2-Dichloroethene	3.380	96	16237271	1574.424	ug/L	97
22) cis-1,2-Dichloroethene	4.640	96	176124367m	13951.151	ug/L	
25) Chloroform	5.174	83	317016	13.657	ug/L	98
27) 1,2-Dichloroethane	5.846	62	223037	15.742	ug/L	95
30) Cyclohexane	5.451	56	107042	5.985	ug/L	97
33) Benzene	5.833	78	854545	17.269	ug/L	100
34) Trichloroethene	6.553	95	87969932m	6396.592	ug/L	
35) Methylcyclohexane	6.824	83	370661m	19.209	ug/L	
40) 4-Methyl-2-pentanone	7.817	43	16559	2.155	ug/L #	90
42) Toluene	7.991	91	262911	4.984	ug/L	97
45) 1,1,2-Trichloroethane	8.412	97	865573	95.389	ug/L	97
47) Tetrachloroethene	8.566	164	174494	18.358	ug/L	97
51) Chlorobenzene	9.454	112	178129	5.098	ug/L	97
52) Ethylbenzene	9.579	91	191878	3.251	ug/L	99
53) m,p-Xylene	9.704	106	58706	2.688	ug/L	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

54) o-Xylene	10.106	106	437086	20.338	ug/L	97
60) Isopropylbenzene	10.486	105	84723	1.346	ug/L	98
61) 1,2,3-Trichloropropane	10.823	75	13733	1.533	ug/L	99
62) 1,3,5-Trimethylbenzene	11.090	105	114837	2.193	ug/L	99
63) 1,2,4-Trimethylbenzene	11.470	105	475603	9.215	ug/L	98
64) 1,3-Dichlorobenzene	11.746	146	48509	1.605	ug/L	97
65) 1,4-Dichlorobenzene	11.836	146	713441	23.686	ug/L	98
67) 1,2-Dichlorobenzene	12.212	146	156073	5.508	ug/L	98
70) 1,2,4-trichlorobenzene	13.839	180	2697851	125.976	ug/L	97
72) 1,2,3-Trichlorobenzene	14.328	180	804660	43.289	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055206.D
 Acq On : 07 Sep 2023 23:44
 Operator : MD/SY
 Sample : 04306-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH4H7

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 09/08/2023
 Supervised By :Mahesh Dadoda 09/14/2023

Quant Time: Sep 08 06:37:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 06:18:43 2023
 Response via : Initial Calibration

