

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
 Data File : VU055182.D
 Acq On : 07 Sep 2023 12:37
 Operator : MD/SY
 Sample : 04230-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Sep 08 05:06:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 08 05:04:57 2023
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.248	114	159865	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.418	117	168190	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.814	152	81927	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.595	65	40444	5.398	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.000%	
7) Chloroethane-d5		1.907	69	45868	5.289	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.800%	
11) 1,1-Dichloroethene-d2		2.563	65	21383	5.009	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.200%	
20) 2-Butanone-d5		4.624	46	119133	54.792	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.580%	
24) Chloroform-d		5.062	84	100946	5.077	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4		5.701	65	51539	5.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%	
32) Benzene-d6		5.724	84	199247	4.799	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6		6.689	67	68176	5.163	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%	
41) Toluene-d8		7.898	98	174457	4.562	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.200%	
43) trans-1,3-Dichloroprop...		8.180	79	16387	4.506	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.200%	
46) 2-Hexanone-d5		8.634	63	68785	46.593	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.180%	
56) 1,1,2,2-Tetrachloroeth...		10.756	84	47352	5.099	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.000%	
66) 1,2-Dichlorobenzene-d4		12.193	152	60623	5.070	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%	
Target Compounds							
16) Methylene chloride		3.042	84	3631	0.322	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU090723\
Data File : VU055182.D
Acq On : 07 Sep 2023 12:37
Operator : MD/SY
Sample : 04230-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Sep 08 05:06:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR090123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 08 05:04:57 2023
Response via : Initial Calibration

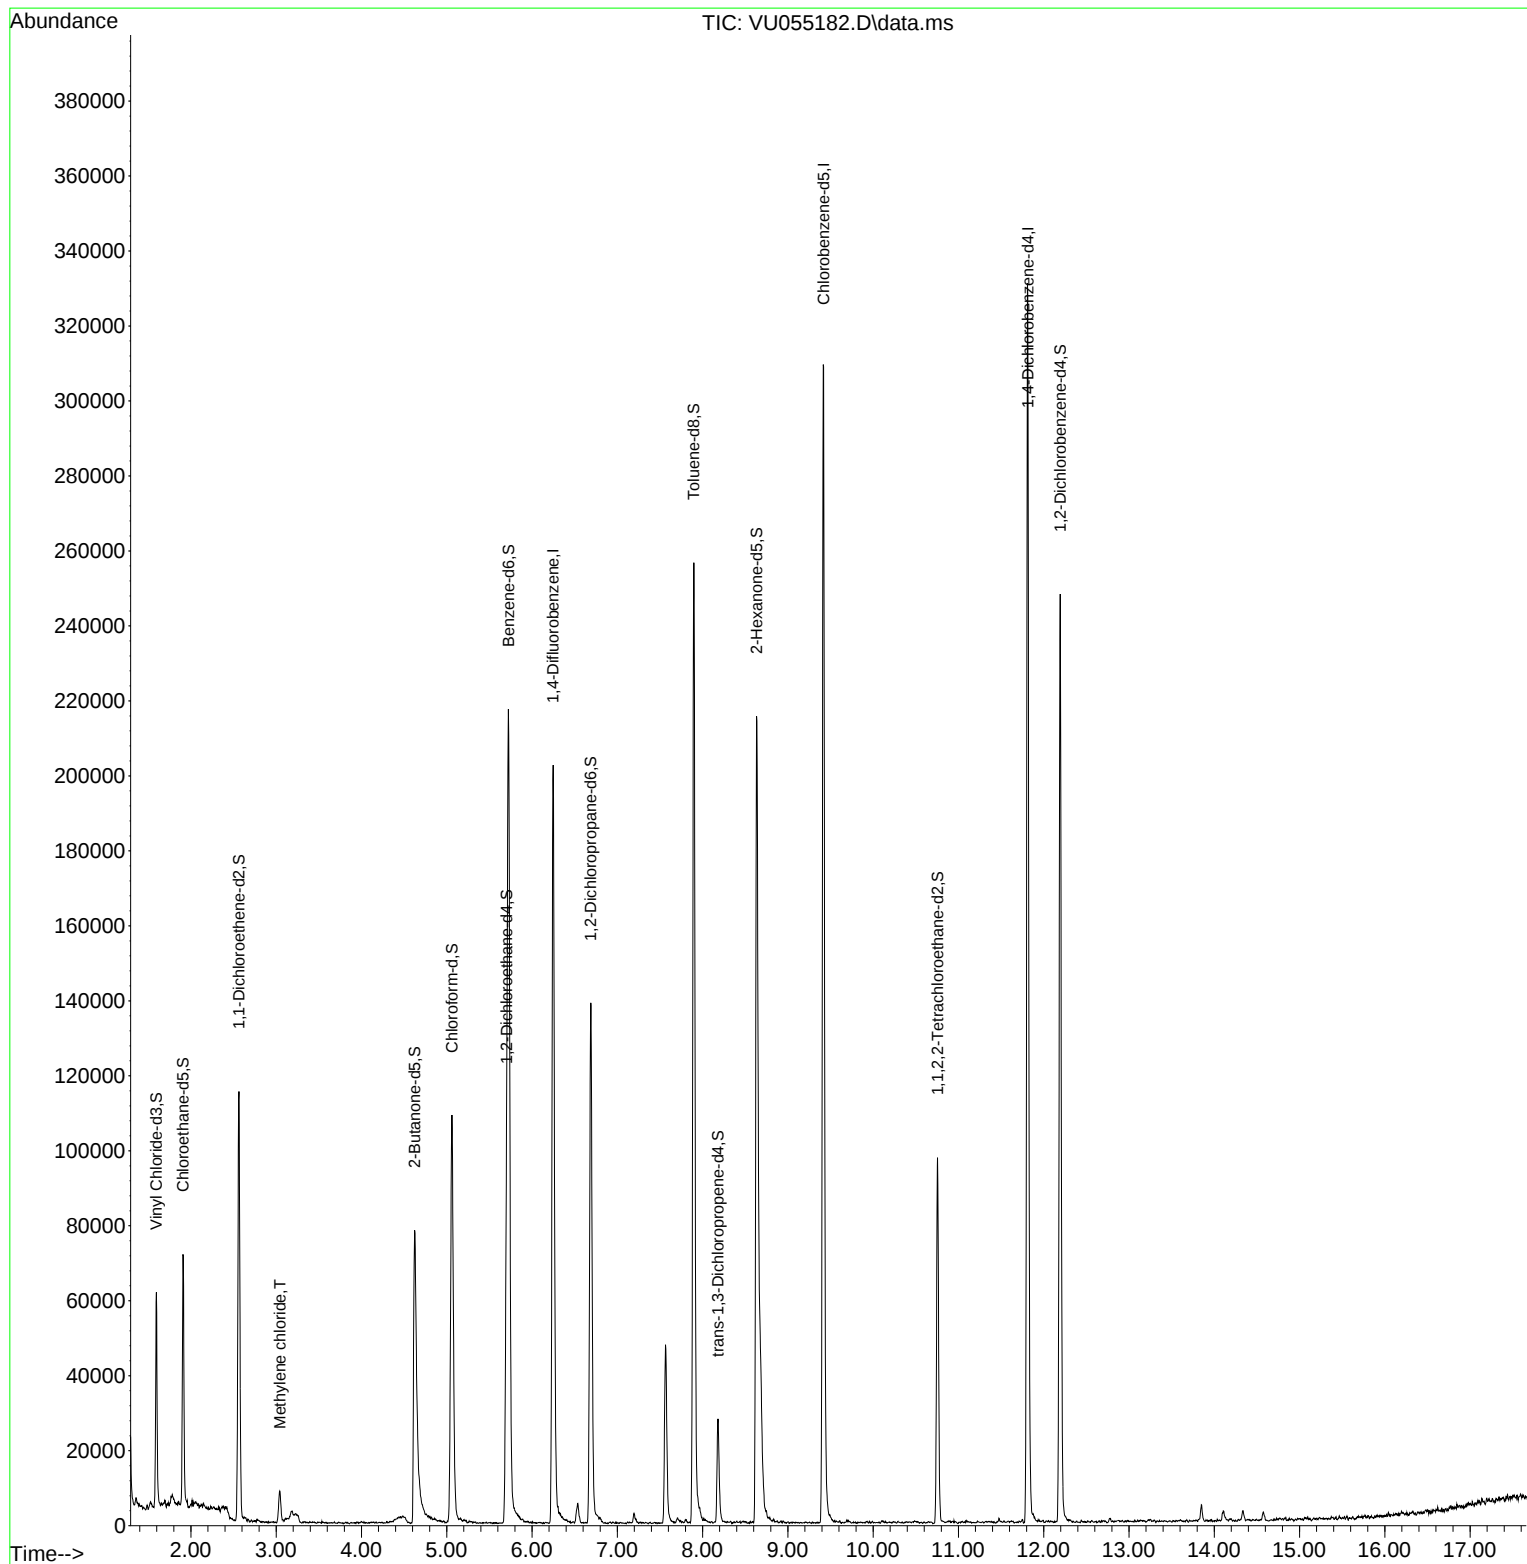

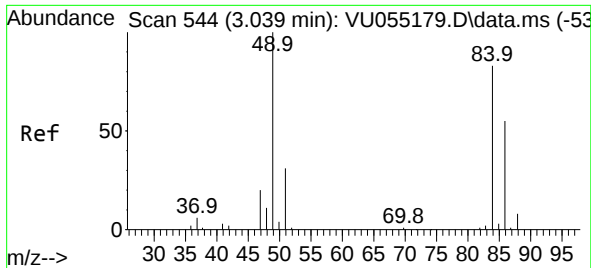

#16
Methylene chloride
Concen: 0.322 ug/L
RT: 3.042 min Scan# 54
Delta R.T. 0.003 min
Lab File: VU055182.D
Acq: 07 Sep 2023 12:37

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

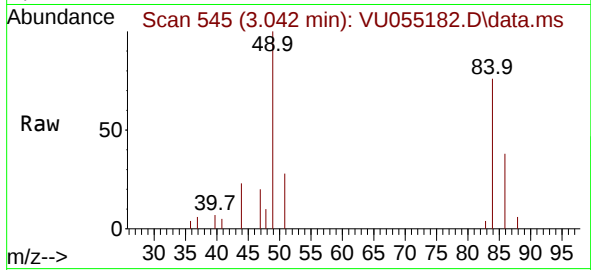

Tgt Ion:	84	Resp:	3631
Ion	Ratio	Lower	Upper
84	100		
86	49.9	43.4	80.6
49	132.2	87.7	162.9

